

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031919\
 Data File : PD051877.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Mar 2019 8:37
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 11:03:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	29650677	616.1E6	22.362	21.485
28)	SA Decachlor...	7.821	9.154	24476516	375.9E6	21.533	20.577
Target Compounds							
4)	MA Heptachlor	0.000	5.238	0	3217695	N.D.	0.084 #
7)	B delta-BHC	0.000	5.086f	0	23587208	N.D.	0.686 #
8)	B Heptachlo...	4.873f	5.922	867102	35638358	0.441	1.111 #
10)	B gamma-Chl...	0.000	6.166	0	151.3E6	N.D.	4.732 #
12)	B 4,4'-DDE	0.000	6.412f	0	18108150	N.D.	0.585 #
14)	MA Endrin	0.000	6.759	0	21134473	N.D.	0.809 #
15)	B Endosulfa...	0.000	6.983	0	761379	N.D.	0.030 #
17)	MA 4,4'-DDT	0.000	7.159f	0	946156	N.D.	0.047 #
22)	Mirex	0.000	8.269	0	2702441	N.D.	0.175 #
25)	Chlordane-3	0.000	6.166	0	151.3E6	N.D.	33.981 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031919\
Data File : PD051877.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Mar 2019 8:37
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 11:03:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

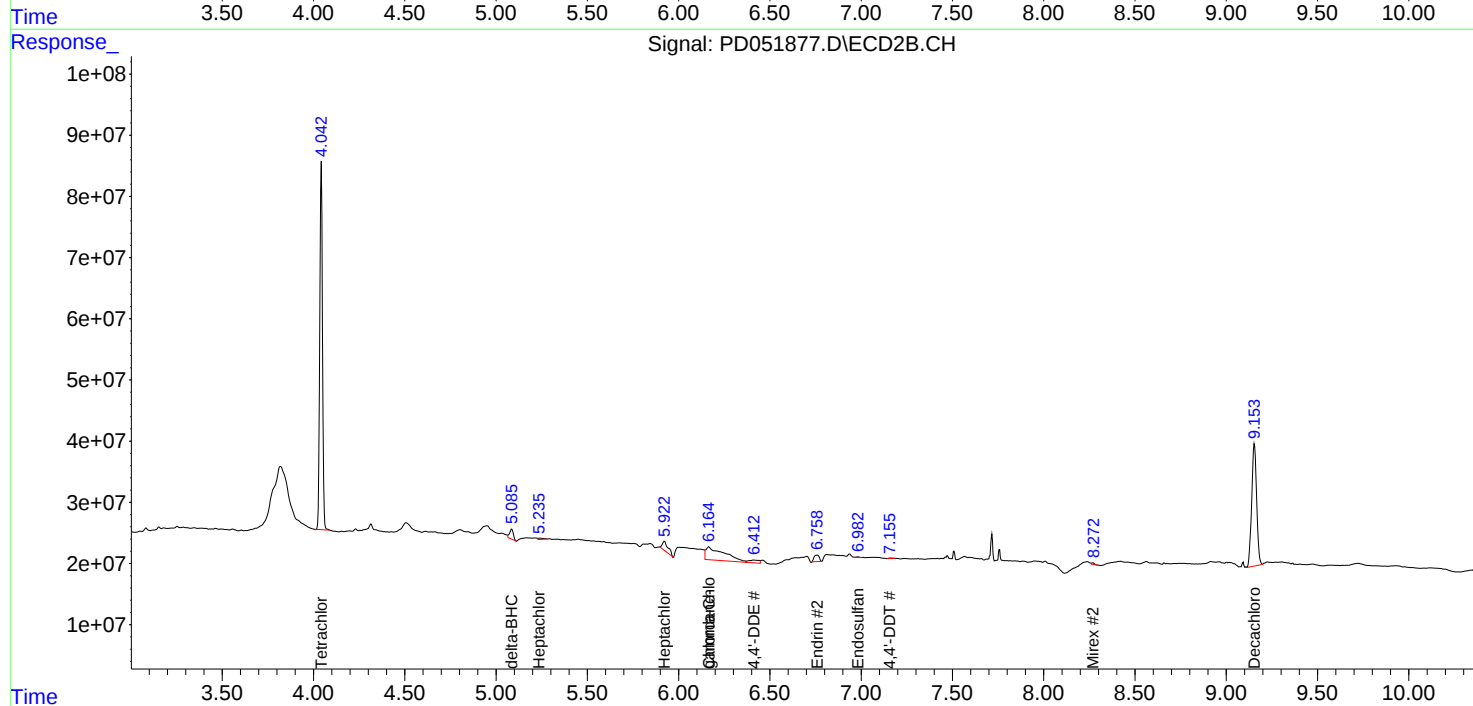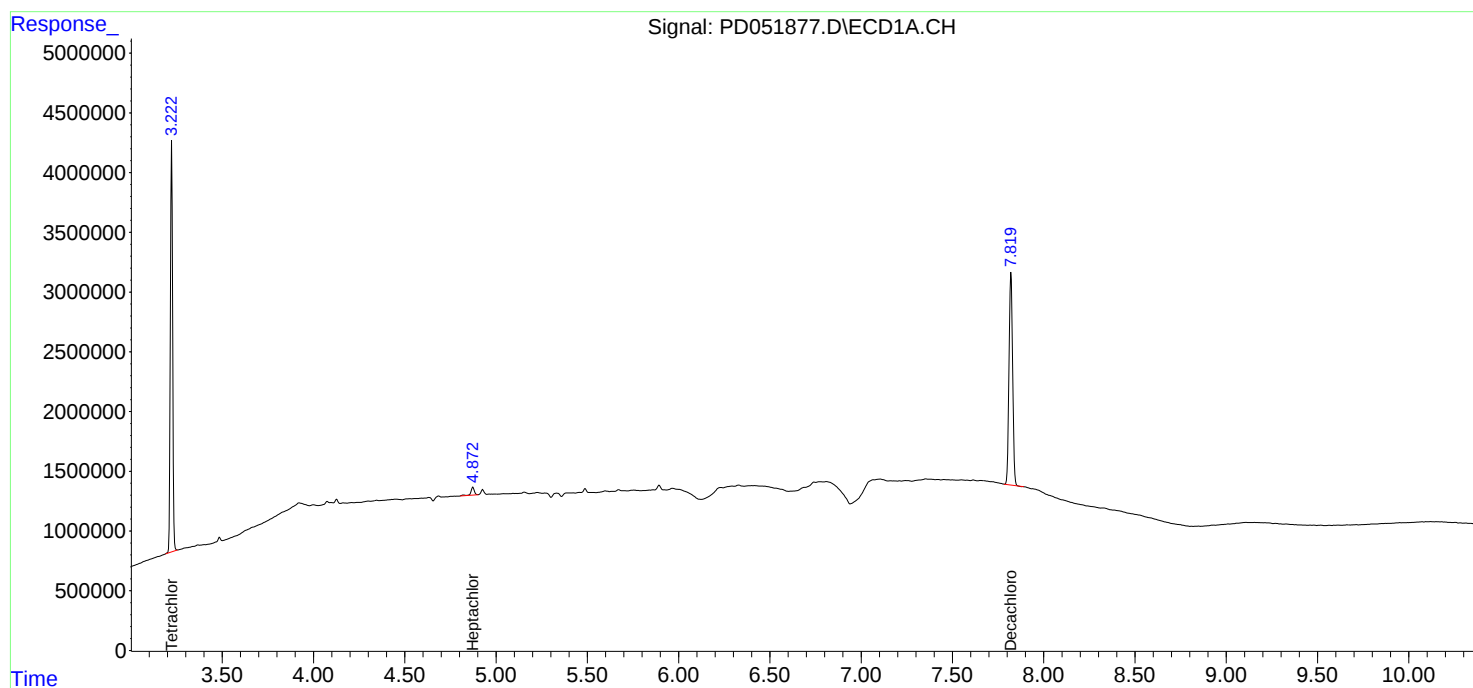


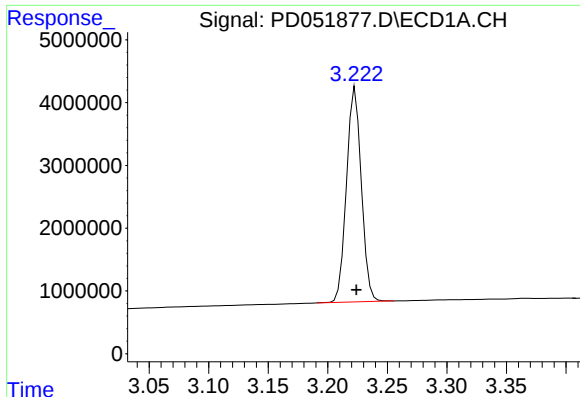

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 29650677
Conc: 22.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

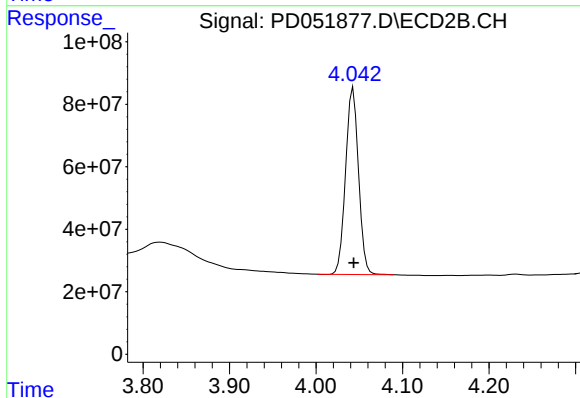


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 616114470
Conc: 21.48 ng/ml

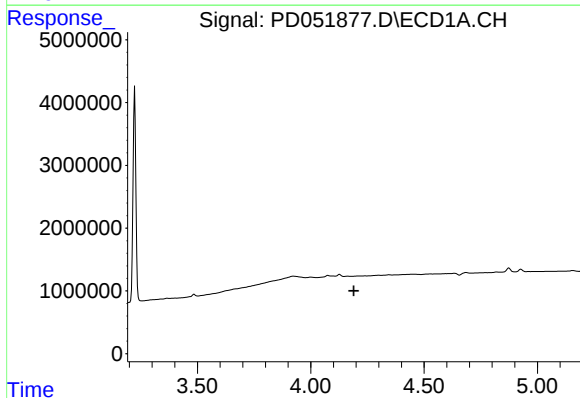


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.190 min
Response: 0
Conc: N.D.

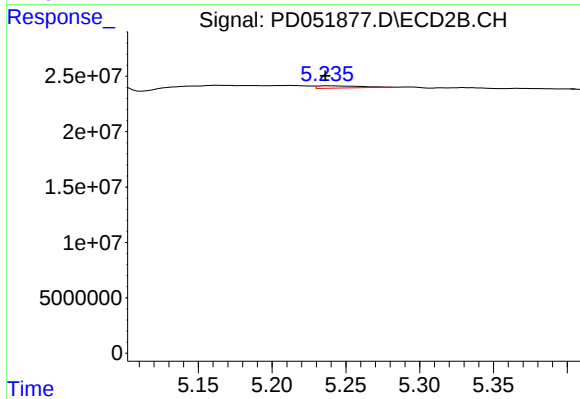

#4 Heptachlor


R.T.: 5.238 min
Delta R.T.: 0.002 min
Response: 3217695
Conc: 0.08 ng/ml

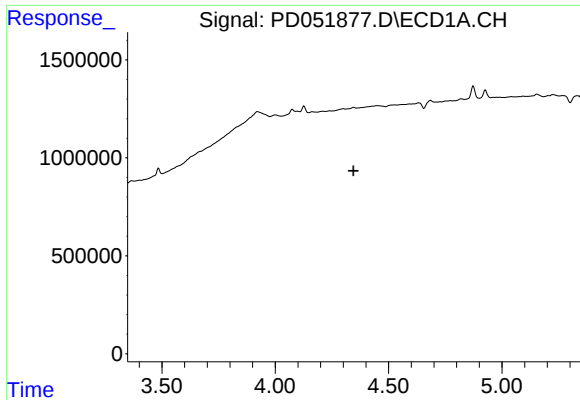

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

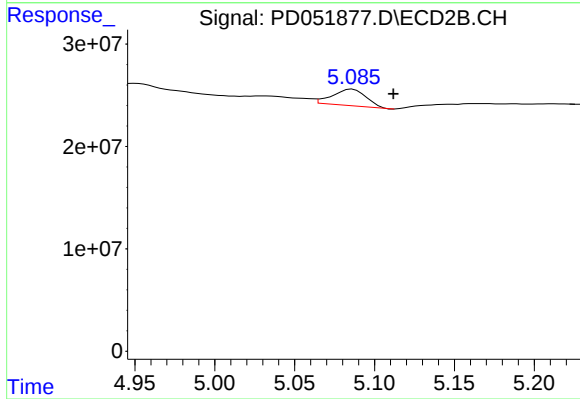


#7 delta-BHC

R.T.: 5.086 min
Delta R.T.: -0.026 min
Response: 23587208
Conc: 0.69 ng/ml

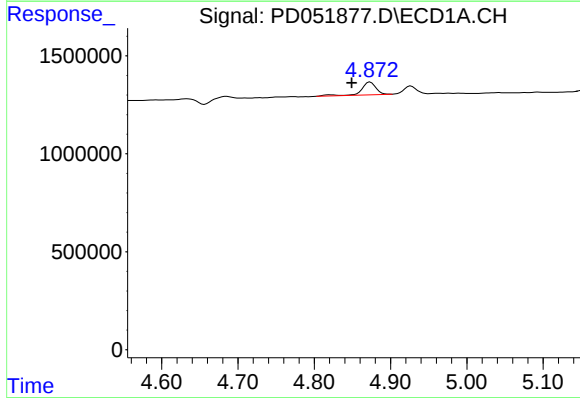


#8 Heptachlor epoxide

R.T.: 4.873 min
Delta R.T.: 0.024 min
Response: 867102
Conc: 0.44 ng/ml

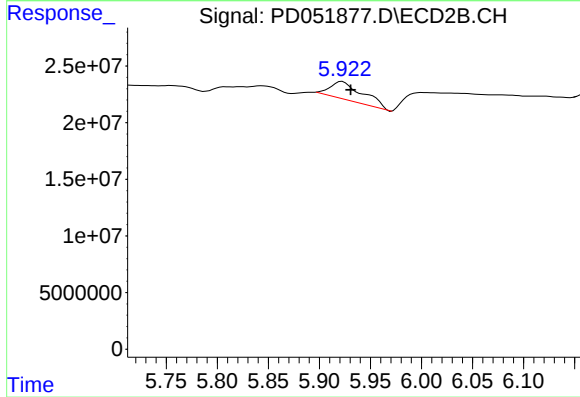

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 35638358
Conc: 1.11 ng/ml

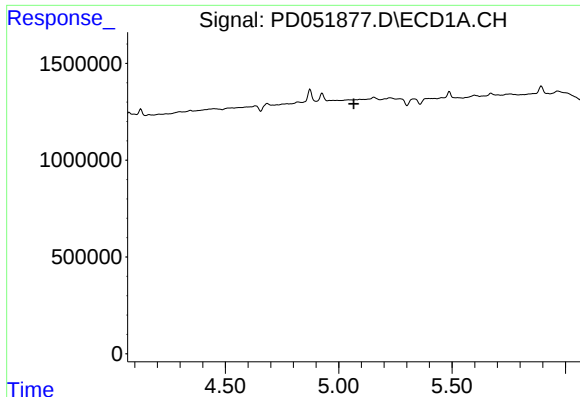

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

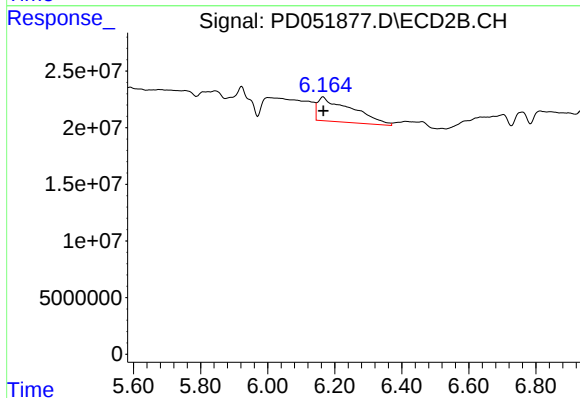


#10 gamma-Chlordane

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 151319441
Conc: 4.73 ng/ml

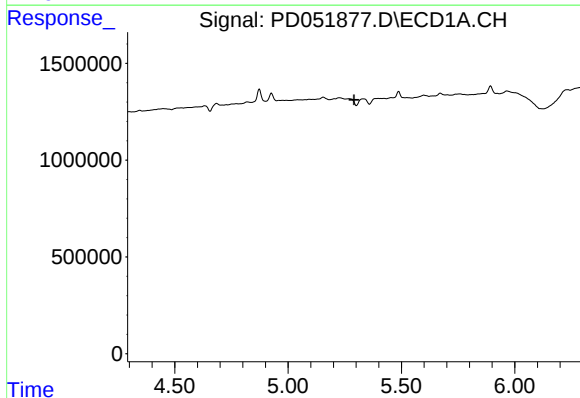


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.292 min
Response: 0
Conc: N.D.

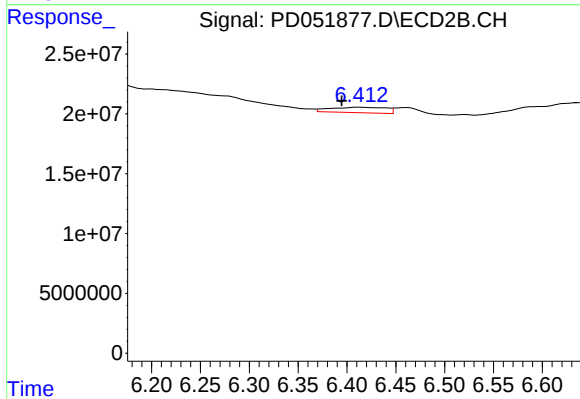

#12 4,4'-DDE


R.T.: 6.412 min
Delta R.T.: 0.018 min
Response: 18108150
Conc: 0.59 ng/ml

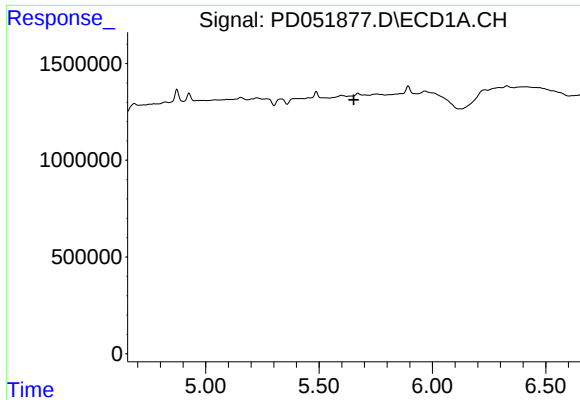

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.653 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

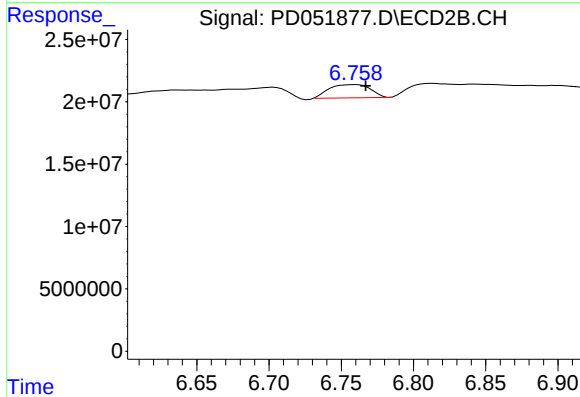


#14 Endrin

R.T.: 6.759 min
Delta R.T.: -0.008 min
Response: 21134473
Conc: 0.81 ng/ml

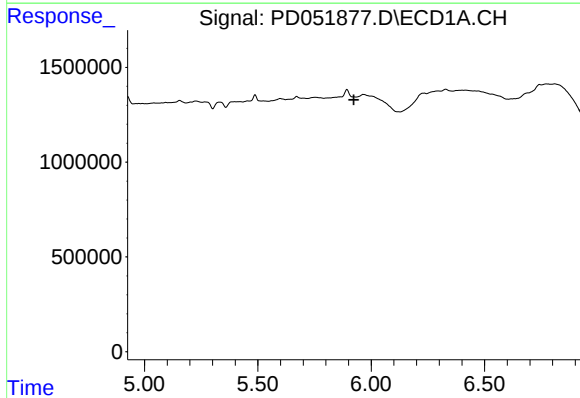


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.923 min
Response: 0
Conc: N.D.

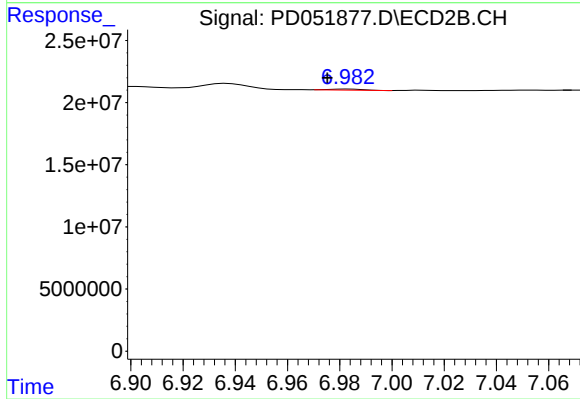

#15 Endosulfan II


R.T.: 6.983 min
Delta R.T.: 0.008 min
Response: 761379
Conc: 0.03 ng/ml

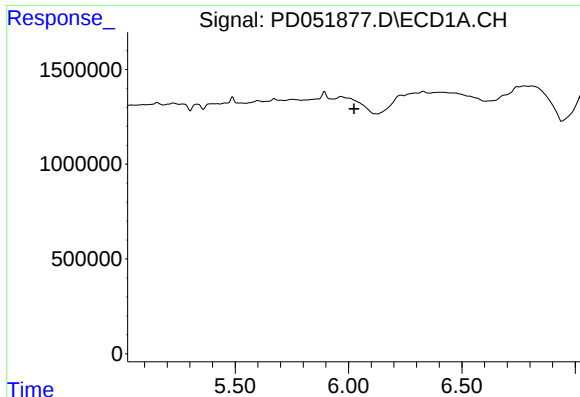

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

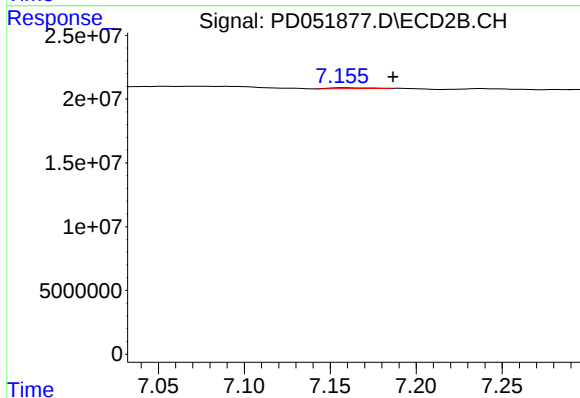


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: -0.028 min
Response: 946156
Conc: 0.05 ng/ml

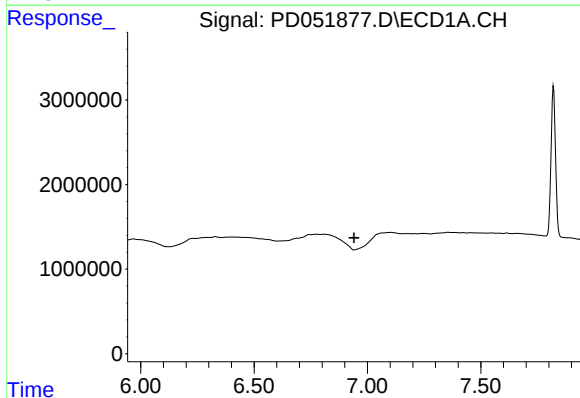


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 6.942 min
Response: 0
Conc: N.D.

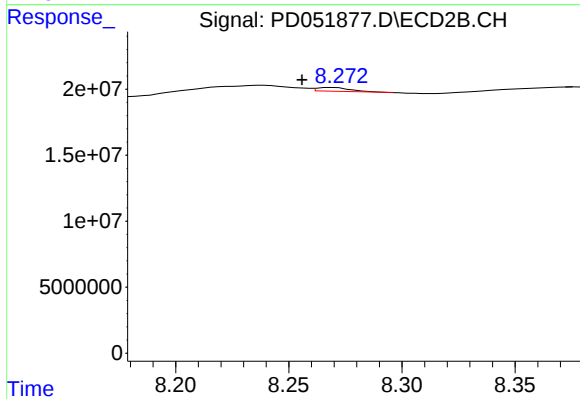

#22 Mirex


R.T.: 8.269 min
Delta R.T.: 0.014 min
Response: 2702441
Conc: 0.17 ng/ml

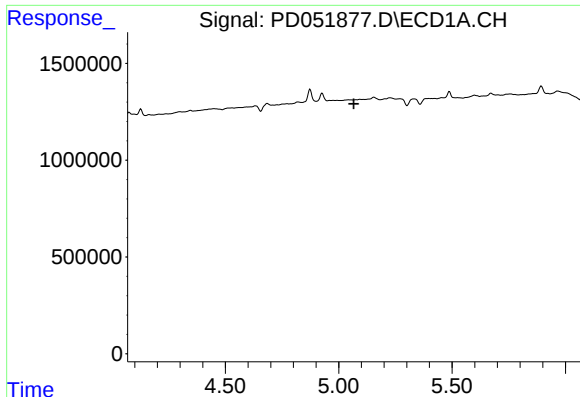

#25 Chloroform-3


R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

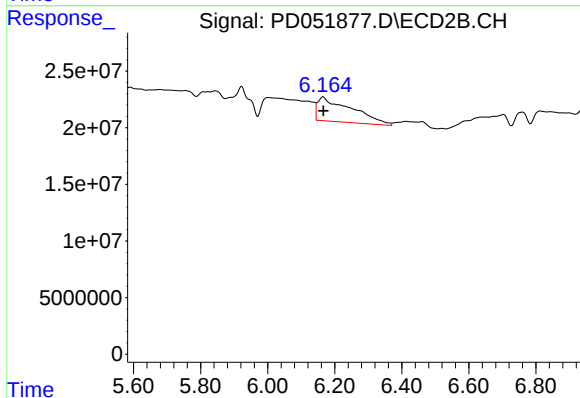


#25 Chloroform-3

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 151319441
Conc: 33.98 ng/ml

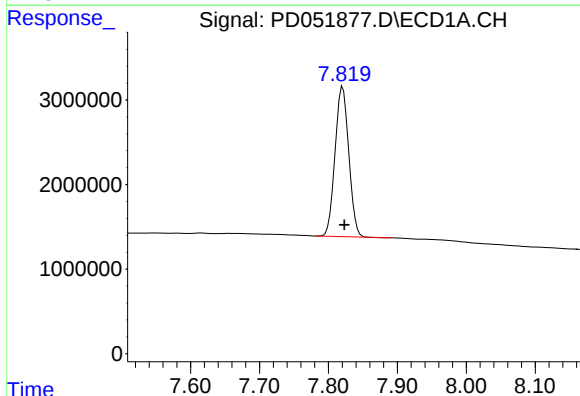

#28 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: -0.003 min
Response: 24476516
Conc: 21.53 ng/ml

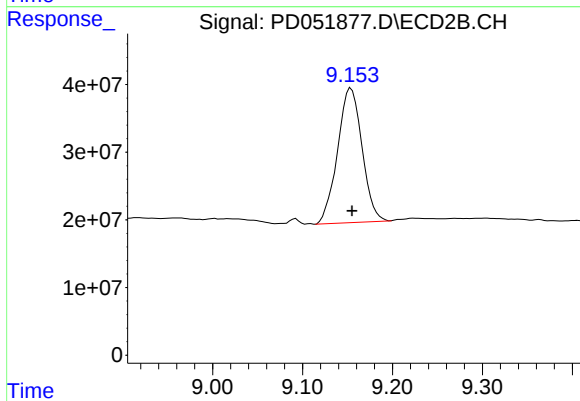

#28 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.001 min
Response: 375876009
Conc: 20.58 ng/ml