

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031924\
 Data File : PD082192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2024 04:02
 Operator : AR\AJ
 Sample : INDA6081
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA6081

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/19/2024
 Supervised By : Ankita Jodhani 03/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:10:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 19 06:10:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.778	243.7E6	356.9E6	164.685	159.946
27)	SA Decachlor...	9.124	7.912	540.3E6	670.4E6	298.410	317.011
Target Compounds							
2)	A alpha-BHC	4.024	3.278	475.4E6	591.1E6	185.386	177.429
3)	MA gamma-BHC...	4.359	3.607	434.8E6	522.2E6	178.692	173.395
4)	MA Heptachlor	4.951	3.946	407.9E6	471.3E6	167.539	166.025
9)	A Endosulfan I	6.110	5.097	340.8E6	405.0E6	162.065	165.921
13)	MA Dieldrin	6.386	5.361	755.4E6	890.0E6	344.550	334.225
14)	MA Endrin	6.616	5.635	569.4E6	712.6E6	343.239	332.531m
16)	A 4,4'-DDD	6.749	5.784	539.6E6	679.6E6	348.242	334.010
17)	MA 4,4'-DDT	7.064	6.035	538.5E6	707.9E6	352.667	344.593
20)	A Methoxychlor	7.541	6.610	1232.5E6	1475.5E6	1587.342	1429.805

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031924\
Data File : PD082192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2024 04:02
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:10:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 19 06:10:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

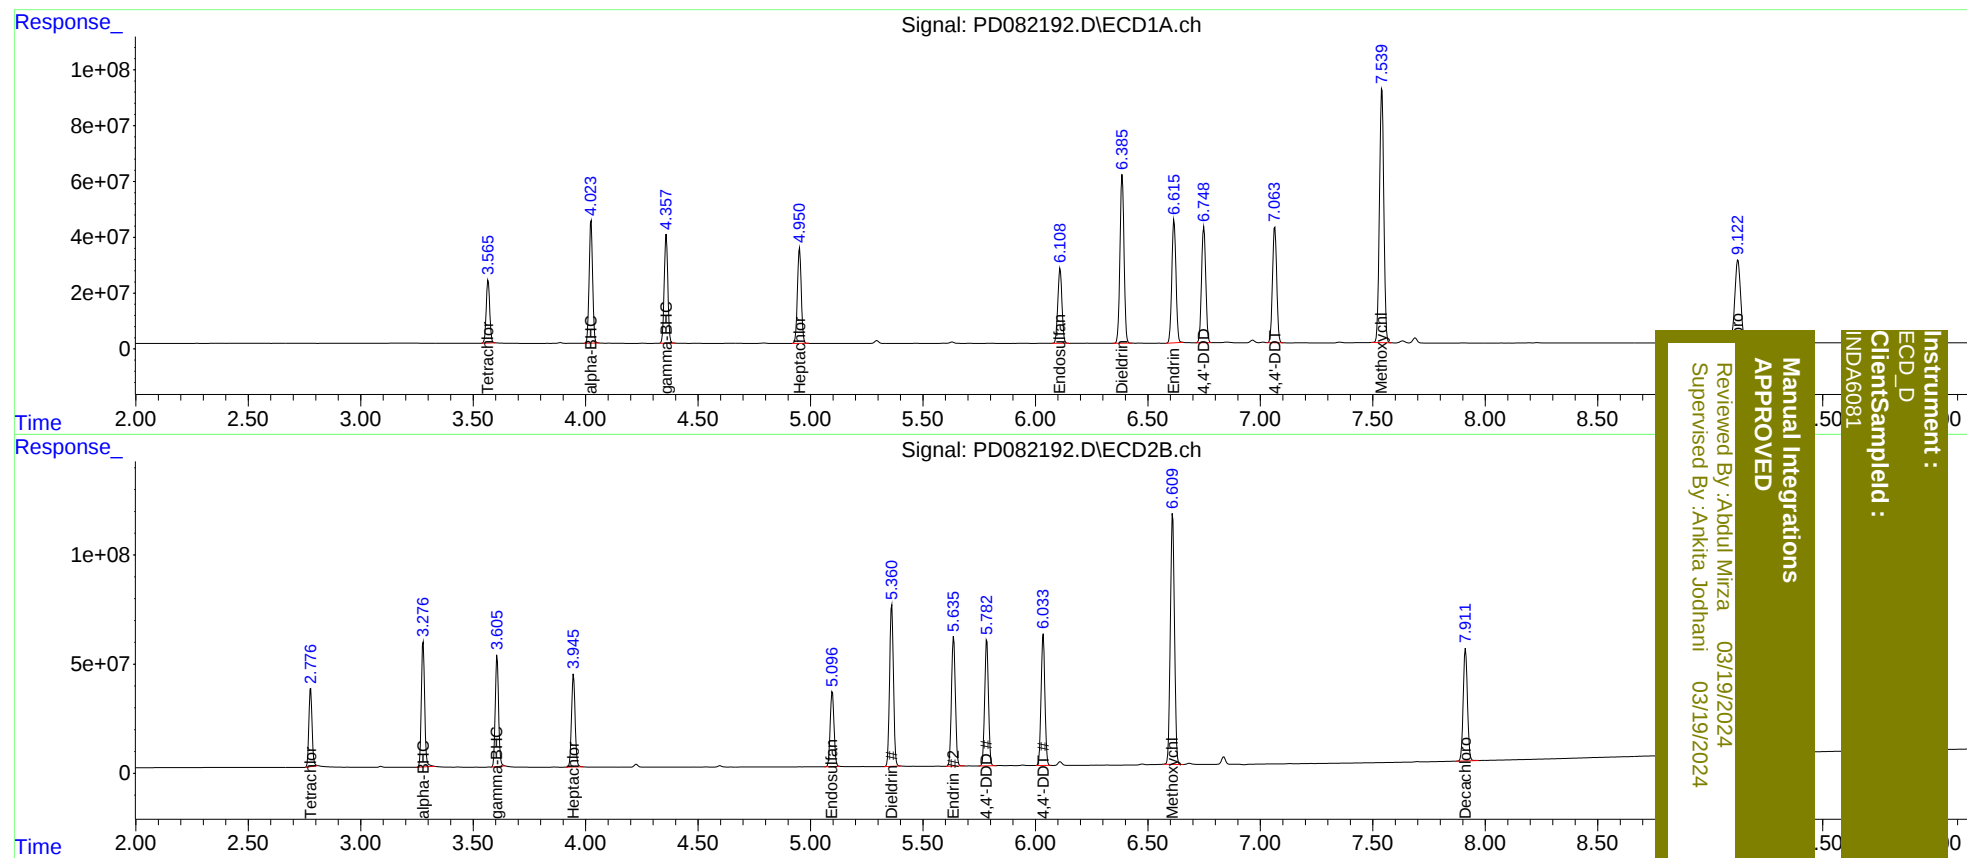

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/19/2024
Supervised By: Ankita Jodhani 03/19/2024

Instrument :
ECD_D
Client Sampled :
INDA6081