

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
 Data File : PD051893.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 9:06
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 11:16:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4) MA	Heptachlor	4.169f	5.238	677977	1140267	0.316 0.030 #
6) B	beta-BHC	4.169	0.000	677977	0	0.770 N.D. #
7) B	delta-BHC	0.000	5.135f	0	2031334	N.D. 0.059 #
8) B	Heptachlo...	0.000	5.922	0	6398680	N.D. 0.200 #
9) A	Endosulfan I	0.000	6.285	0	16097574	N.D. 0.543 #
12) B	4,4'-DDE	0.000	6.388	0	16846940	N.D. 0.545 #
17) MA	4,4'-DDT	0.000	7.192	0	24174393	N.D. 1.193 #
18) B	Endrin al...	0.000	7.096	0	617931	N.D. 0.029 #
21) B	Endrin ke...	0.000	7.794	0	3352166	N.D. 0.148 #
24)	Chlordane-2	4.509f	0.000	8788377	0	112.287 N.D. #
27)	Chlordane-5	0.000	7.079f	0	1156759	N.D. 1.142 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
Data File : PD051893.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 9:06
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 11:16:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

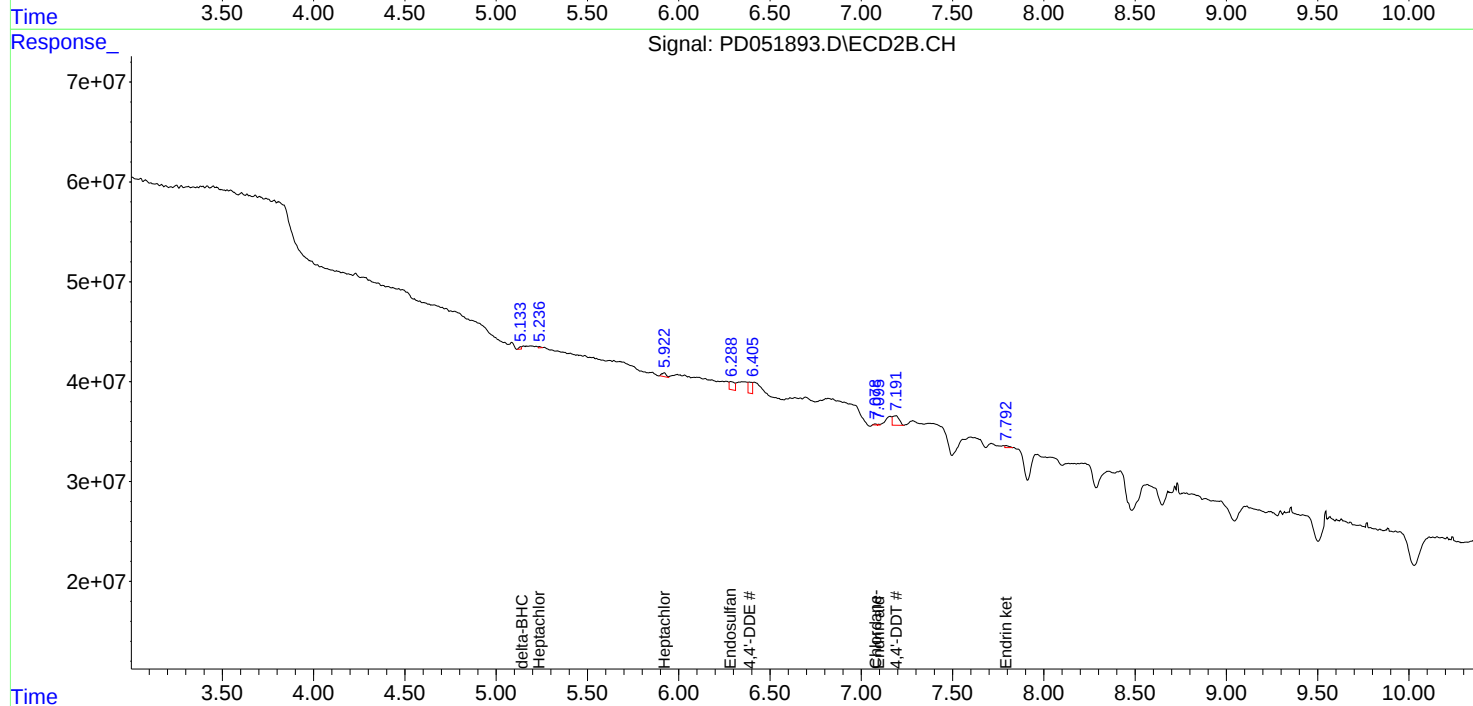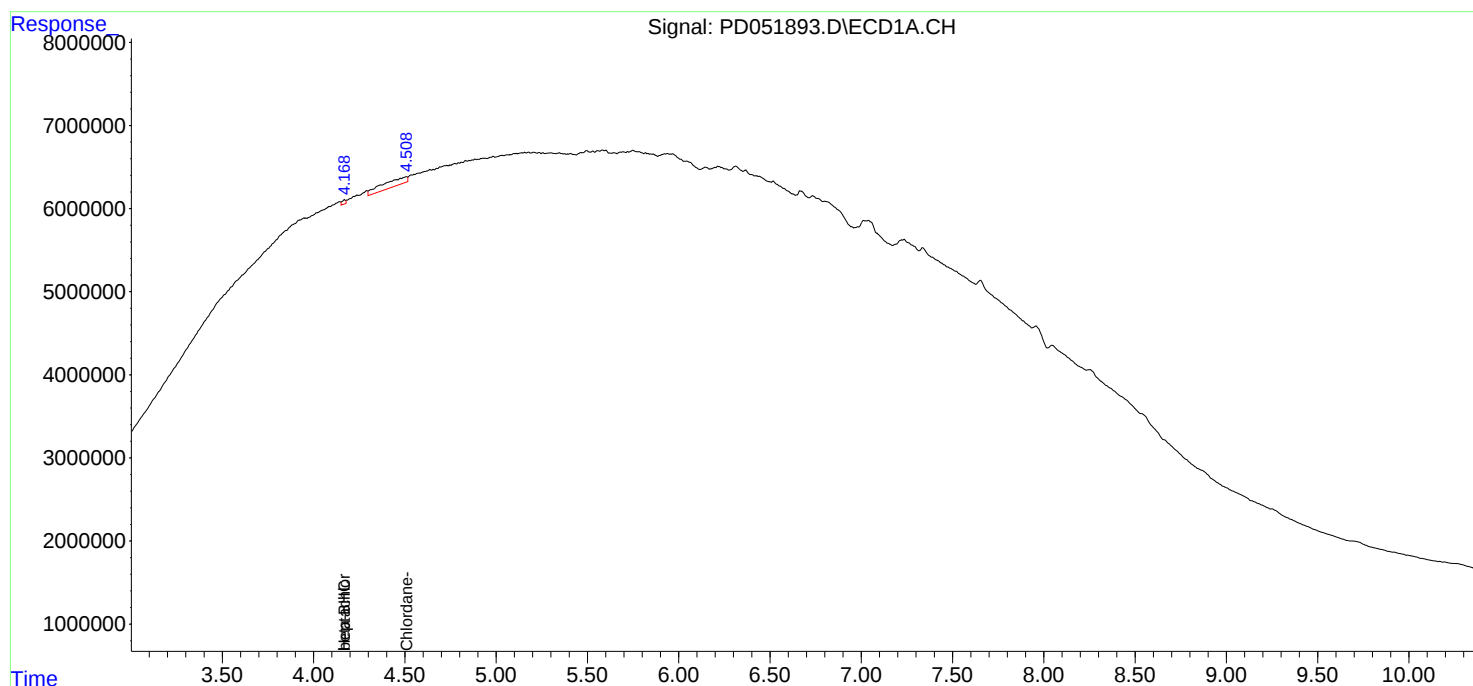


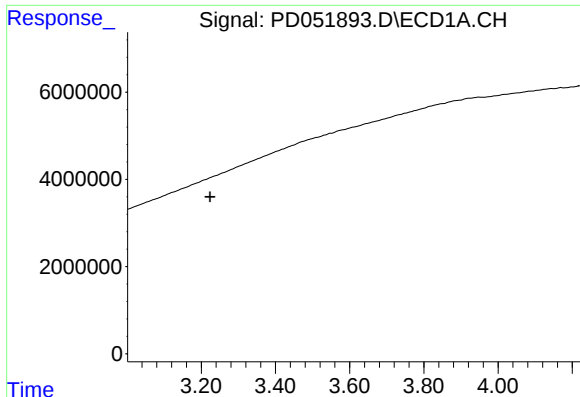

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.224 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

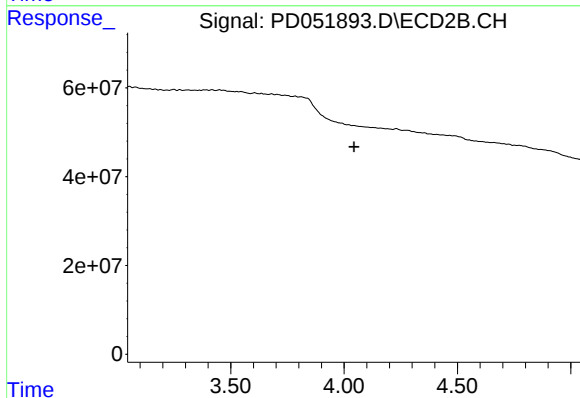


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.044 min
Response: 0
Conc: N.D.

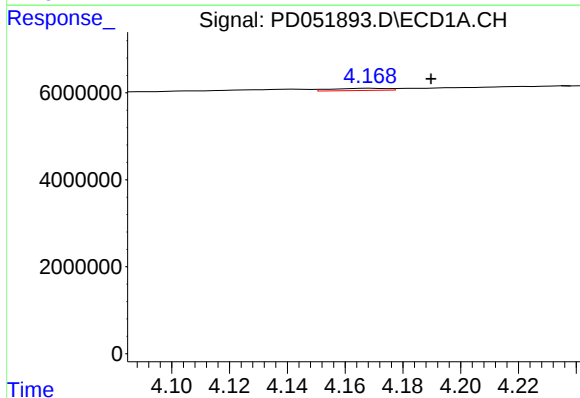


#4 Heptachlor

R.T.: 4.169 min
Delta R.T.: -0.020 min
Response: 677977
Conc: 0.32 ng/ml

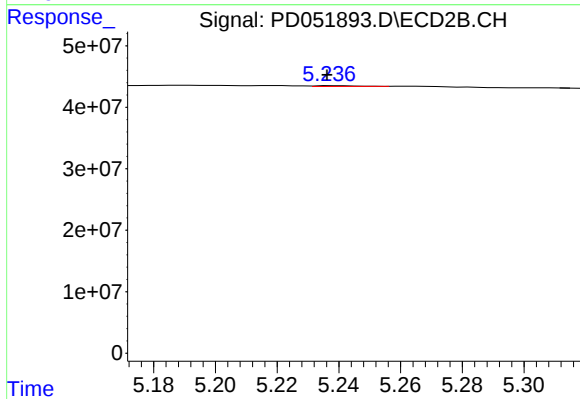

#4 Heptachlor


R.T.: 5.238 min
Delta R.T.: 0.001 min
Response: 1140267
Conc: 0.03 ng/ml

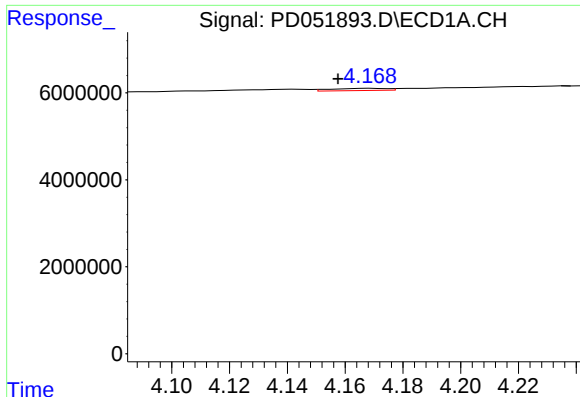

#6 beta-BHC


R.T.: 4.169 min
Delta R.T.: 0.012 min
Response: 677977
Conc: 0.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

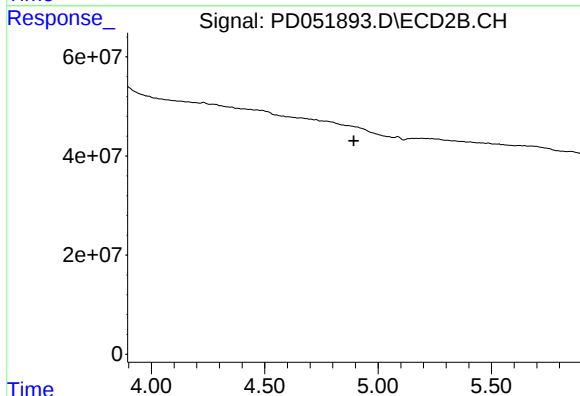


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

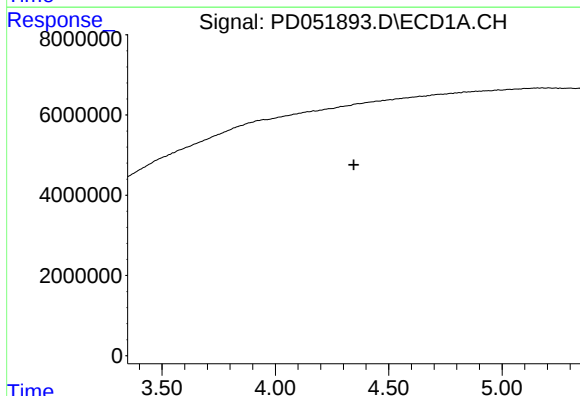


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.346 min
Response: 0
Conc: N.D.

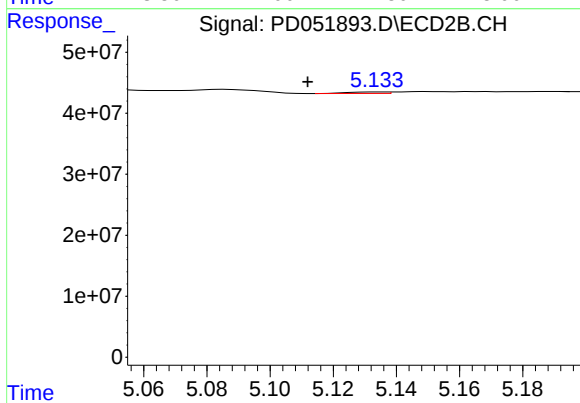

#7 delta-BHC


R.T.: 5.135 min
Delta R.T.: 0.023 min
Response: 2031334
Conc: 0.06 ng/ml

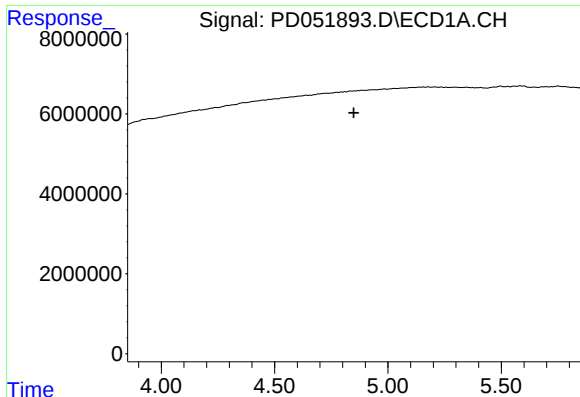

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.849 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

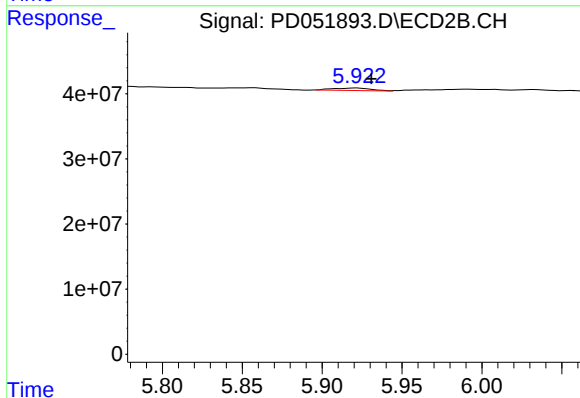


#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.009 min
Response: 6398680
Conc: 0.20 ng/ml

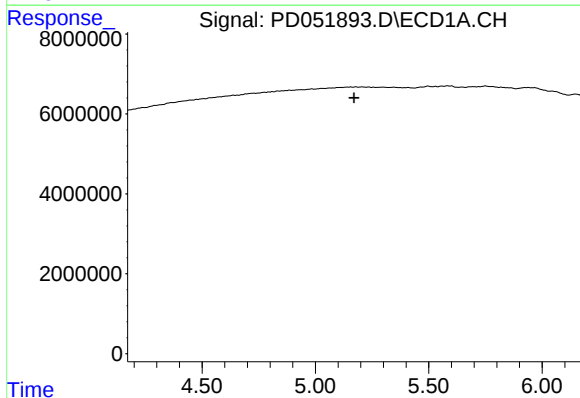


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.170 min
Response: 0
Conc: N.D.

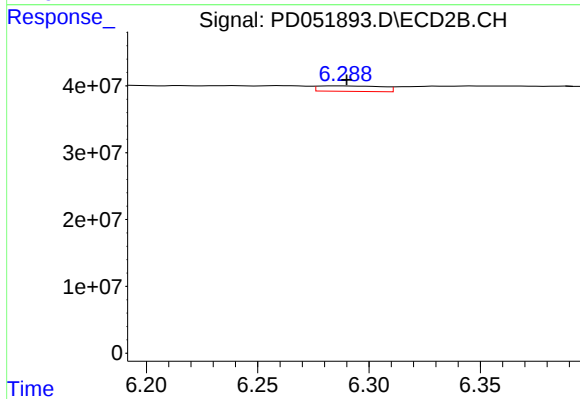

#9 Endosulfan I


R.T.: 6.285 min
Delta R.T.: -0.005 min
Response: 16097574
Conc: 0.54 ng/ml

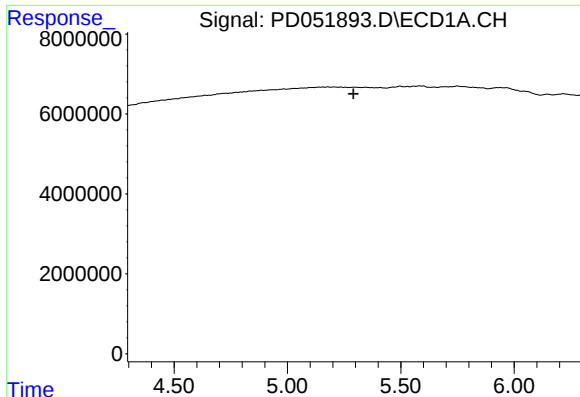

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.292 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

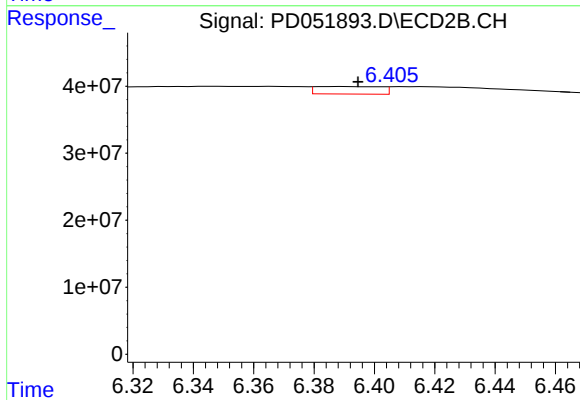


#12 4,4'-DDE

R.T.: 6.388 min
Delta R.T.: -0.006 min
Response: 16846940
Conc: 0.54 ng/ml

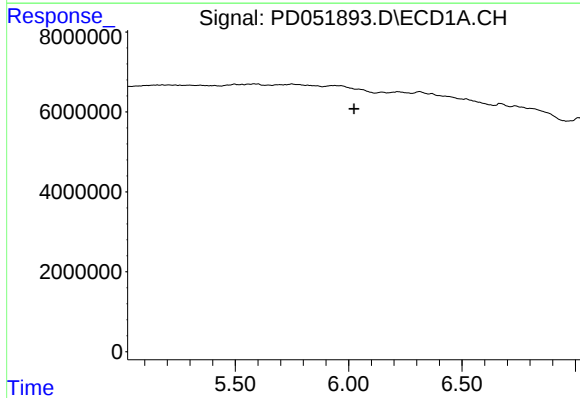


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

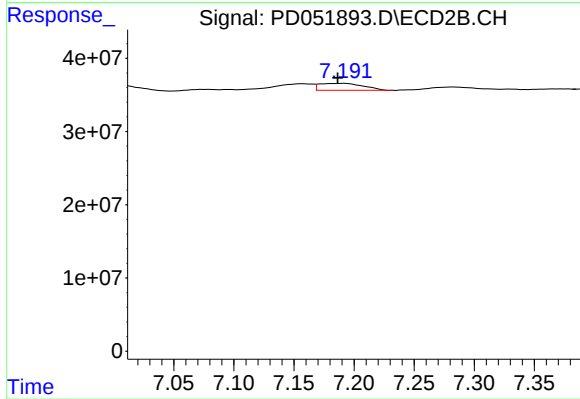

#17 4,4'-DDT


R.T.: 7.192 min
Delta R.T.: 0.006 min
Response: 24174393
Conc: 1.19 ng/ml

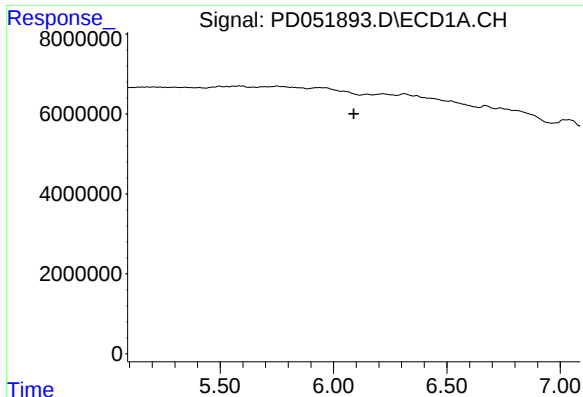

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

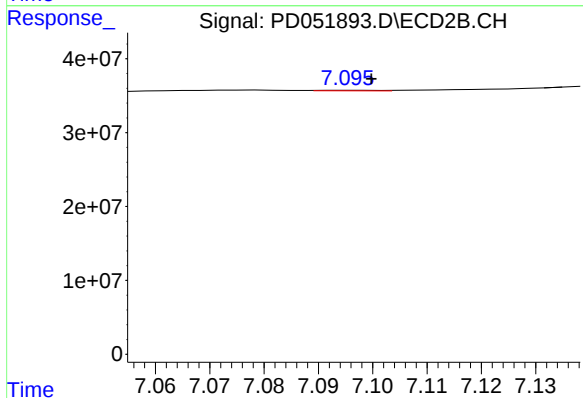


#18 Endrin aldehyde

R.T.: 7.096 min
Delta R.T.: -0.003 min
Response: 617931
Conc: 0.03 ng/ml

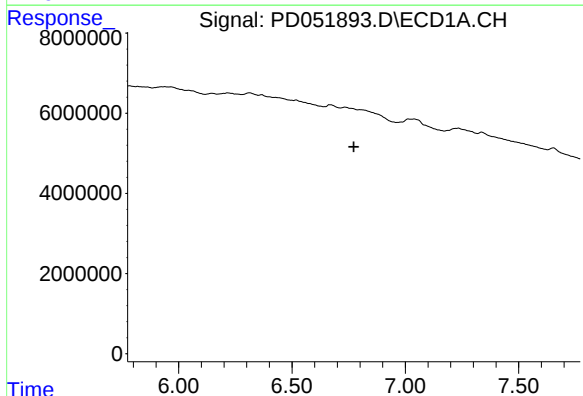


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.773 min
Response: 0
Conc: N.D.

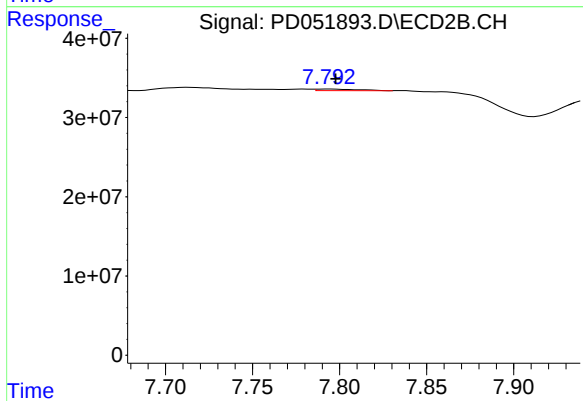

#21 Endrin ketone


R.T.: 7.794 min
Delta R.T.: -0.004 min
Response: 3352166
Conc: 0.15 ng/ml

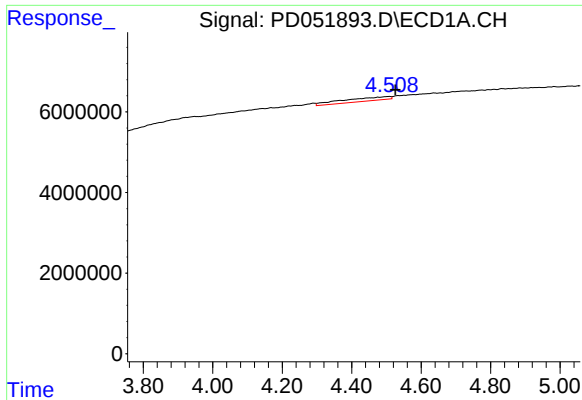

#24 Chlordane-2


R.T.: 4.509 min
Delta R.T.: -0.017 min
Response: 8788377
Conc: 112.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

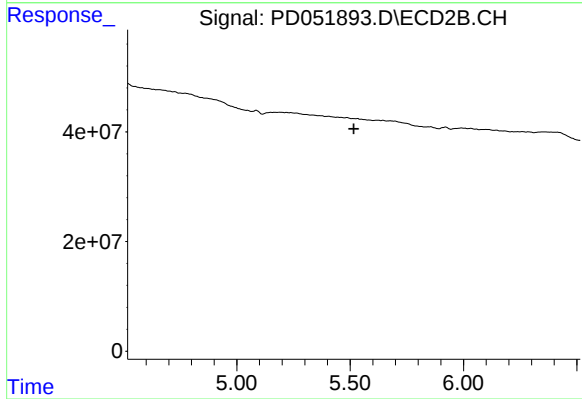


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.517 min
Response: 0
Conc: N.D.

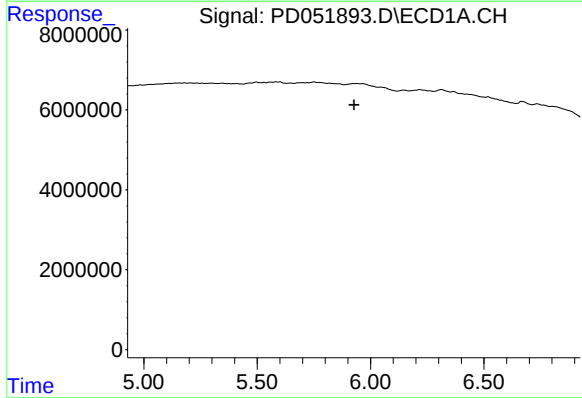


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.927 min
Response: 0
Conc: N.D.

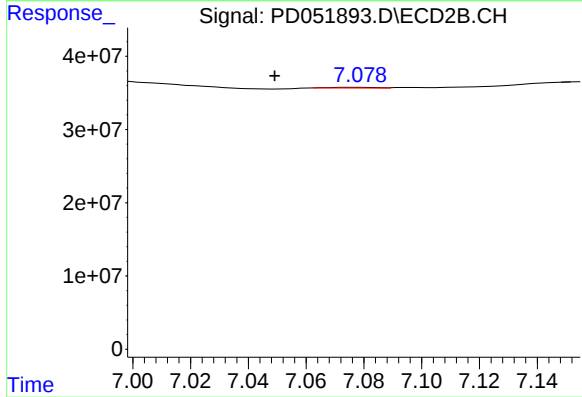

#27 Chlordane-5


R.T.: 7.079 min
Delta R.T.: 0.030 min
Response: 1156759
Conc: 1.14 ng/ml

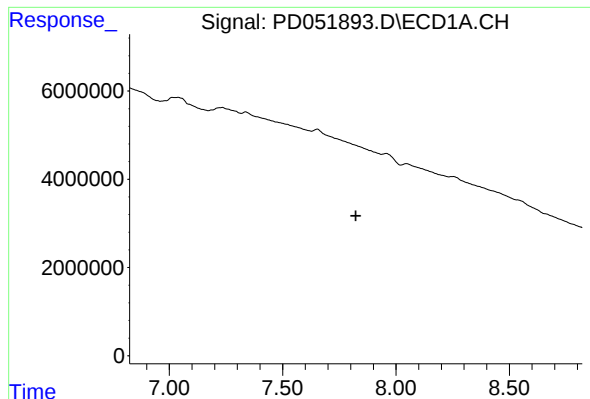

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

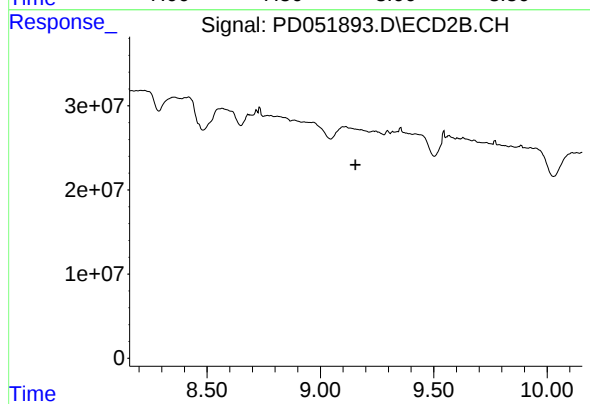

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.155 min
Response: 0
Conc: N.D.