

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
 Data File : PD051900.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 10:47
 Operator : AJ\SJ
 Sample : K1692-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-02-031819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 11:18:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	26416133	530.8E6	19.923	18.511
28)	SA Decachlor...	7.819	9.154	18019650	287.6E6	15.853	15.744
Target Compounds							
3)	MA gamma-BHC...	3.918	4.702f	4736870	9968224	2.267	0.252 #
4)	MA Heptachlor	0.000	5.246	0	4011350	N.D.	0.105 #
7)	B delta-BHC	0.000	5.087f	0	61443334	N.D.	1.788 #
8)	B Heptachlo...	0.000	5.918	0	11099061	N.D.	0.346 #
10)	B gamma-Chl...	0.000	6.170	0	4861335	N.D.	0.152 #
13)	MA Dieldrin	0.000	6.534	0	5131906	N.D.	0.166 #
14)	MA Endrin	0.000	6.771	0	978937	N.D.	0.037 #
15)	B Endosulfa...	0.000	6.983	0	19147684	N.D.	0.743 #
25)	Chlordane-3	0.000	6.170	0	4861335	N.D.	1.092 #
27)	Chlordane-5	0.000	7.044	0	507391	N.D.	0.501 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
Data File : PD051900.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 10:47
Operator : AJ\SJ
Sample : K1692-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 11:18:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

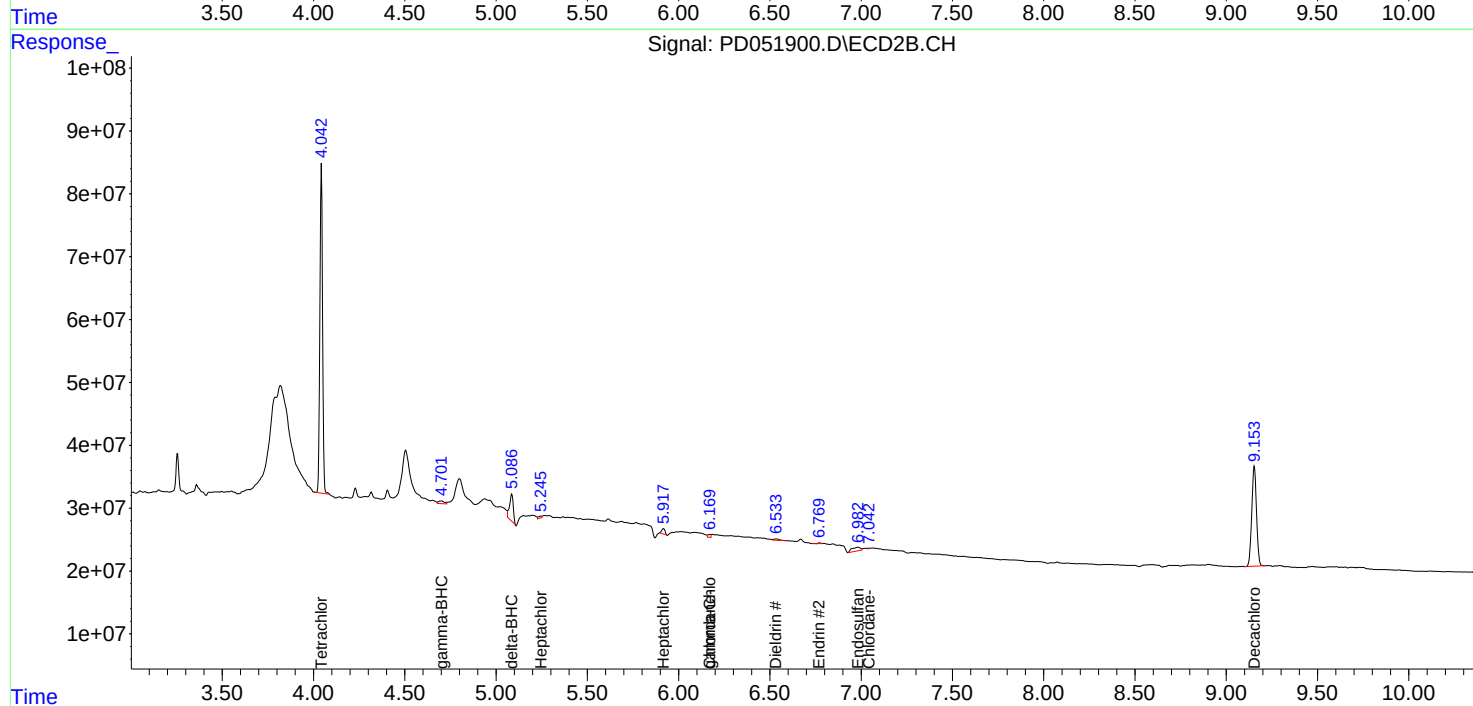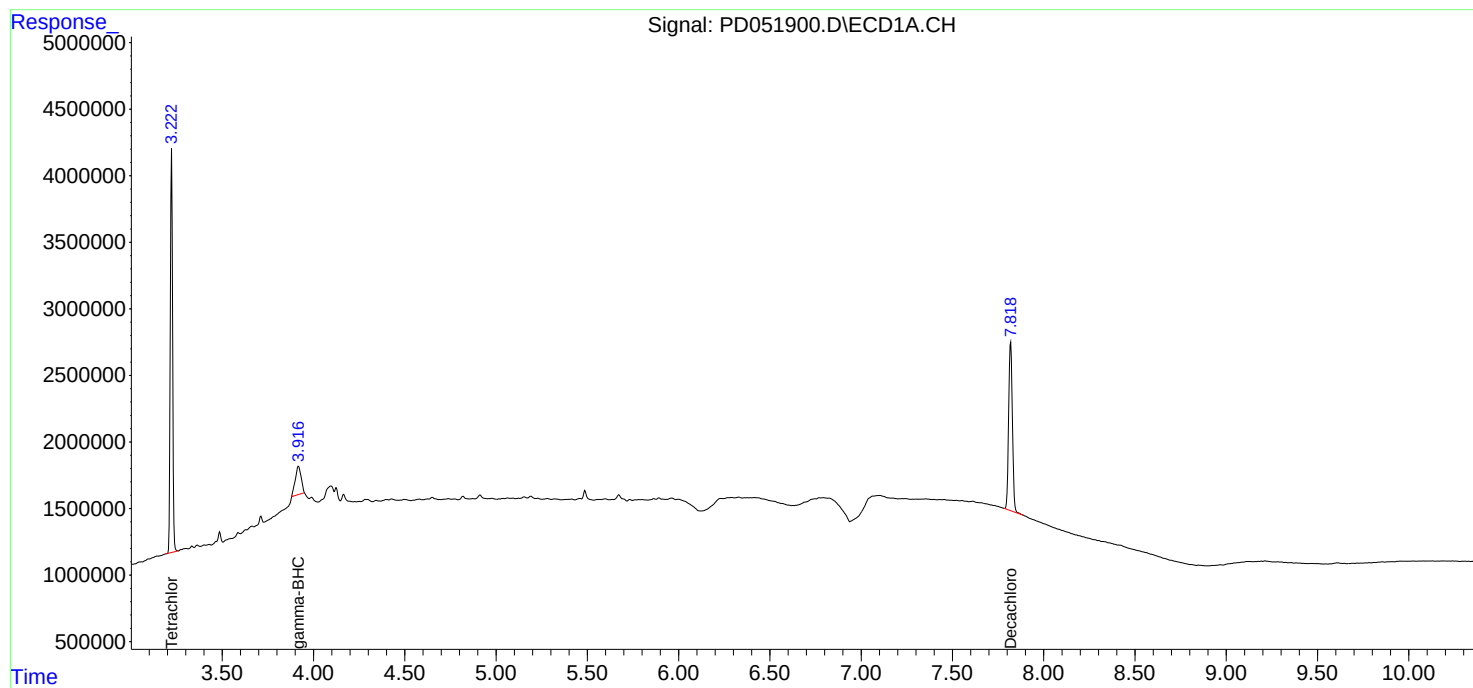


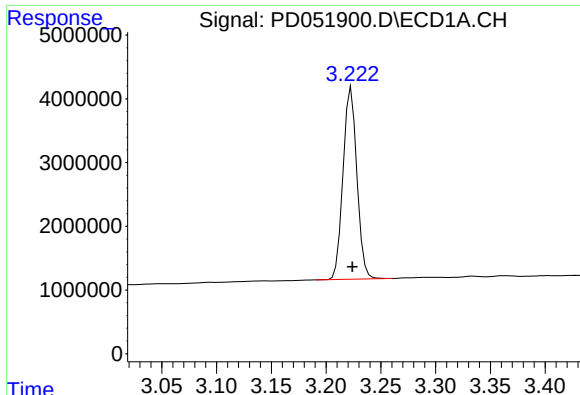

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 26416133
Conc: 19.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

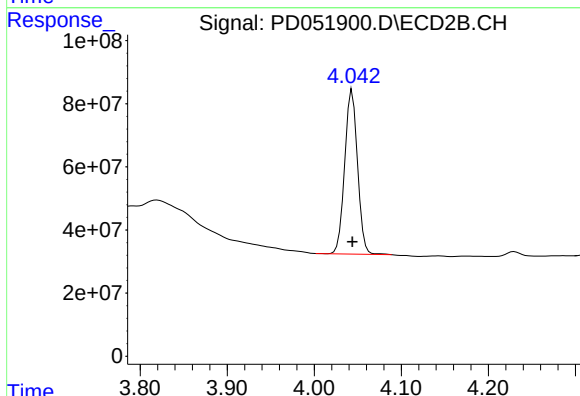


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 530826968
Conc: 18.51 ng/ml

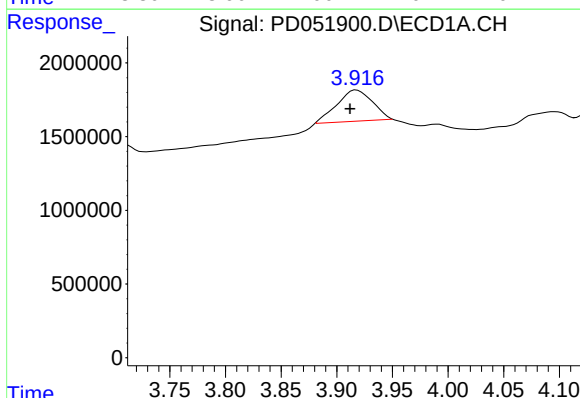


#3 gamma-BHC (Lindane)

R.T.: 3.918 min
Delta R.T.: 0.006 min
Response: 4736870
Conc: 2.27 ng/ml

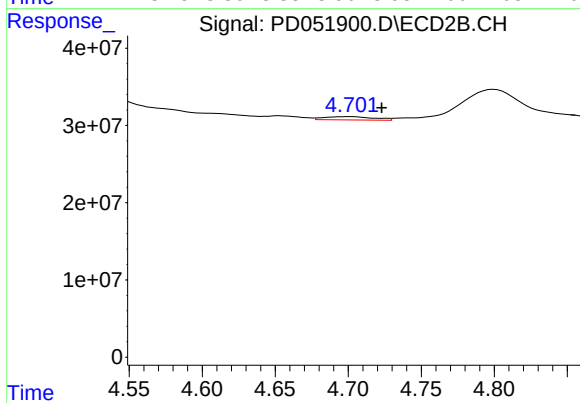

#3 gamma-BHC (Lindane)


R.T.: 4.702 min
Delta R.T.: -0.021 min
Response: 9968224
Conc: 0.25 ng/ml

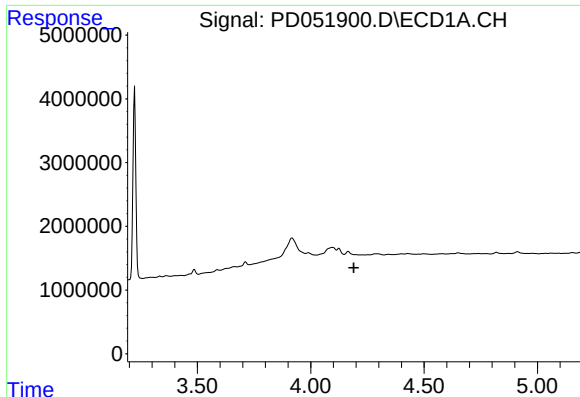

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

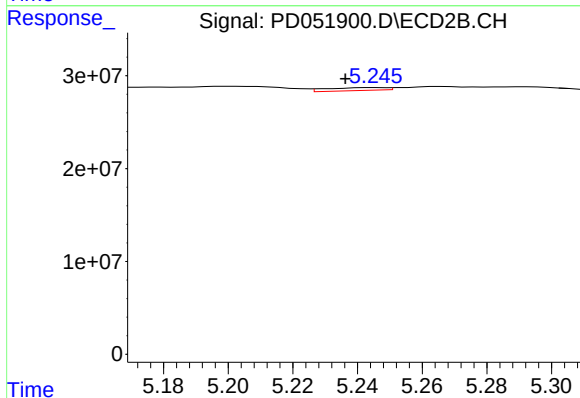


#4 Heptachlor

R.T.: 5.246 min
Delta R.T.: 0.010 min
Response: 4011350
Conc: 0.10 ng/ml

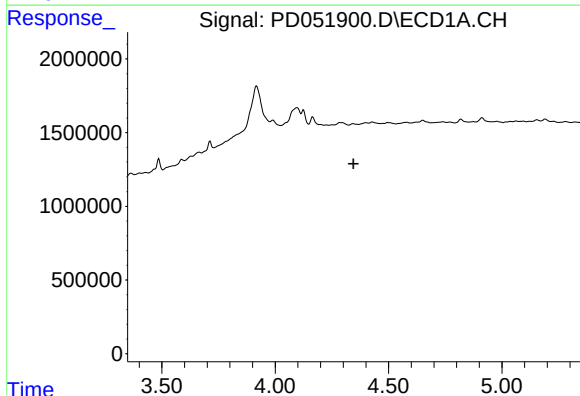


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

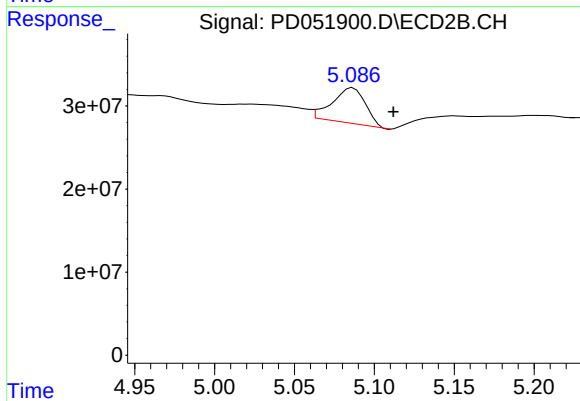

#7 delta-BHC


R.T.: 5.087 min
Delta R.T.: -0.025 min
Response: 61443334
Conc: 1.79 ng/ml

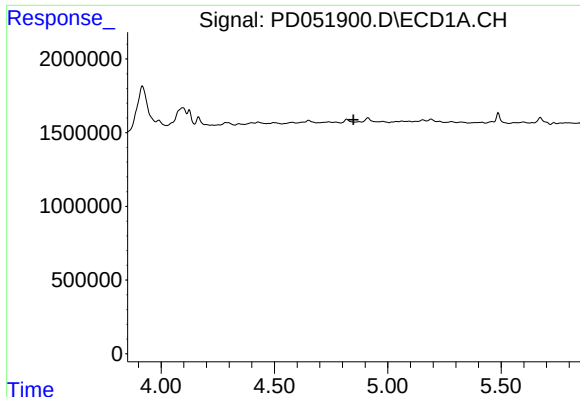

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.849 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

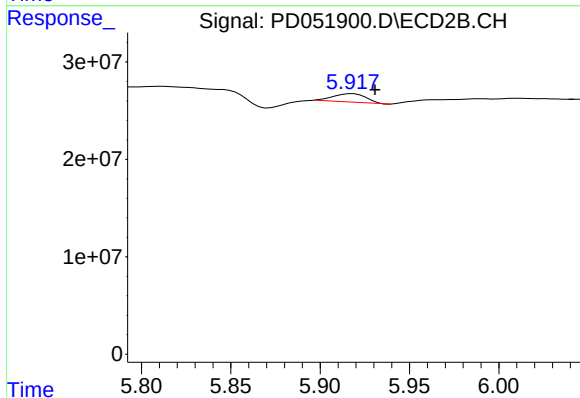


#8 Heptachlor epoxide

R.T.: 5.918 min
Delta R.T.: -0.013 min
Response: 11099061
Conc: 0.35 ng/ml

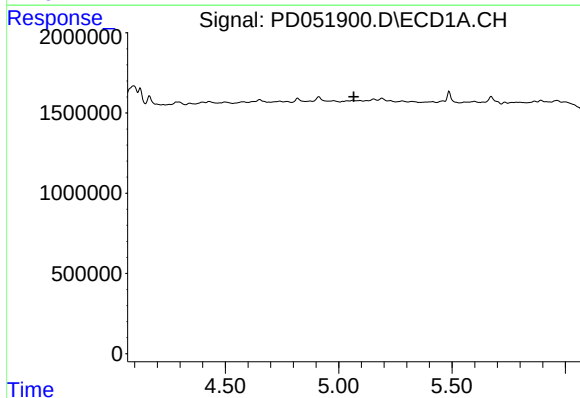


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

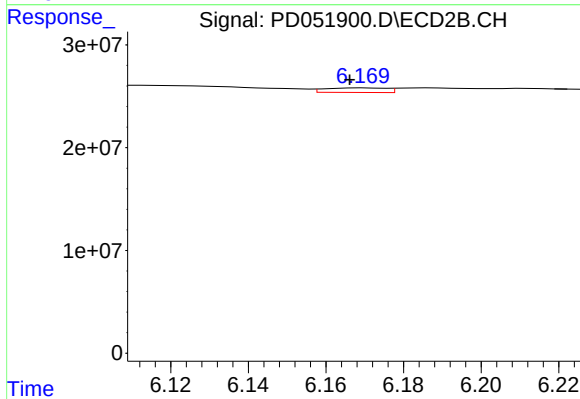

#10 gamma-Chlordane


R.T.: 6.170 min
Delta R.T.: 0.004 min
Response: 4861335
Conc: 0.15 ng/ml

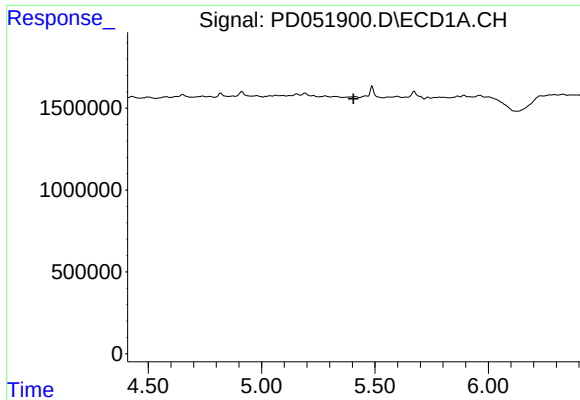

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

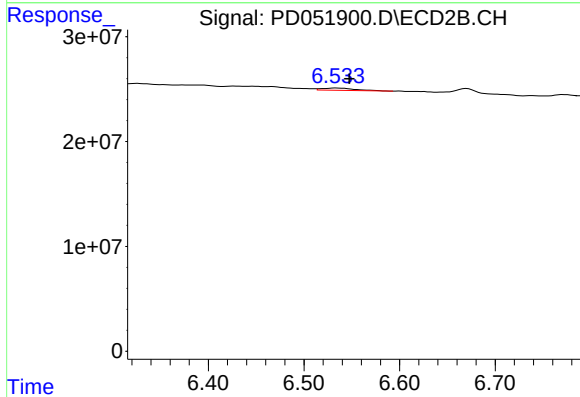


#13 Dieldrin

R.T.: 6.534 min
Delta R.T.: -0.013 min
Response: 5131906
Conc: 0.17 ng/ml

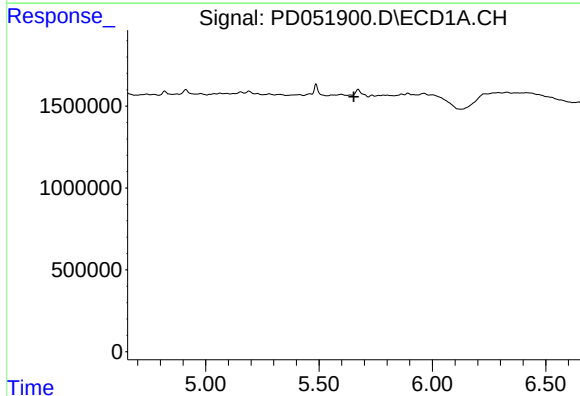


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.653 min
Response: 0
Conc: N.D.

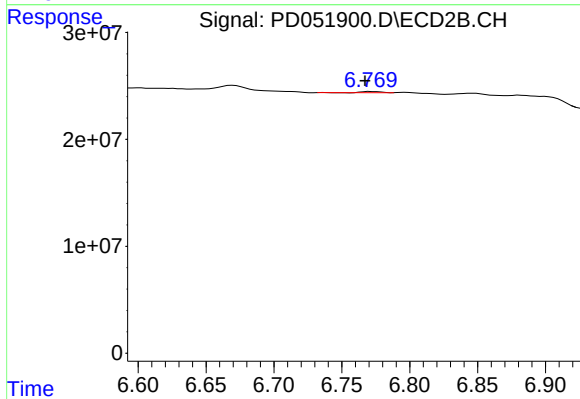

#14 Endrin


R.T.: 6.771 min
Delta R.T.: 0.004 min
Response: 978937
Conc: 0.04 ng/ml

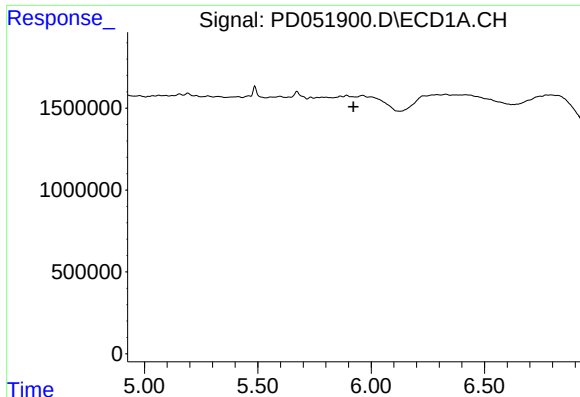

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.923 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

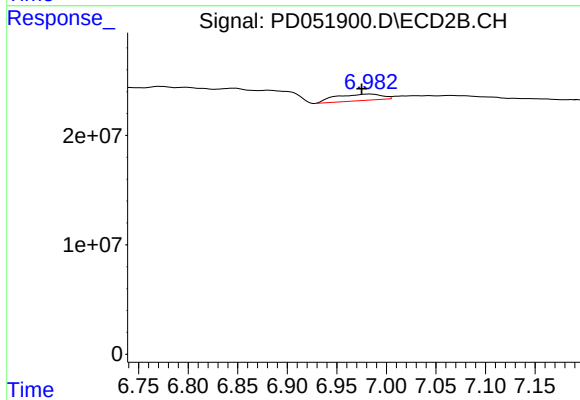


#15 Endosulfan II

R.T.: 6.983 min
Delta R.T.: 0.008 min
Response: 19147684
Conc: 0.74 ng/ml

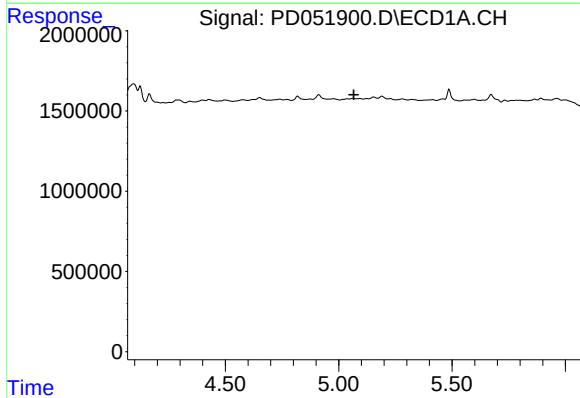


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.067 min
Response: 0
Conc: N.D.

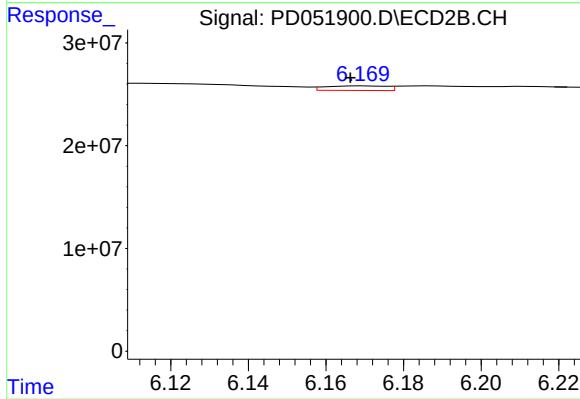

#25 Chlordane-3


R.T.: 6.170 min
Delta R.T.: 0.004 min
Response: 4861335
Conc: 1.09 ng/ml

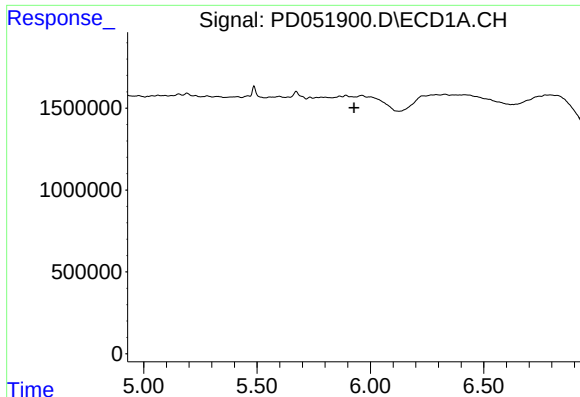

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 5.927 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OK-02-031819

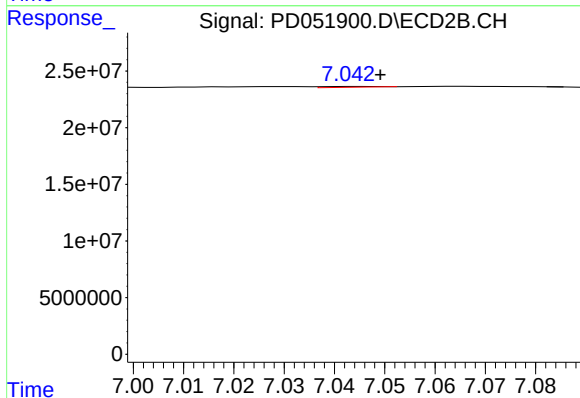


#27 Chlorodane-5

R.T.: 7.044 min
Delta R.T.: -0.005 min
Response: 507391
Conc: 0.50 ng/ml

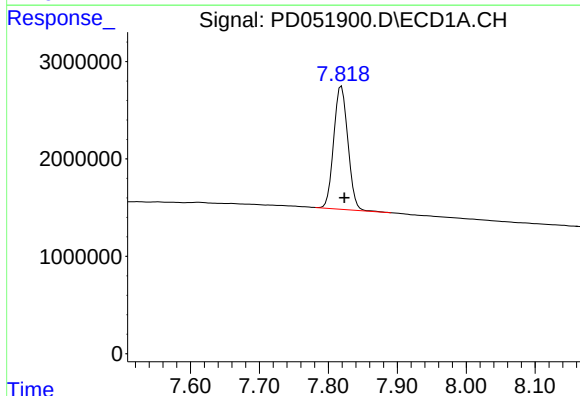

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: -0.004 min
Response: 18019650
Conc: 15.85 ng/ml

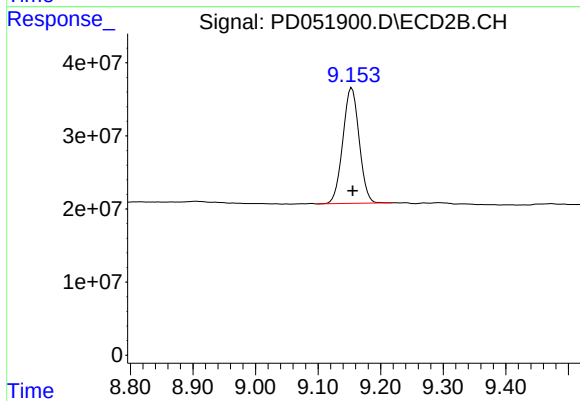

#28 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.001 min
Response: 287596782
Conc: 15.74 ng/ml