

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
 Data File : PD051905.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 11:57
 Operator : AJ\SJ
 Sample : K1941-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 13:18:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	24941363	500.7E6	18.811	17.459
28)	SA Decachlor...	7.819	9.153	13877539	220.5E6	12.209	12.072
Target Compounds							
3)	MA gamma-BHC...	3.915	4.735	3960077	2835465	1.895	0.072 #
4)	MA Heptachlor	0.000	5.243	0	4511519	N.D.	0.118 #
7)	B delta-BHC	0.000	5.086f	0	49777511	N.D.	1.448 #
8)	B Heptachlo...	0.000	5.917	0	6606898	N.D.	0.206 #
10)	B gamma-Chl...	0.000	6.176	0	22123402	N.D.	0.692 #
13)	MA Dieldrin	0.000	6.541	0	4273139	N.D.	0.138 #
25)	Chlordane-3	0.000	6.176	0	22123402	N.D.	4.968 #
27)	Chlordane-5	0.000	7.044	0	292262	N.D.	0.289 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
Data File : PD051905.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 11:57
Operator : AJ\SJ
Sample : K1941-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 13:18:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

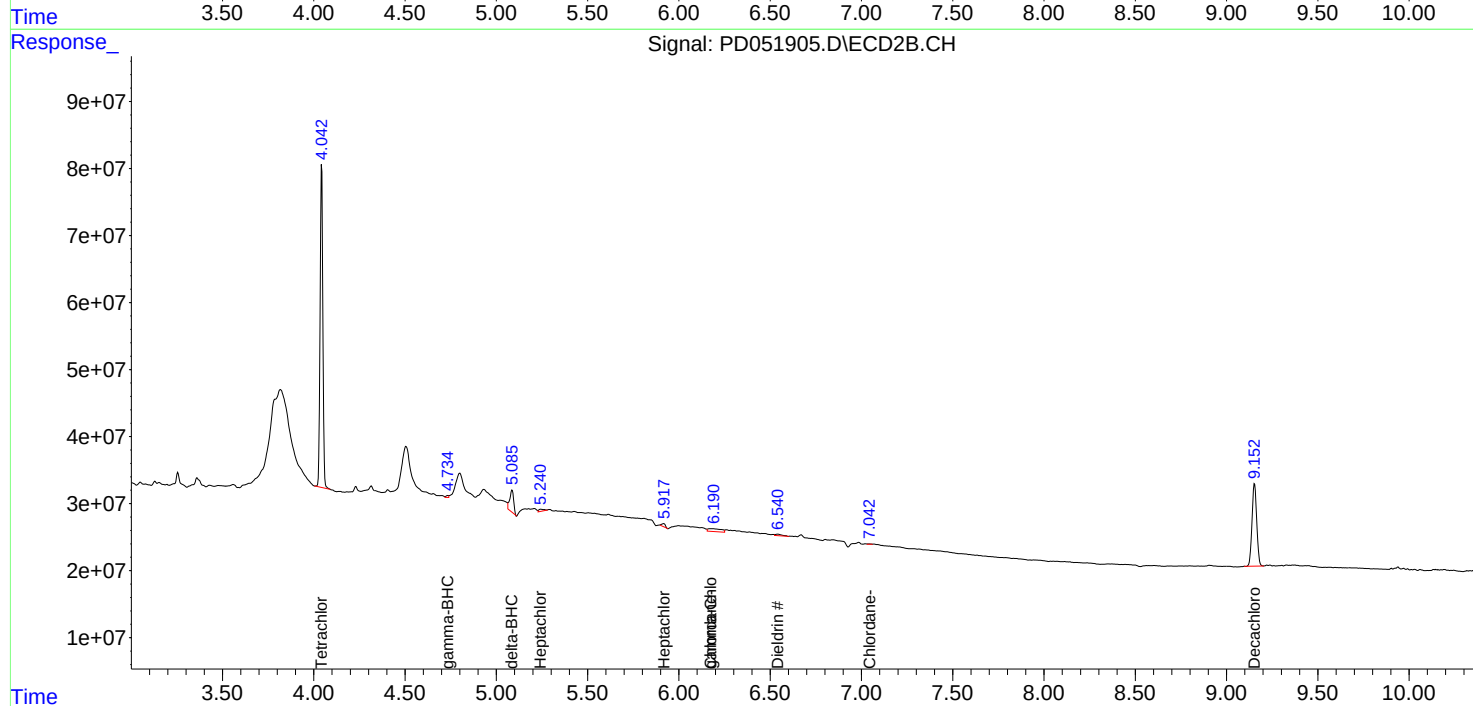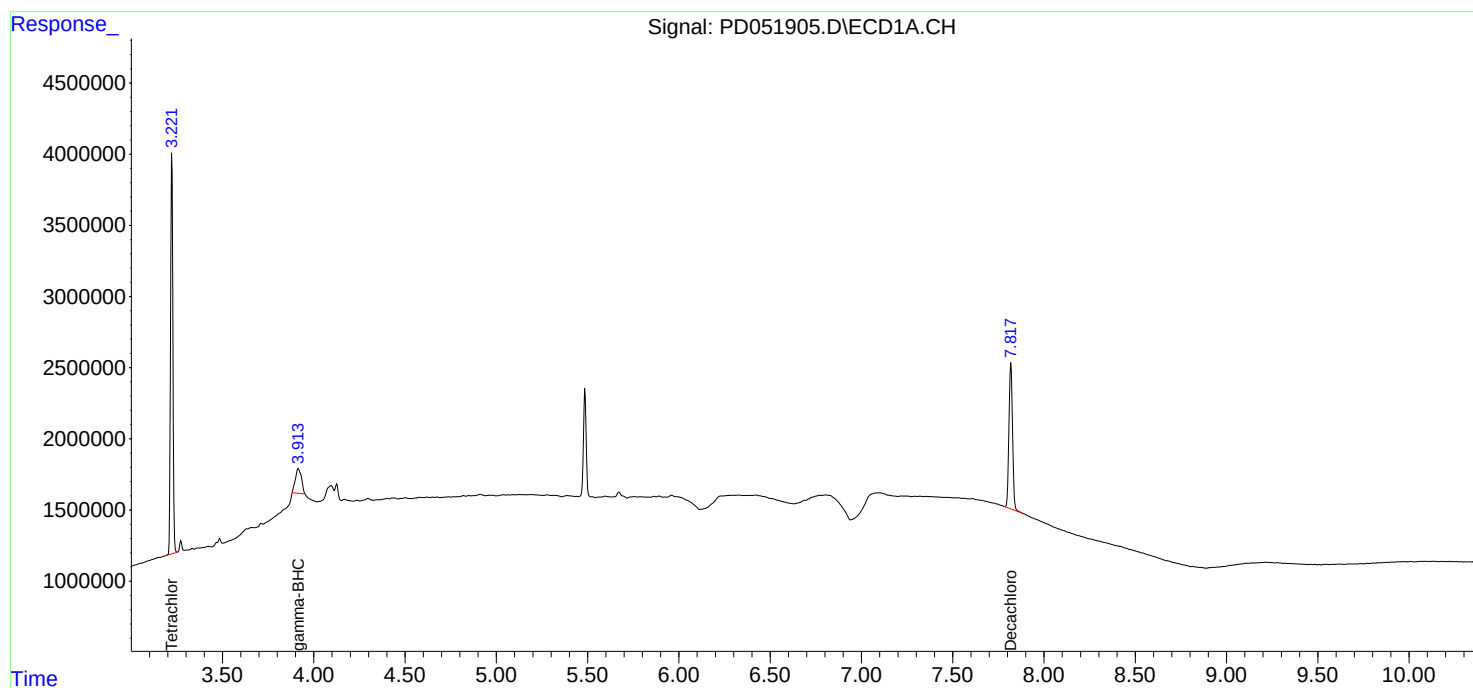


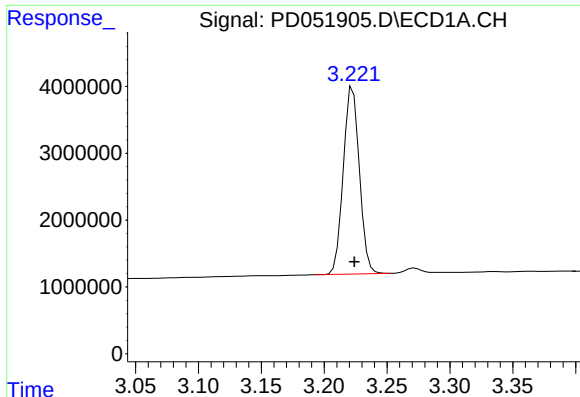

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.001 min
Response: 24941363
Conc: 18.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
SP

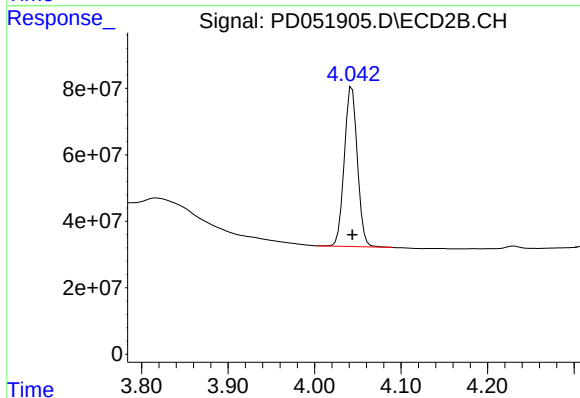


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 500681527
Conc: 17.46 ng/ml

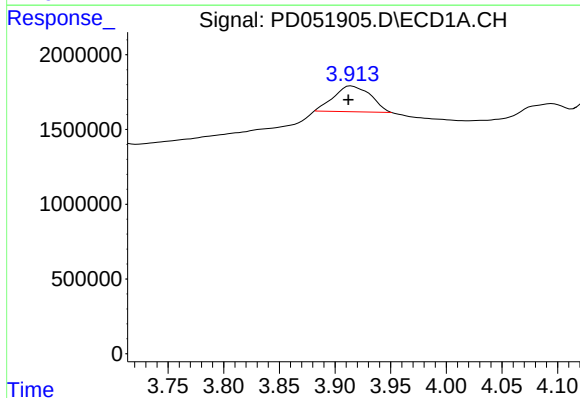


#3 gamma-BHC (Lindane)

R.T.: 3.915 min
Delta R.T.: 0.003 min
Response: 3960077
Conc: 1.90 ng/ml

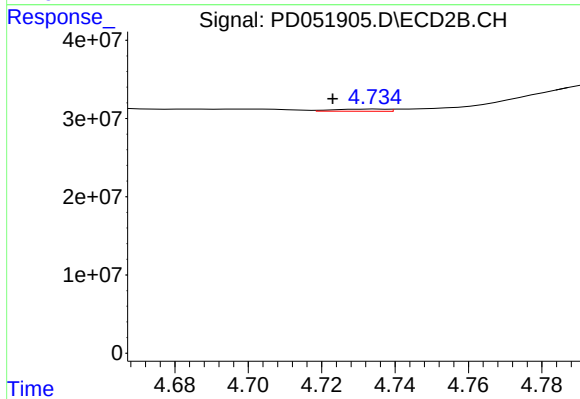

#3 gamma-BHC (Lindane)


R.T.: 4.735 min
Delta R.T.: 0.012 min
Response: 2835465
Conc: 0.07 ng/ml

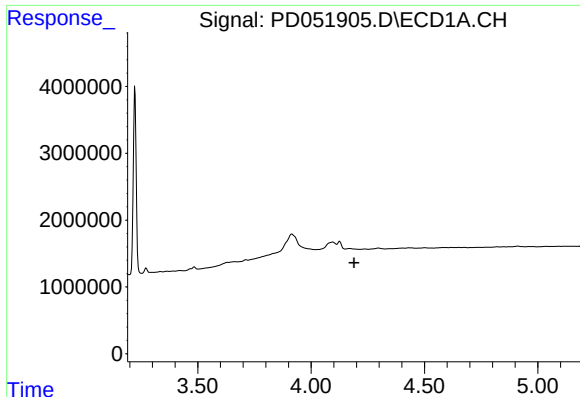

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SP

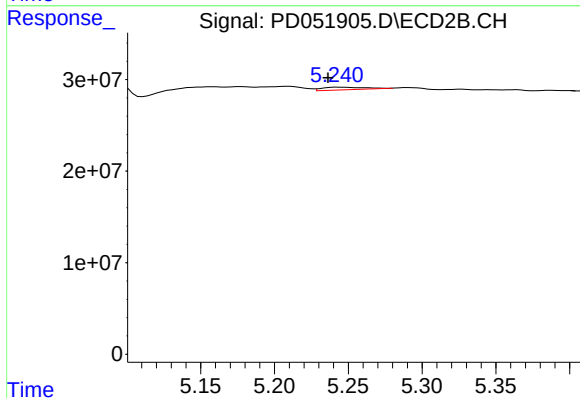


#4 Heptachlor

R.T.: 5.243 min
Delta R.T.: 0.007 min
Response: 4511519
Conc: 0.12 ng/ml

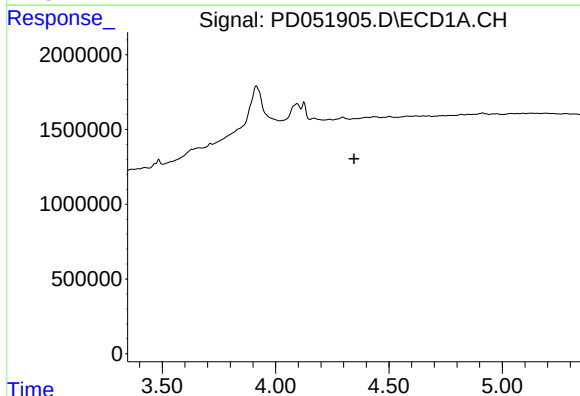


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

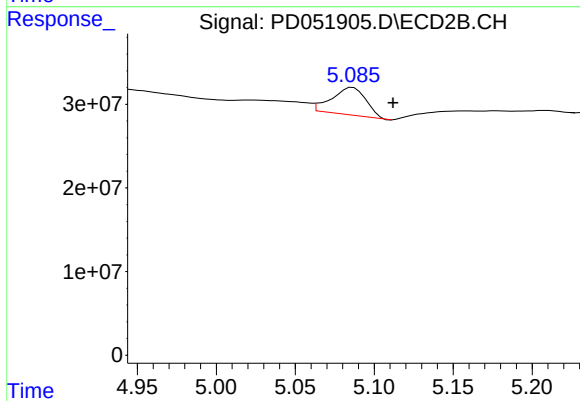

#7 delta-BHC


R.T.: 5.086 min
Delta R.T.: -0.026 min
Response: 49777511
Conc: 1.45 ng/ml

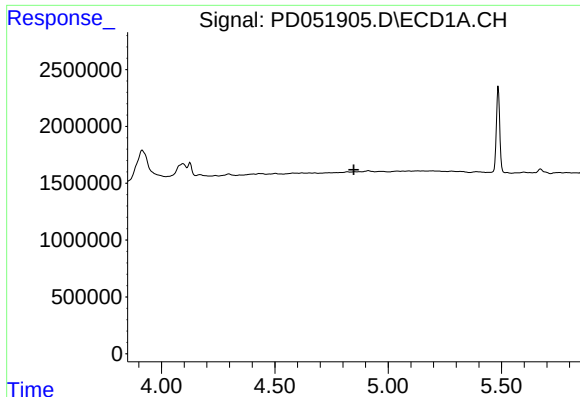

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.849 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SP

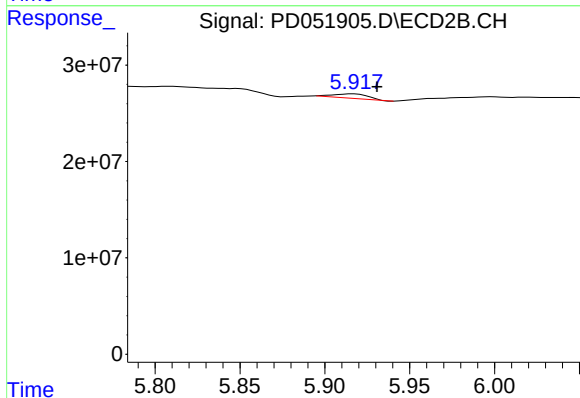


#8 Heptachlor epoxide

R.T.: 5.917 min
Delta R.T.: -0.014 min
Response: 6606898
Conc: 0.21 ng/ml

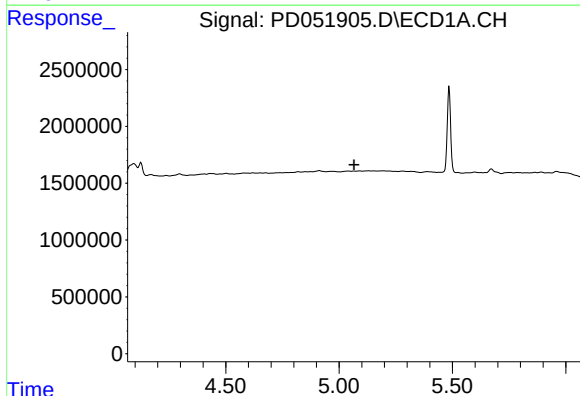


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

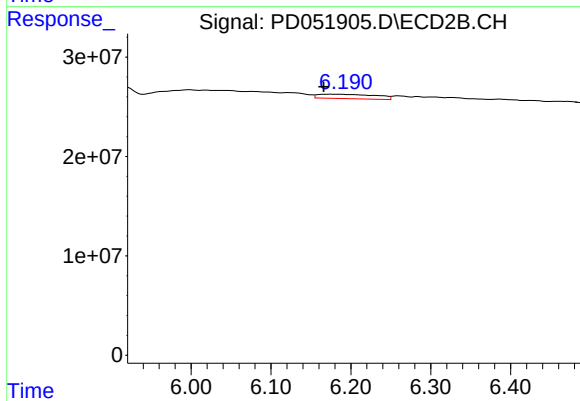

#10 gamma-Chlordane


R.T.: 6.176 min
Delta R.T.: 0.010 min
Response: 22123402
Conc: 0.69 ng/ml

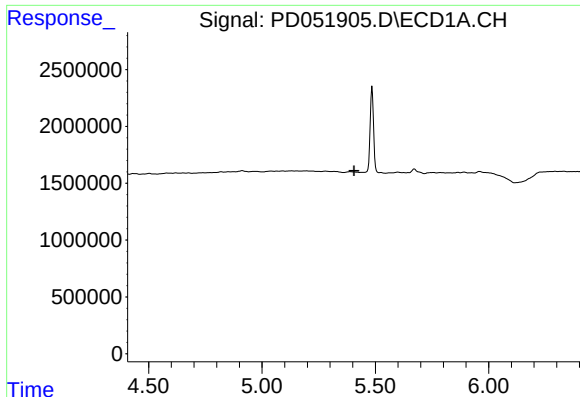

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SP

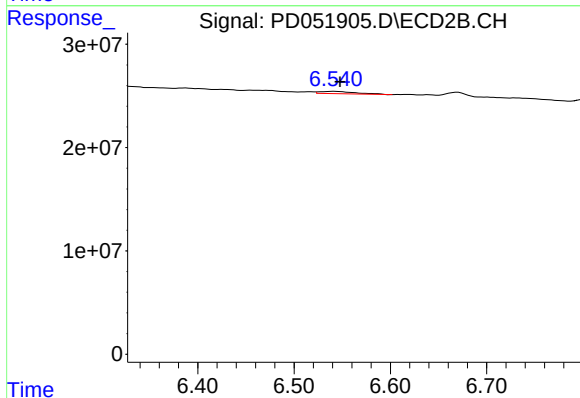


#13 Dieldrin

R.T.: 6.541 min
Delta R.T.: -0.006 min
Response: 4273139
Conc: 0.14 ng/ml

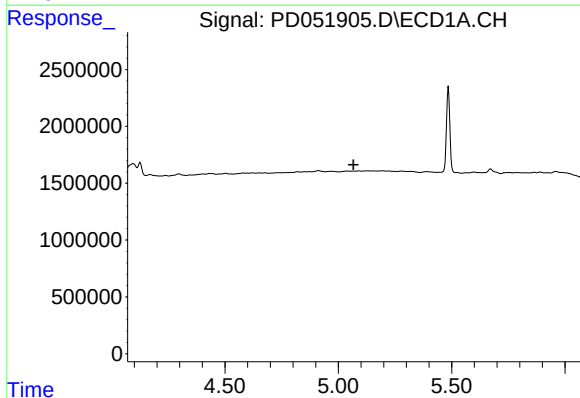


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

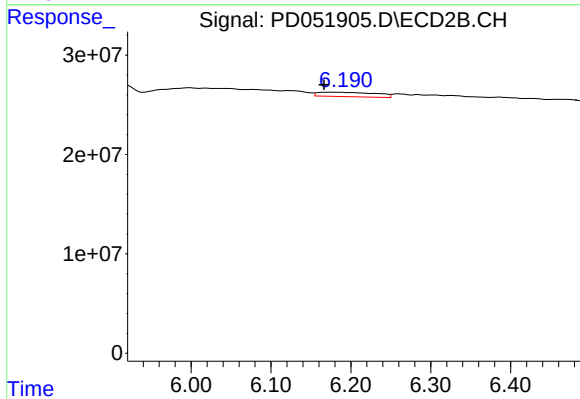

#25 Chlordane-3


R.T.: 6.176 min
Delta R.T.: 0.010 min
Response: 22123402
Conc: 4.97 ng/ml

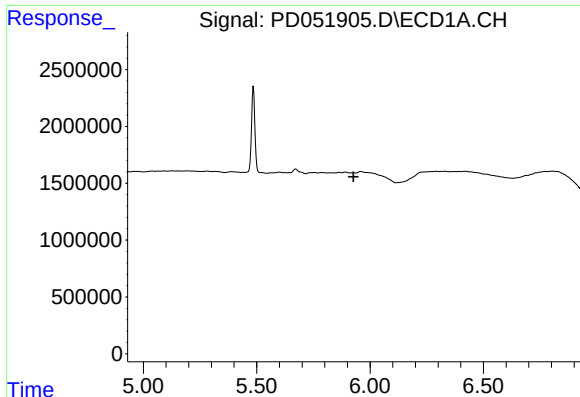

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.927 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SP

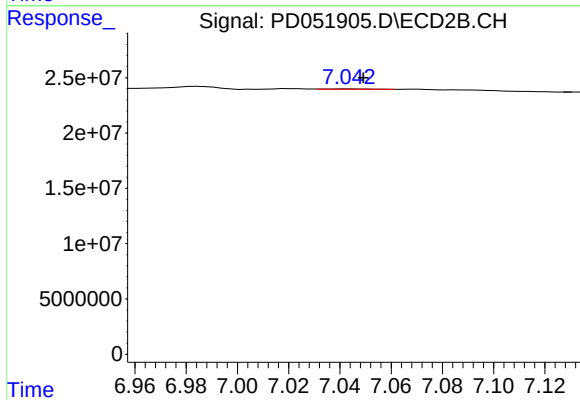


#27 Chlordane-5

R.T.: 7.044 min
Delta R.T.: -0.006 min
Response: 292262
Conc: 0.29 ng/ml

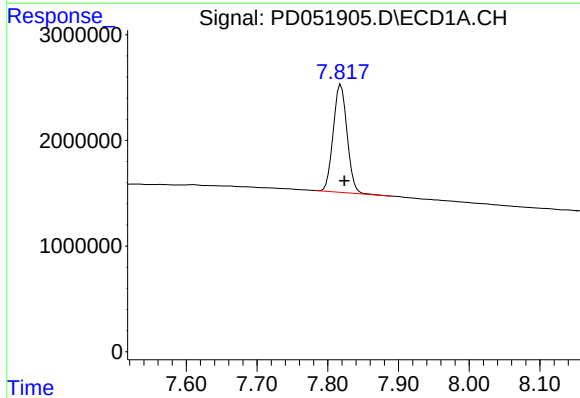

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: -0.005 min
Response: 13877539
Conc: 12.21 ng/ml

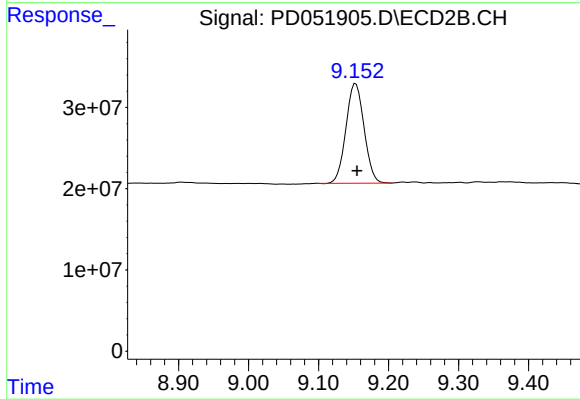

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: -0.002 min
Response: 220515203
Conc: 12.07 ng/ml