

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
 Data File : PD051910.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 13:08
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 13:39:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	30284499	615.7E6	22.840	21.472
28)	SA Decachlor...	7.819	9.153	23413762	370.5E6	20.598	20.280
Target Compounds							
3)	MA gamma-BHC...	3.923	0.000	3004542	0	1.438	N.D. #
4)	MA Heptachlor	0.000	5.243	0	3236761	N.D.	0.084 #
7)	B delta-BHC	0.000	5.084f	0	20287327	N.D.	0.590 #
8)	B Heptachlo...	4.871f	5.921	694907	20828330	0.353	0.650 #
9)	A Endosulfan I	0.000	6.284	0	16668244	N.D.	0.562 #
10)	B gamma-Chl...	0.000	6.165	0	43758852	N.D.	1.368 #
14)	MA Endrin	0.000	6.756	0	17304851	N.D.	0.663 #
22)	Mirex	0.000	8.244	0	7847291	N.D.	0.507 #
25)	Chlordane-3	0.000	6.165	0	43758852	N.D.	9.827 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
Data File : PD051910.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 13:08
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 13:39:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

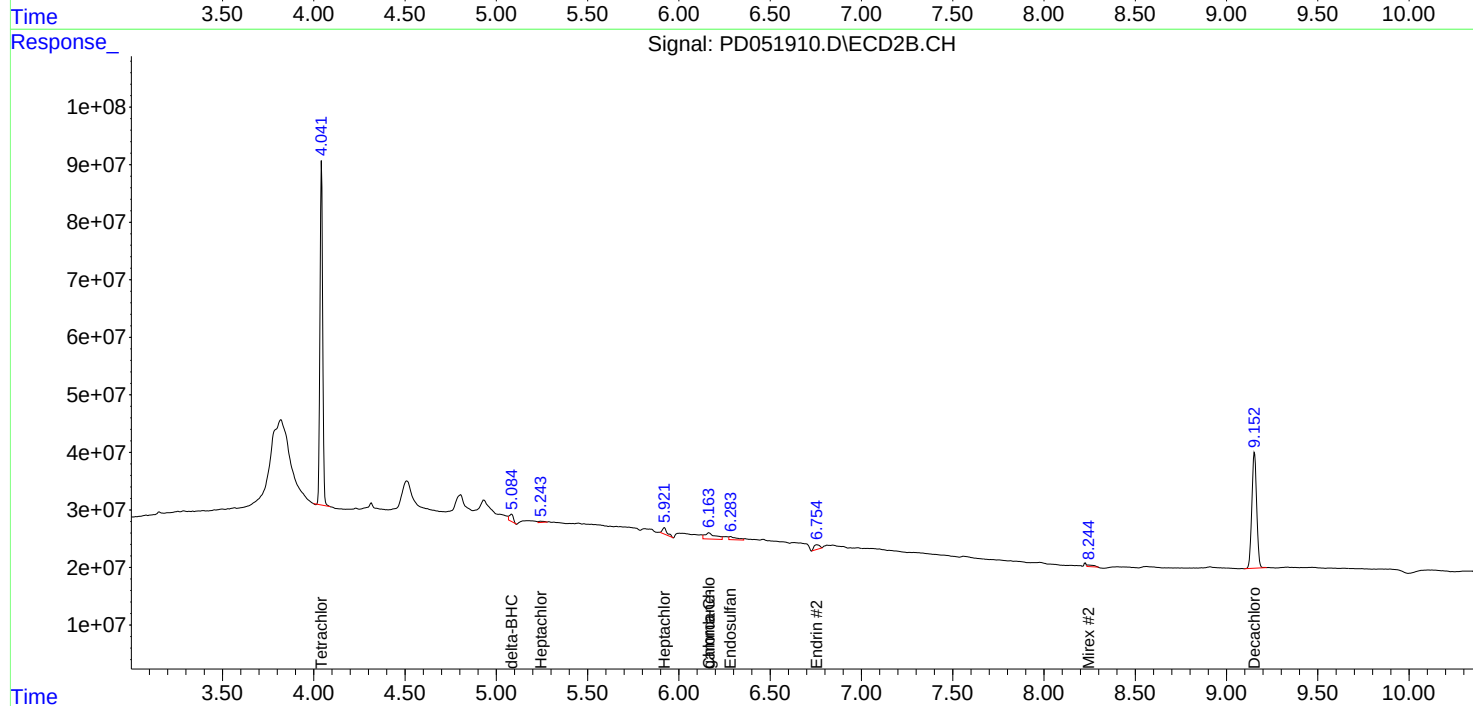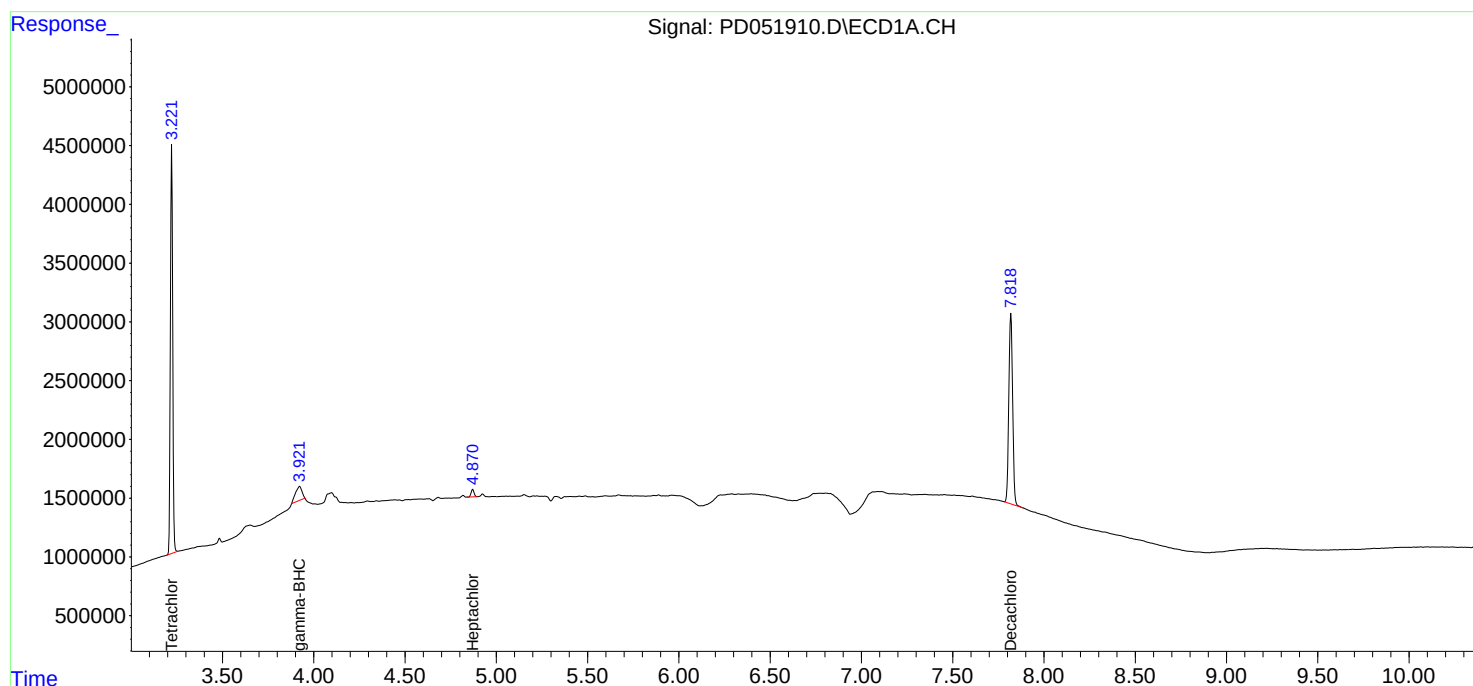


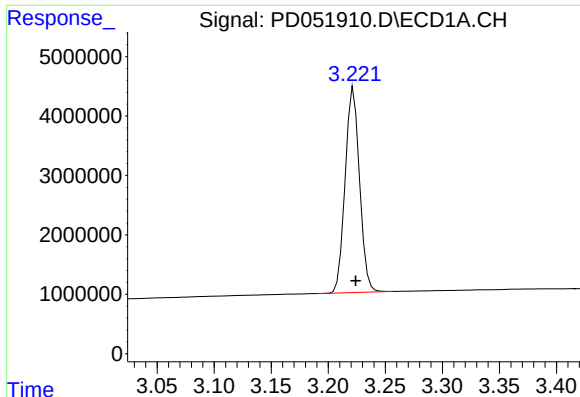

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: -0.002 min
Response: 30284499
Conc: 22.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

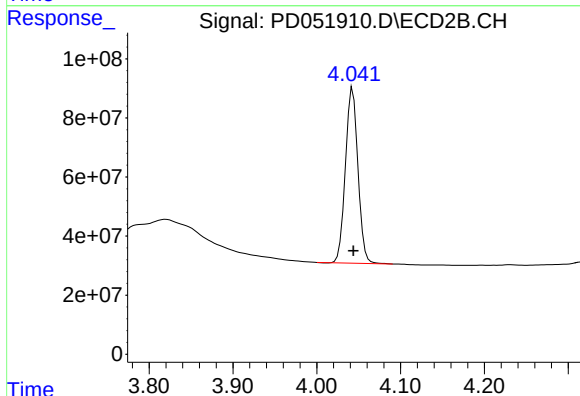


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 615742292
Conc: 21.47 ng/ml

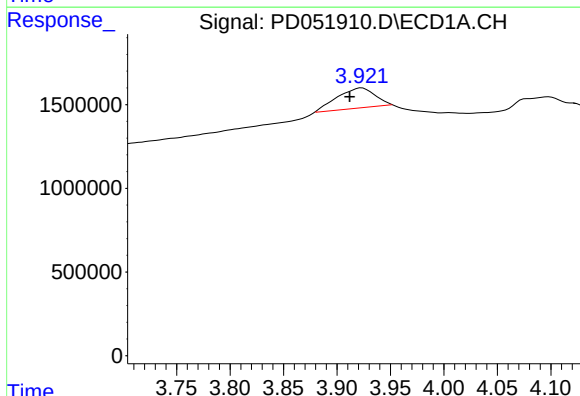


#3 gamma-BHC (Lindane)

R.T.: 3.923 min
Delta R.T.: 0.011 min
Response: 3004542
Conc: 1.44 ng/ml

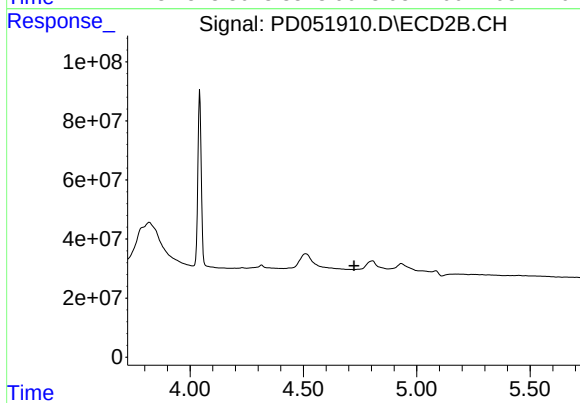

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

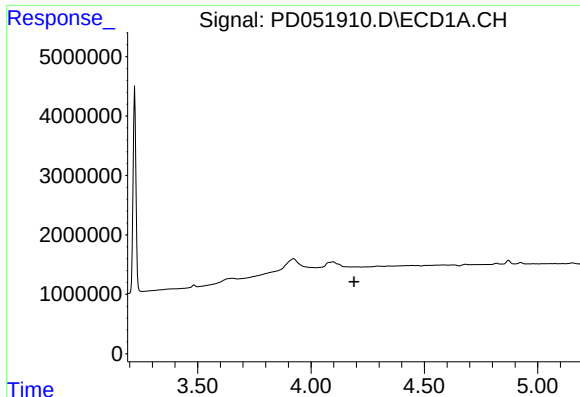

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

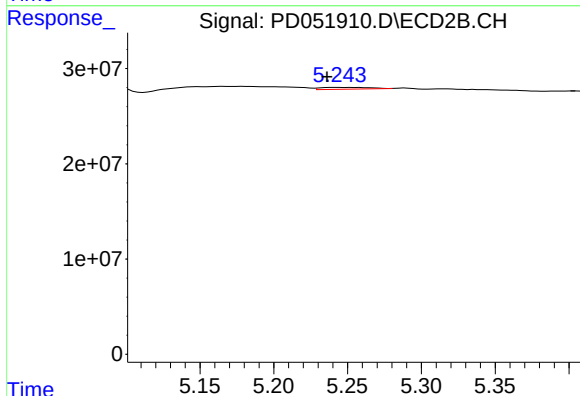


#4 Heptachlor

R.T.: 5.243 min
Delta R.T.: 0.007 min
Response: 3236761
Conc: 0.08 ng/ml

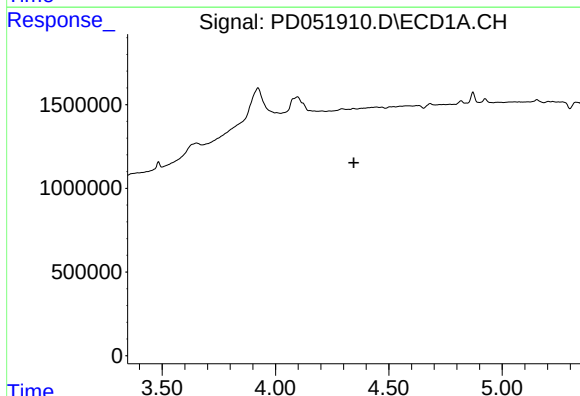


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

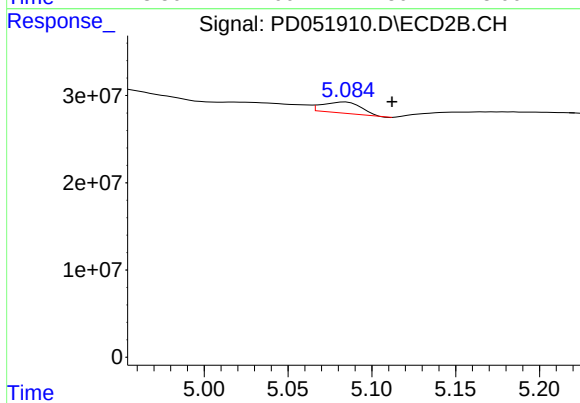

#7 delta-BHC


R.T.: 5.084 min
Delta R.T.: -0.027 min
Response: 20287327
Conc: 0.59 ng/ml

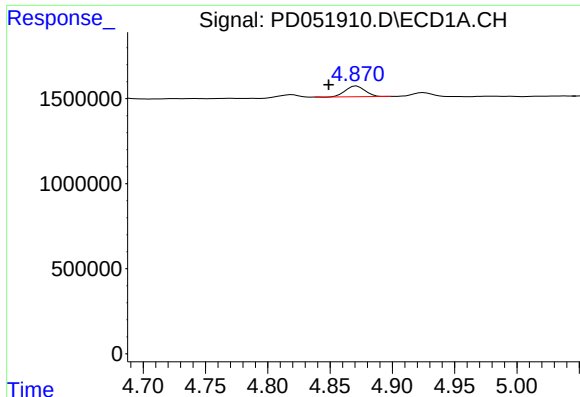

#8 Heptachlor epoxide


R.T.: 4.871 min
Delta R.T.: 0.022 min
Response: 694907
Conc: 0.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

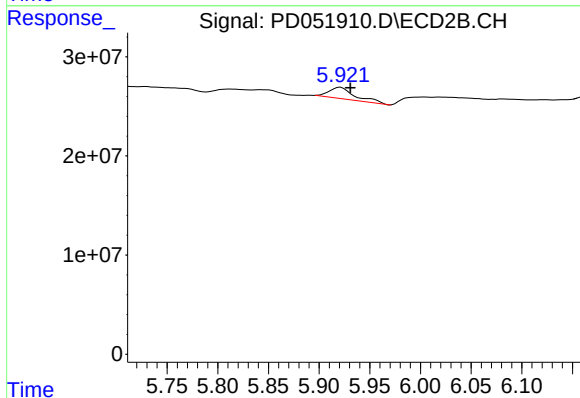


#8 Heptachlor epoxide

R.T.: 5.921 min
Delta R.T.: -0.010 min
Response: 20828330
Conc: 0.65 ng/ml

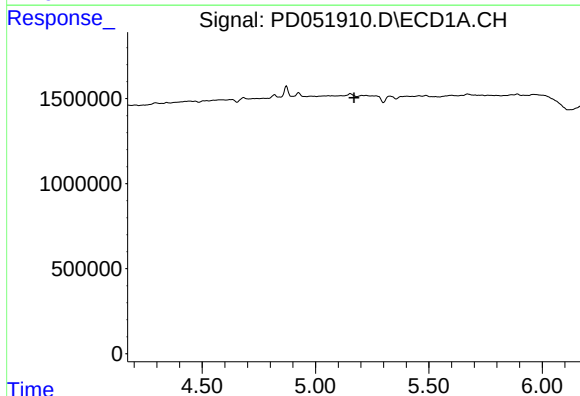


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.170 min
Response: 0
Conc: N.D.

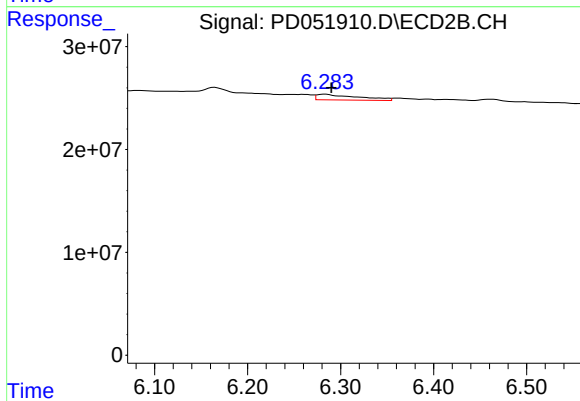

#9 Endosulfan I


R.T.: 6.284 min
Delta R.T.: -0.006 min
Response: 16668244
Conc: 0.56 ng/ml

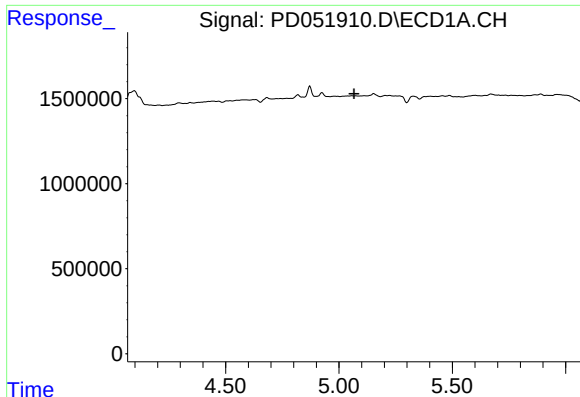

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

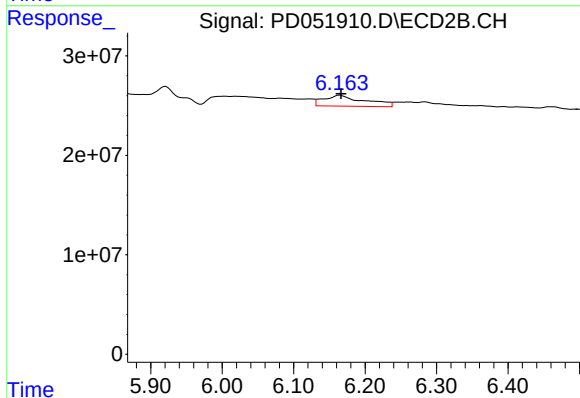


#10 gamma-Chlordane

R.T.: 6.165 min
Delta R.T.: -0.001 min
Response: 43758852
Conc: 1.37 ng/ml

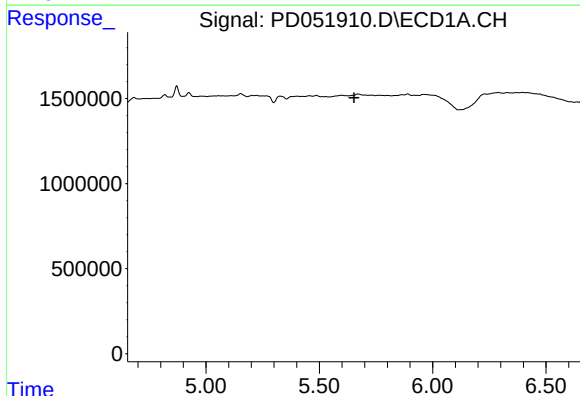


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.653 min
Response: 0
Conc: N.D.

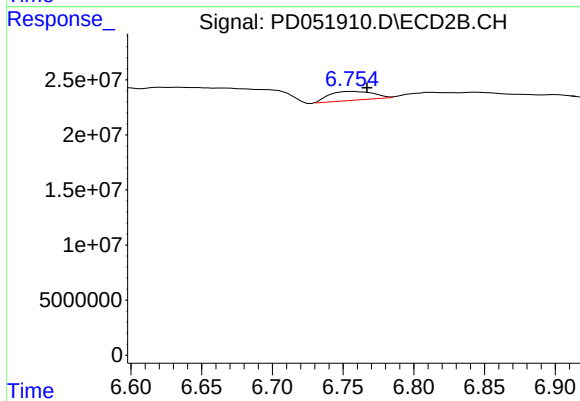

#14 Endrin


R.T.: 6.756 min
Delta R.T.: -0.011 min
Response: 17304851
Conc: 0.66 ng/ml

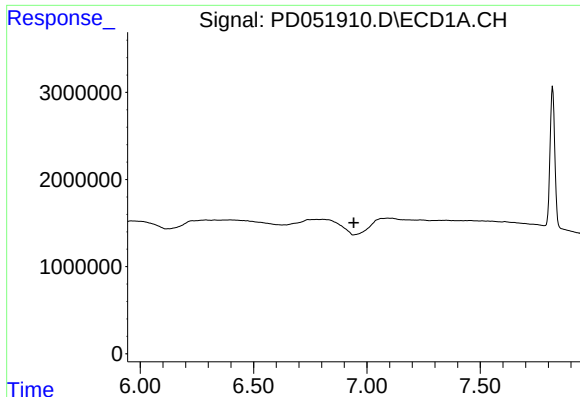

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 6.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

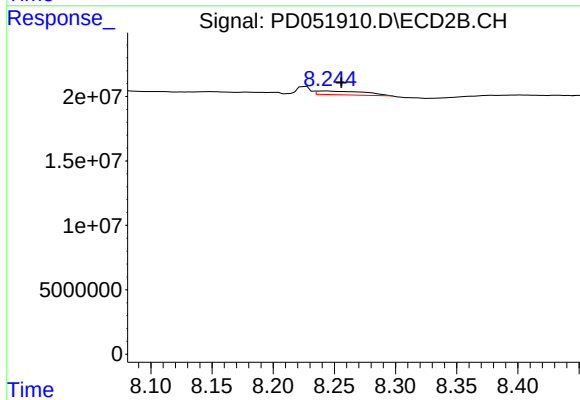


#22 Mirex

R.T.: 8.244 min
Delta R.T.: -0.012 min
Response: 7847291
Conc: 0.51 ng/ml

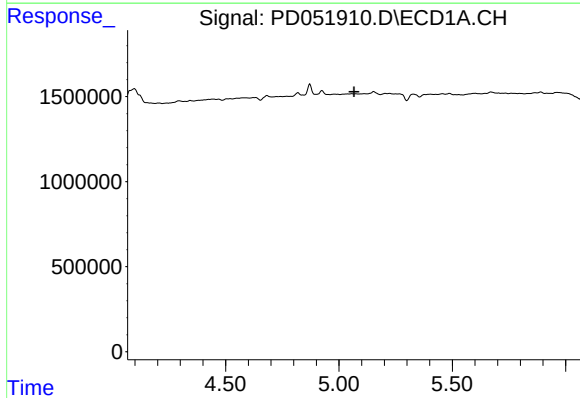


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

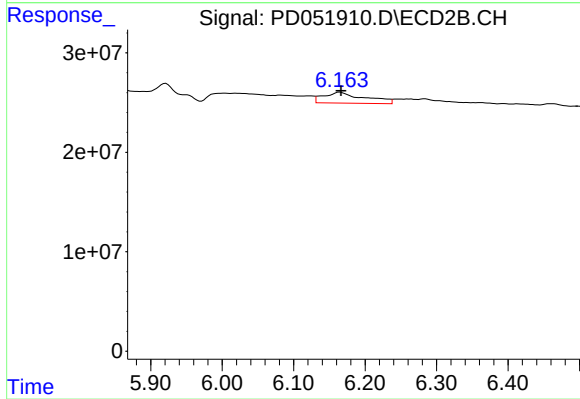

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: -0.002 min
Response: 43758852
Conc: 9.83 ng/ml

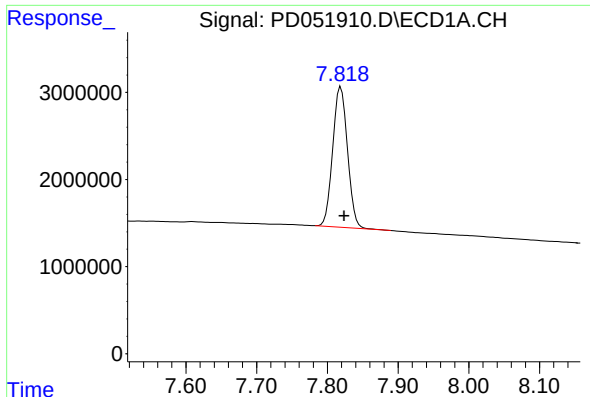

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: -0.004 min
Response: 23413762
Conc: 20.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

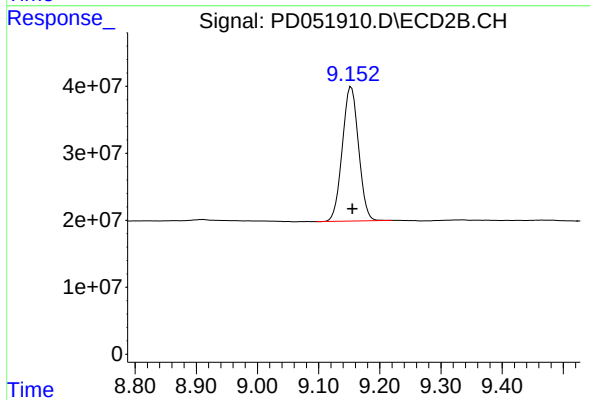

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: -0.002 min
Response: 370462157
Conc: 20.28 ng/ml