

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
 Data File : PD051922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Mar 2019 16:47
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 17:05:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	30174678	536.0E6	22.757	18.692
28)	SA Decachlor...	7.820	9.155	18781086	206.5E6	16.523	11.307 #
Target Compounds							
3)	MA gamma-BHC...	3.922	0.000	2888735	0	1.383	N.D. #
7)	B delta-BHC	0.000	5.086f	0	8346911	N.D.	0.243 #
8)	B Heptachlo...	4.872f	5.922	634792	18651563	0.323	0.582 #
9)	A Endosulfan I	0.000	6.285	0	2843244	N.D.	0.096 #
10)	B gamma-Chl...	0.000	6.164	0	5993614	N.D.	0.187 #
14)	MA Endrin	0.000	6.760	0	7563921	N.D.	0.290 #
25)	Chlordane-3	0.000	6.164	0	5993614	N.D.	1.346 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032019\
Data File : PD051922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Mar 2019 16:47
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 17:05:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

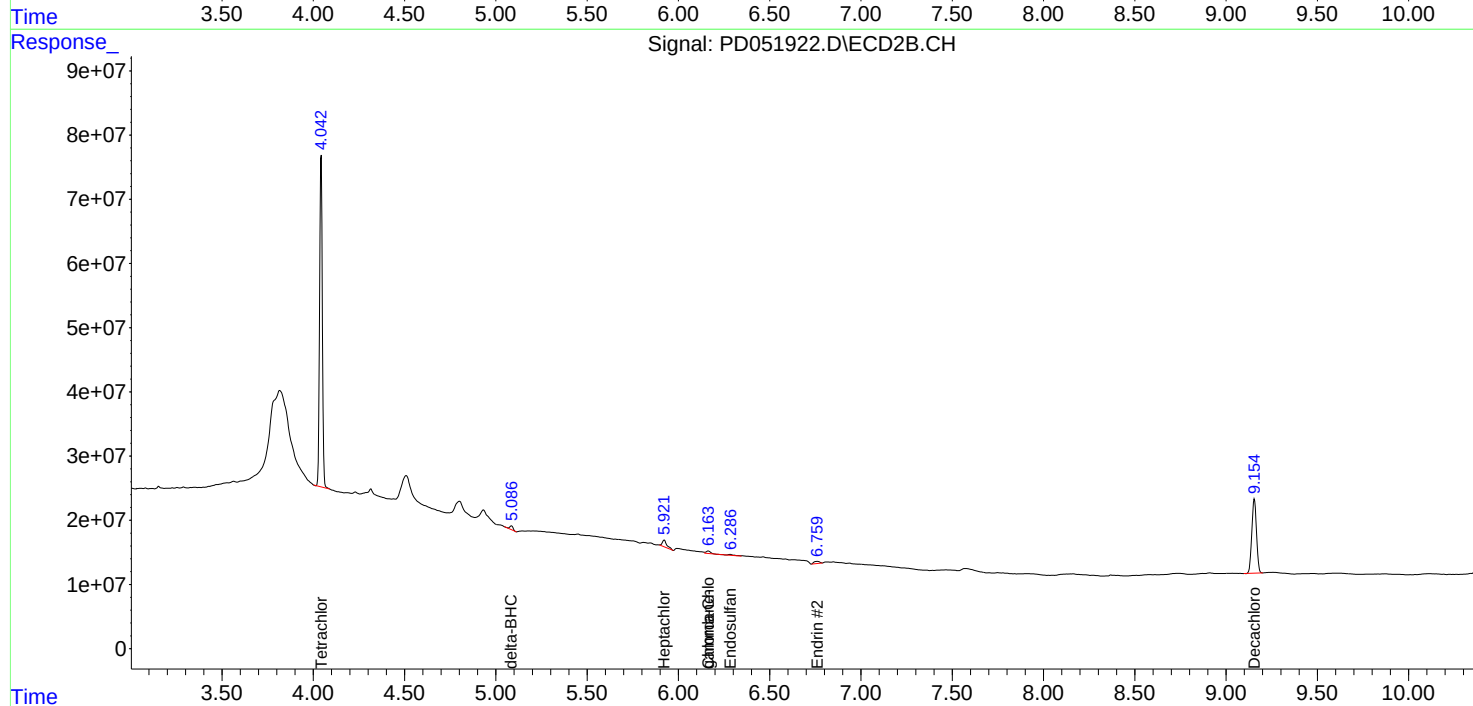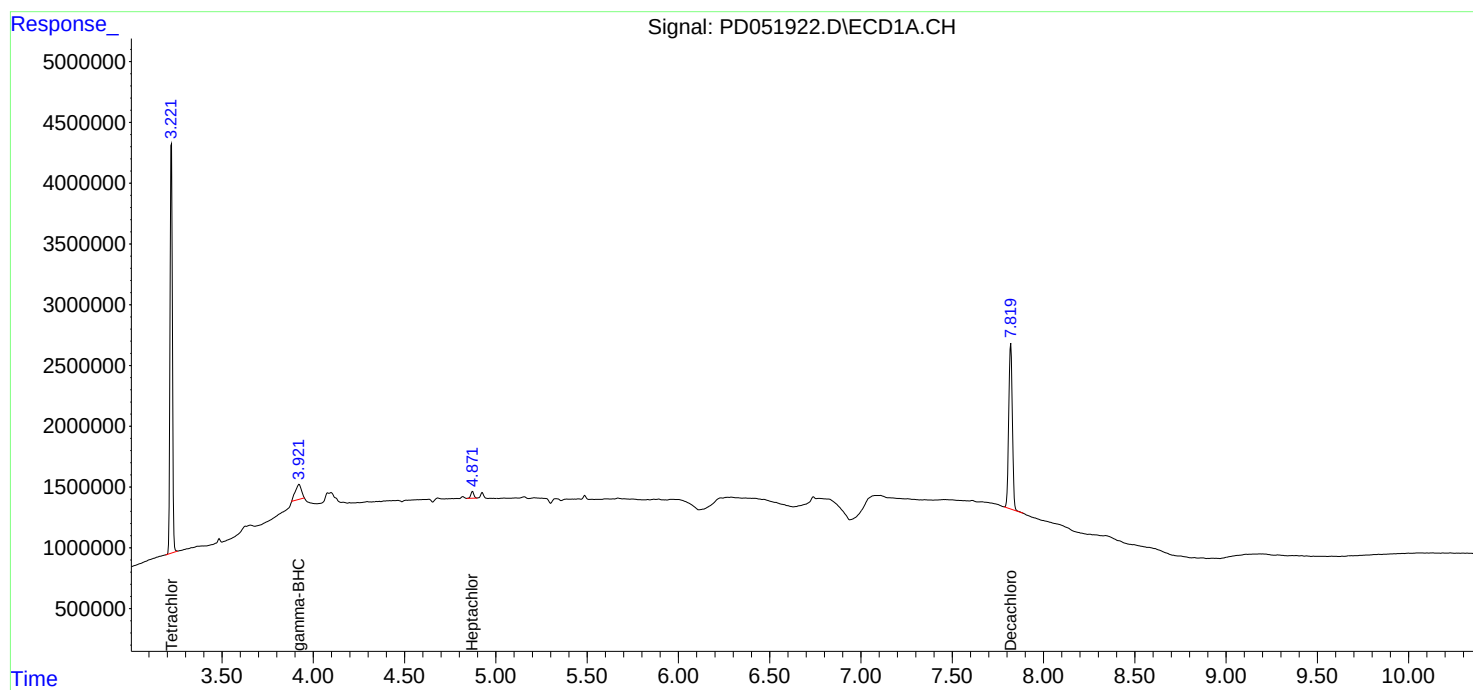


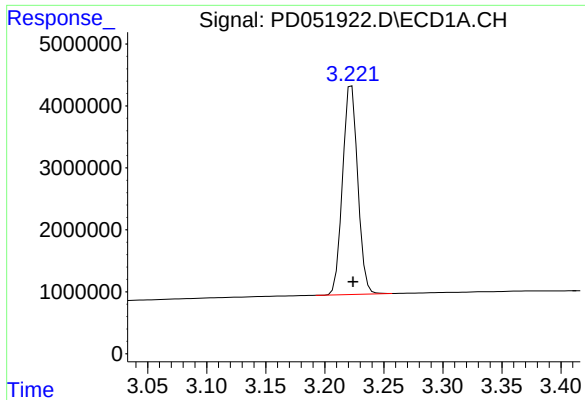

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.001 min
Response: 30174678
Conc: 22.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

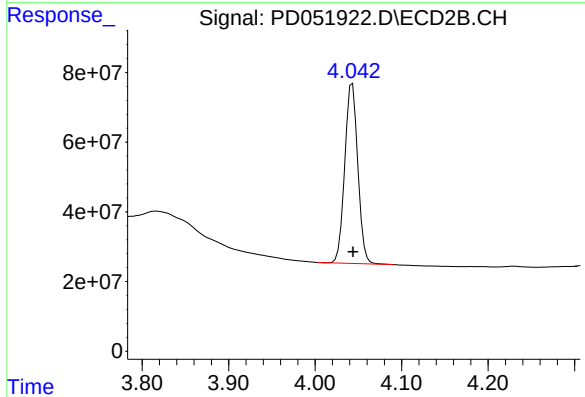


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 536042156
Conc: 18.69 ng/ml

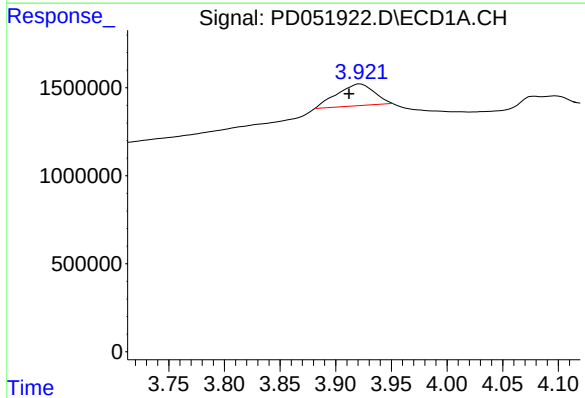


#3 gamma-BHC (Lindane)

R.T.: 3.922 min
Delta R.T.: 0.010 min
Response: 2888735
Conc: 1.38 ng/ml

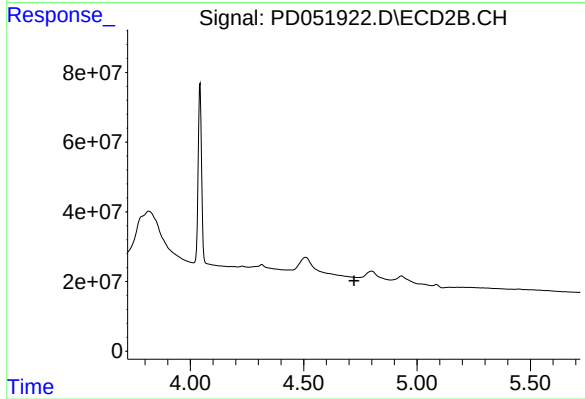

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

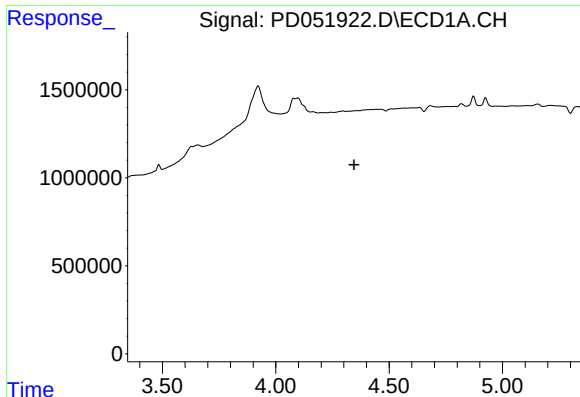

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

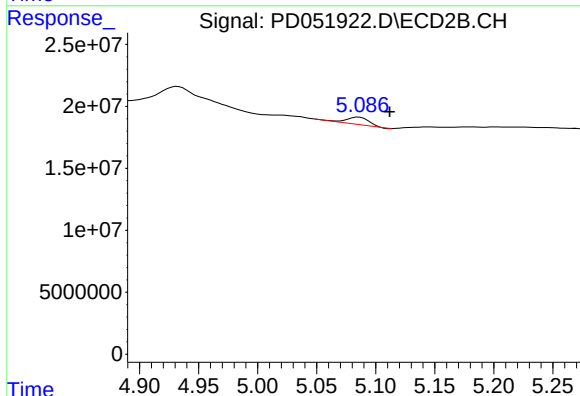


#7 delta-BHC

R.T.: 5.086 min
Delta R.T.: -0.026 min
Response: 8346911
Conc: 0.24 ng/ml

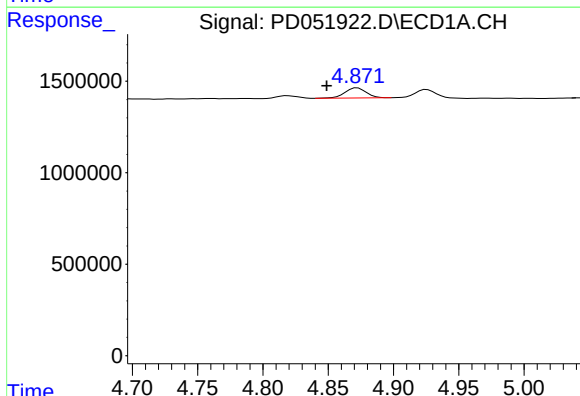


#8 Heptachlor epoxide

R.T.: 4.872 min
Delta R.T.: 0.023 min
Response: 634792
Conc: 0.32 ng/ml

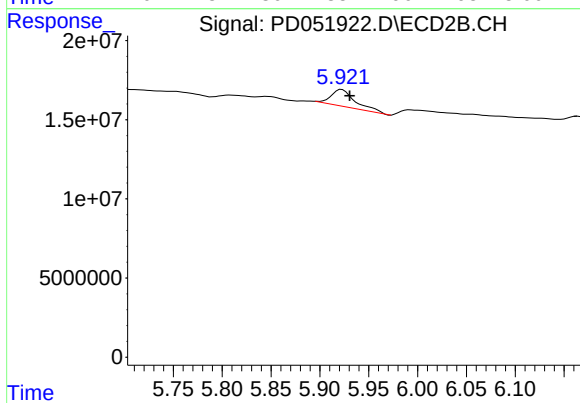

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 18651563
Conc: 0.58 ng/ml

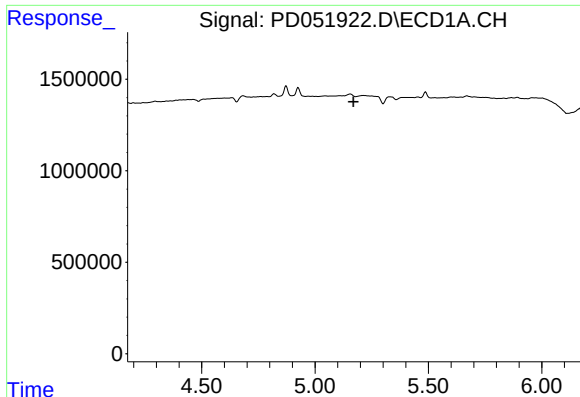

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

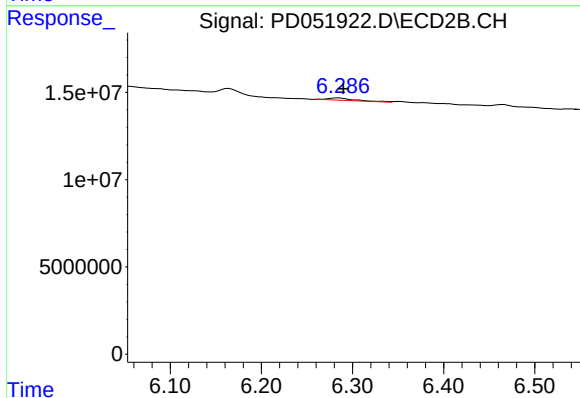


#9 Endosulfan I

R.T.: 6.285 min
Delta R.T.: -0.005 min
Response: 2843244
Conc: 0.10 ng/ml

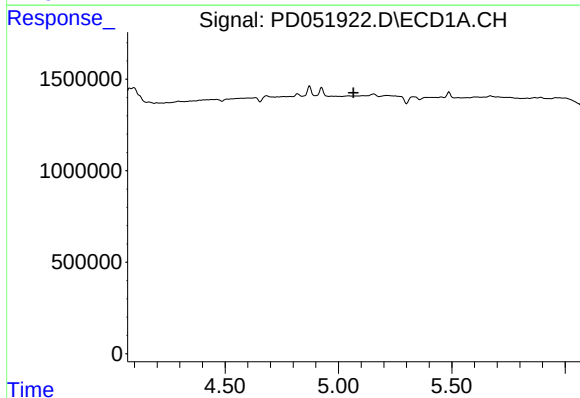


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

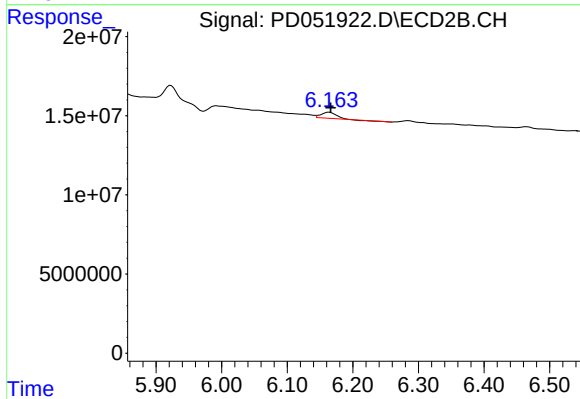

#10 gamma-Chlordane


R.T.: 6.164 min
Delta R.T.: -0.002 min
Response: 5993614
Conc: 0.19 ng/ml

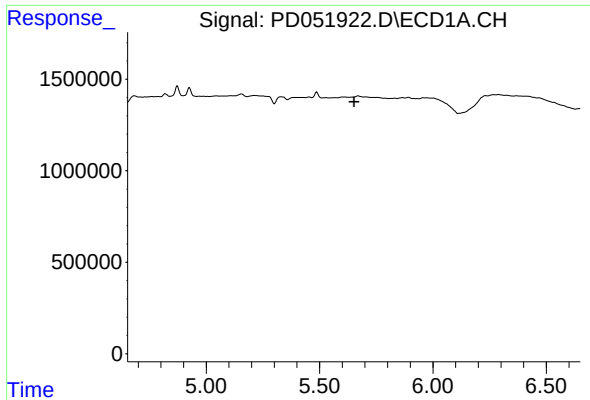

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.653 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

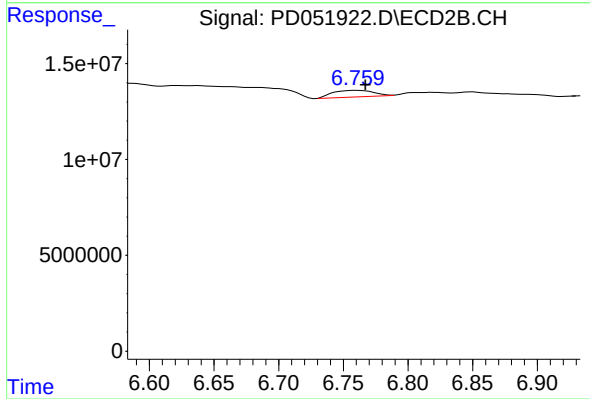


#14 Endrin

R.T.: 6.760 min
Delta R.T.: -0.007 min
Response: 7563921
Conc: 0.29 ng/ml

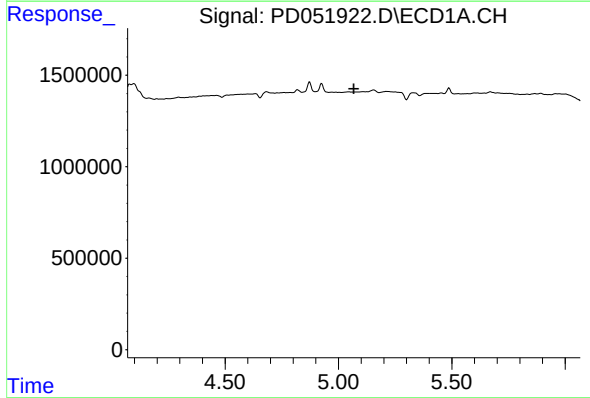


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

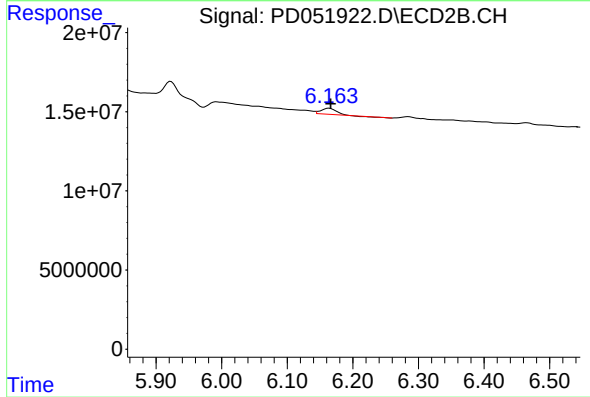

#25 Chlordane-3


R.T.: 6.164 min
Delta R.T.: -0.003 min
Response: 5993614
Conc: 1.35 ng/ml

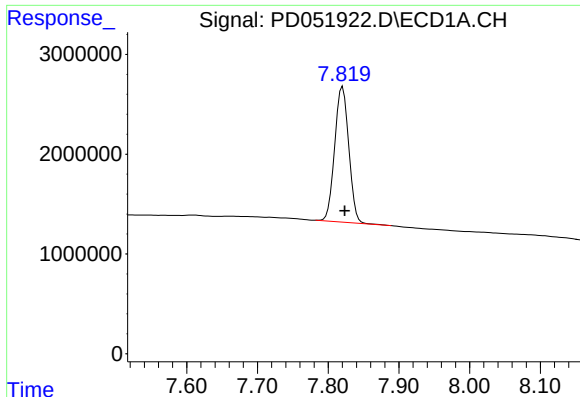

#28 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: -0.003 min
Response: 18781086
Conc: 16.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

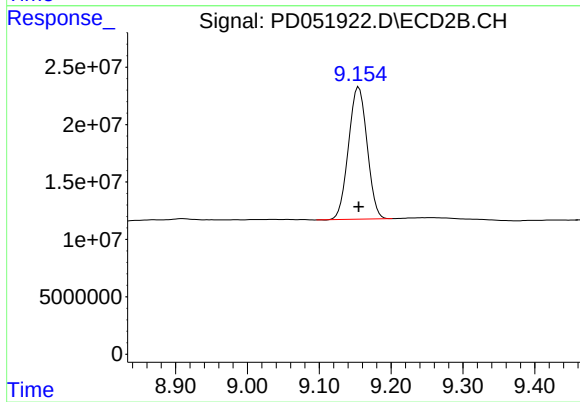

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 206545151
Conc: 11.31 ng/ml