

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032023\
 Data File : PD074285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2023 09:08
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 21:17:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:23:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
4)	MA	Heptachlor	4.956f	0.000	1429710	0	0.417	N.D.	#
7)	B	delta-BHC	4.786	0.000	2280762	0	0.831	N.D.	#
8)	B	Heptachlo...	5.709	0.000	144156	0	0.051	N.D.	#
11)	B	alpha-Chl...	6.034	0.000	203508	0	0.067	N.D.	#
12)	B	4,4'-DDE	6.234f	0.000	91414	0	0.033	N.D.	#
13)	MA	Dieldrin	6.370	0.000	109781	0	0.037	N.D.	#
14)	MA	Endrin	6.621f	0.000	11622	0	0.005	N.D.	#
15)	B	Endosulfa...	6.800f	0.000	278844	0	0.108	N.D.	#
19)	B	Endosulfa...	7.205f	0.000	34478	0	0.014	N.D.	#
21)	B	Endrin ke...	7.690f	0.000	977438	0	0.351	N.D.	#
26)		Chlordane-4	6.056	0.000	45176	0	0.075	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032023\
Data File : PD074285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2023 09:08
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 21:17:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:23:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

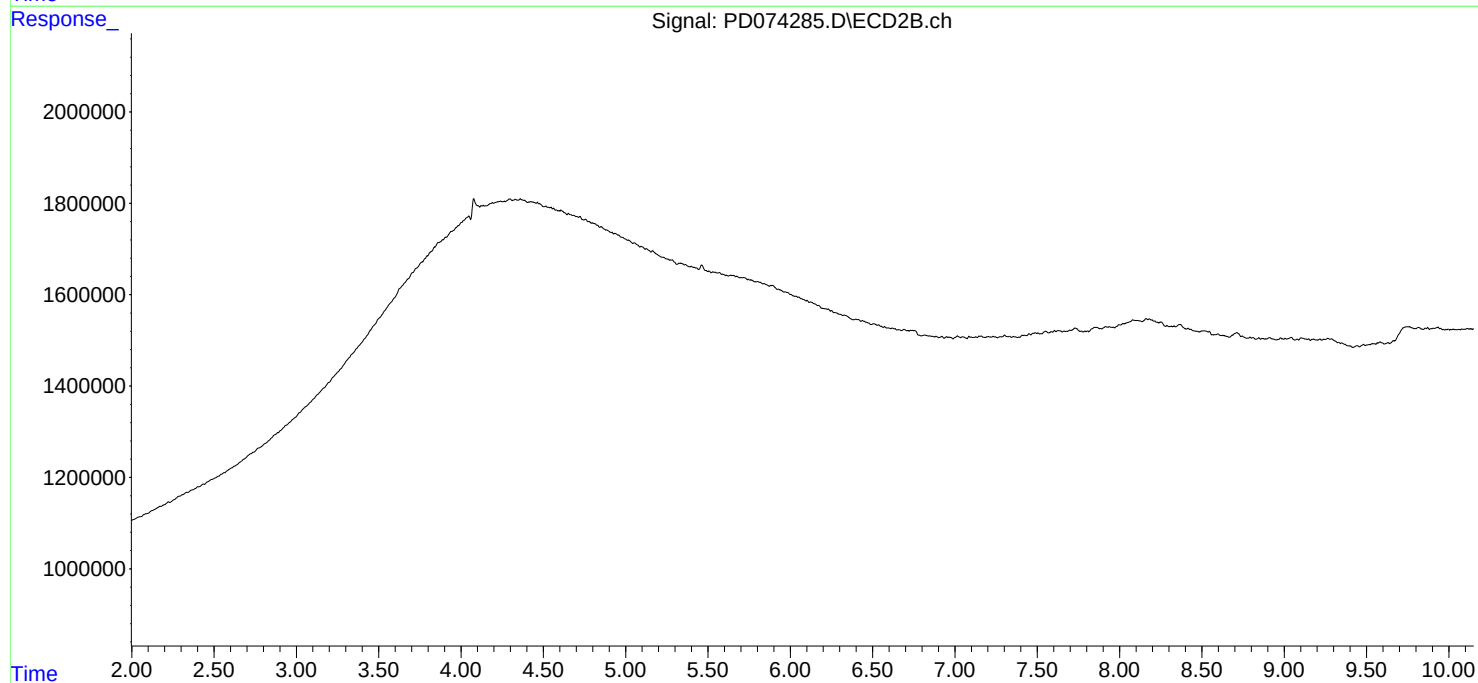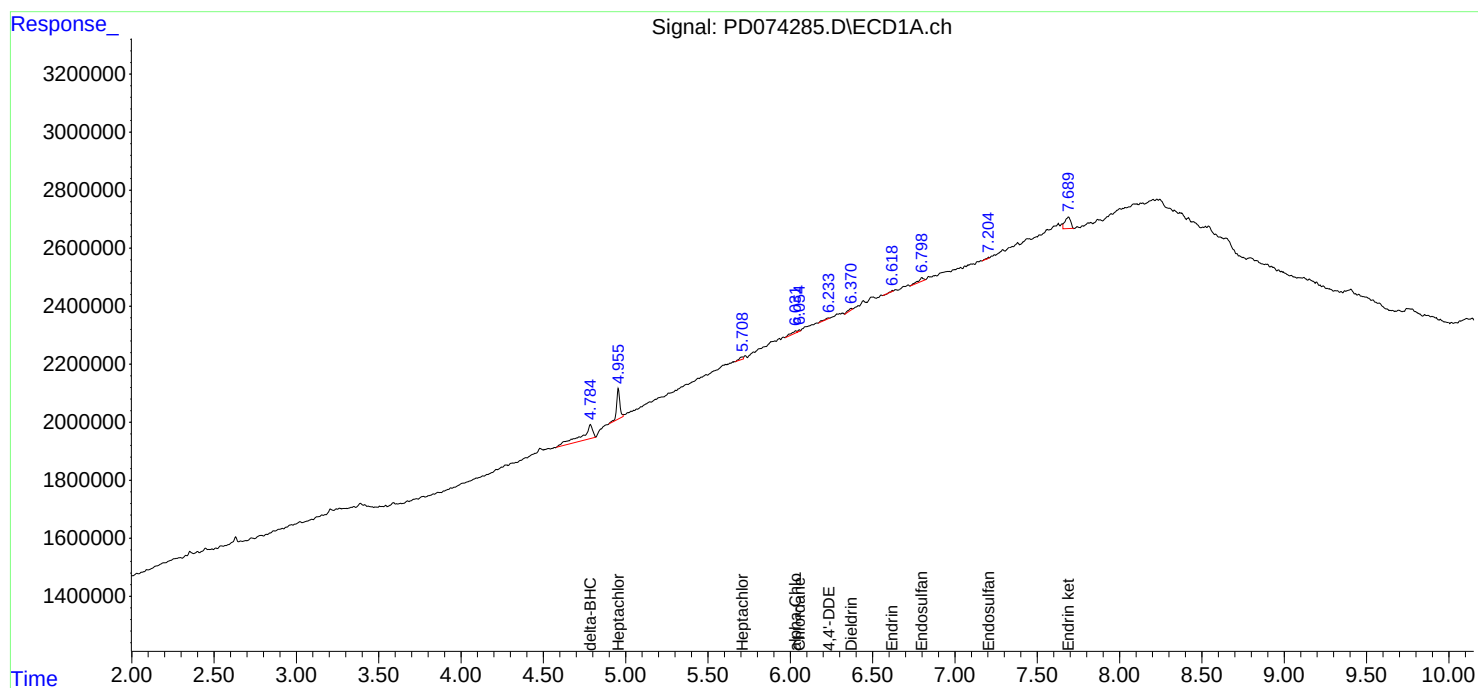


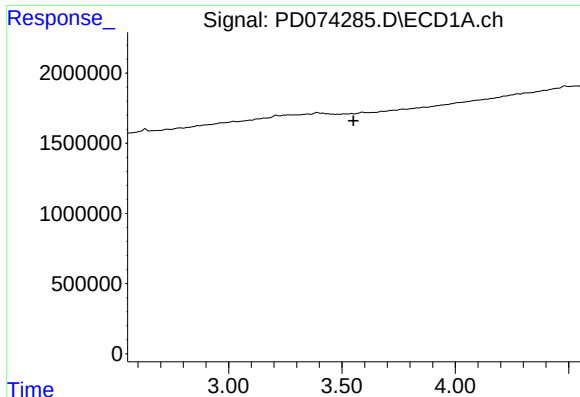

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

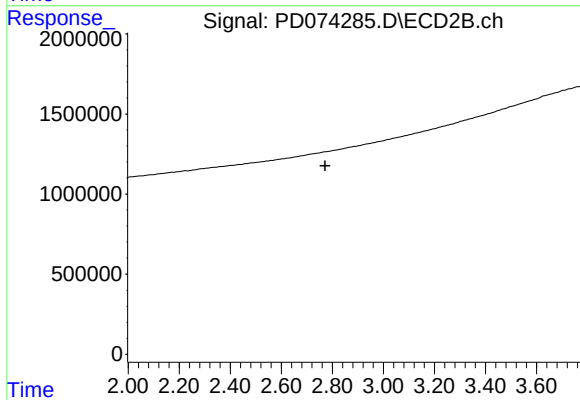


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.772 min
Response: 0
Conc: N.D.

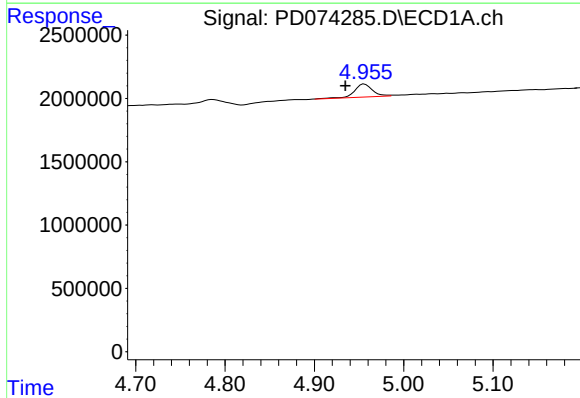


#4 Heptachlor

R.T.: 4.956 min
Delta R.T.: 0.021 min
Response: 1429710
Conc: 0.42 ng/ml

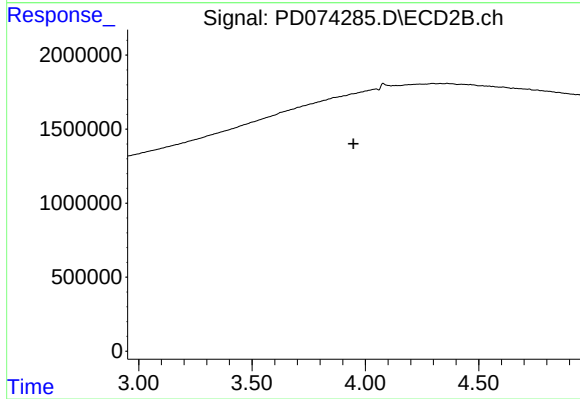

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.948 min
Response: 0
Conc: N.D.

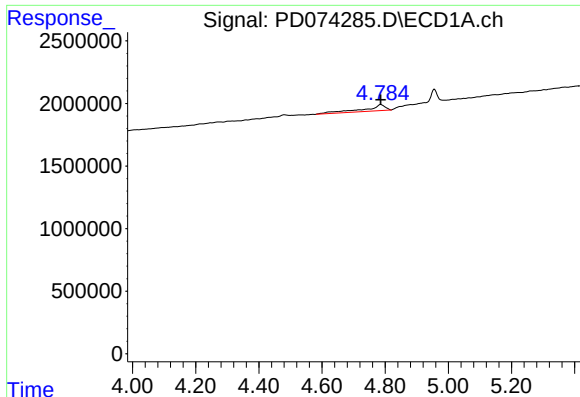

#7 delta-BHC


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 2280762
Conc: 0.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

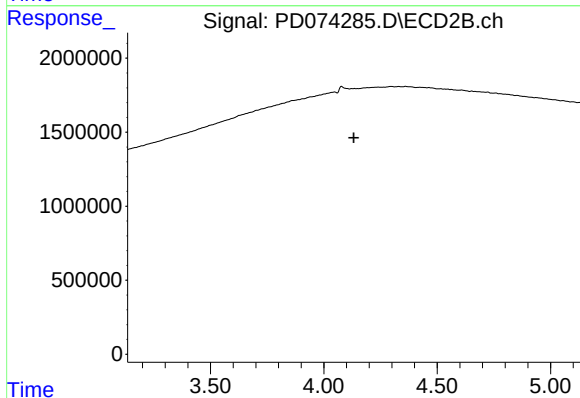


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

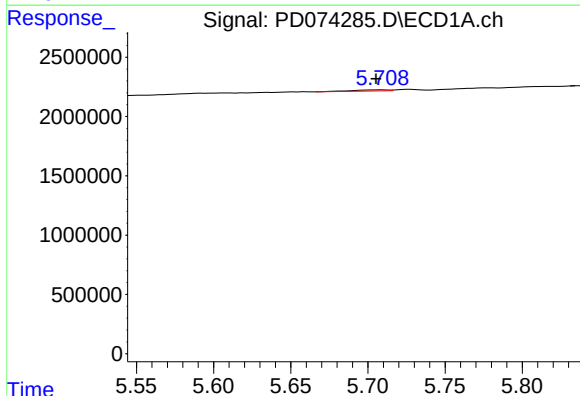


#8 Heptachlor epoxide

R.T.: 5.709 min
Delta R.T.: 0.004 min
Response: 144156
Conc: 0.05 ng/ml

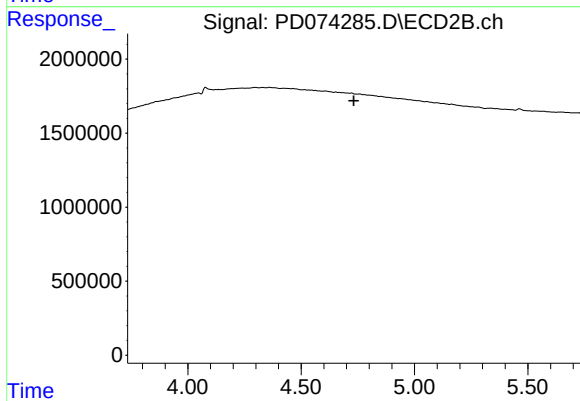

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

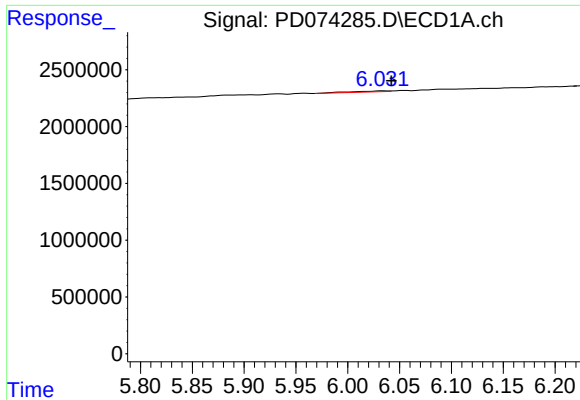

#11 alpha-Chlordane


R.T.: 6.034 min
Delta R.T.: -0.009 min
Response: 203508
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

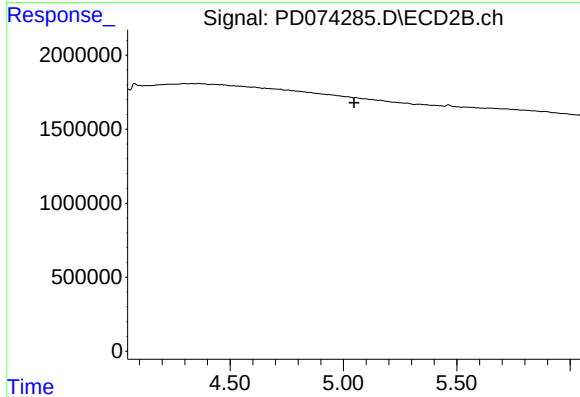


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.047 min
Response: 0
Conc: N.D.

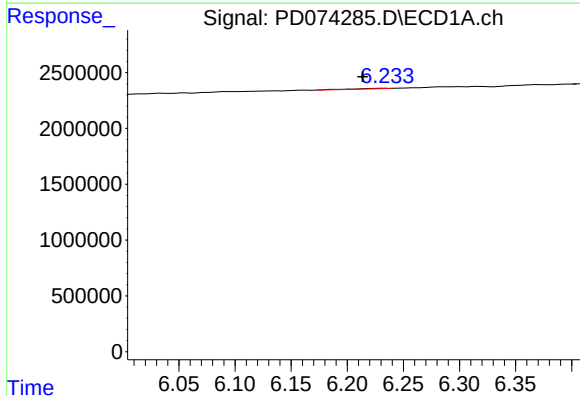


#12 4,4'-DDE

R.T.: 6.234 min
Delta R.T.: 0.020 min
Response: 91414
Conc: 0.03 ng/ml

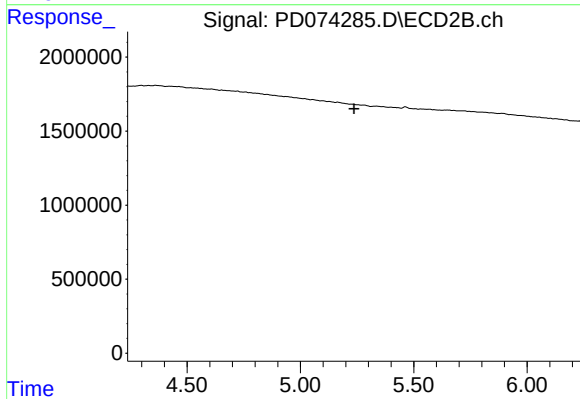

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 5.237 min
Response: 0
Conc: N.D.

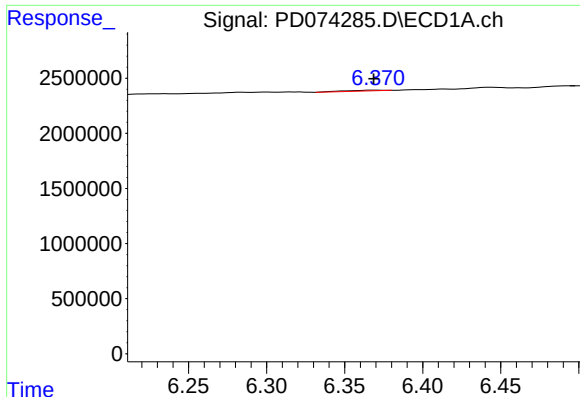

#13 Dieldrin


R.T.: 6.370 min
Delta R.T.: 0.002 min
Response: 109781
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

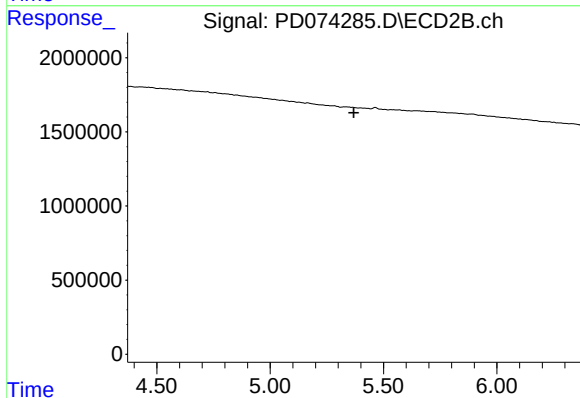


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.369 min
Response: 0
Conc: N.D.

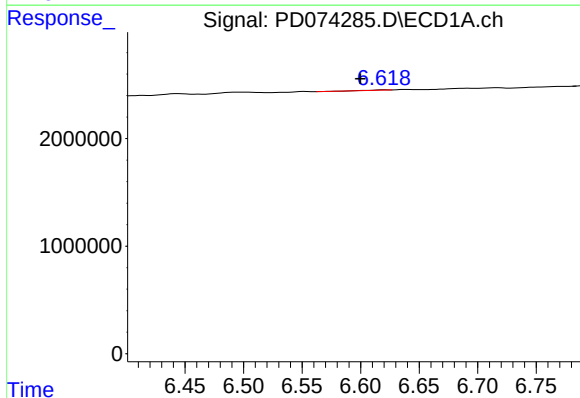


#14 Endrin

R.T.: 6.621 min
Delta R.T.: 0.021 min
Response: 11622
Conc: 0.00 ng/ml

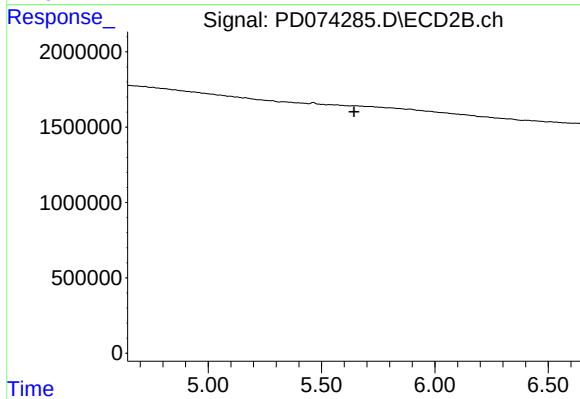

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

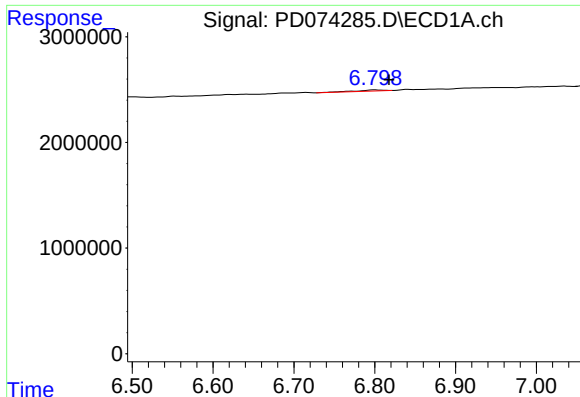

#15 Endosulfan II


R.T.: 6.800 min
Delta R.T.: -0.018 min
Response: 278844
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

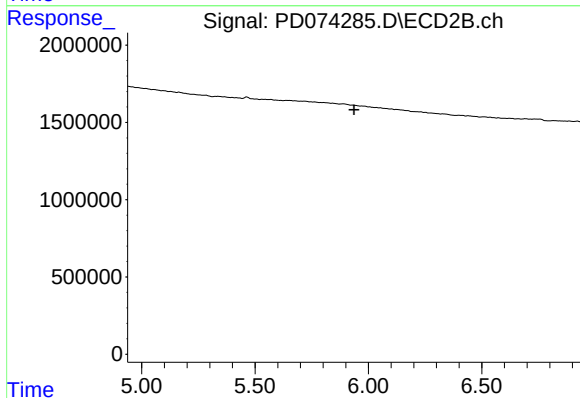


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.937 min
Response: 0
Conc: N.D.

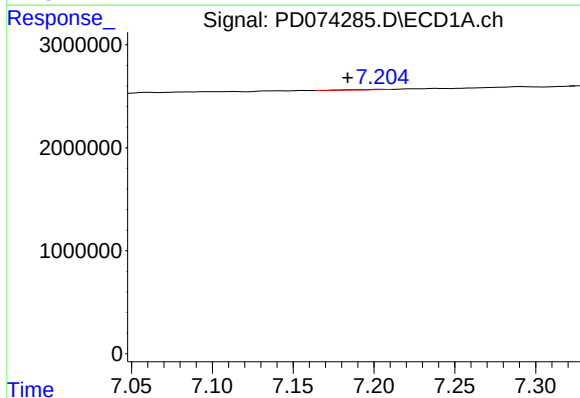


#19 Endosulfan Sulfate

R.T.: 7.205 min
Delta R.T.: 0.021 min
Response: 34478
Conc: 0.01 ng/ml

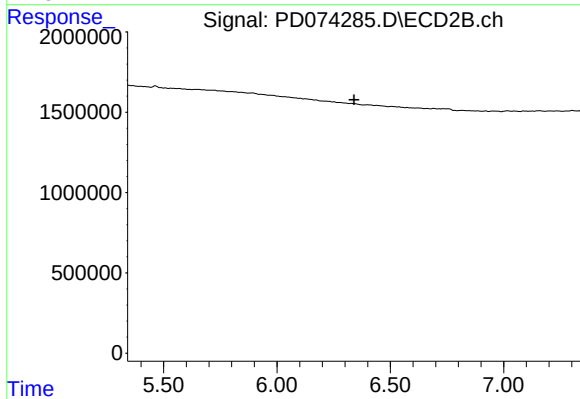

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.340 min
Response: 0
Conc: N.D.

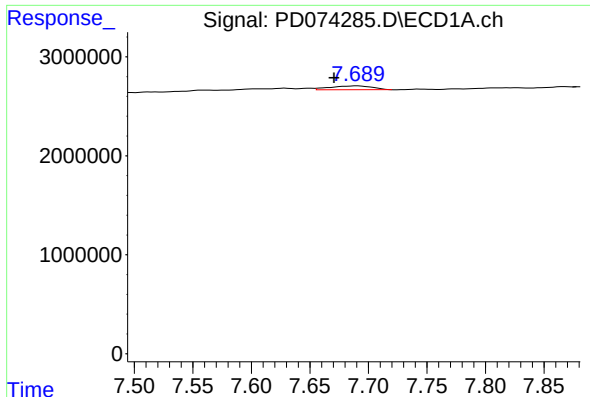

#21 Endrin ketone


R.T.: 7.690 min
Delta R.T.: 0.019 min
Response: 977438
Conc: 0.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

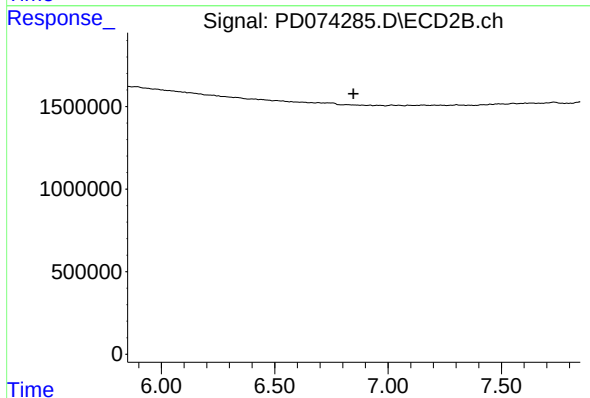


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

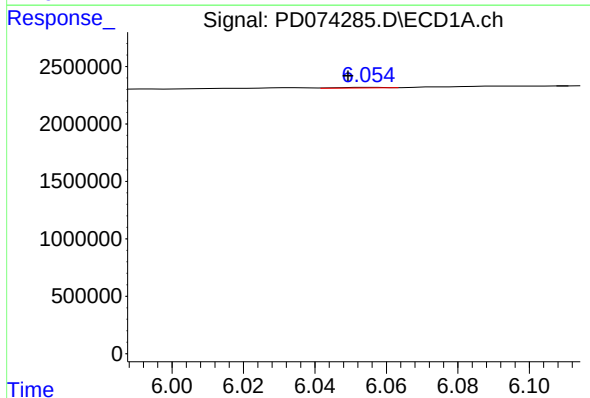


#26 Chlordane-4

R.T.: 6.056 min
Delta R.T.: 0.007 min
Response: 45176
Conc: 0.08 ng/ml

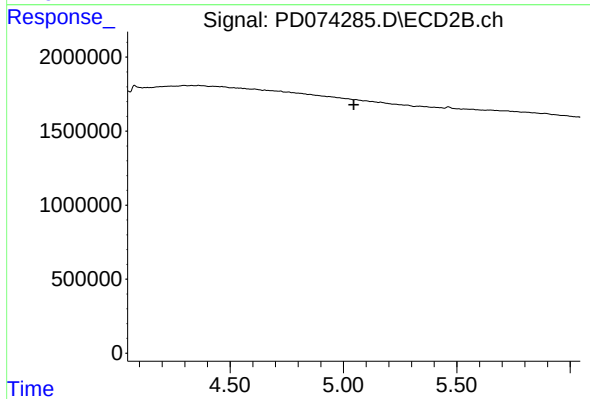

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.045 min
Response: 0
Conc: N.D.

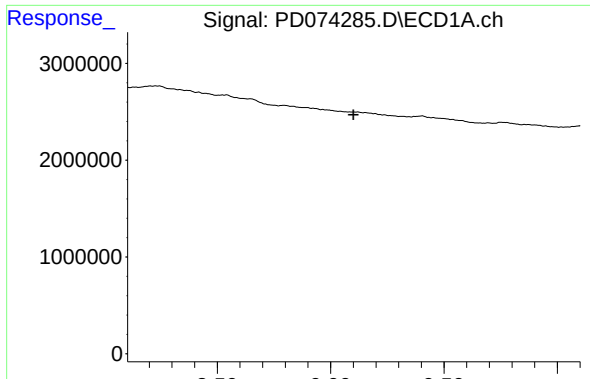

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

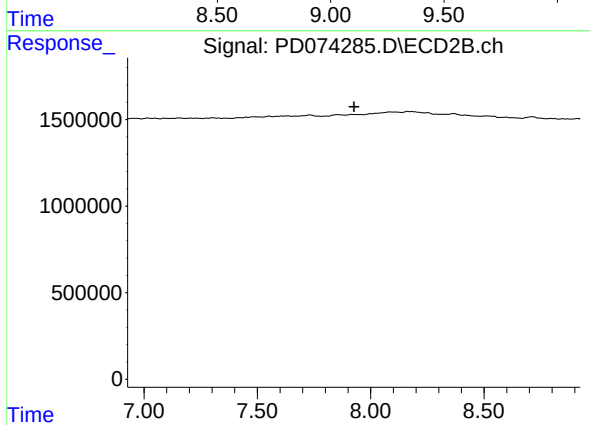

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.927 min
Response: 0
Conc: N.D.