

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032119\
 Data File : PD051942.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Mar 2019 18:38
 Operator : AJ\SJ
 Sample : PIBLK35
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK35

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 08:49:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032119CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 08:47:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	34568794	789.5E6	24.689	24.633
27)	SA Decachlor...	7.822	9.158	53255633	932.2E6	45.562	46.405
Target Compounds							
6)	B beta-BHC	0.000	4.938f	0 44765784	N.D.	2.124	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032119\
Data File : PD051942.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Mar 2019 18:38
Operator : AJ\SJ
Sample : PIBLK35
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 08:49:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032119CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 08:47:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

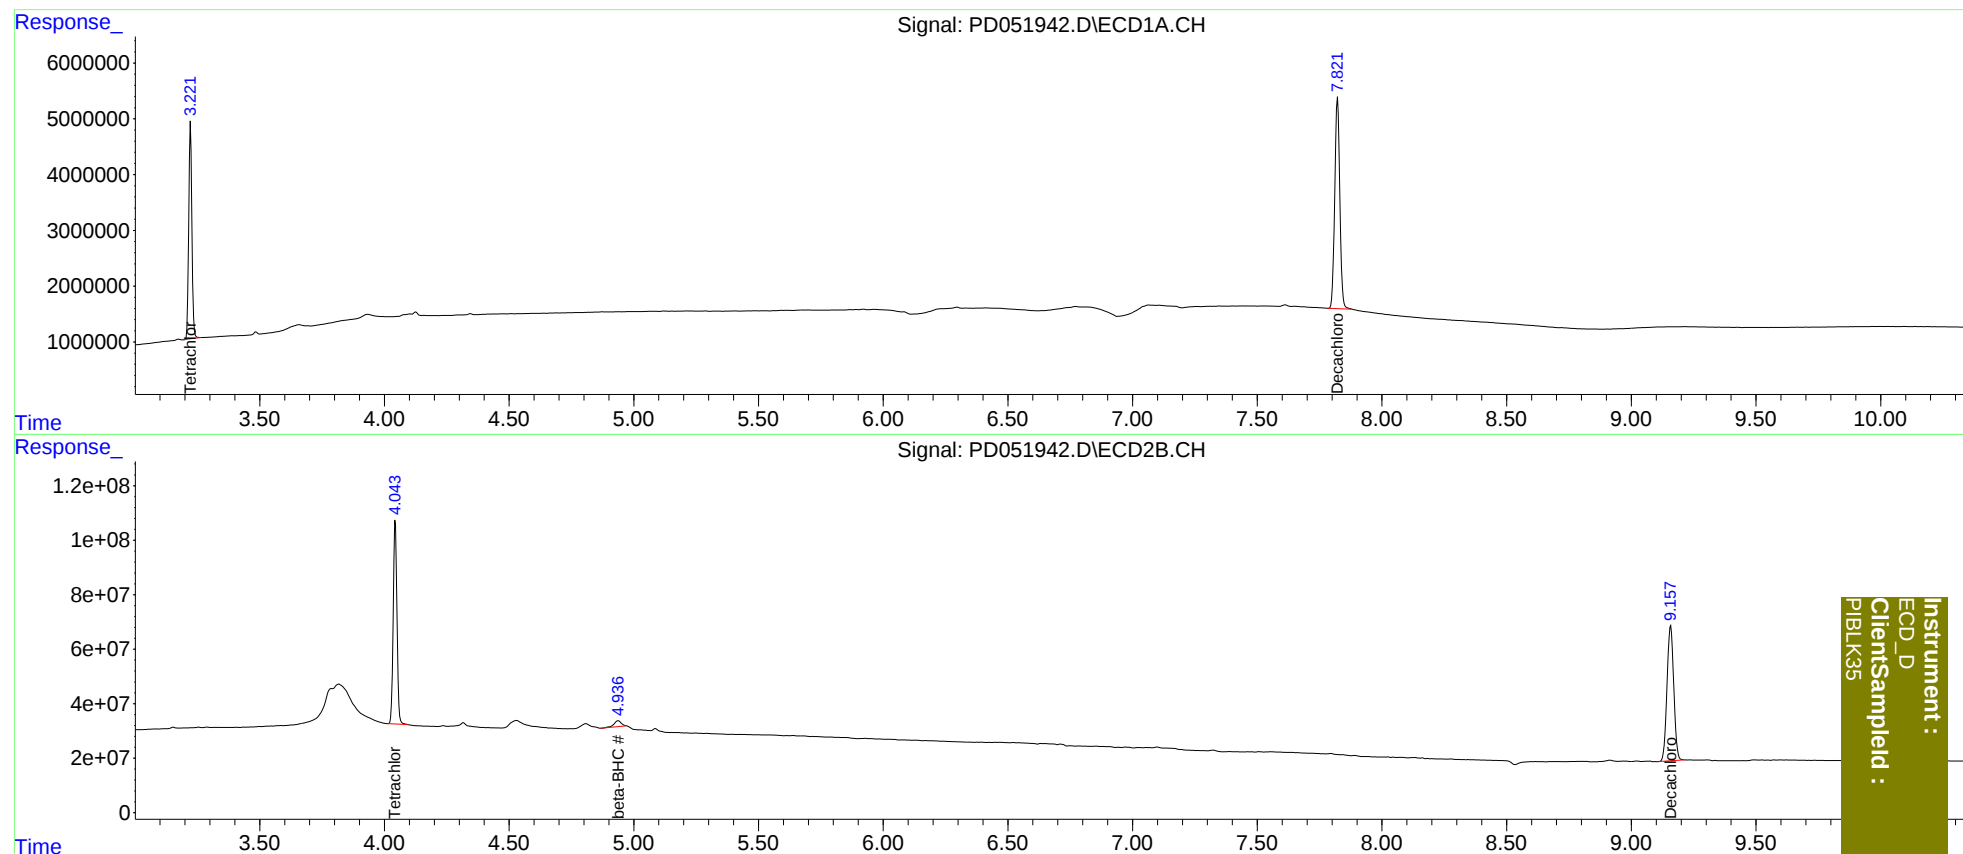


Instrument :
ECD_D
ClientSampleId :
PIBLK35

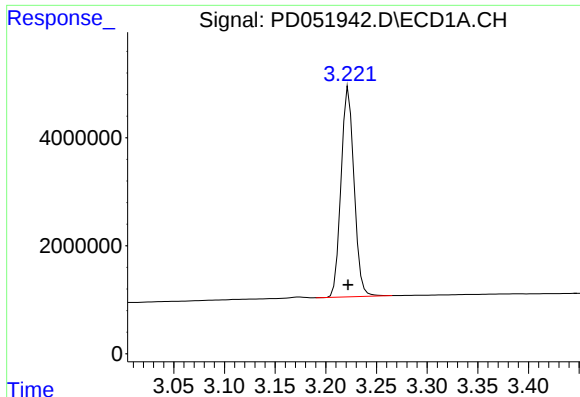

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 34568794
Conc: 24.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK35

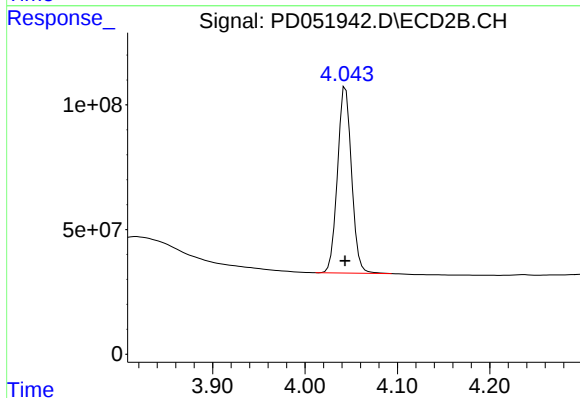


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 789485261
Conc: 24.63 ng/ml

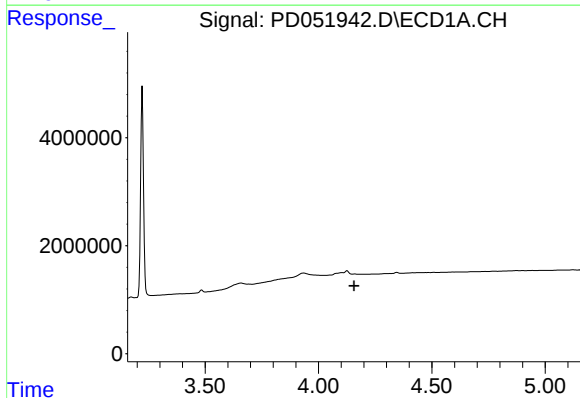


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.157 min
Response: 0
Conc: N.D.

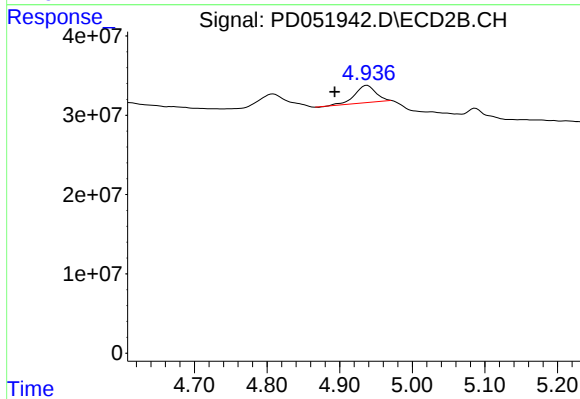

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.044 min
Response: 44765784
Conc: 2.12 ng/ml

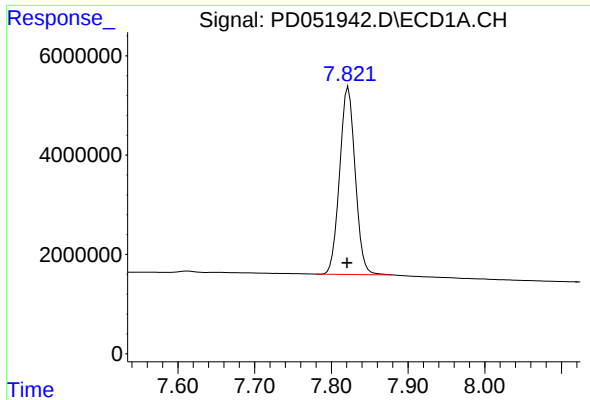

#27 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: 0.002 min
Response: 53255633
Conc: 45.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK35

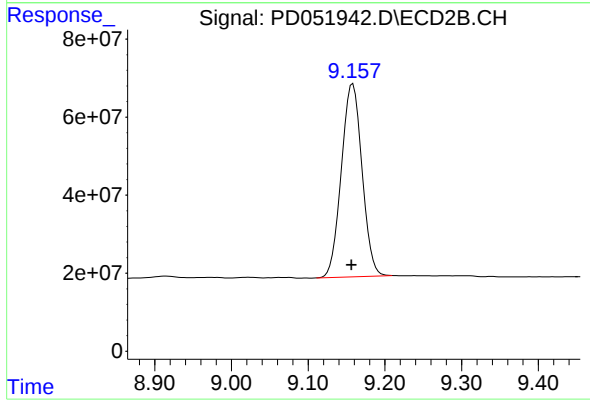

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.002 min
Response: 932201984
Conc: 46.41 ng/ml