

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032122\
 Data File : PD068708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2022 13:03
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:14:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	4.176	63541539	440.7E6	52.333	46.091
28)	SA Decachlor...	8.217	9.373	54728037	245.1E6	43.319	43.254
Target Compounds							
23)	Chlordane-1	4.327	5.199	19650570	178.5E6	463.061	452.376
24)	Chlordane-2	4.829	5.672	23219563	175.0E6	462.681	457.812
25)	Chlordane-3	5.398	6.328	64004215	603.4E6	459.033	449.103
26)	Chlordane-4	5.456	6.405	53175790	702.2E6	449.307	451.703
27)	Chlordane-5	6.293	7.216	22047750	127.0E6	441.311	435.145m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2022 13:03
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:14:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

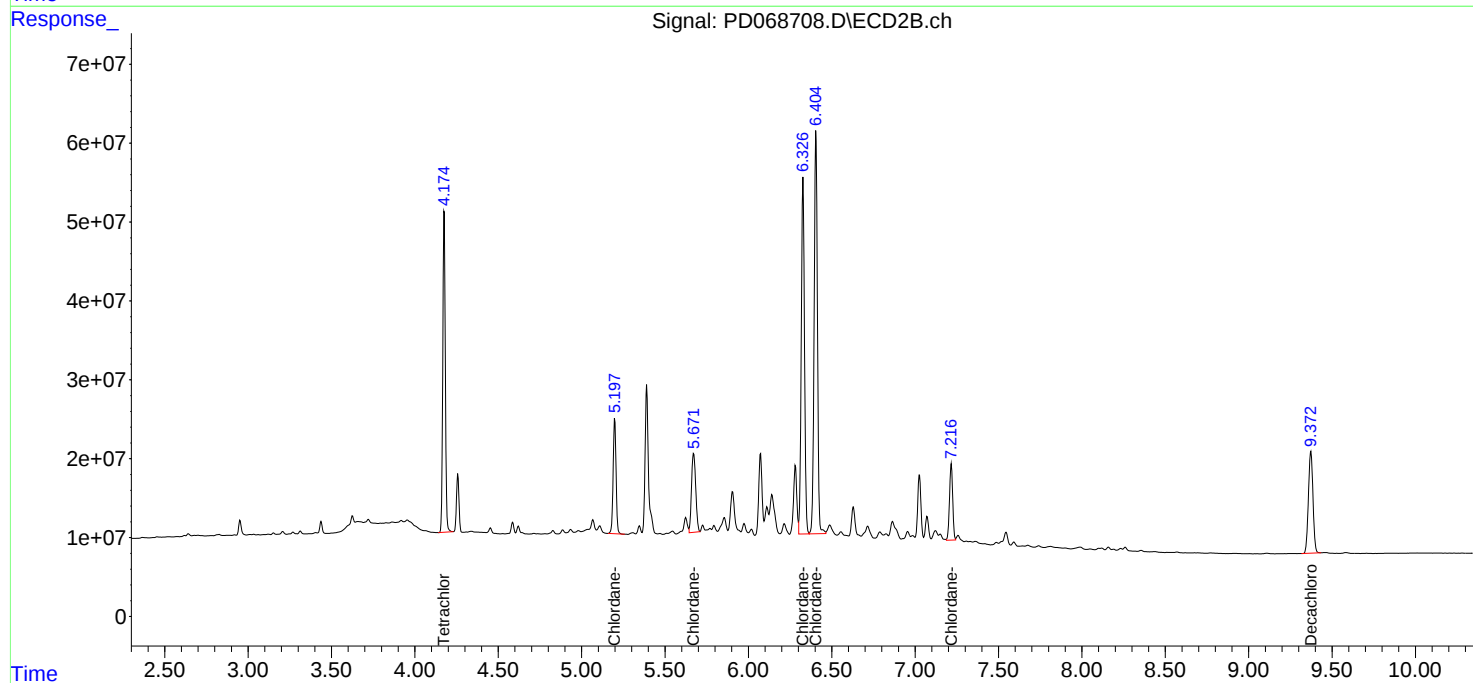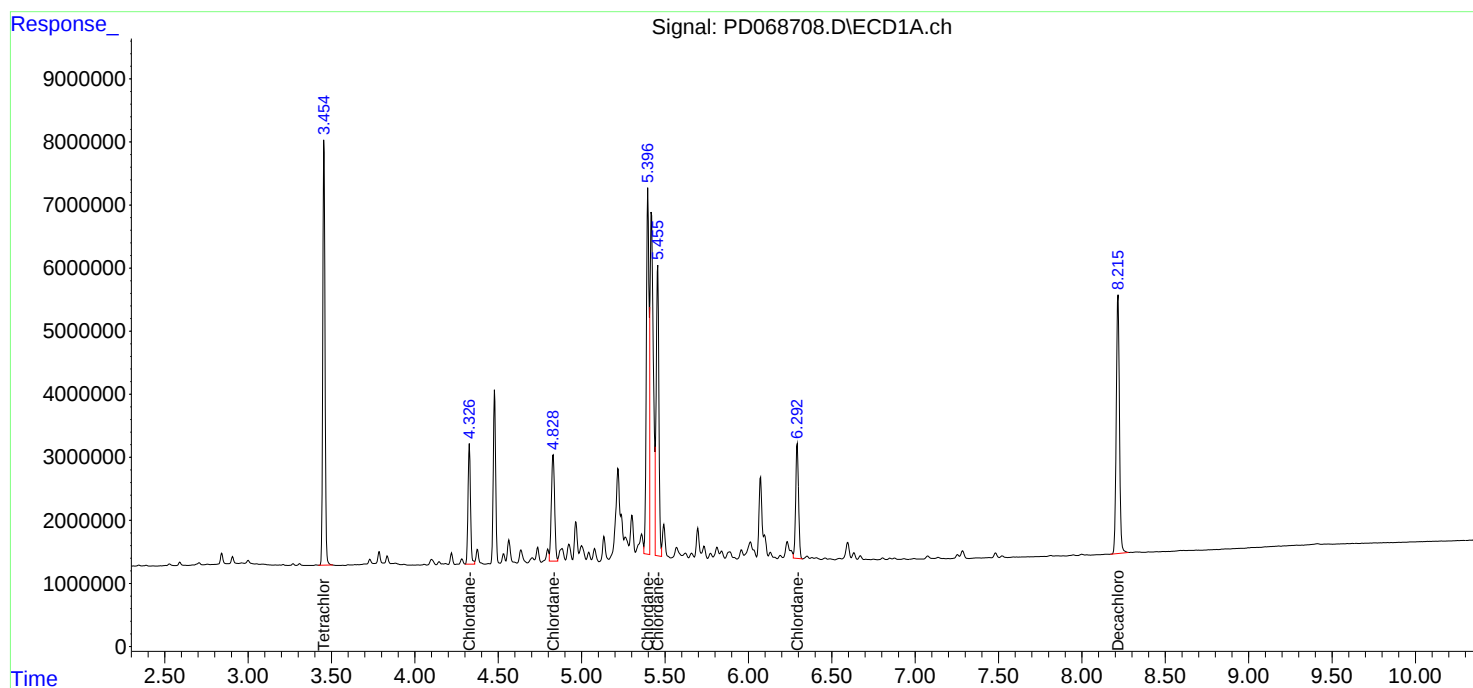


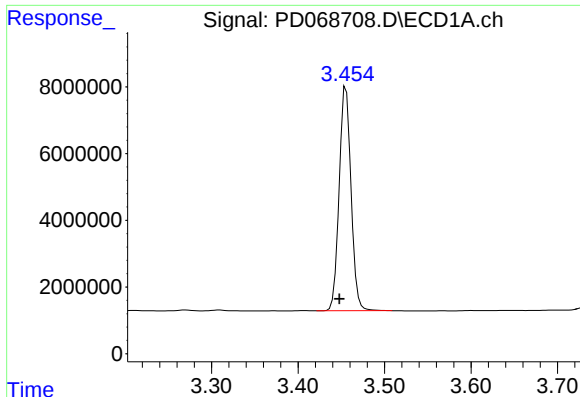

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: 0.008 min
Response: 63541539
Conc: 52.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

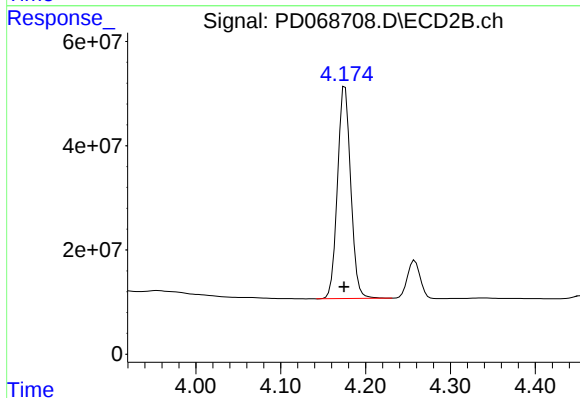


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.001 min
Response: 440668792
Conc: 46.09 ng/ml

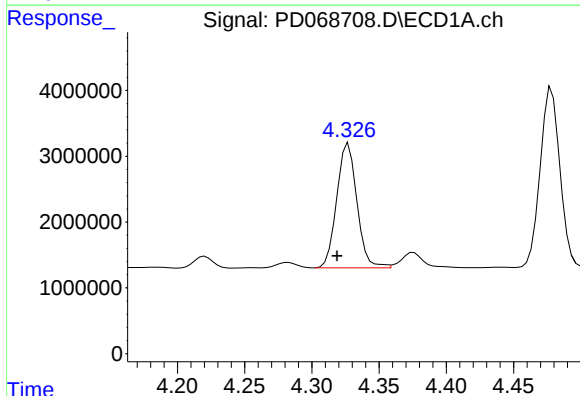


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.008 min
Response: 19650570
Conc: 463.06 ng/ml

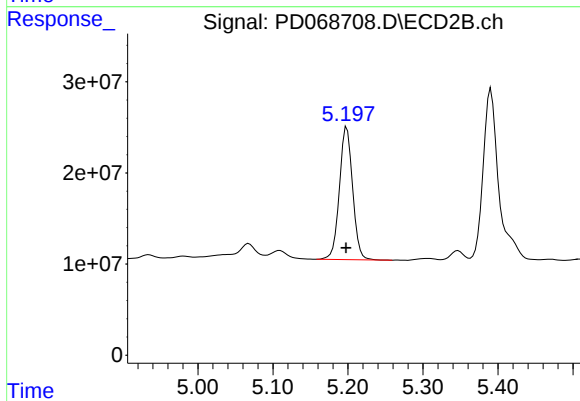

#23 Chlordane-1


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 178477121
Conc: 452.38 ng/ml

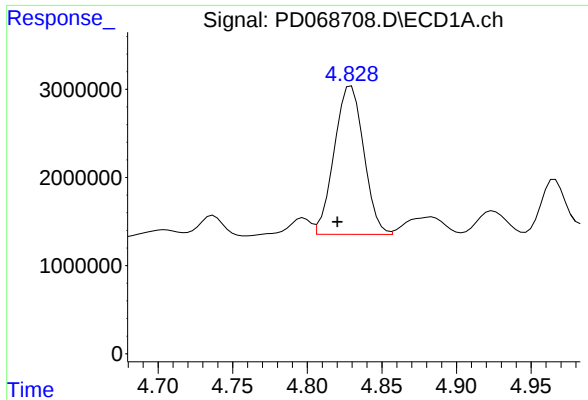

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.009 min
Response: 23219563
Conc: 462.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

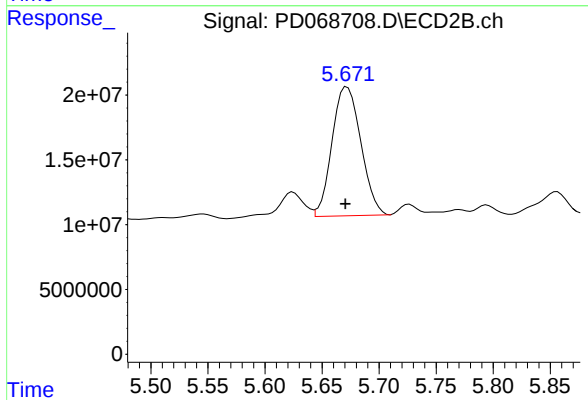


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.001 min
Response: 175015914
Conc: 457.81 ng/ml

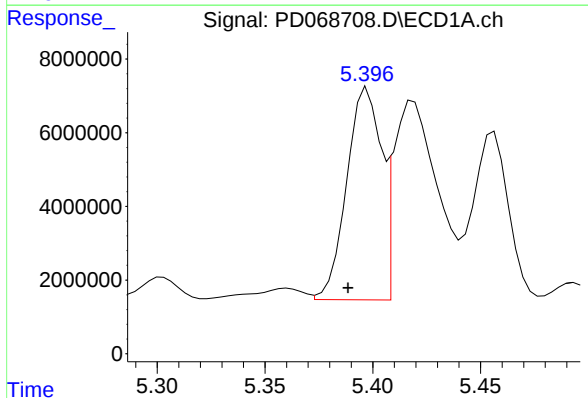


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.009 min
Response: 64004215
Conc: 459.03 ng/ml

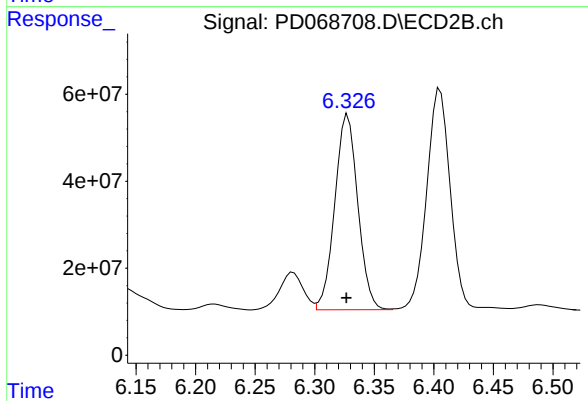

#25 Chlordane-3


R.T.: 6.328 min
Delta R.T.: 0.001 min
Response: 603407002
Conc: 449.10 ng/ml

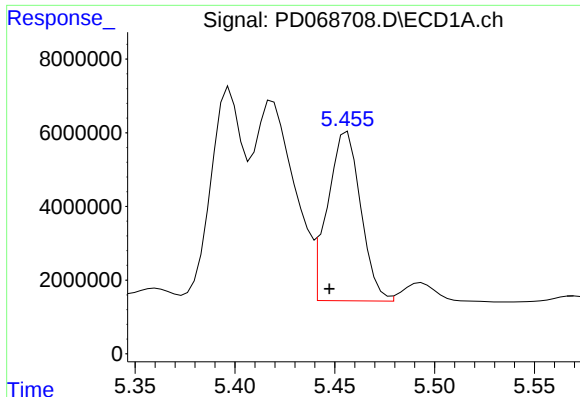

#26 Chlordane-4


R.T.: 5.456 min
Delta R.T.: 0.009 min
Response: 53175790
Conc: 449.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

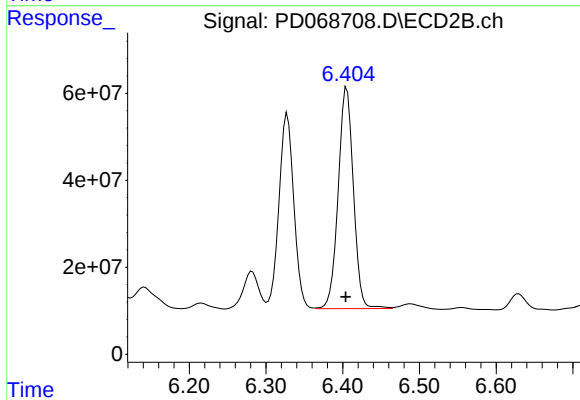


#26 Chlordane-4

R.T.: 6.405 min
Delta R.T.: 0.001 min
Response: 702211382
Conc: 451.70 ng/ml

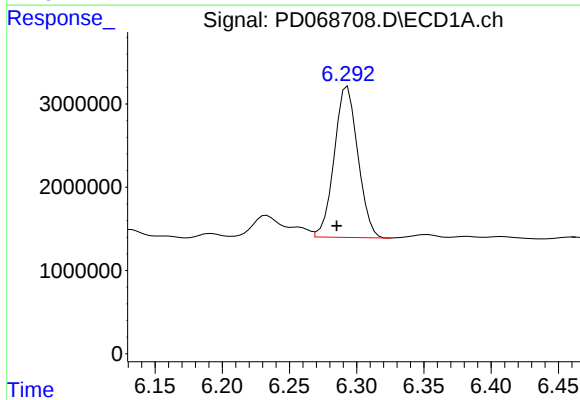


#27 Chlordane-5

R.T.: 6.293 min
Delta R.T.: 0.008 min
Response: 22047750
Conc: 441.31 ng/ml

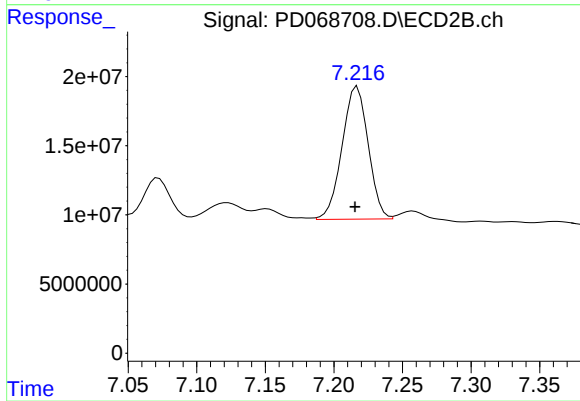

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 126970483
Conc: 435.15 ng/ml m

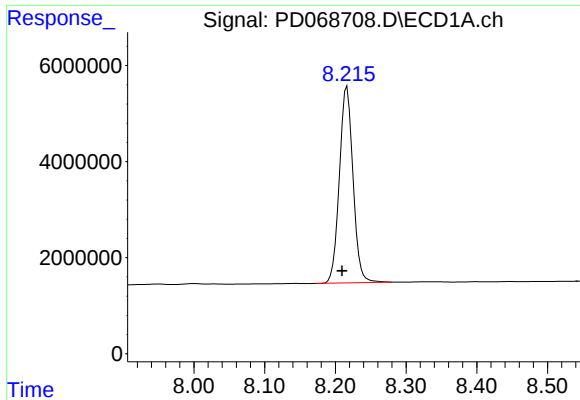

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: 0.007 min
Response: 54728037
Conc: 43.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

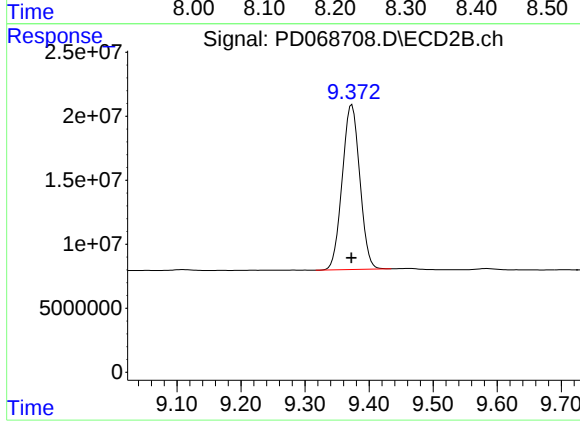

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 245107488
Conc: 43.25 ng/ml