

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032122\
 Data File : PD068717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2022 18:26
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:24:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.173	62896822	425.6E6	51.802	44.514
28)	SA Decachlor...	8.205	9.368	56736158	256.3E6	44.908	45.234
Target Compounds							
23)	Chlordane-1	4.315	5.195	19324423	178.5E6	455.375	452.369
24)	Chlordane-2	4.817	5.668	22452805	171.0E6	447.402	447.323
25)	Chlordane-3	5.385	6.323	63647374	595.8E6	456.474	443.427
26)	Chlordane-4	5.444	6.401	53193706	697.2E6	449.458	448.470
27)	Chlordane-5	6.281	7.211	22692781	129.4E6	454.222	443.471m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031222\
Data File : PD068717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2022 18:26
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:24:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

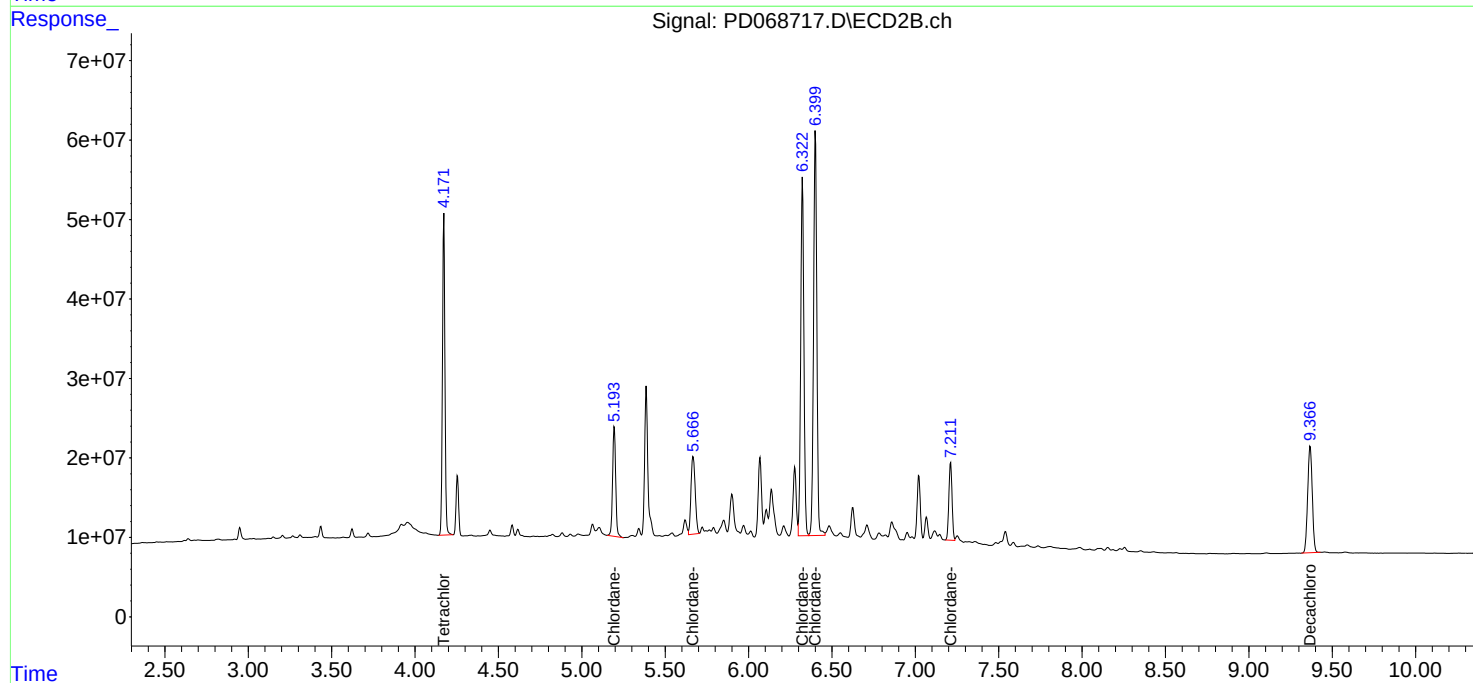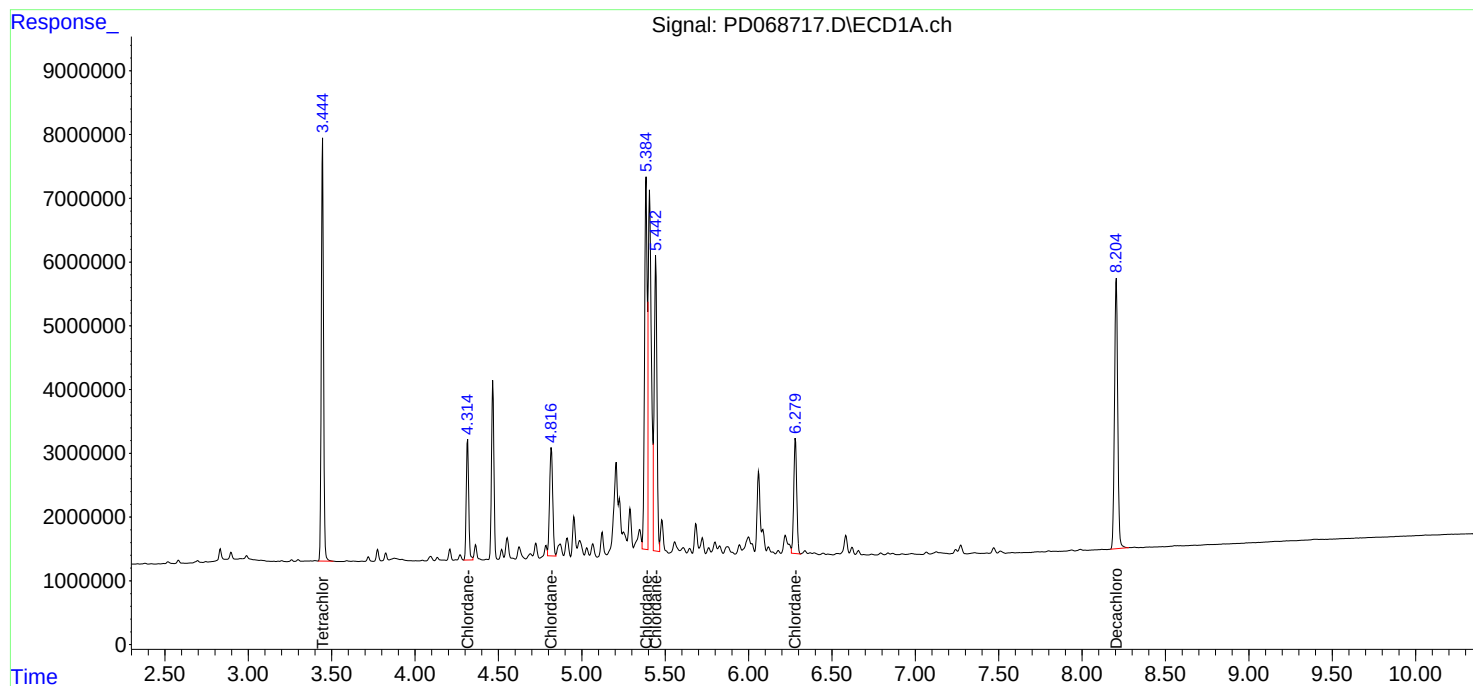


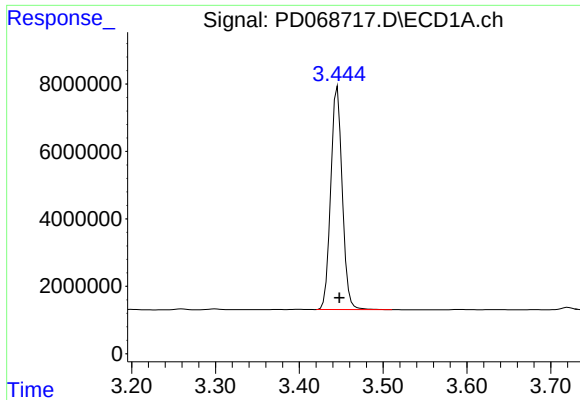

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.002 min
Response: 62896822
Conc: 51.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

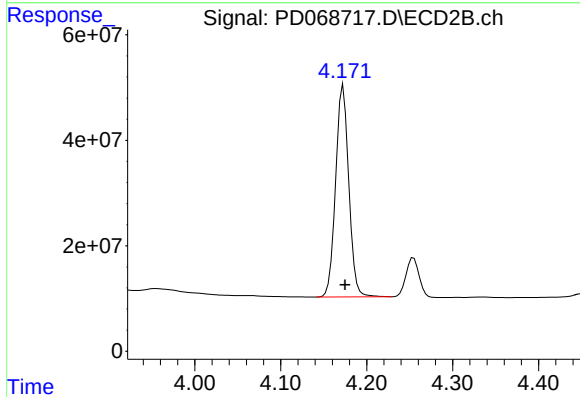


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.002 min
Response: 425585740
Conc: 44.51 ng/ml

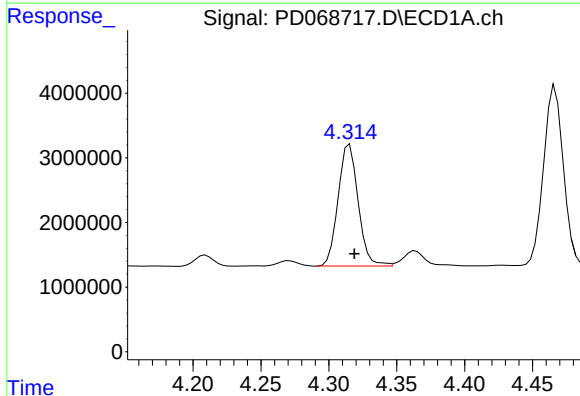


#23 Chlordane-1

R.T.: 4.315 min
Delta R.T.: -0.004 min
Response: 19324423
Conc: 455.38 ng/ml

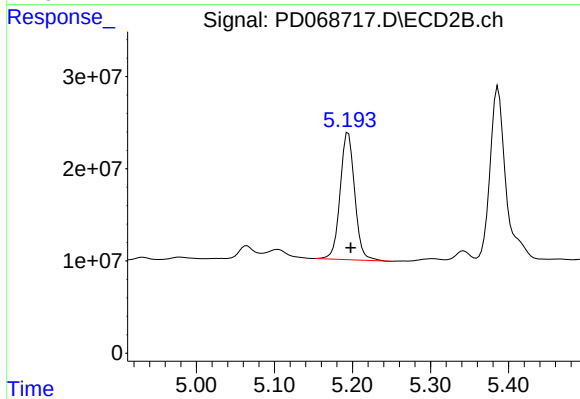

#23 Chlordane-1


R.T.: 5.195 min
Delta R.T.: -0.003 min
Response: 178474303
Conc: 452.37 ng/ml

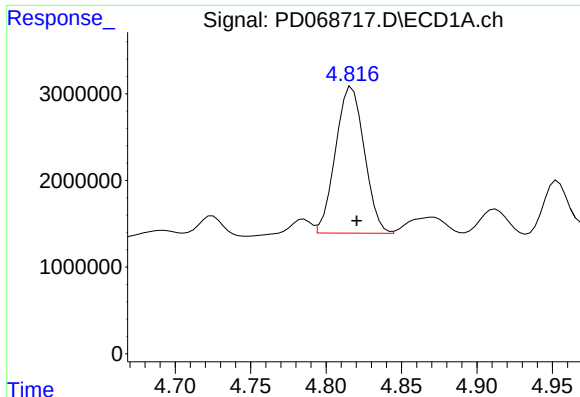

#24 Chlordane-2


R.T.: 4.817 min
Delta R.T.: -0.003 min
Response: 22452805
Conc: 447.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

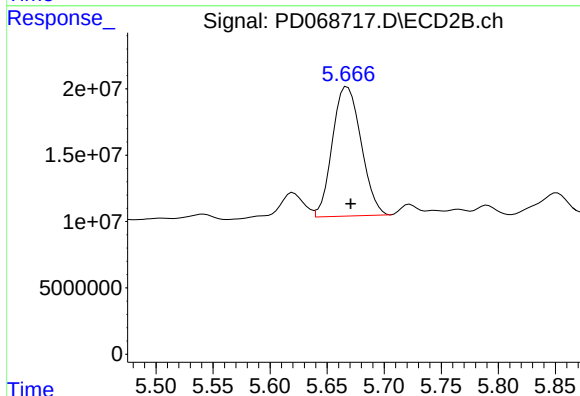


#24 Chlordane-2

R.T.: 5.668 min
Delta R.T.: -0.003 min
Response: 171006055
Conc: 447.32 ng/ml

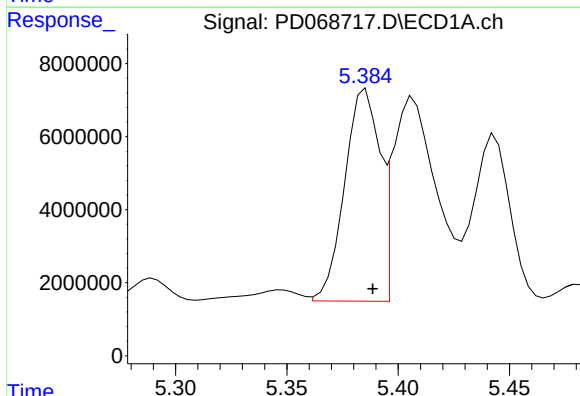


#25 Chlordane-3

R.T.: 5.385 min
Delta R.T.: -0.003 min
Response: 63647374
Conc: 456.47 ng/ml

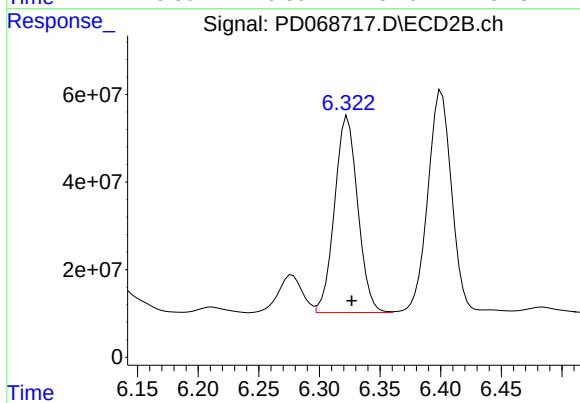

#25 Chlordane-3


R.T.: 6.323 min
Delta R.T.: -0.003 min
Response: 595779752
Conc: 443.43 ng/ml

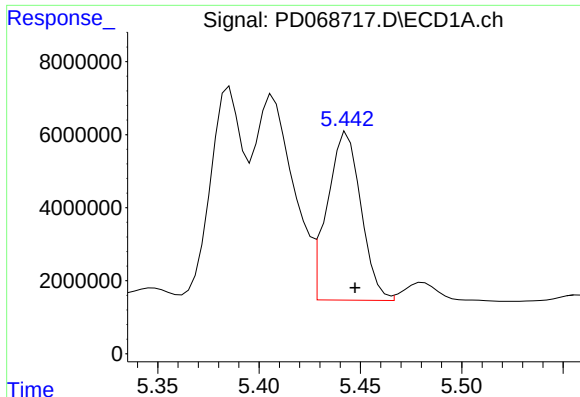

#26 Chlordane-4


R.T.: 5.444 min
Delta R.T.: -0.004 min
Response: 53193706
Conc: 449.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

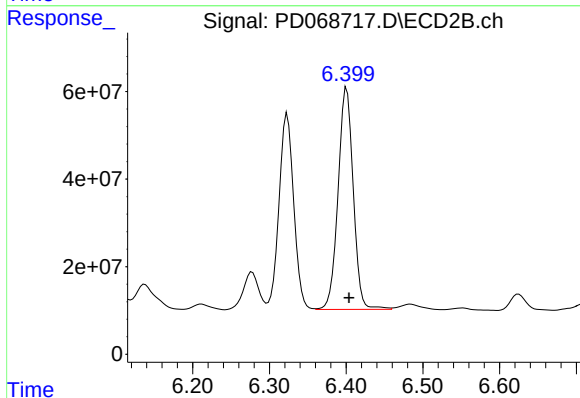


#26 Chlordane-4

R.T.: 6.401 min
Delta R.T.: -0.003 min
Response: 697185622
Conc: 448.47 ng/ml

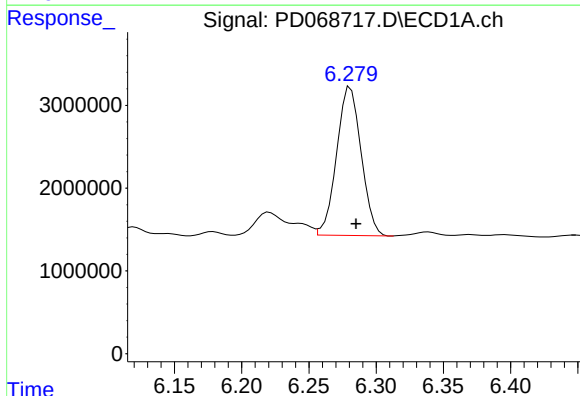


#27 Chlordane-5

R.T.: 6.281 min
Delta R.T.: -0.004 min
Response: 22692781
Conc: 454.22 ng/ml

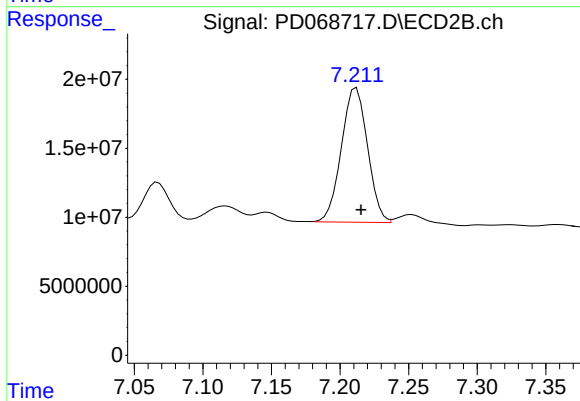

#27 Chlordane-5


R.T.: 7.211 min
Delta R.T.: -0.005 min
Response: 129399871
Conc: 443.47 ng/ml m

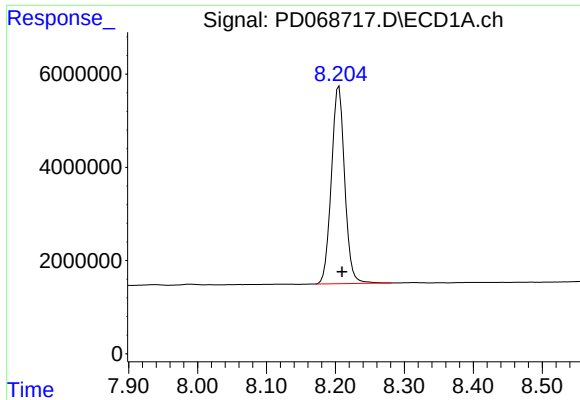

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.005 min
Response: 56736158
Conc: 44.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

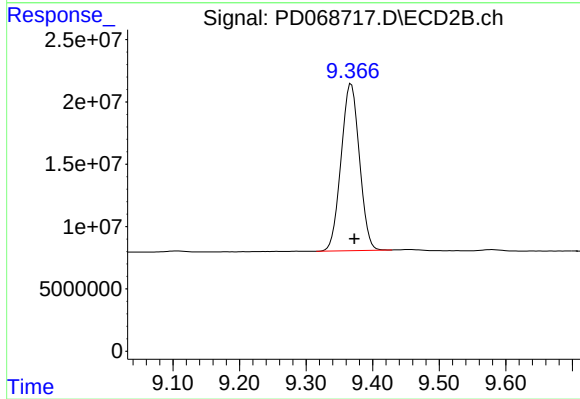

#28 Decachlorobiphenyl

R.T.: 9.368 min
Delta R.T.: -0.005 min
Response: 256331118
Conc: 45.23 ng/ml