

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\Pd032125\
 Data File : PD087983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2025 08:37
 Operator : AR\AJ
 Sample : RESC203
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 12:39:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032125CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 21 12:36:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.884	40078258	316.9E6	20.322	20.617
2)	SA Decachlor...	9.084	8.082	131.7E6	713.3E6	39.303	40.175
Target Compounds							
2)	A alpha-BHC	4.003	3.397	39659229	262.1E6	9.649	10.814
3)	MA gamma-BHC...	4.335	3.734	39416842	242.1E6	9.886	10.880
4)	MA Heptachlor	4.935	4.089	40763573	244.1E6	9.966	10.695
5)	MB Aldrin	5.277	4.375	37739116	236.5E6	10.079	11.088
6)	B beta-BHC	4.519	4.030	16715194	107.2E6	10.316	10.916
7)	B delta-BHC	4.768	4.267	39807261	231.0E6	10.060	10.544
8)	B Heptachlo...	5.697	4.879	34727060	212.2E6	9.969	10.787
9)	A Endosulfan I	6.080	5.253	34263324	212.6E6	10.245	12.254
10)	B trans-Chl...	5.952	5.132	33751822	222.1E6	9.884	10.766
11)	B cis-Chlor...	6.033	5.197	34041480	215.7E6	9.949	10.839
12)	B 4,4'-DDE	6.202	5.382	62531790	410.7E6	19.204	21.385
13)	MA Dieldrin	6.353	5.519	72833753	441.0E6	19.832	21.792
14)	MA Endrin	6.581	5.796	60826892	393.5E6	19.841	21.681
15)	B Endosulfa...	6.792	6.087	60139663	370.1E6	19.942	21.581
16)	A 4,4'-DDD	6.711	5.936	50522295	354.1E6	19.604	21.671
17)	MA 4,4'-DDT	7.028	6.191	55076240	360.3E6	20.387	21.509
18)	B Endrin al...	6.921	6.266	46709055	291.6E6	20.317	21.915
19)	B Endosulfa...	7.155	6.489	56077848	362.8E6	19.965	21.654
20)	A Methoxychlor	7.500	6.762	153.7E6	821.4E6	103.125	110.241
21)	B Endrin ke...	7.637	6.999	61588938	403.4E6	20.235	22.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\Pd032125\
Data File : PD087983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2025 08:37
Operator : AR\AJ
Sample : RESC203
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 12:39:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032125CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 21 12:36:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

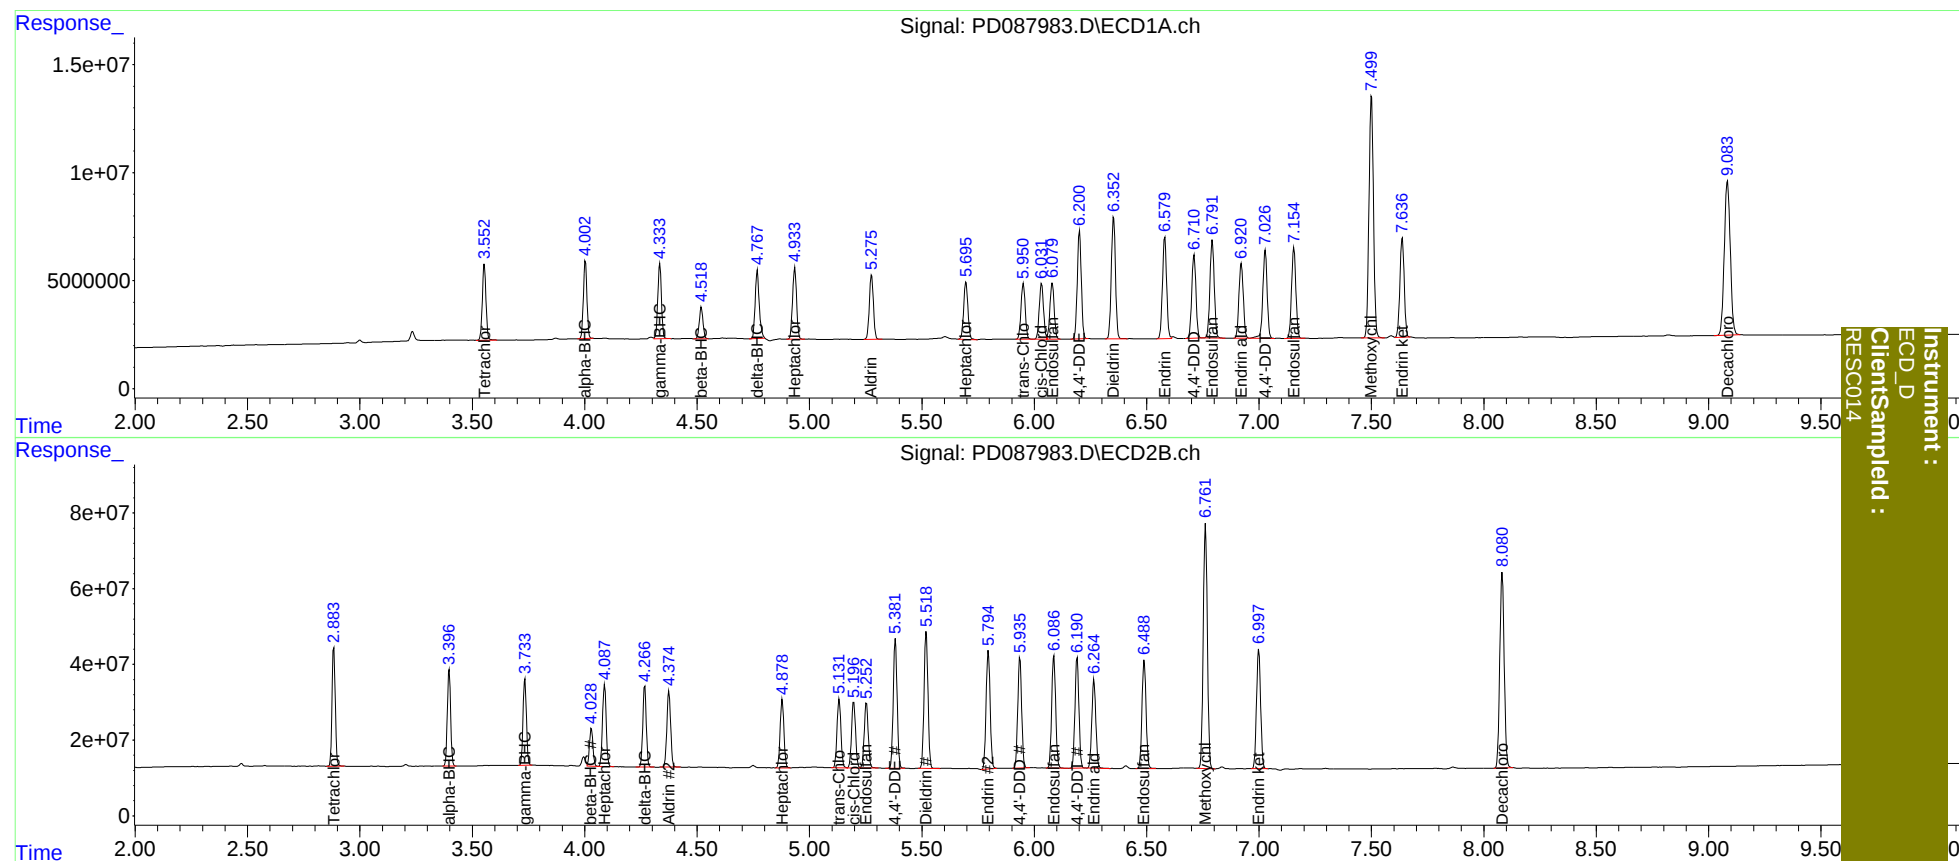

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032125\
Data File : PD087983.D
Acq On : 21 Mar 2025 08:37
Operator : AR\AJ
Sample : RESC203
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032125CLP.M
Title : GC Extractables
Last Update : Fri Mar 21 12:36:13 2025
Integrator: ChemStation

RT#1	RT#2	Resolution
3.554	4.003	100.00%
4.003	4.335	100.00%
4.335	4.519	100.00%
4.519	4.768	100.00%
4.768	4.935	100.00%
4.935	5.277	100.00%
5.277	5.697	100.00%
5.697	5.952	100.00%
5.952	6.033	100.00%
6.033	6.080	95.69%
6.080	6.202	100.00%
6.202	6.353	100.00%
6.353	6.581	100.00%
6.581	6.711	100.00%
6.711	6.792	100.00%
6.792	6.921	100.00%
6.921	7.028	100.00%
7.028	7.155	100.00%
7.155	7.500	100.00%
7.500	7.637	100.00%
7.637	9.084	100.00%

Signal #2

2.884	3.397	100.00%
3.397	3.734	100.00%
3.734	4.030	100.00%
4.030	4.089	100.00%
4.089	4.267	100.00%
4.267	4.375	100.00%
4.375	4.879	100.00%
4.879	5.132	100.00%
5.132	5.197	99.11%
5.197	5.253	99.29%
5.253	5.382	100.00%
5.382	5.519	100.00%
5.519	5.796	100.00%
5.796	5.936	100.00%
5.936	6.087	100.00%
6.087	6.191	100.00%
6.191	6.266	100.00%
6.266	6.489	100.00%
6.489	6.762	100.00%
6.762	6.999	100.00%
6.999	8.082	100.00%