

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032219\
 Data File : PD051967.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Mar 2019 19:04
 Operator : AJ\SJ
 Sample : K2050-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CS-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 23:18:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.222	4.045	11508969	281.0E6	8.680	9.799
28) SA Decachlor...	7.824	9.164	8649417	145.7E6	7.609	7.974
Target Compounds						
17) MA 4,4'-DDT	6.022	7.190	1654923	18271006	1.036	0.902



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032219\
Data File : PD051967.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Mar 2019 19:04
Operator : AJ\SJ
Sample : K2050-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
CS-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 23:18:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

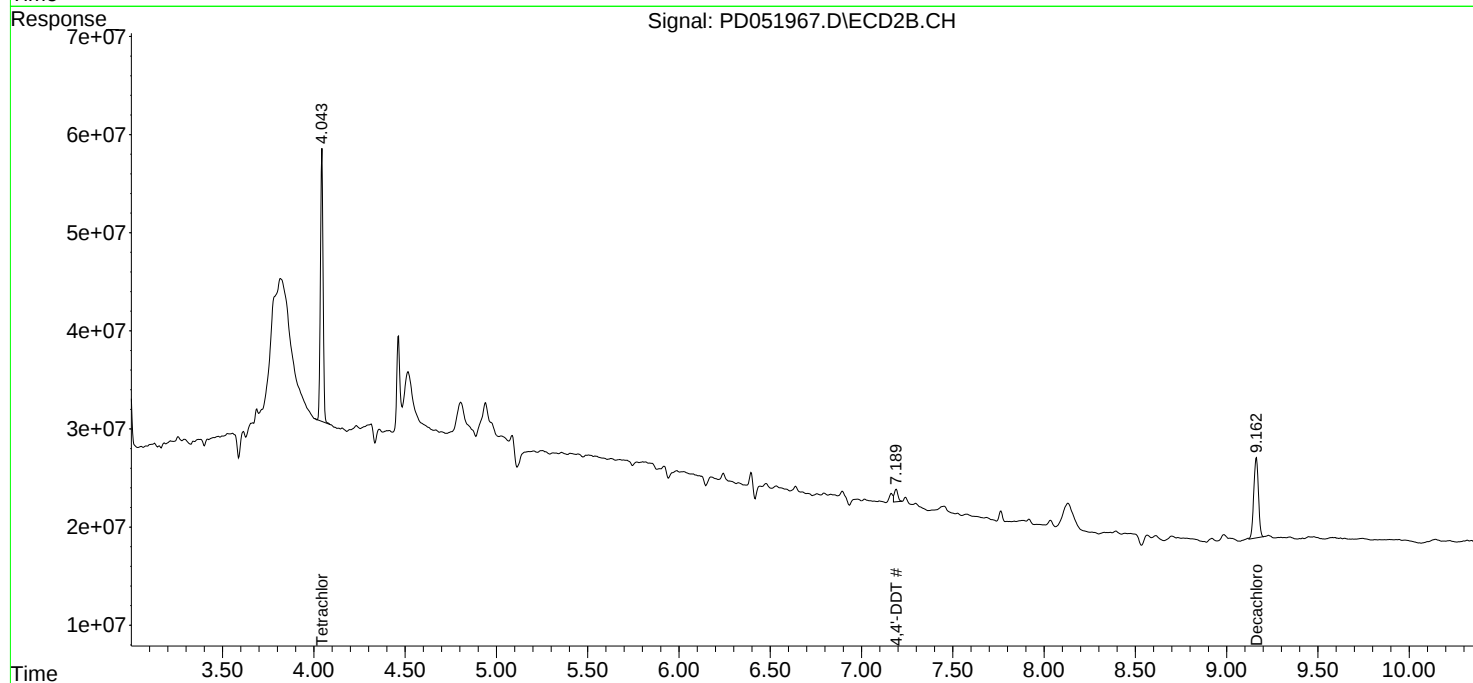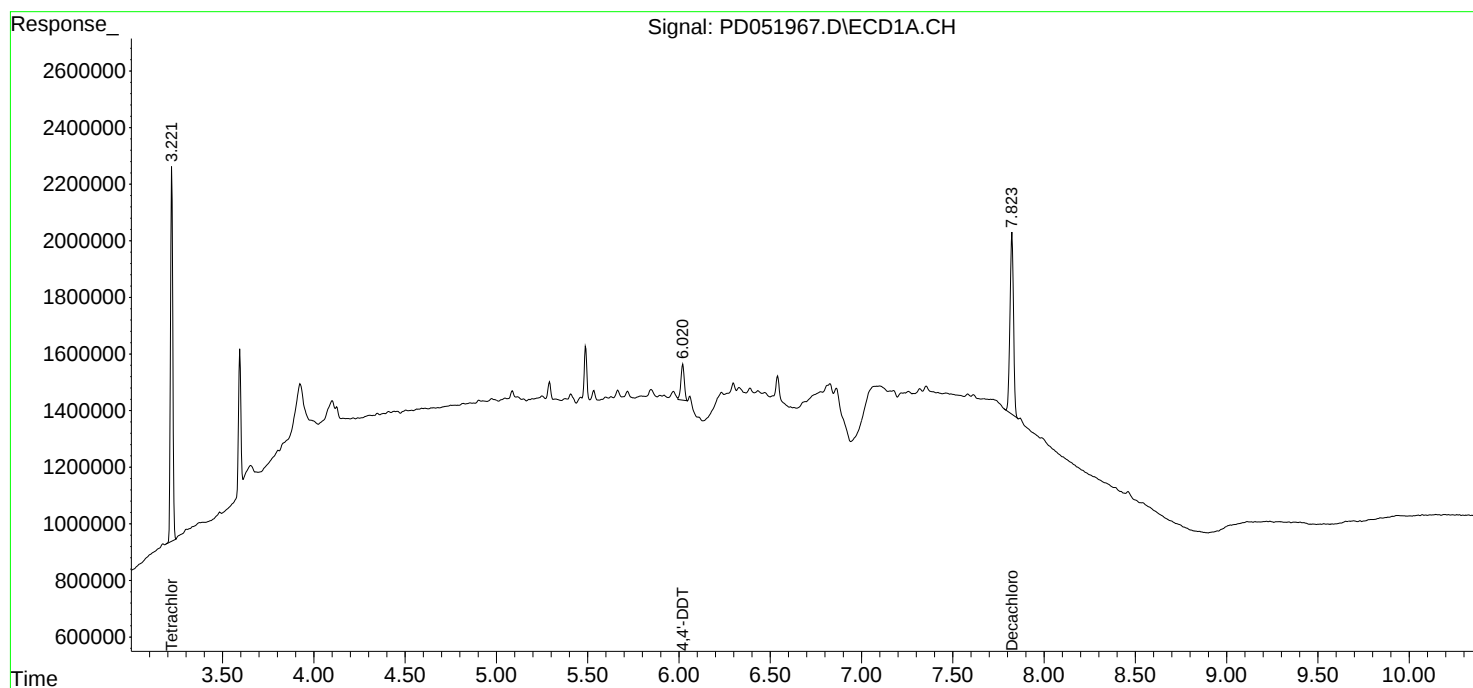


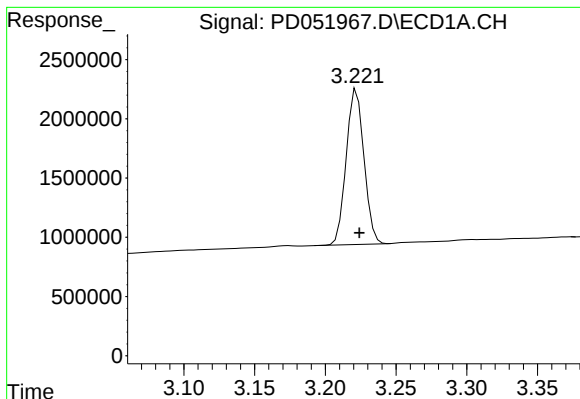

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: -0.002 min
Response: 11508969
Conc: 8.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
CS-3

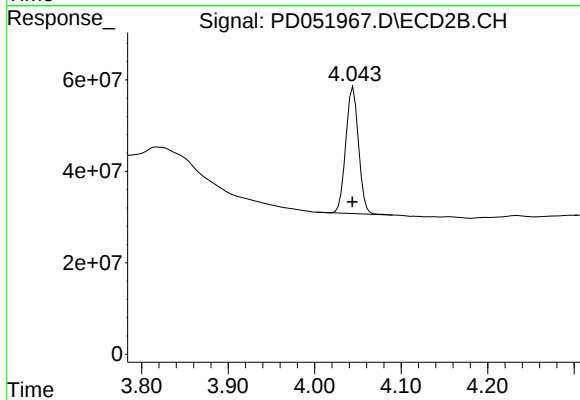


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 281015052
Conc: 9.80 ng/ml

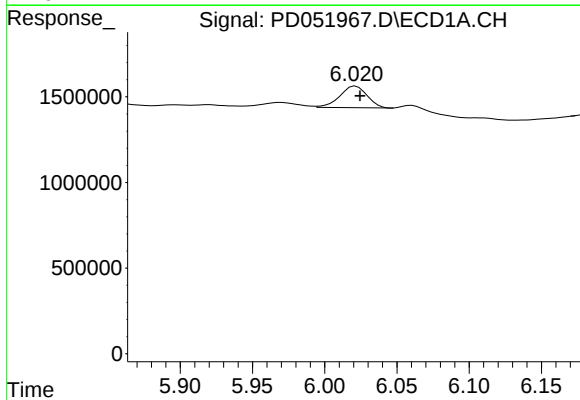


#17 4,4'-DDT

R.T.: 6.022 min
Delta R.T.: -0.003 min
Response: 1654923
Conc: 1.04 ng/ml

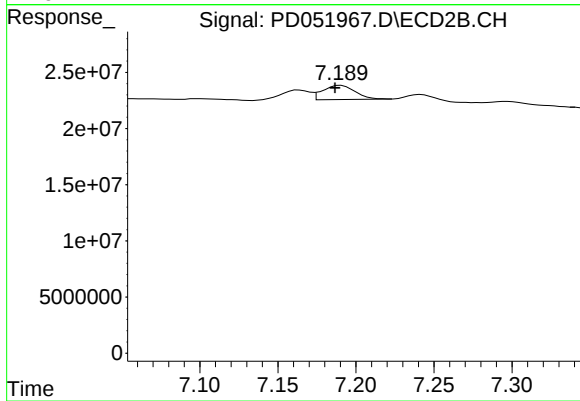

#17 4,4'-DDT


R.T.: 7.190 min
Delta R.T.: 0.004 min
Response: 18271006
Conc: 0.90 ng/ml

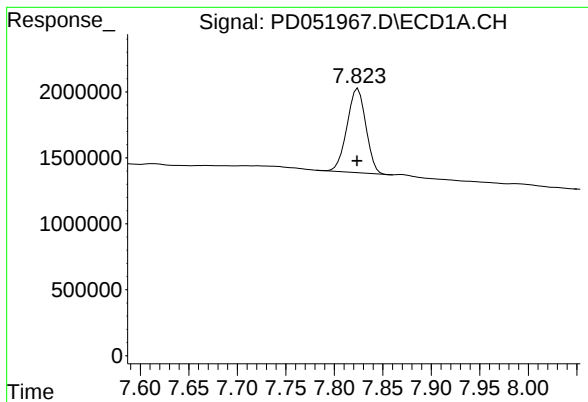

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.001 min
Response: 8649417
Conc: 7.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
CS-3

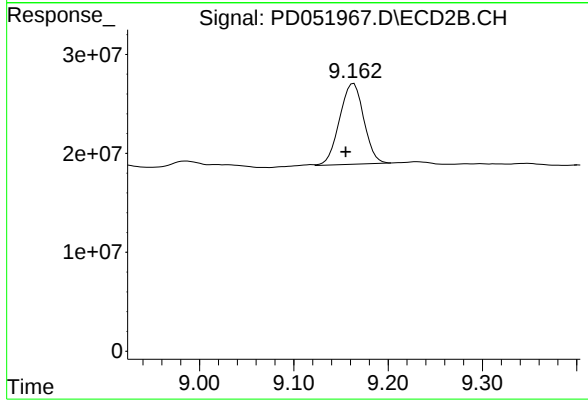

#28 Decachlorobiphenyl

R.T.: 9.164 min
Delta R.T.: 0.008 min
Response: 145659101
Conc: 7.97 ng/ml