

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032222\
 Data File : PD068730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 15:45
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:47:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	63317660	439.5E6	52.149	45.972
28)	SA Decachlor...	8.203	9.365	59118074	270.5E6	46.794	47.731
Target Compounds							
23)	Chlordane-1	4.315	5.193	19612171	182.4E6	462.156	462.404
24)	Chlordane-2	4.817	5.666	23494716	178.0E6	468.164	465.737
25)	Chlordane-3	5.384	6.322	64319623	624.4E6	461.295	464.710
26)	Chlordane-4	5.443	6.399	53891748	722.3E6	455.356	464.627
27)	Chlordane-5	6.280	7.210	22738089	133.1E6	455.129	456.137m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032222\
Data File : PD068730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 15:45
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:47:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

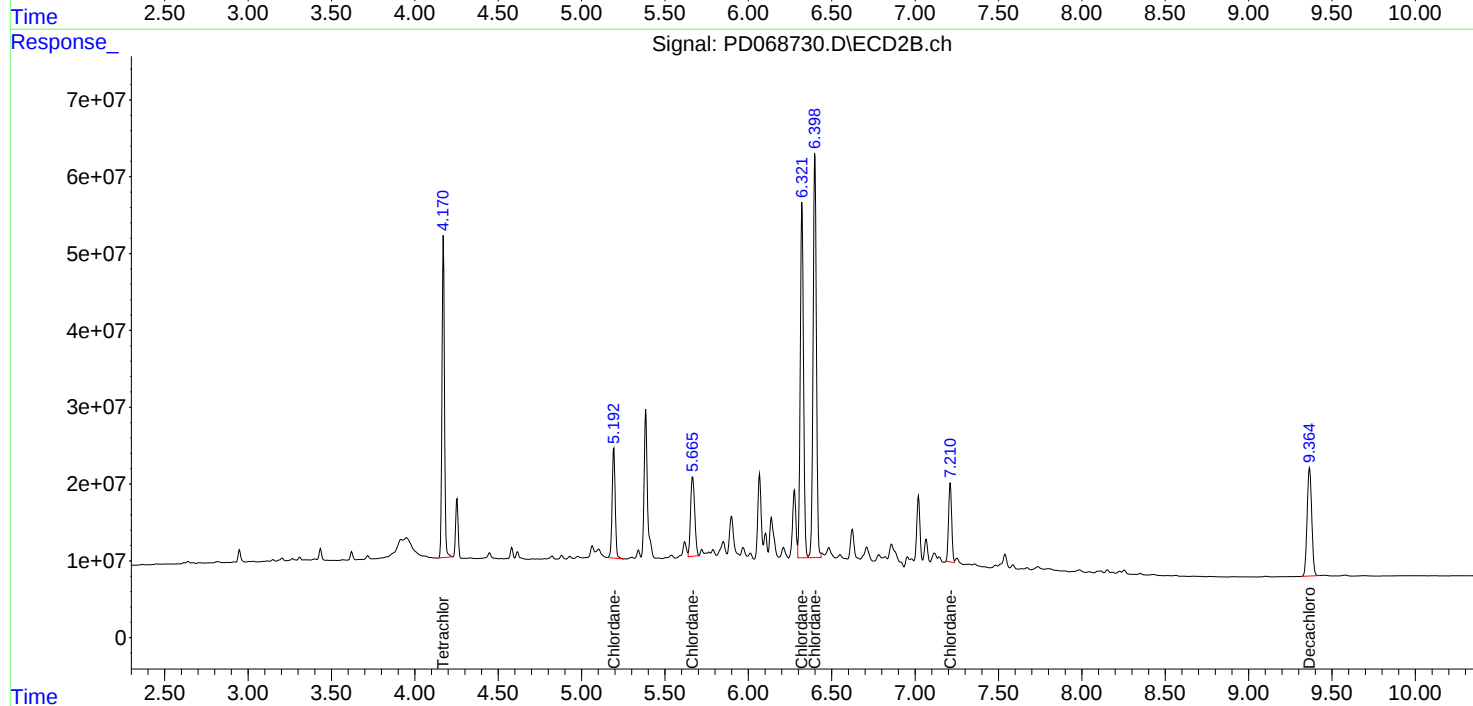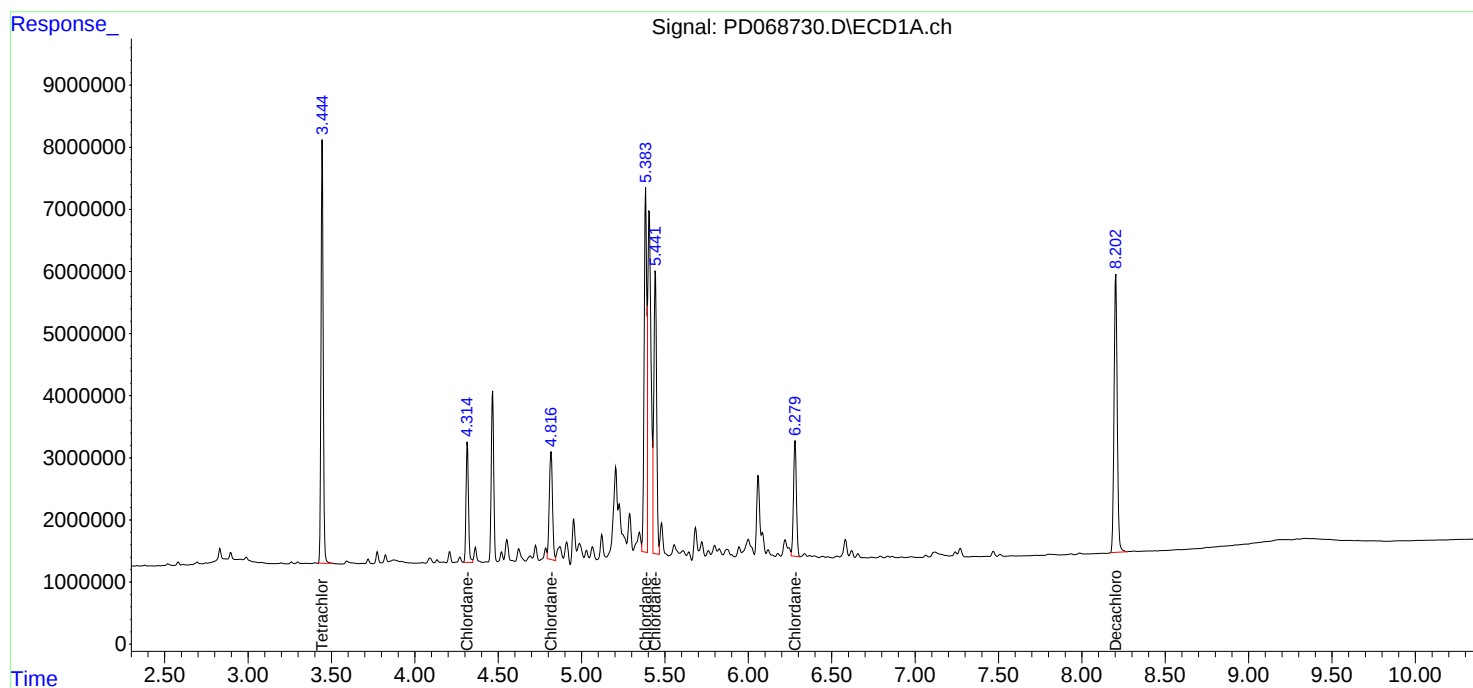


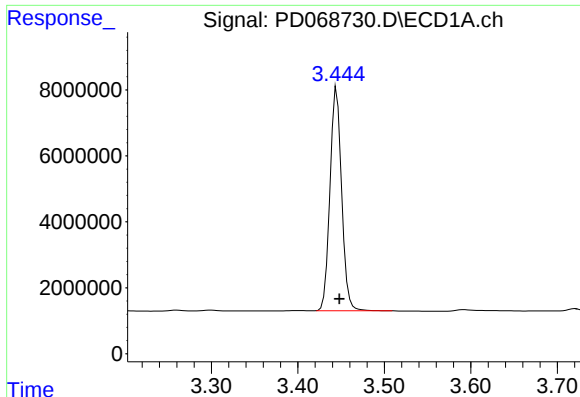

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: -0.003 min
Response: 63317660
Conc: 52.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

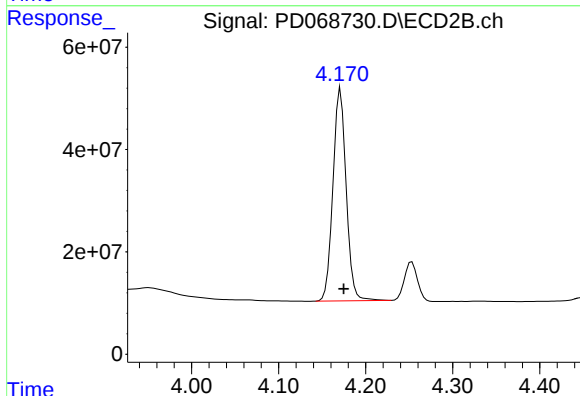


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: -0.004 min
Response: 439524823
Conc: 45.97 ng/ml

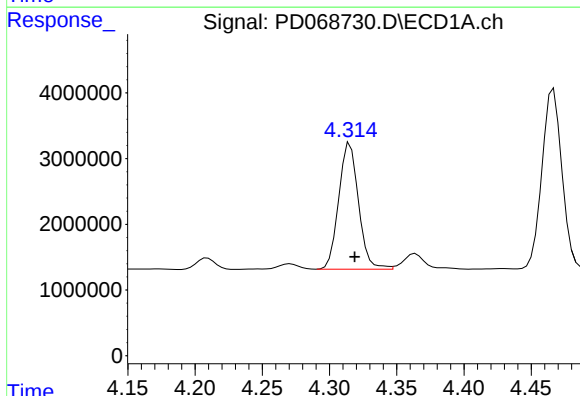


#23 Chlordane-1

R.T.: 4.315 min
Delta R.T.: -0.004 min
Response: 19612171
Conc: 462.16 ng/ml

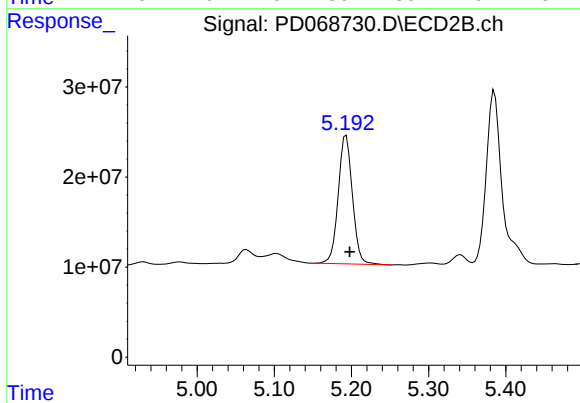

#23 Chlordane-1


R.T.: 5.193 min
Delta R.T.: -0.004 min
Response: 182433494
Conc: 462.40 ng/ml

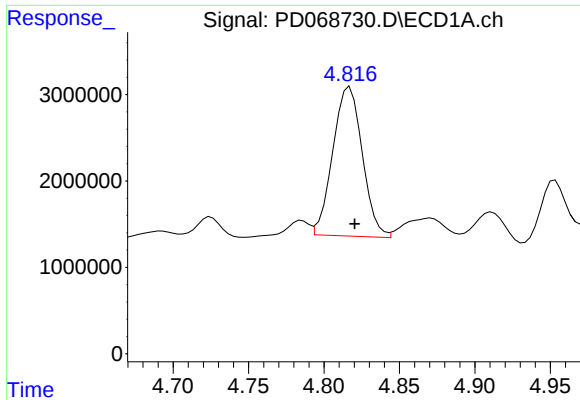

#24 Chlordane-2


R.T.: 4.817 min
Delta R.T.: -0.003 min
Response: 23494716
Conc: 468.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

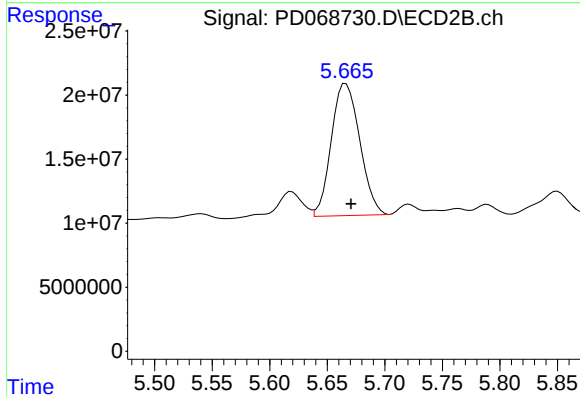


#24 Chlordane-2

R.T.: 5.666 min
Delta R.T.: -0.005 min
Response: 178045869
Conc: 465.74 ng/ml

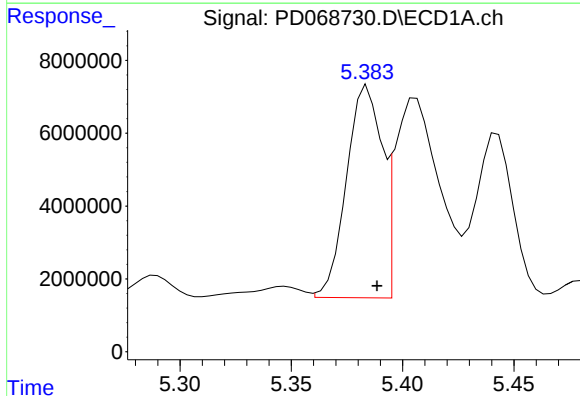


#25 Chlordane-3

R.T.: 5.384 min
Delta R.T.: -0.004 min
Response: 64319623
Conc: 461.29 ng/ml

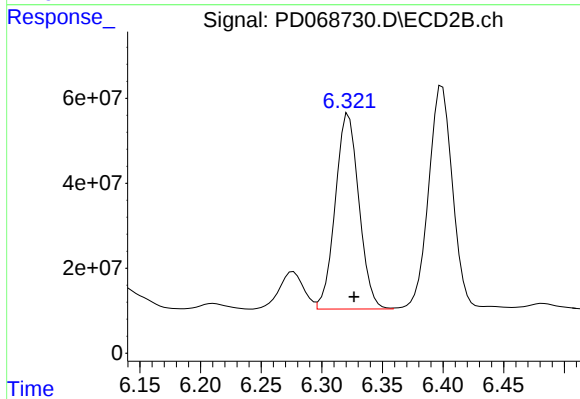

#25 Chlordane-3


R.T.: 6.322 min
Delta R.T.: -0.005 min
Response: 624375092
Conc: 464.71 ng/ml

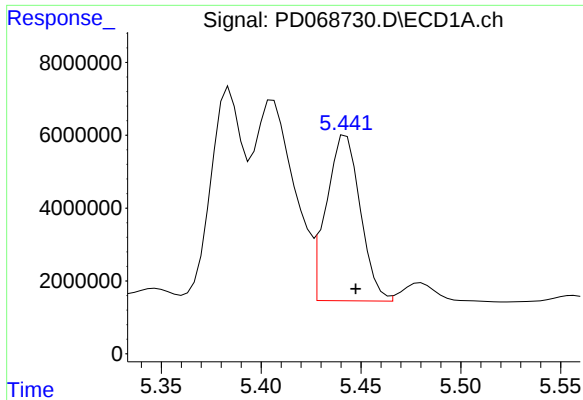

#26 Chlordane-4


R.T.: 5.443 min
Delta R.T.: -0.005 min
Response: 53891748
Conc: 455.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

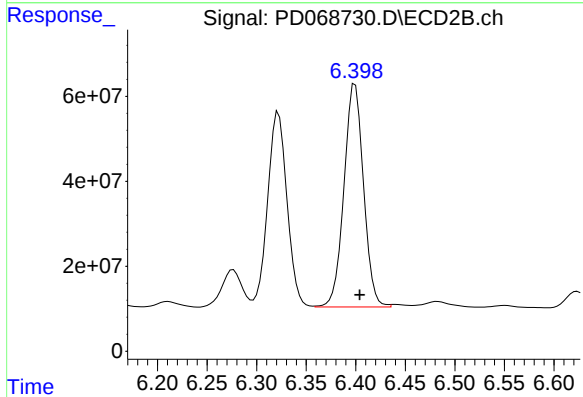


#26 Chlordane-4

R.T.: 6.399 min
Delta R.T.: -0.005 min
Response: 722303704
Conc: 464.63 ng/ml

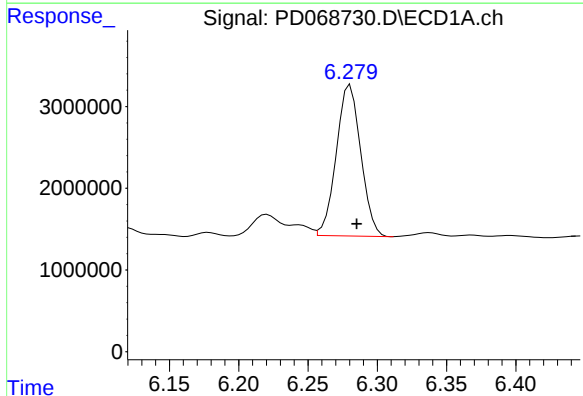


#27 Chlordane-5

R.T.: 6.280 min
Delta R.T.: -0.005 min
Response: 22738089
Conc: 455.13 ng/ml

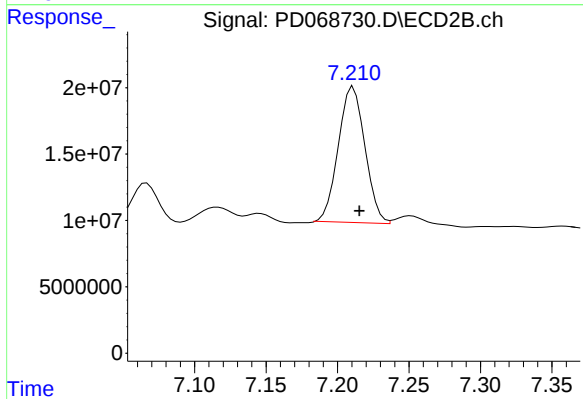

#27 Chlordane-5


R.T.: 7.210 min
Delta R.T.: -0.006 min
Response: 133095801
Conc: 456.14 ng/ml m

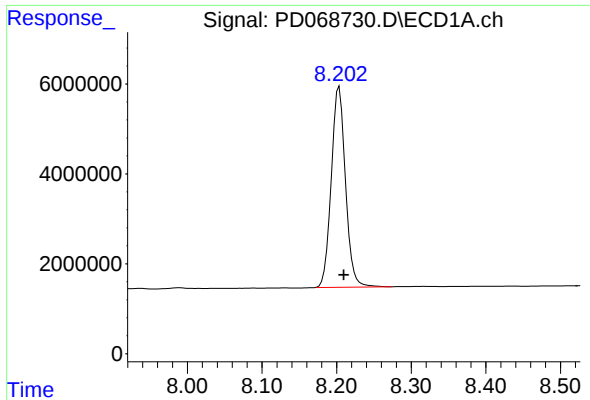

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.006 min
Response: 59118074
Conc: 46.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

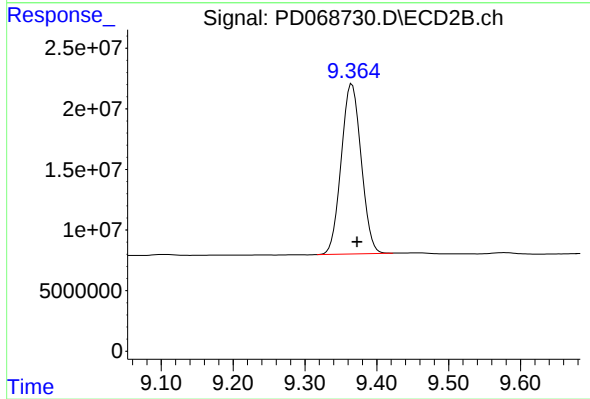

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.007 min
Response: 270477300
Conc: 47.73 ng/ml