

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
 Data File : PD082216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2024 14:01
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 14:09:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 14:09:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	36941715	78001898	25.253	25.612
28)	SA Decachlor...	9.118	7.909	49757344	55062532	26.737	25.678
Target Compounds							
23)	Chlordane-1	4.734	3.771	19393156	24948034	253.880	258.605
24)	Chlordane-2	5.265	4.346	20930940	28418173	264.678	264.193
25)	Chlordane-3	5.977	4.975	78163820	73260838	245.478	248.661
26)	Chlordane-4	6.059	5.039	94045633	71156291	247.937	249.888
27)	Chlordane-5	6.912	5.933	15654926	24527255	253.864	252.448



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
Data File : PD082216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2024 14:01
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 14:09:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 14:09:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

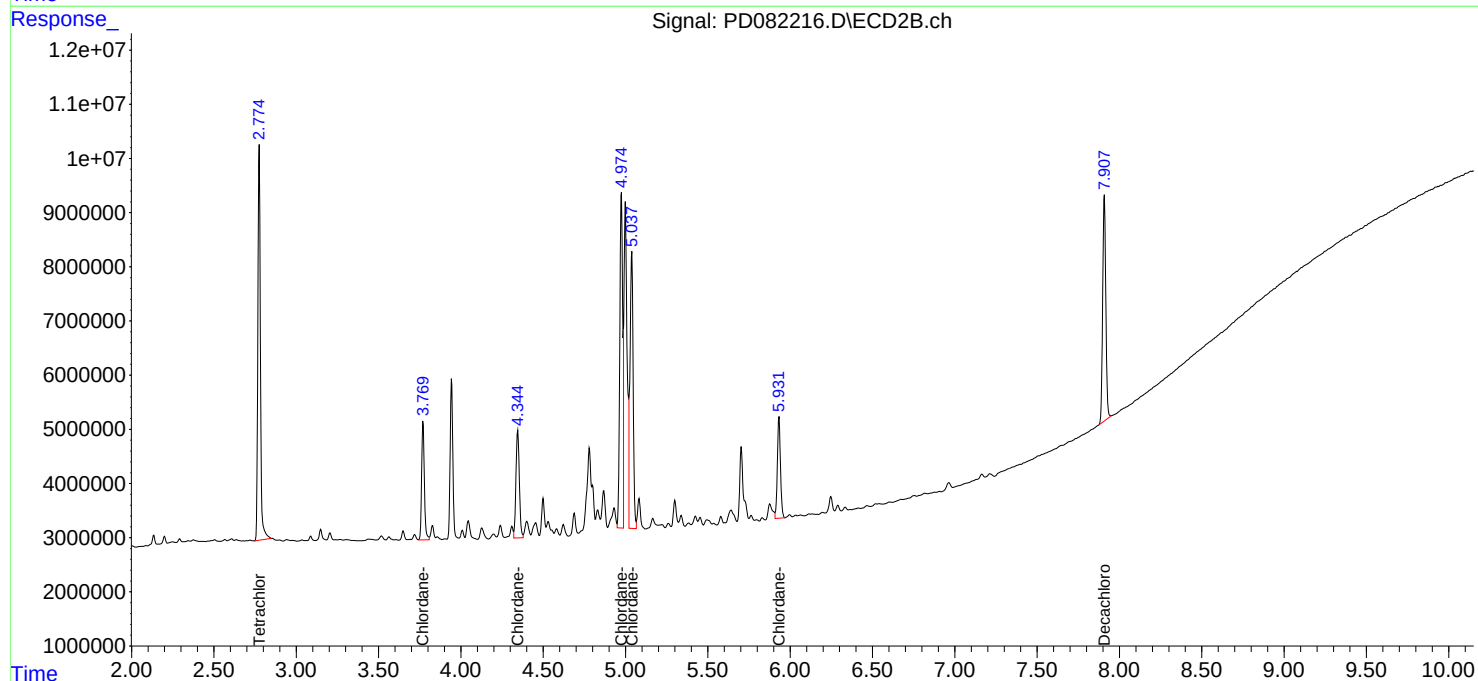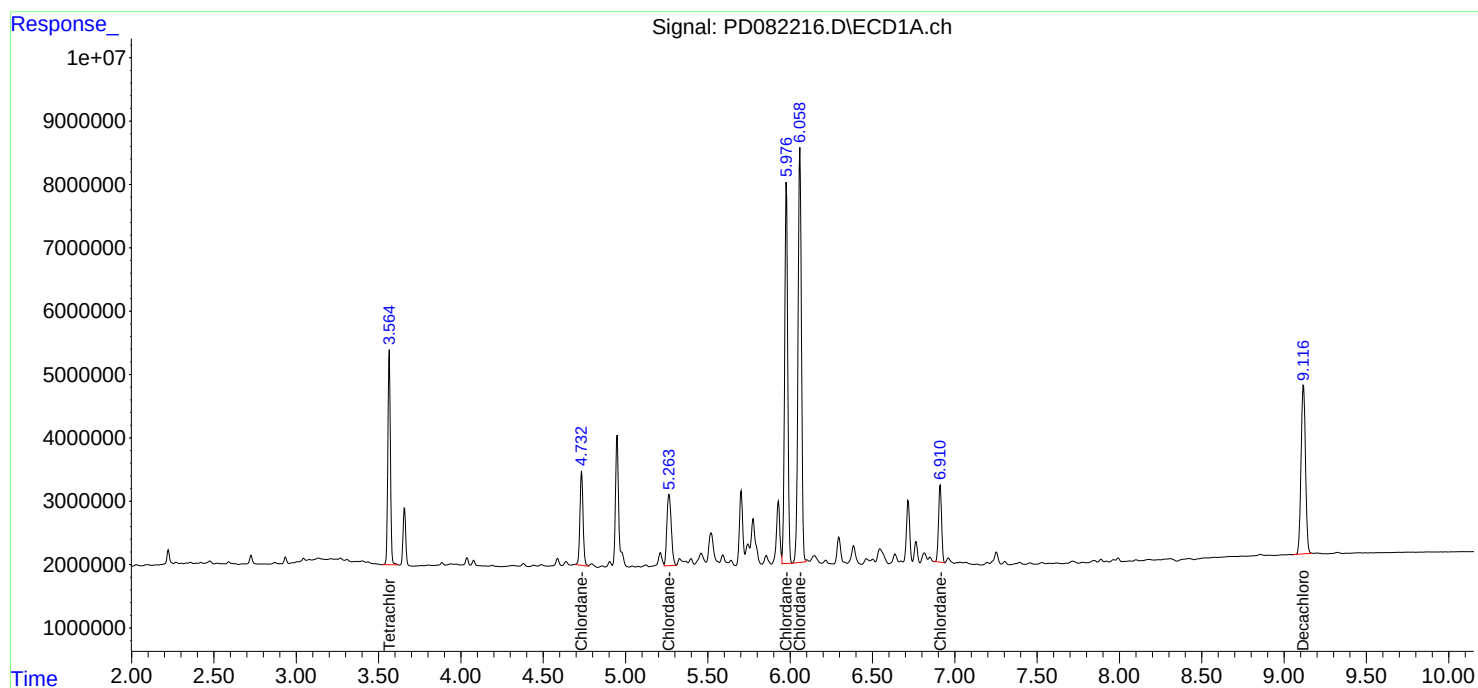


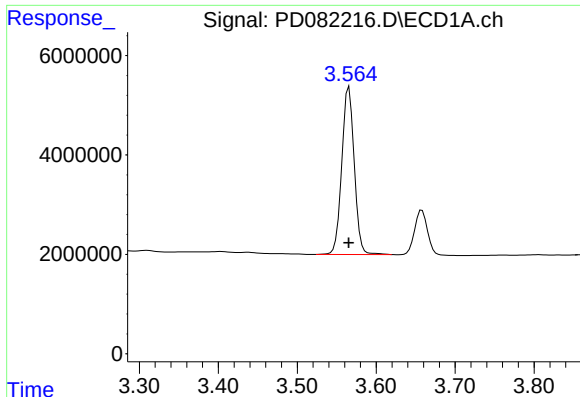

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 36941715
Conc: 25.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

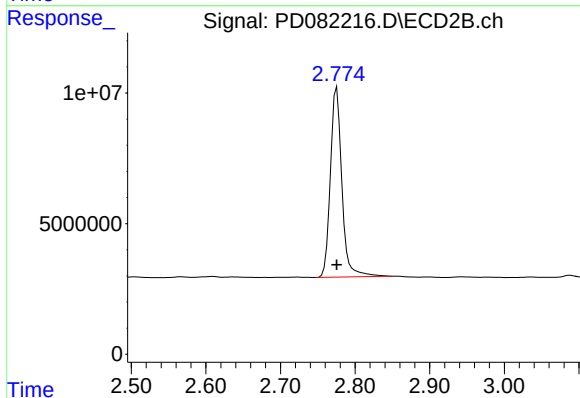


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 78001898
Conc: 25.61 ng/ml

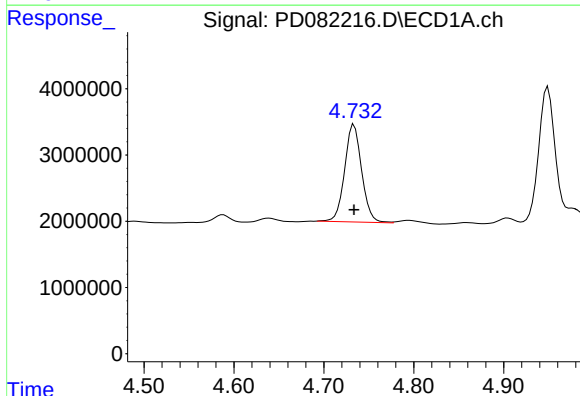


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 19393156
Conc: 253.88 ng/ml

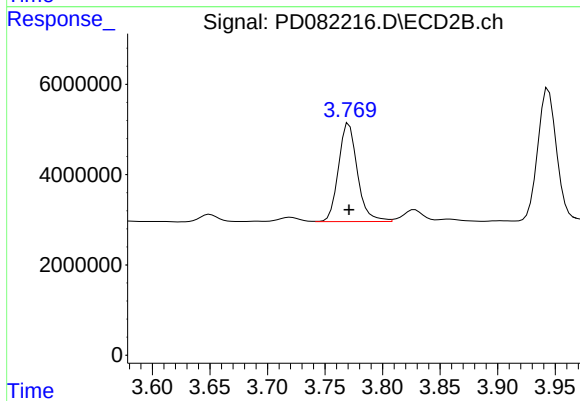

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 24948034
Conc: 258.61 ng/ml

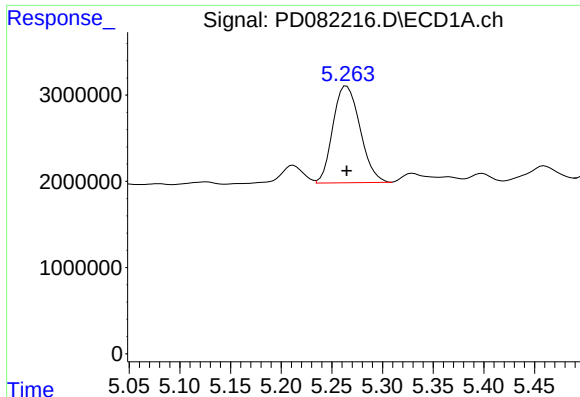

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 20930940
Conc: 264.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

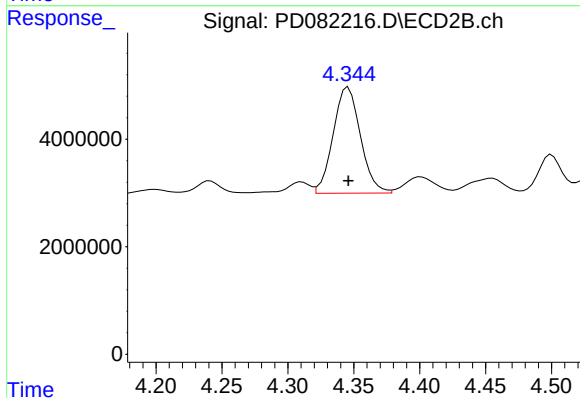


#24 Chlordane-2

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 28418173
Conc: 264.19 ng/ml

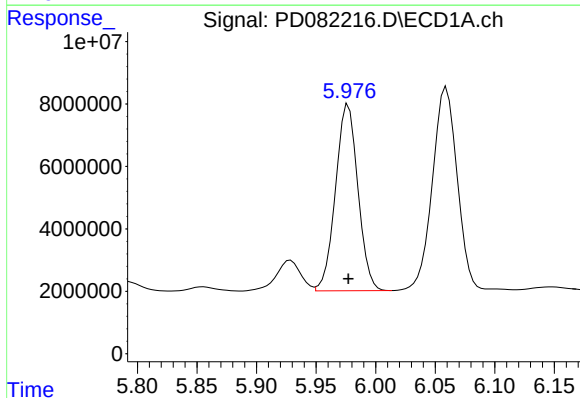


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 78163820
Conc: 245.48 ng/ml

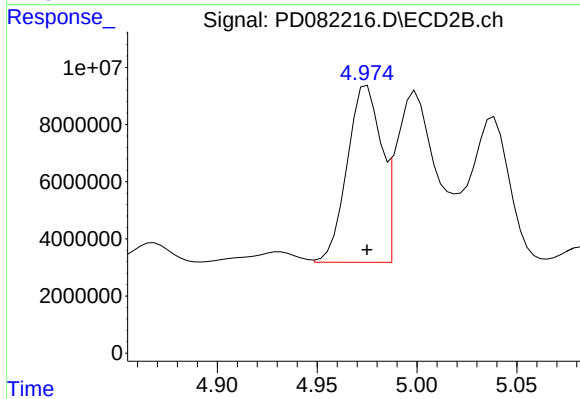

#25 Chlordane-3


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 73260838
Conc: 248.66 ng/ml

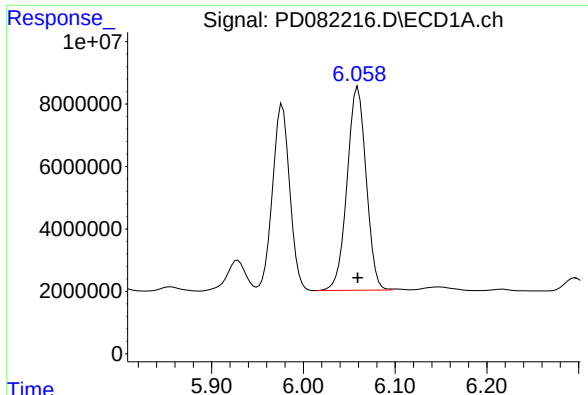

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 94045633
Conc: 247.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

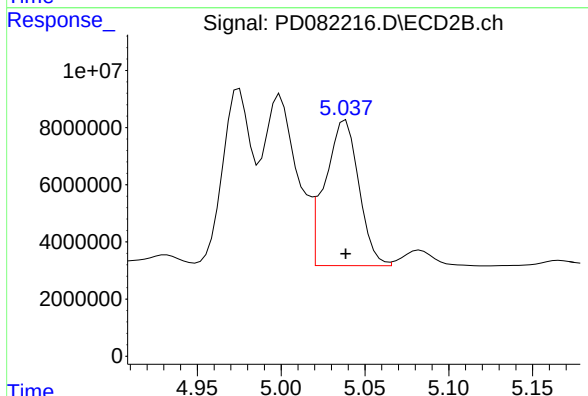


#26 Chlordane-4

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 71156291
Conc: 249.89 ng/ml

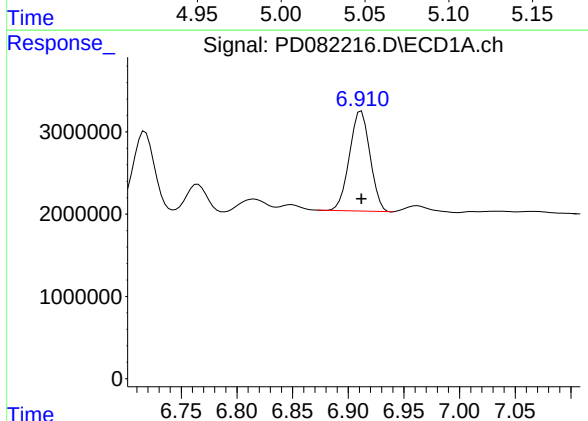


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 15654926
Conc: 253.86 ng/ml

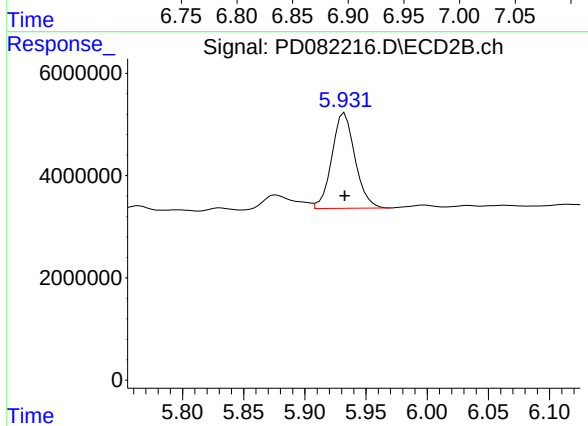

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 24527255
Conc: 252.45 ng/ml

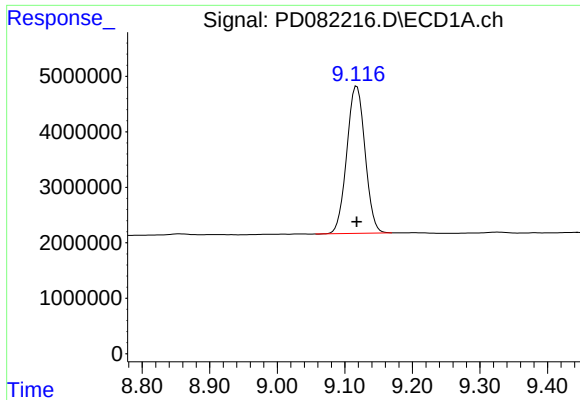

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 49757344
Conc: 26.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

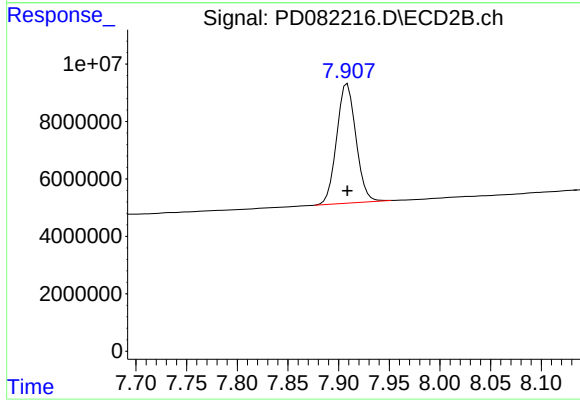

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 55062532
Conc: 25.68 ng/ml