

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
 Data File : PD082207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2024 12:01
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 14:40:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 14:38:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.775	28546962	46861860	19.927	19.068
28)	SA Decachlor...	9.118	7.908	38073124	41618270	20.059	19.119
Target Compounds							
9)	A Endosulfan I	6.106	5.094	19058386	22601774	9.091	8.376
10)	B gamma-Chl...	5.976	4.974	21271240	26414452	9.625	9.039
12)	B 4,4'-DDE	6.228	5.227	40416992	48074002	19.165	18.224
13)	MA Dieldrin	6.382	5.358	40155982	50677852	18.521	17.774
19)	B Endosulfa...	7.197	6.328	32629167	42379003	19.243	18.317
20)	A Methoxychlor	7.537	6.607	80737797	102.9E6	90.946	90.096
21)	B Endrin ke...	7.684	6.834	34307990	47986672	18.978	18.075



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
Data File : PD082207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2024 12:01
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 14:40:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 14:38:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

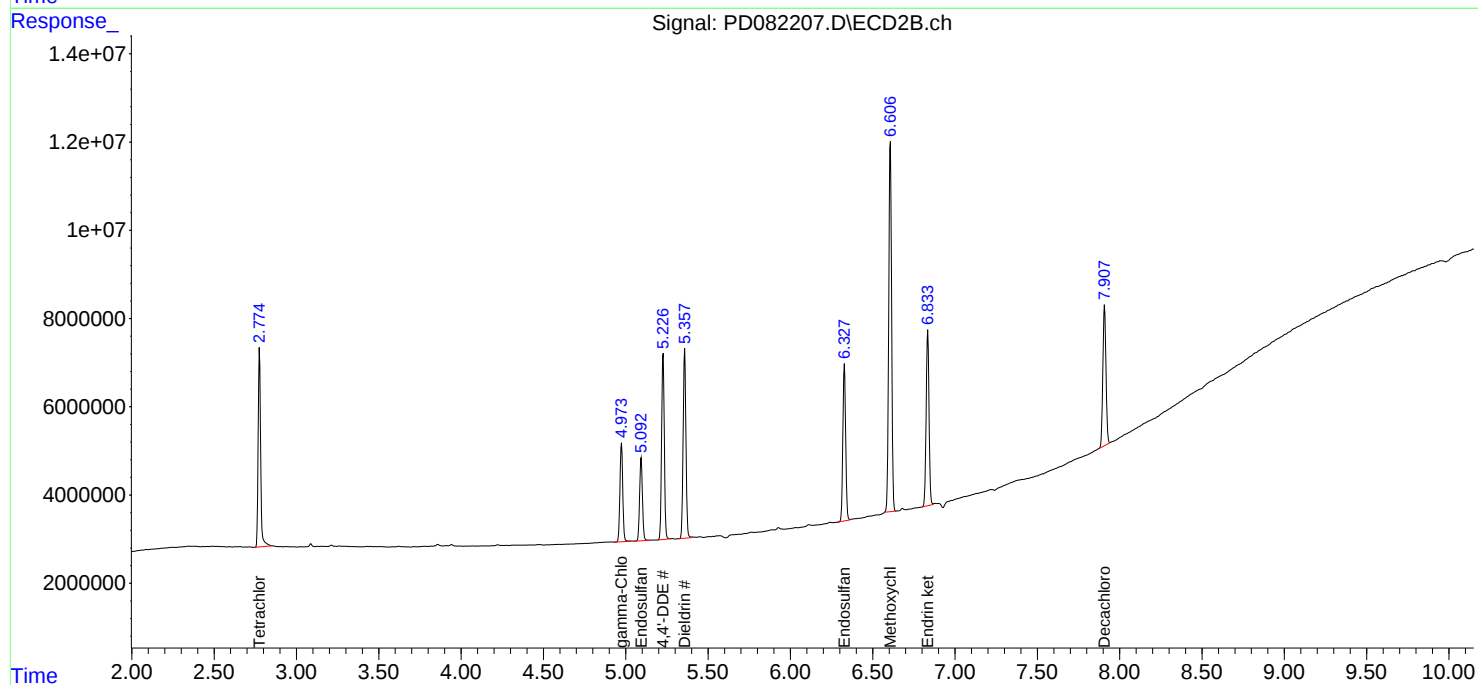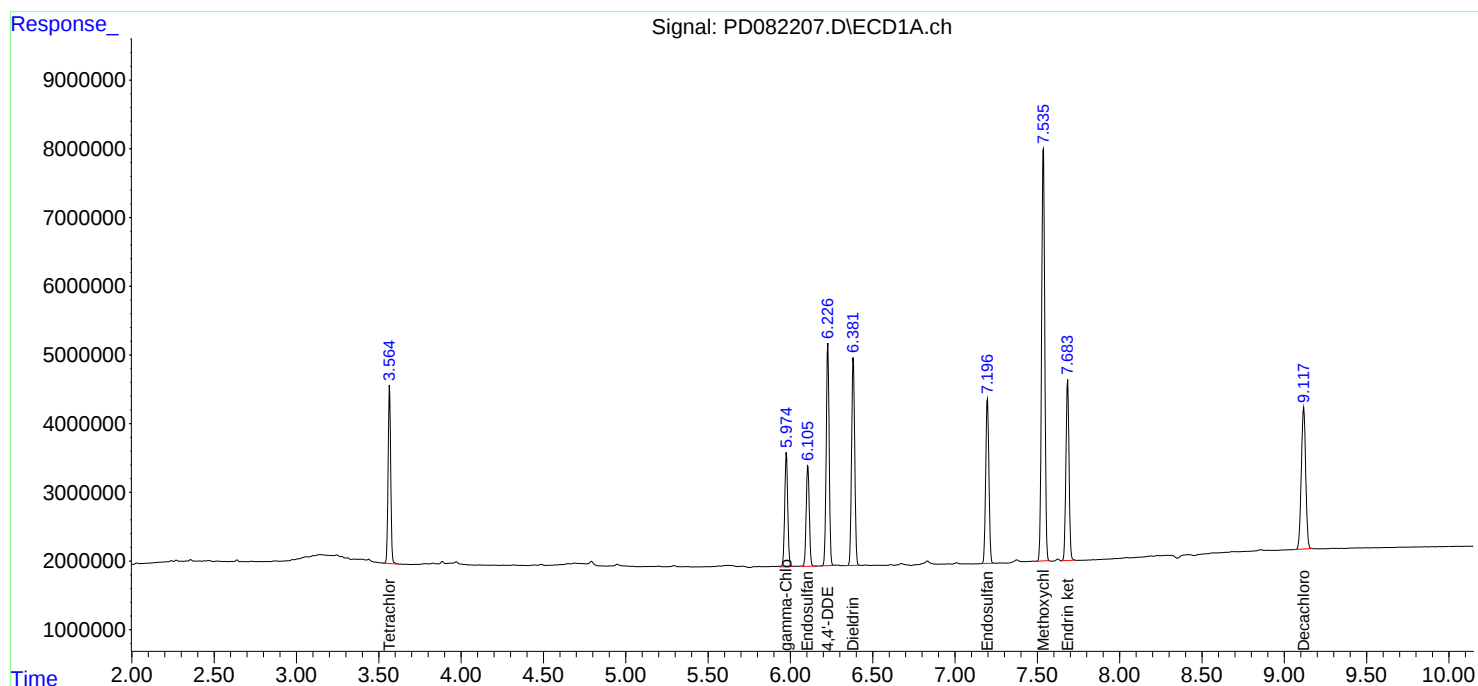


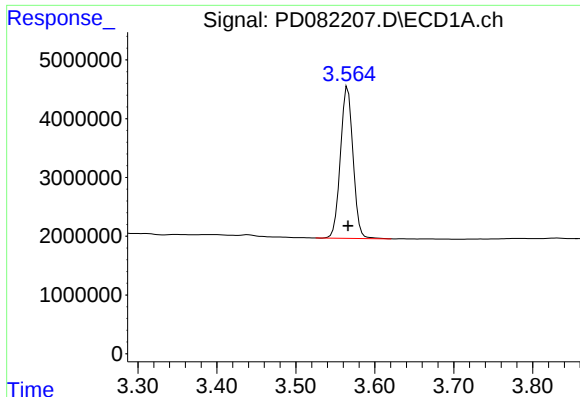

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 28546962
Conc: 19.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

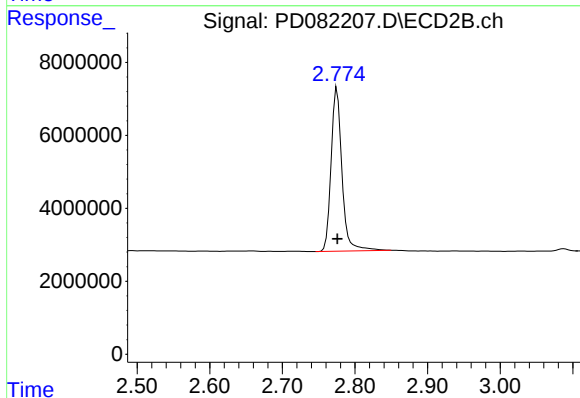


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 46861860
Conc: 19.07 ng/ml

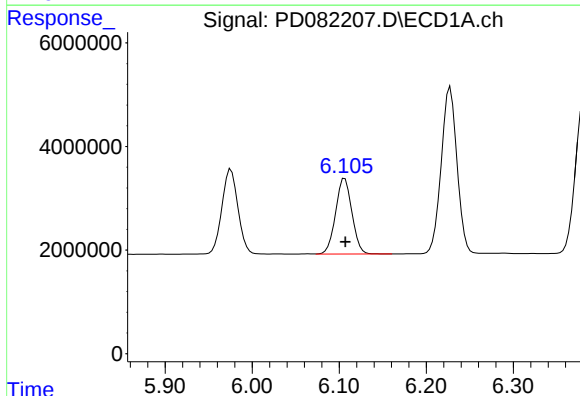


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 19058386
Conc: 9.09 ng/ml

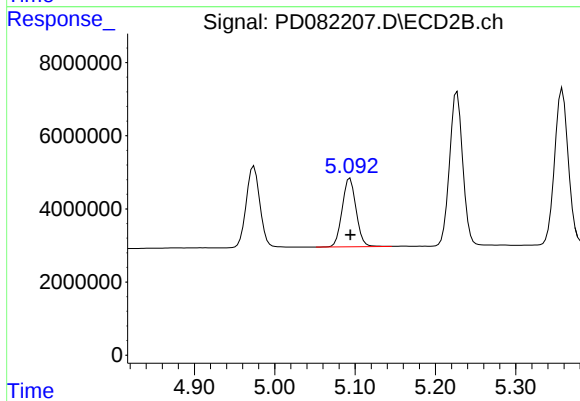

#9 Endosulfan I


R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 22601774
Conc: 8.38 ng/ml

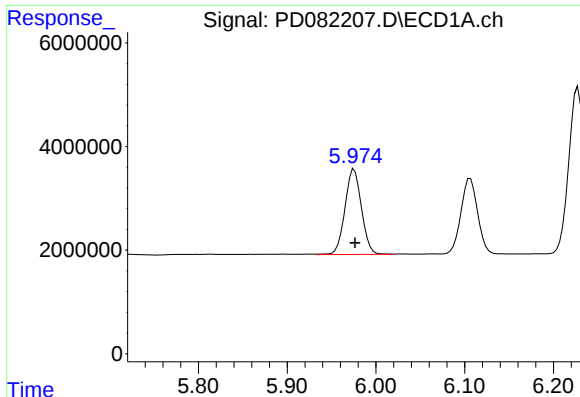

#10 gamma-Chlordane


R.T.: 5.976 min
Delta R.T.: -0.001 min
Response: 21271240
Conc: 9.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

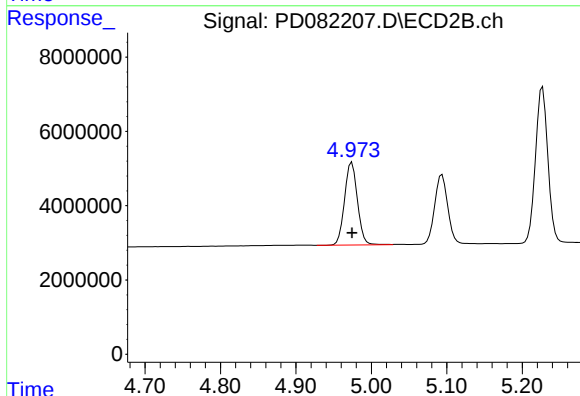


#10 gamma-Chlordane

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 26414452
Conc: 9.04 ng/ml

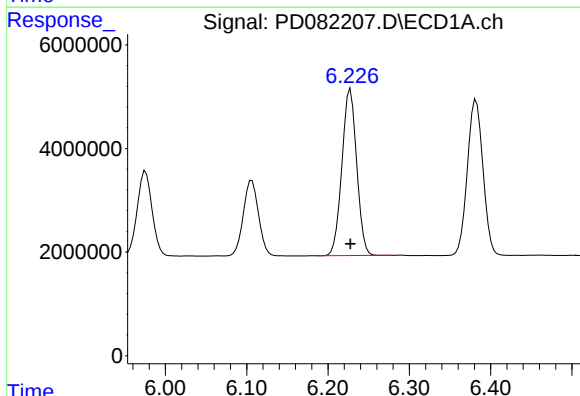


#12 4,4'-DDE

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 40416992
Conc: 19.17 ng/ml

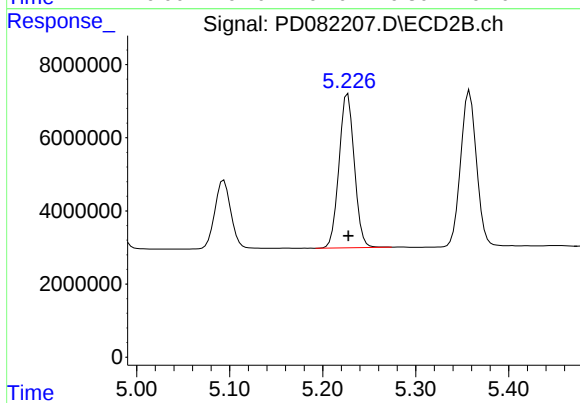

#12 4,4'-DDE


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 48074002
Conc: 18.22 ng/ml

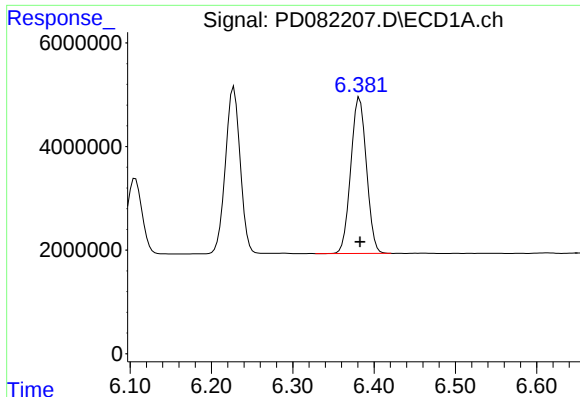

#13 Dieldrin


R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 40155982
Conc: 18.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

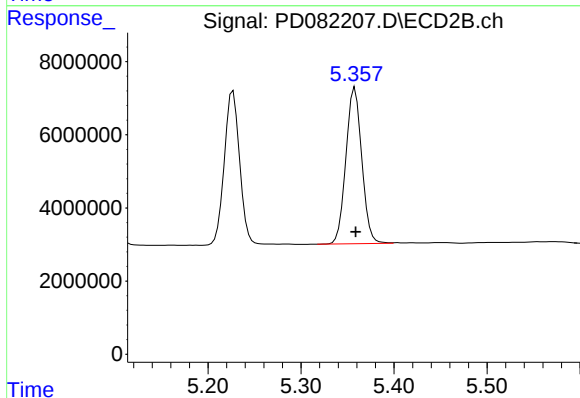


#13 Dieldrin

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 50677852
Conc: 17.77 ng/ml

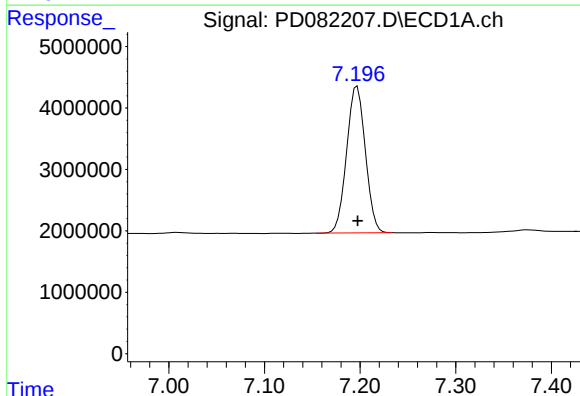


#19 Endosulfan Sulfate

R.T.: 7.197 min
Delta R.T.: 0.000 min
Response: 32629167
Conc: 19.24 ng/ml

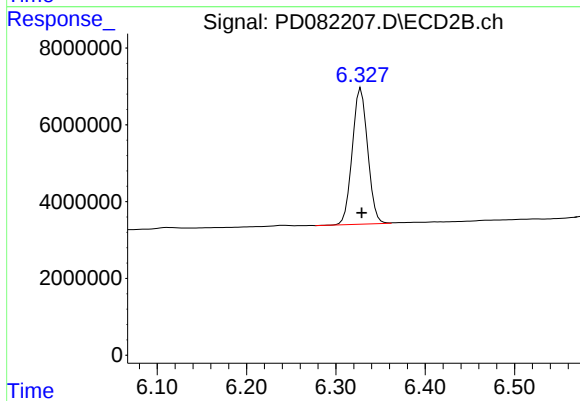

#19 Endosulfan Sulfate


R.T.: 6.328 min
Delta R.T.: -0.001 min
Response: 42379003
Conc: 18.32 ng/ml

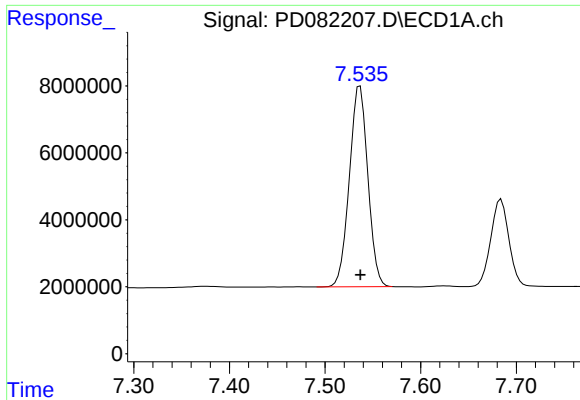

#20 Methoxychlor


R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 80737797
Conc: 90.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

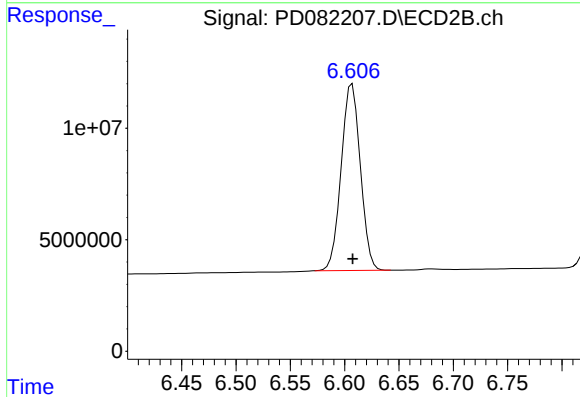


#20 Methoxychlor

R.T.: 6.607 min
Delta R.T.: 0.000 min
Response: 102931813
Conc: 90.10 ng/ml

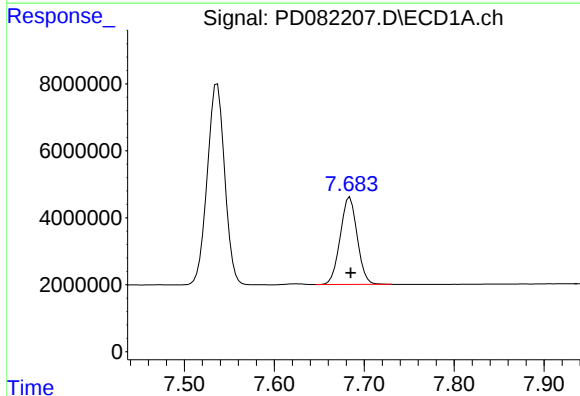


#21 Endrin ketone

R.T.: 7.684 min
Delta R.T.: 0.000 min
Response: 34307990
Conc: 18.98 ng/ml

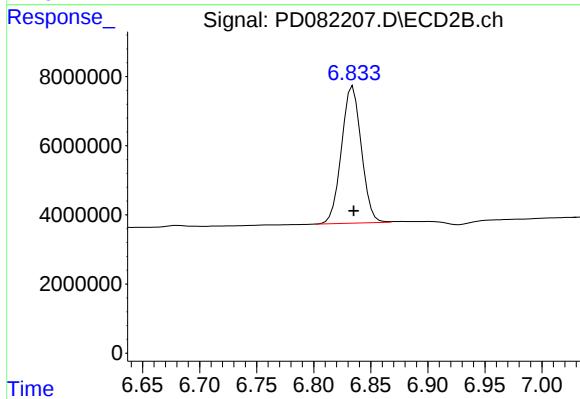

#21 Endrin ketone


R.T.: 6.834 min
Delta R.T.: 0.000 min
Response: 47986672
Conc: 18.07 ng/ml

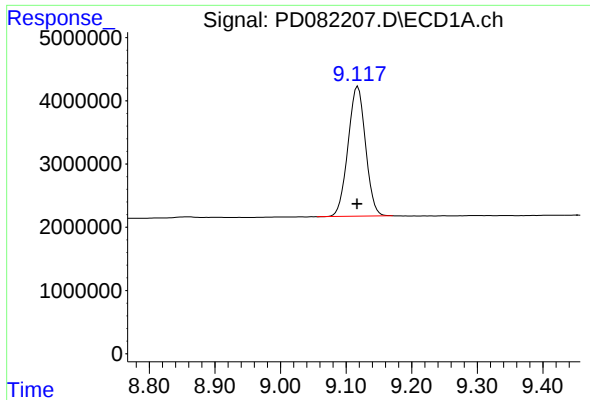

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 38073124
Conc: 20.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

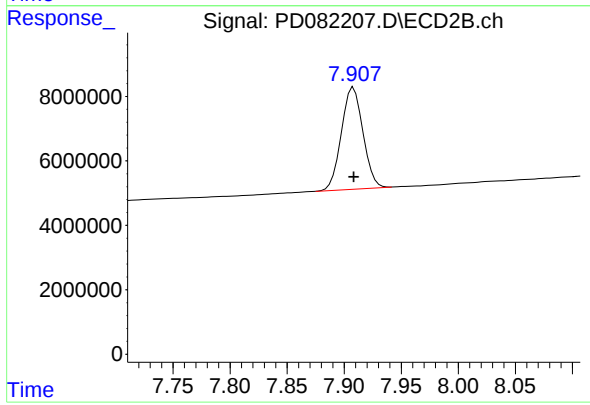

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: 0.000 min
Response: 41618270
Conc: 19.12 ng/ml