

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
 Data File : PD082214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2024 13:34
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 14:03:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:57:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.775	107.1E6	223.3E6	73.440	73.918
28)	SA Decachlor...	9.118	7.909	133.5E6	158.0E6	73.422	74.341
Target Compounds							
23)	Chlordane-1	4.734	3.771	55977651	70670516	736.625	741.055
24)	Chlordane-2	5.264	4.346	56619923	78002231	730.266	739.145
25)	Chlordane-3	5.977	4.975	235.5E6	218.6E6	735.041	740.740
26)	Chlordane-4	6.059	5.038	279.6E6	210.8E6	735.022	740.102
27)	Chlordane-5	6.913	5.932	44950903	71662850	732.710	740.010



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
Data File : PD082214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2024 13:34
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 14:03:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:57:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

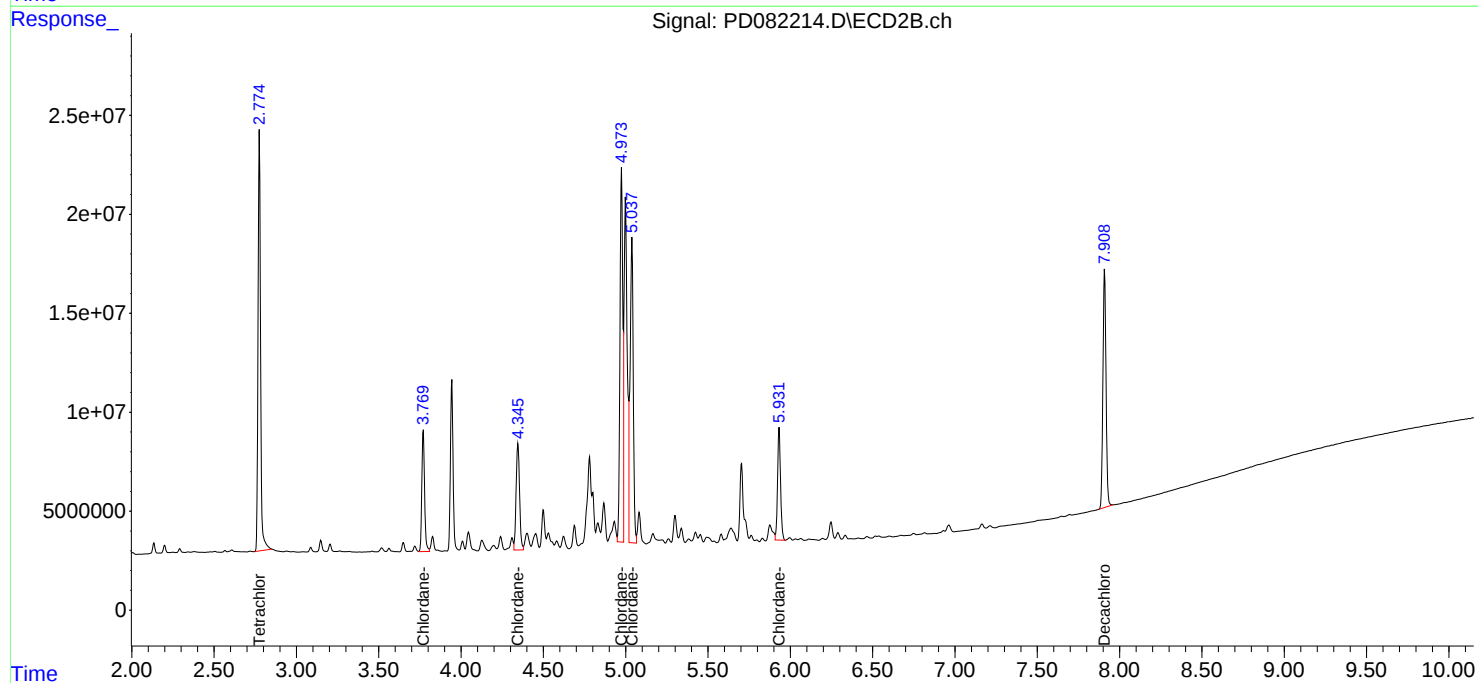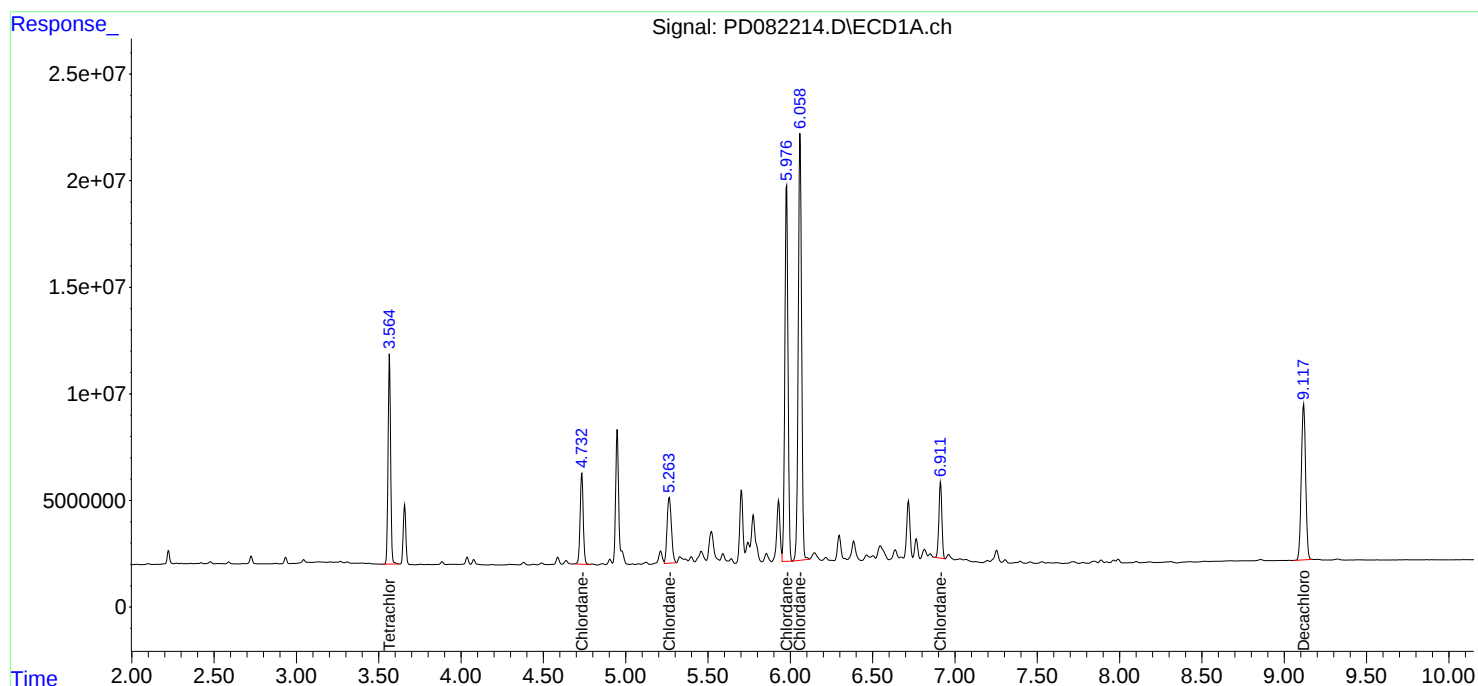


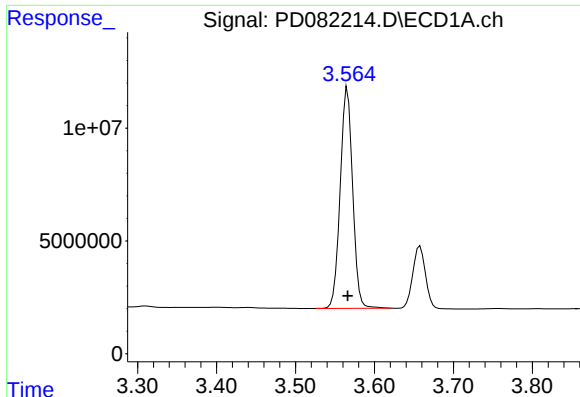

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 107071469
Conc: 73.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

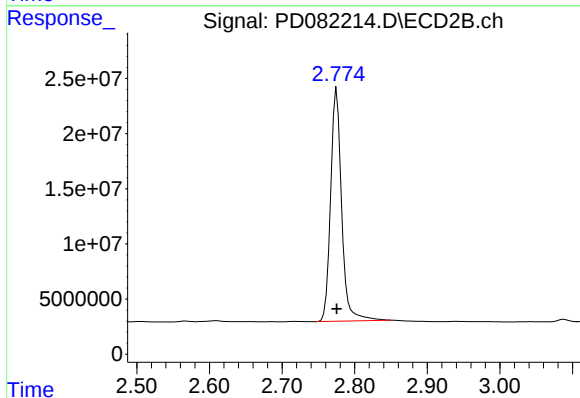


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 223278716
Conc: 73.92 ng/ml

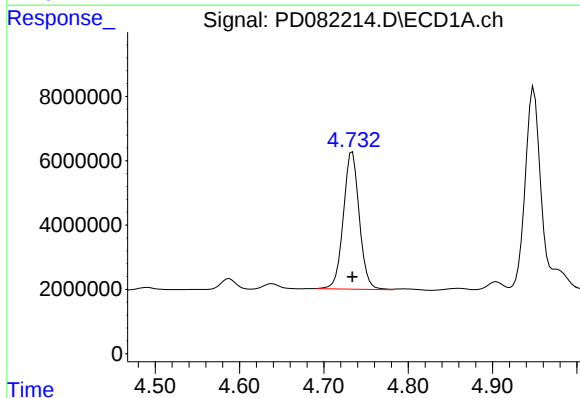


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 55977651
Conc: 736.62 ng/ml

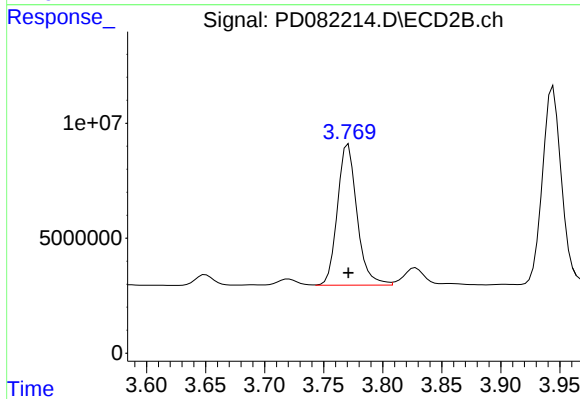

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 70670516
Conc: 741.06 ng/ml

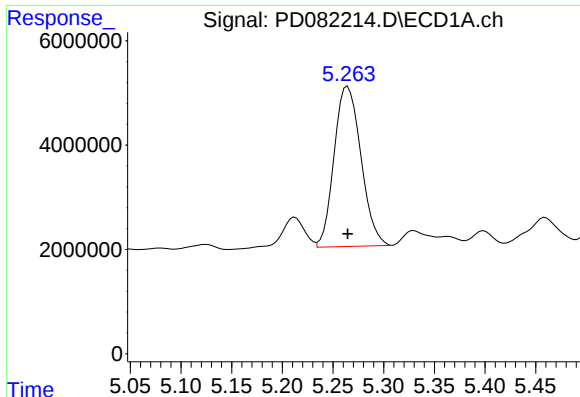

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 56619923
Conc: 730.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

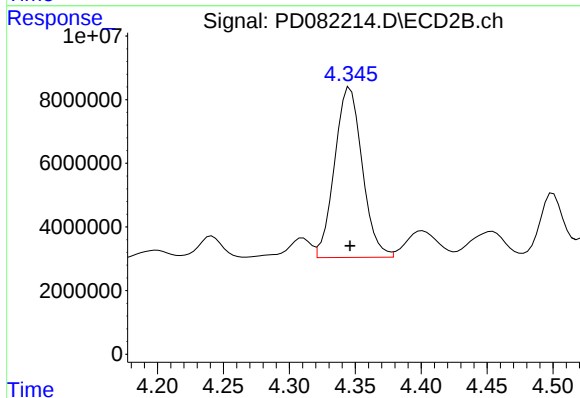


#24 Chlordane-2

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 78002231
Conc: 739.15 ng/ml

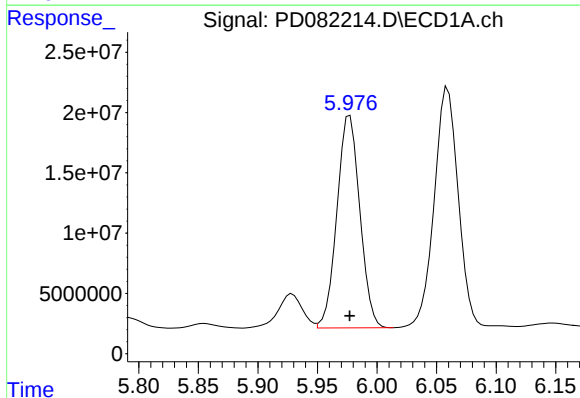


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 235459452
Conc: 735.04 ng/ml

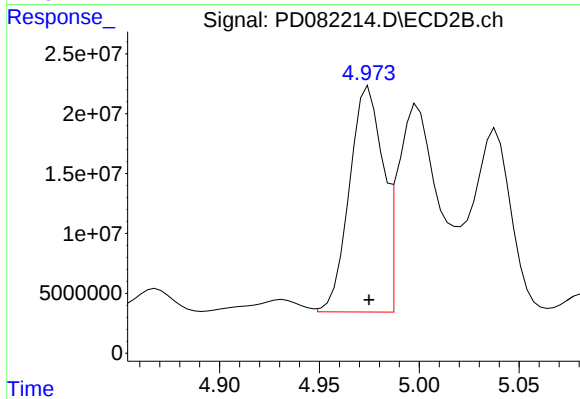

#25 Chlordane-3


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 218628083
Conc: 740.74 ng/ml

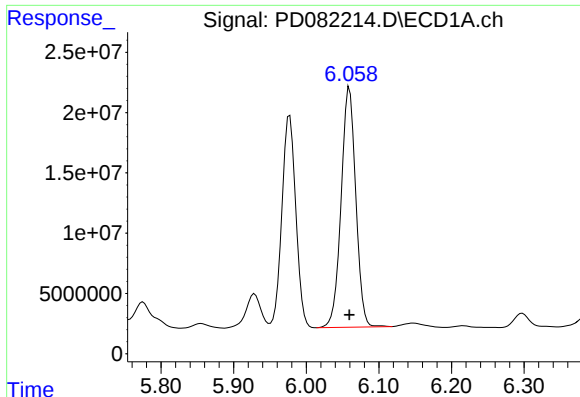

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 279569186
Conc: 735.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

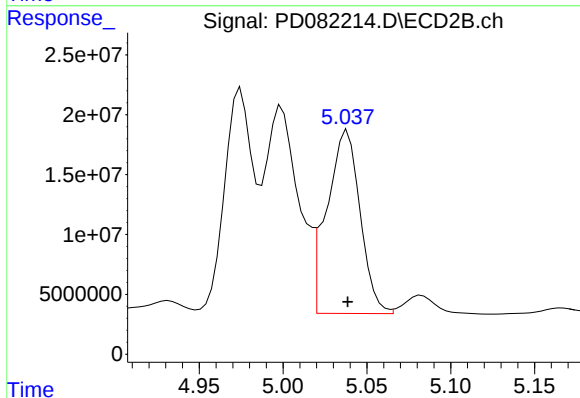


#26 Chlordane-4

R.T.: 5.038 min
Delta R.T.: 0.000 min
Response: 210777701
Conc: 740.10 ng/ml

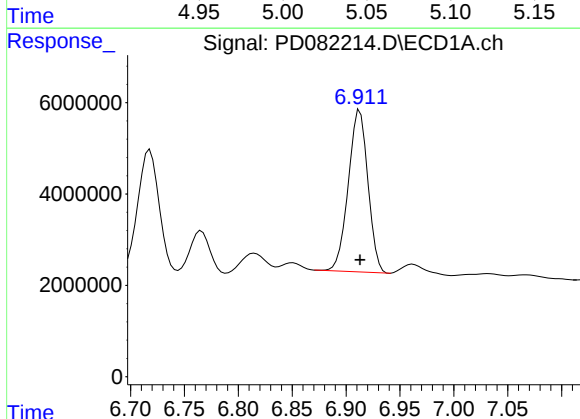


#27 Chlordane-5

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 44950903
Conc: 732.71 ng/ml

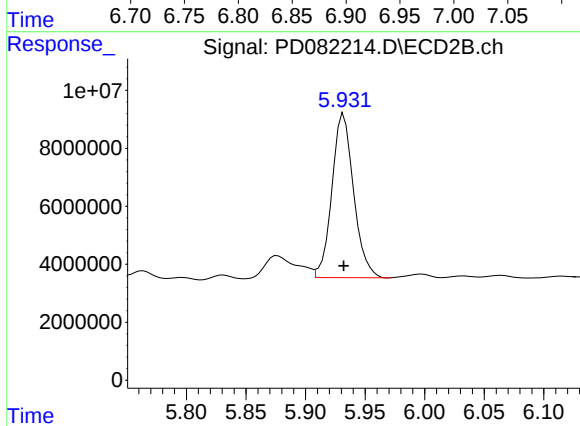

#27 Chlordane-5


R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 71662850
Conc: 740.01 ng/ml

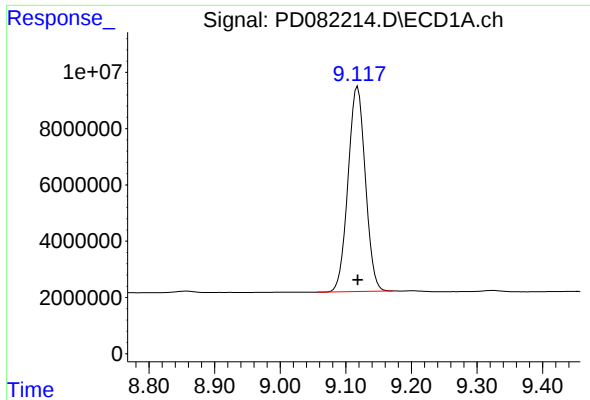

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 133475963
Conc: 73.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

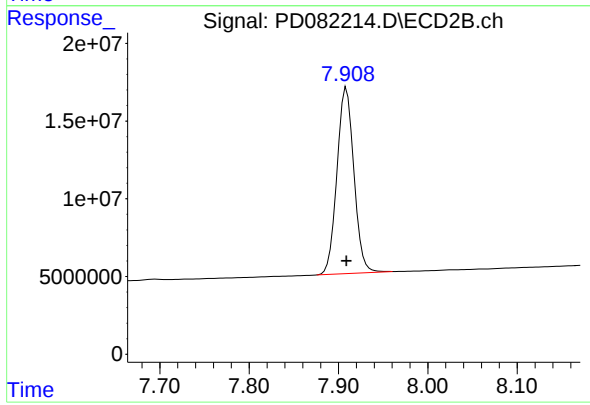

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 157970527
Conc: 74.34 ng/ml