

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
 Data File : PD082217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2024 14:14
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 14:23:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 14:23:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	7713978	16241337	5.216	5.263
28)	SA Decachlor...	9.117	7.909	11257440	11801114	5.805	5.395
Target Compounds							
23)	Chlordane-1	4.734	3.771	4005492	5256551	51.931	53.527
24)	Chlordane-2	5.265	4.346	4650877	6280094	56.809	56.489
25)	Chlordane-3	5.977	4.975	15850408	15223438	49.823	51.328
26)	Chlordane-4	6.059	5.039	19736530	15340106	51.613	53.050
27)	Chlordane-5	6.912	5.933	3147028	5059195	50.823	51.644



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
Data File : PD082217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2024 14:14
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 14:23:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 14:23:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

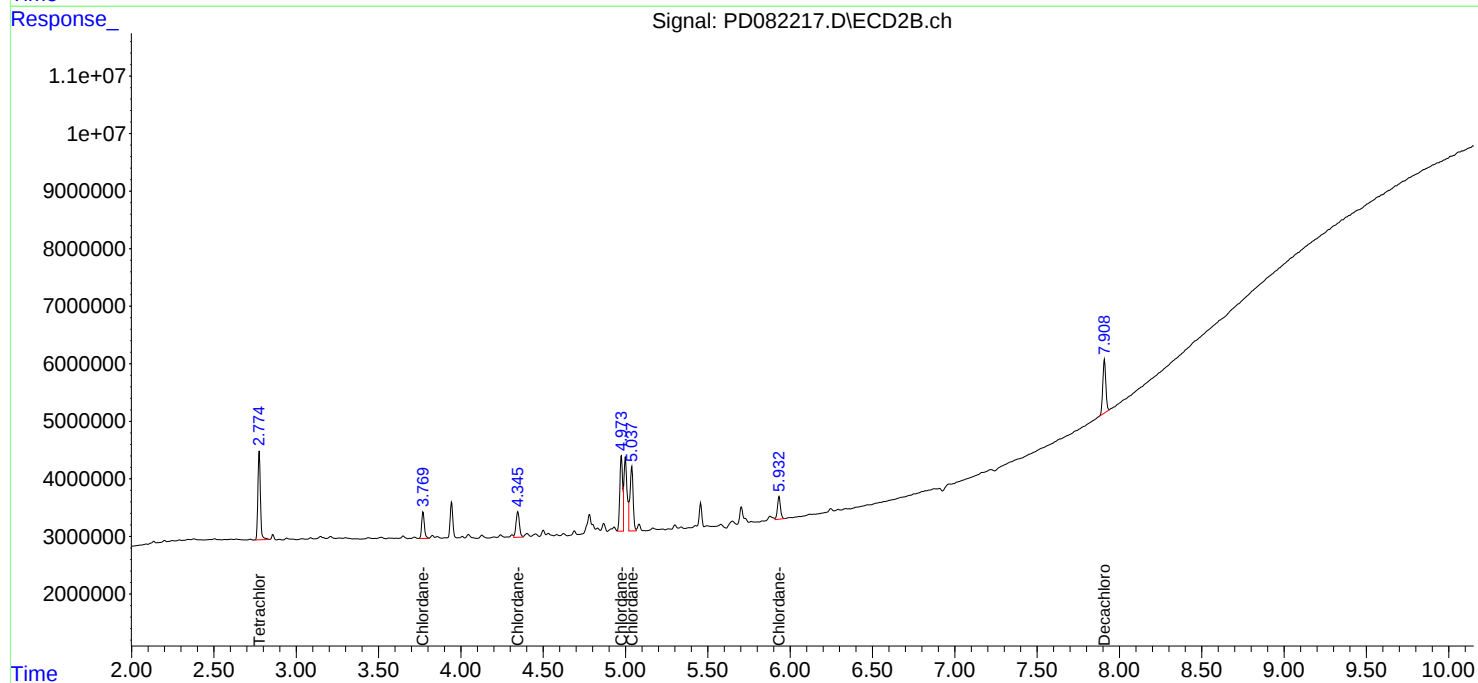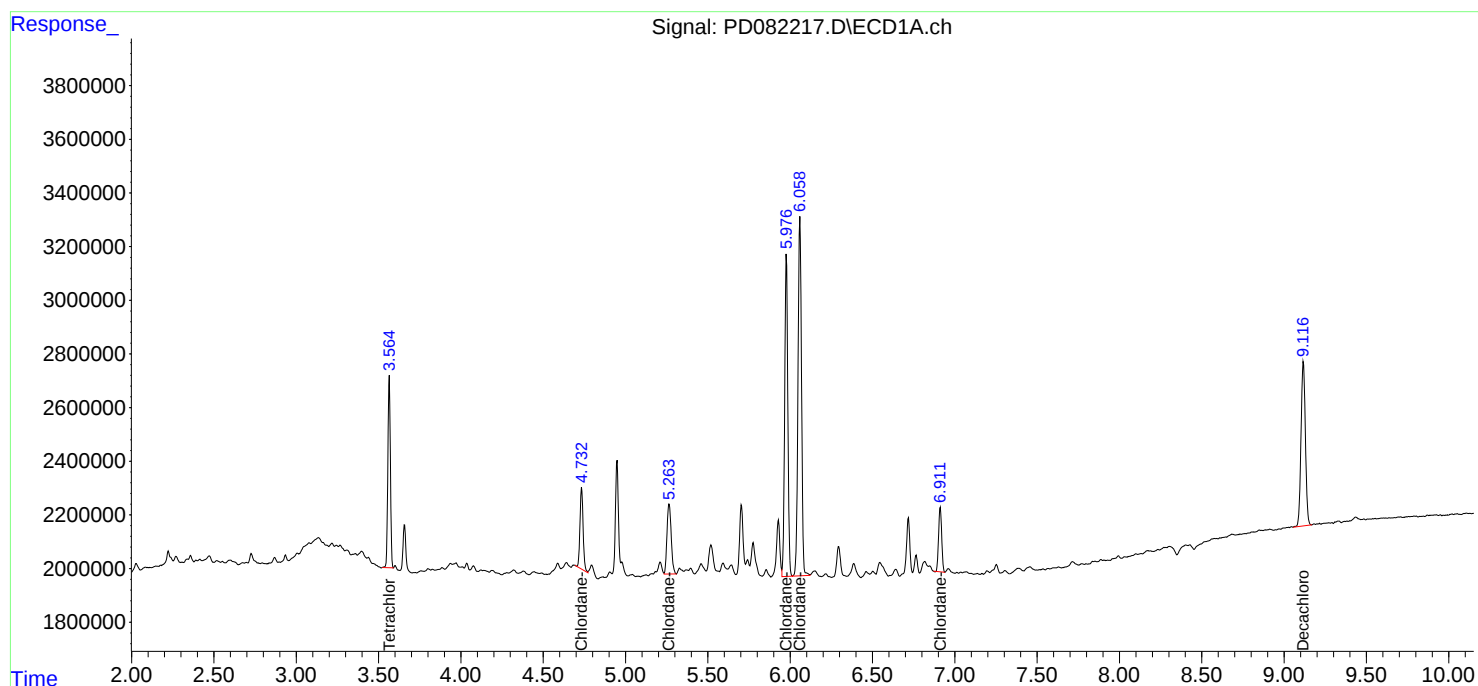


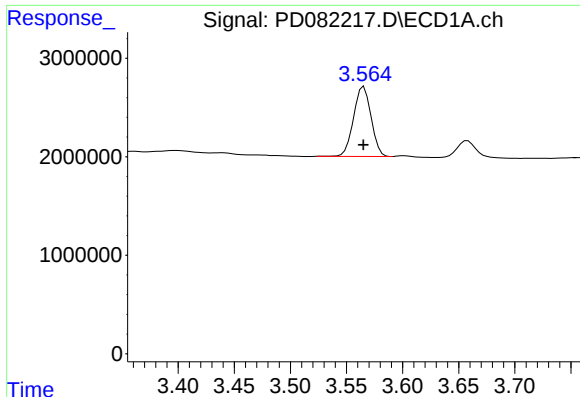

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 7713978
Conc: 5.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

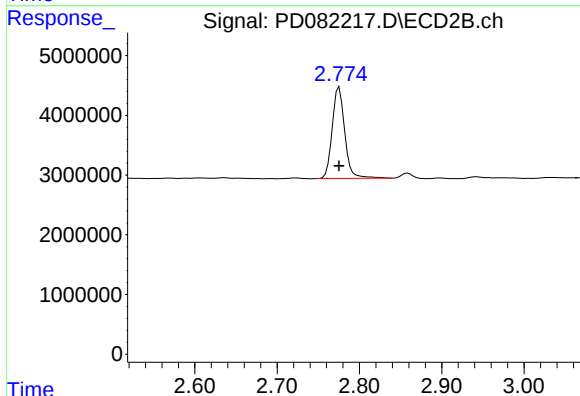


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 16241337
Conc: 5.26 ng/ml

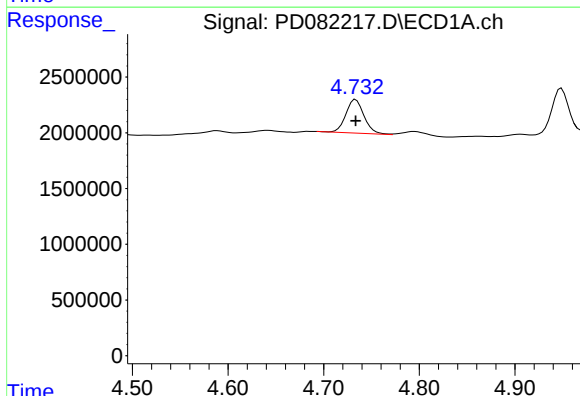


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 4005492
Conc: 51.93 ng/ml

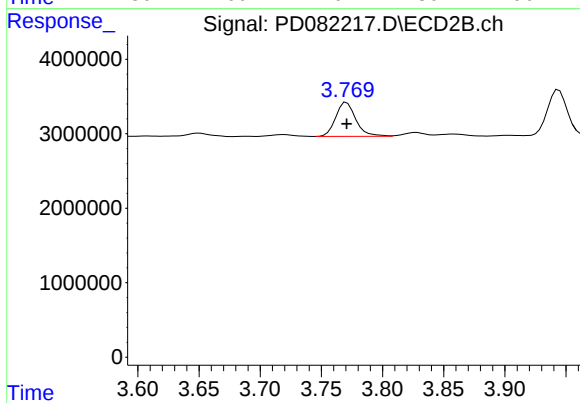

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 5256551
Conc: 53.53 ng/ml

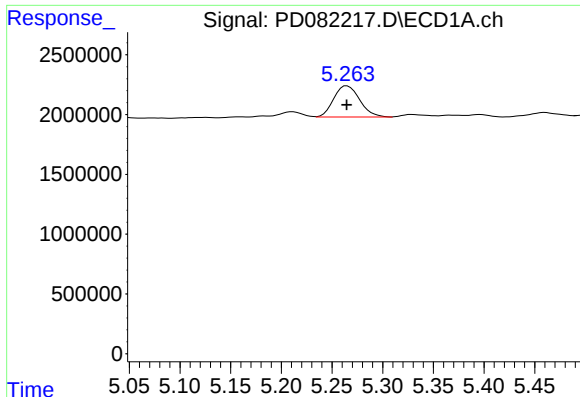

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 4650877
Conc: 56.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

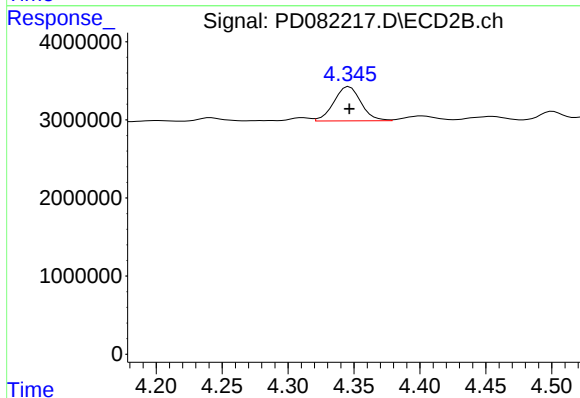


#24 Chlordane-2

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 6280094
Conc: 56.49 ng/ml

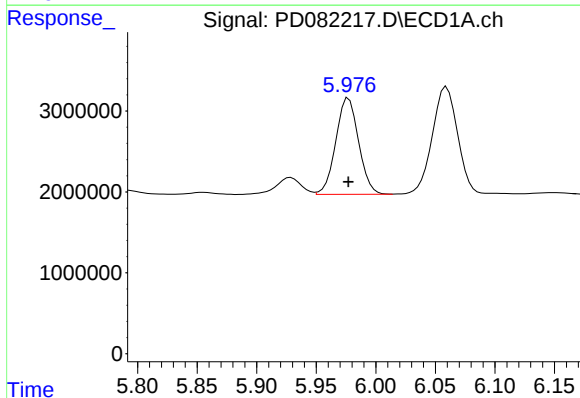


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 15850408
Conc: 49.82 ng/ml

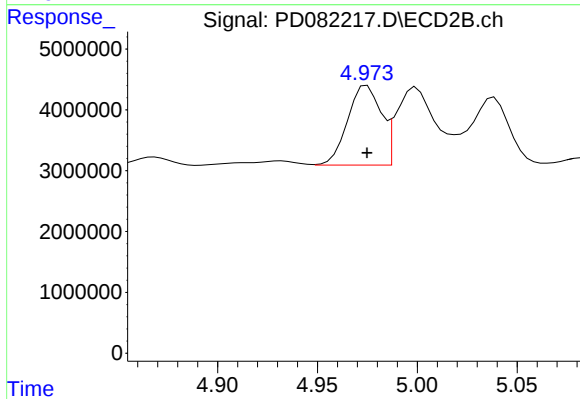

#25 Chlordane-3


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 15223438
Conc: 51.33 ng/ml

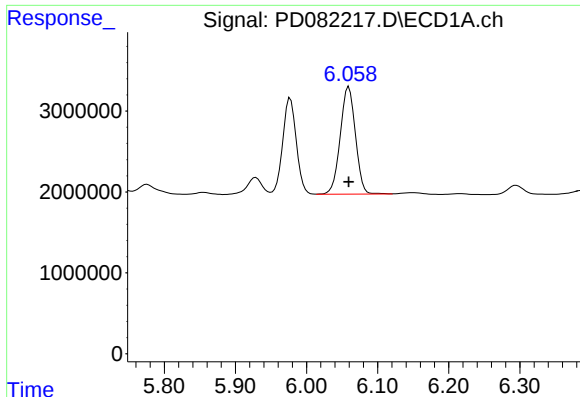

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 19736530
Conc: 51.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

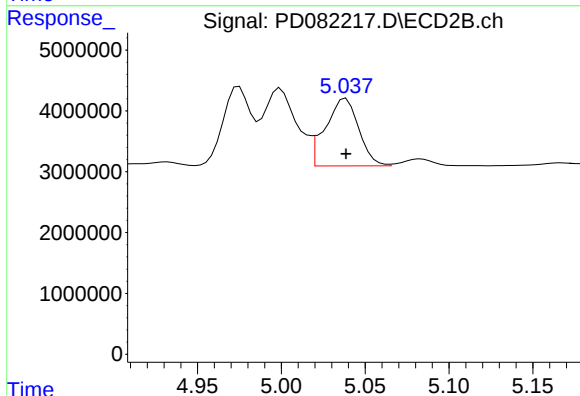


#26 Chlordane-4

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 15340106
Conc: 53.05 ng/ml

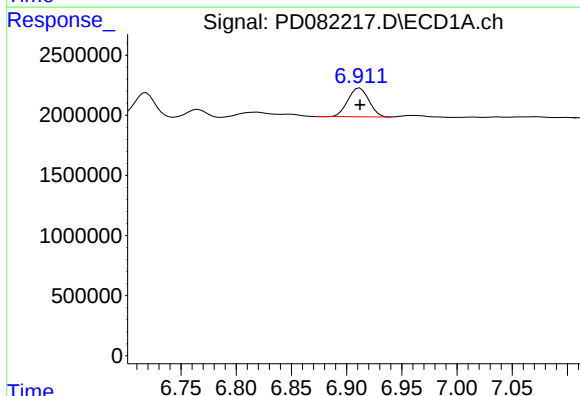


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 3147028
Conc: 50.82 ng/ml

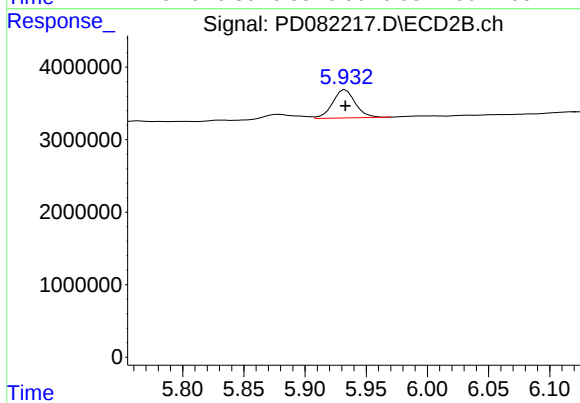

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 5059195
Conc: 51.64 ng/ml

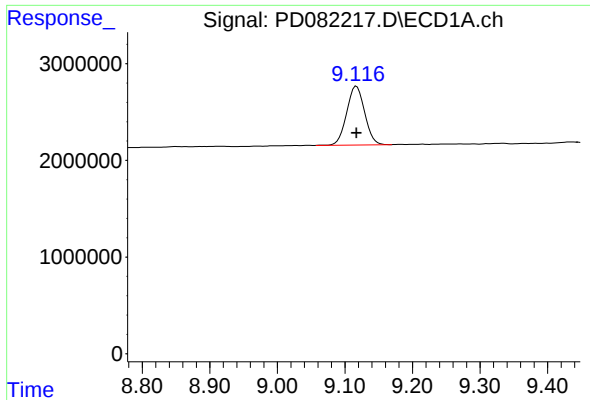

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 11257440
Conc: 5.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

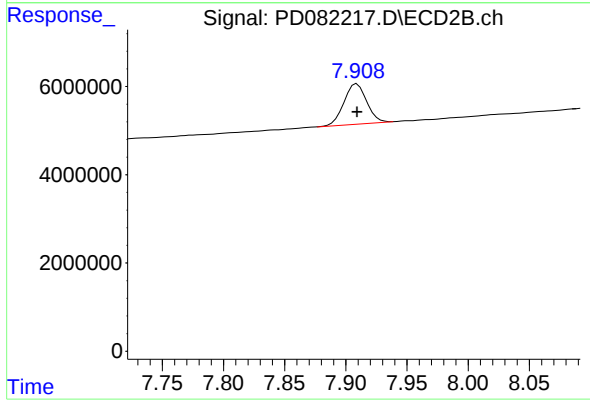

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 11801114
Conc: 5.39 ng/ml