

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
 Data File : PD082224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2024 15:47
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD032224

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 15:58:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 15:58:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.776	74977000	168.4E6	50.699	54.554
28)	SA Decachlor...	9.118	7.909	95841416	117.4E6	49.425	53.690
Target Compounds							
23)	Chlordane-1	4.733	3.771	39254453	53313628	508.927	542.889
24)	Chlordane-2	5.264	4.347	40507147	59610058	494.785	536.191
25)	Chlordane-3	5.977	4.975	161.1E6	162.9E6	506.319	549.325
26)	Chlordane-4	6.059	5.039	191.5E6	154.6E6	500.748	534.677
27)	Chlordane-5	6.912	5.933	31733907	53617902	512.487	547.329



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032224\
Data File : PD082224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2024 15:47
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD032224

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 15:58:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032224.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 15:58:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

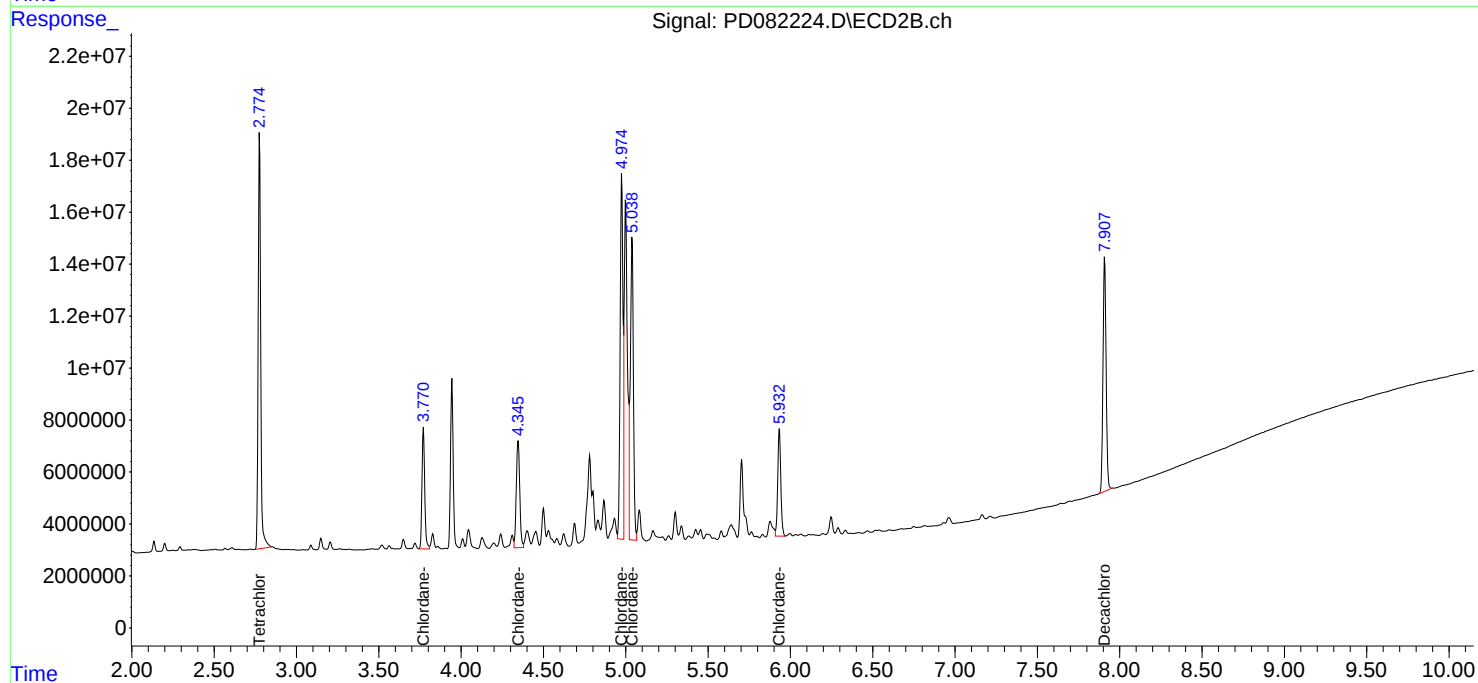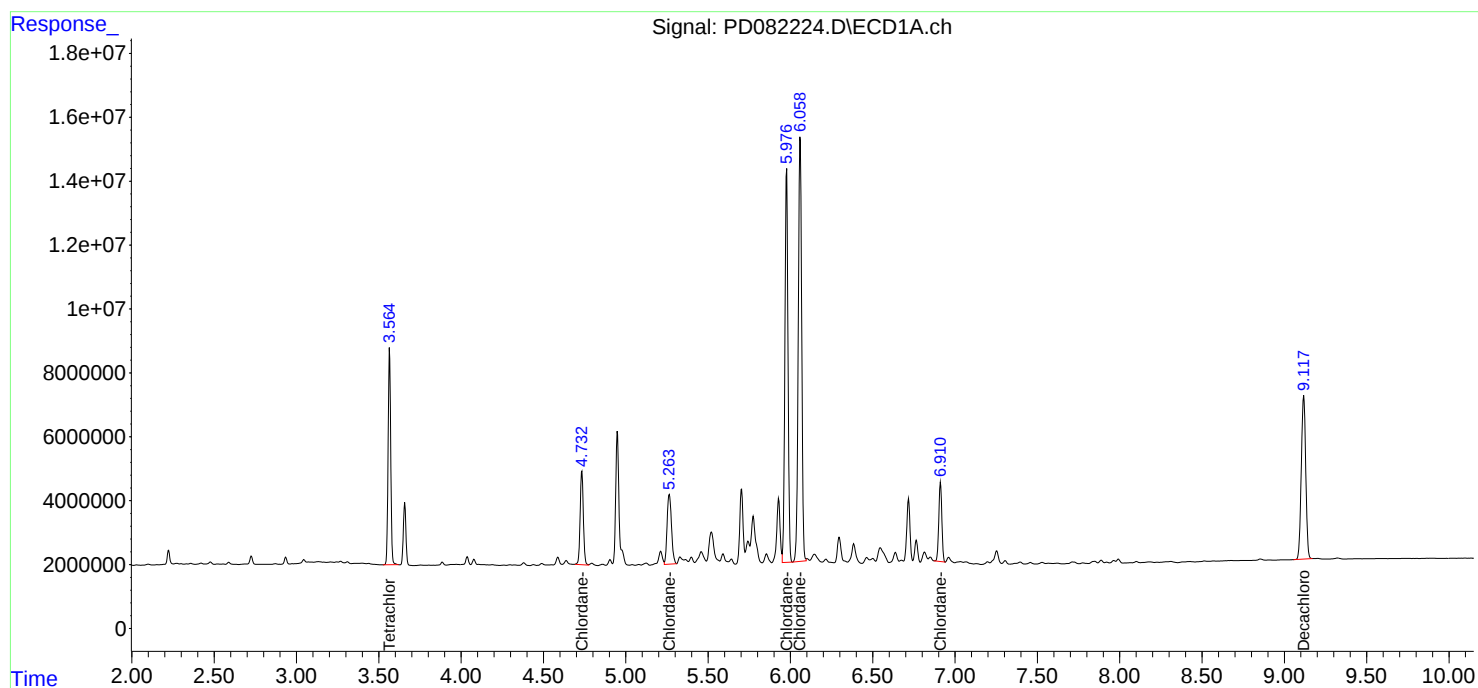


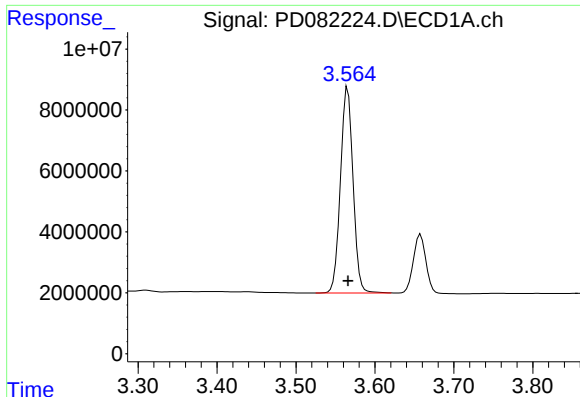

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 74977000
Conc: 50.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032224

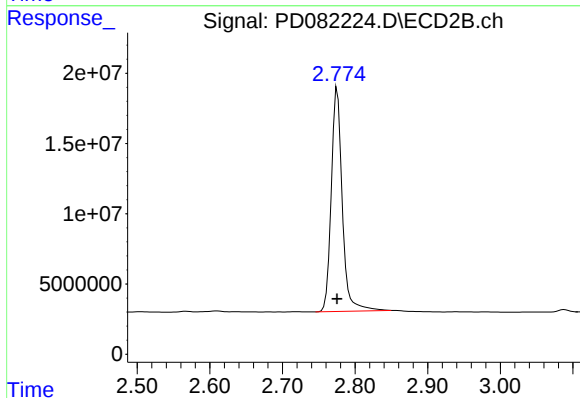


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 168357547
Conc: 54.55 ng/ml

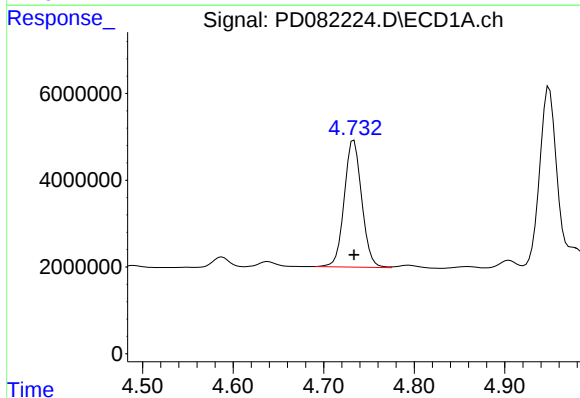


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 39254453
Conc: 508.93 ng/ml

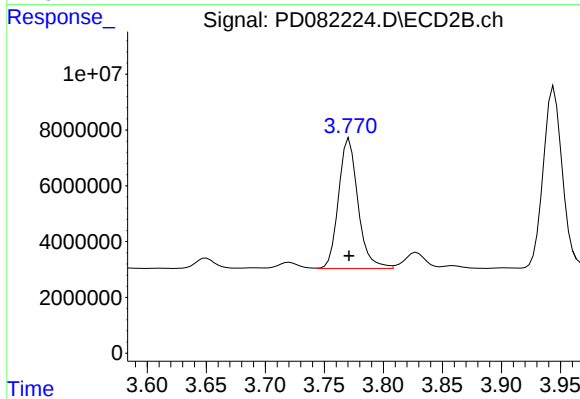

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 53313628
Conc: 542.89 ng/ml

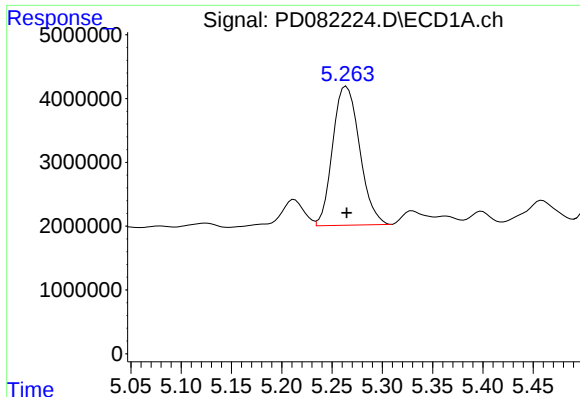

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 40507147
Conc: 494.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032224

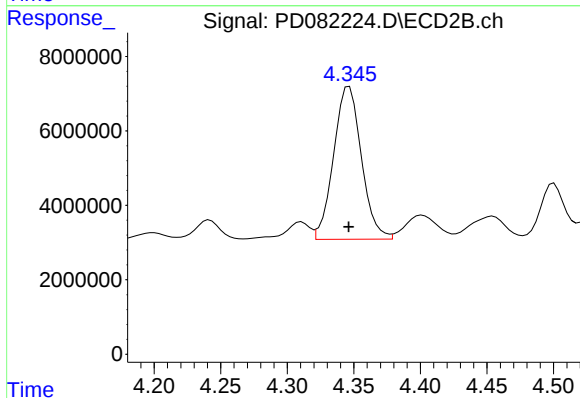


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 59610058
Conc: 536.19 ng/ml

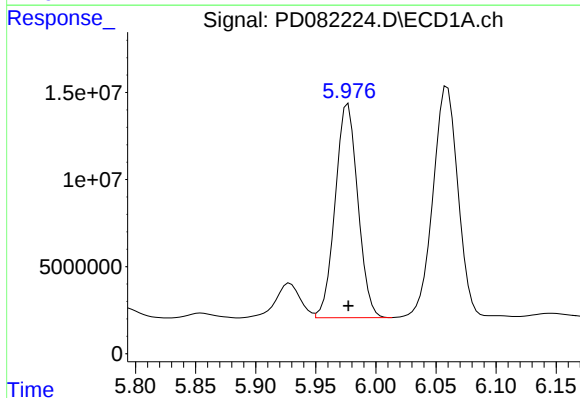


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 161077204
Conc: 506.32 ng/ml

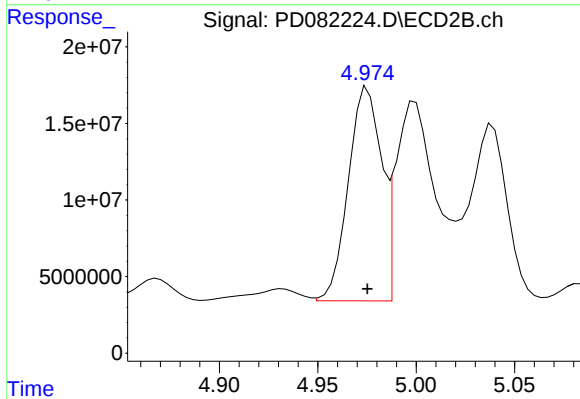

#25 Chlordane-3


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 162924911
Conc: 549.32 ng/ml

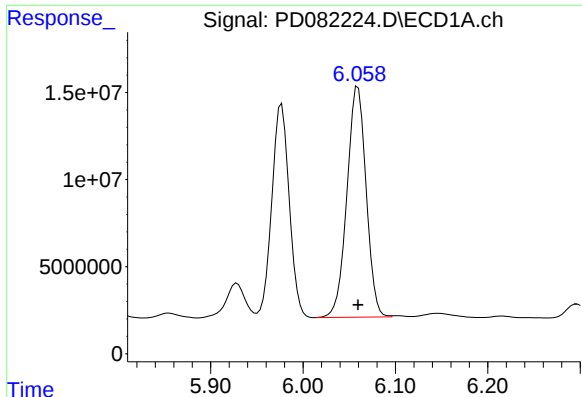

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 191483821
Conc: 500.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032224

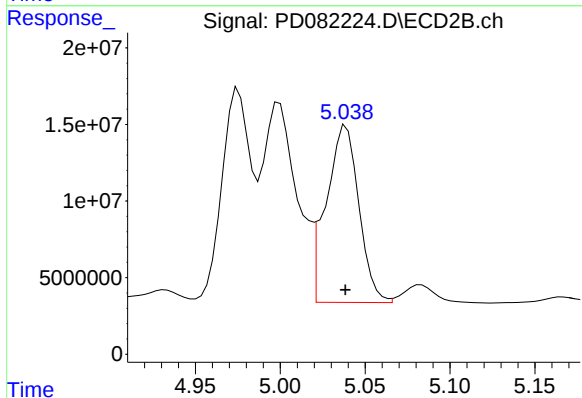


#26 Chlordane-4

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 154608624
Conc: 534.68 ng/ml

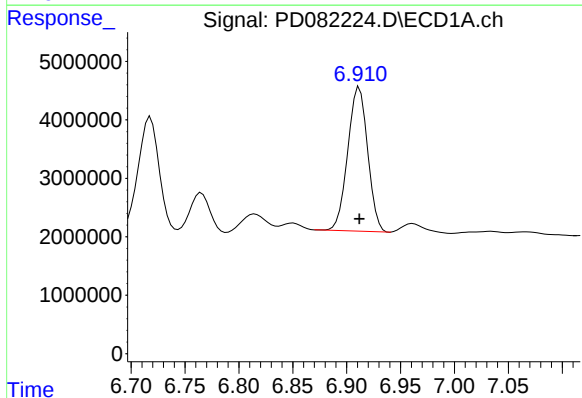


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 31733907
Conc: 512.49 ng/ml

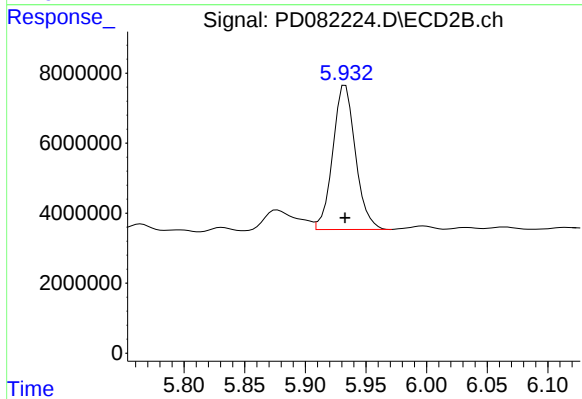

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 53617902
Conc: 547.33 ng/ml

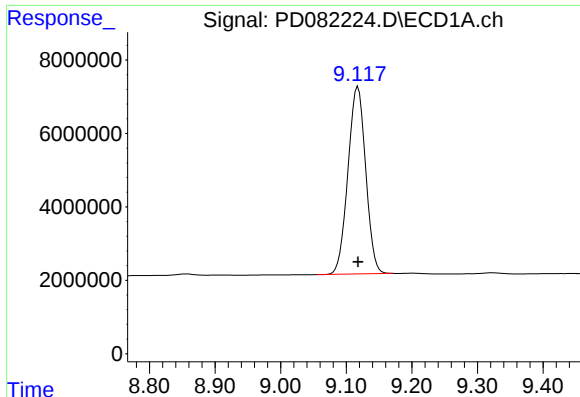

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 95841416
Conc: 49.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD032224

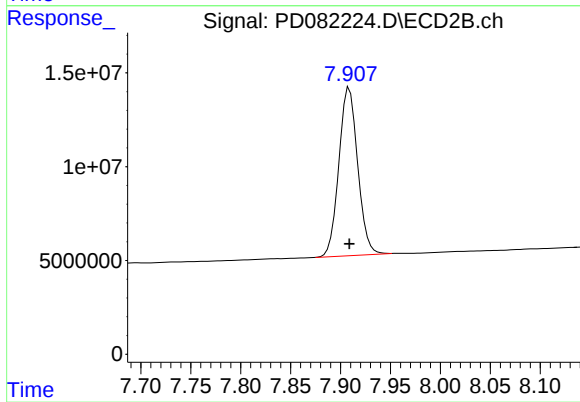

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 117448041
Conc: 53.69 ng/ml