

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032323\
 Data File : PD074376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 11:05
 Operator : AR\AJ
 Sample : PB151544BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS544

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/23/2023
 Supervised By :Ankita Jodhani 03/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 21:15:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	48717080	24119677	19.609	19.171
27)	SA Decachlor...	9.092	7.921	104.8E6	46503600	38.283	38.837
Target Compounds							
2)	A alpha-BHC	4.005	3.273	17815607	8088633	4.566	4.526
3)	MA gamma-BHC...	4.338	3.603	17504901	7824661	4.742	4.581
4)	MA Heptachlor	4.931	3.945	18147369	8071216	4.793	4.868
5)	MB Aldrin	5.274	4.226	18463527	8457248	5.052	4.940
6)	B beta-BHC	4.533	3.899	9083223	4110541	5.373	5.074
7)	B delta-BHC	4.781	4.130	19243413	7439948	5.288	4.206
8)	B Heptachlo...	5.701	4.728	17477490	7604086	5.323	4.800
9)	A Endosulfan I	6.088	5.098	15240856	6944194	5.109	4.952
10)	B trans-Chl...	5.958	4.978	15869531	7695957	4.946	4.975
11)	B cis-Chlor...	6.037	5.043	16421901	7900315	5.012	4.994
12)	B 4,4'-DDE	6.209	5.233	27976386	13546036	9.340	9.326
13)	MA Dieldrin	6.364	5.364	31360054	15510961	9.885	10.005
14)	MA Endrin	6.594	5.639	26360226	13616327	10.003	10.121
15)	B Endosulfa...	6.813	5.931	29097585	12807120	10.542	9.526m
16)	A 4,4'-DDD	6.727	5.787	24116115	12078450	10.204	10.259
17)	MA 4,4'-DDT	7.043	6.039	25845989	12049121	10.300	9.618
18)	B Endrin al...	6.943	6.113	21459146	10535262	9.527	9.584
19)	B Endosulfa...	7.177	6.335	26634710	12730960	10.226	10.114
20)	A Methoxychlor	7.518	6.615	73985211	34083464	53.891	55.413
21)	B Endrin ke...	7.664	6.842	31606704	15868984	10.660	10.429

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032323\
Data File : PD074376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 11:05
Operator : AR\AJ
Sample : PB151544BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 21:15:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

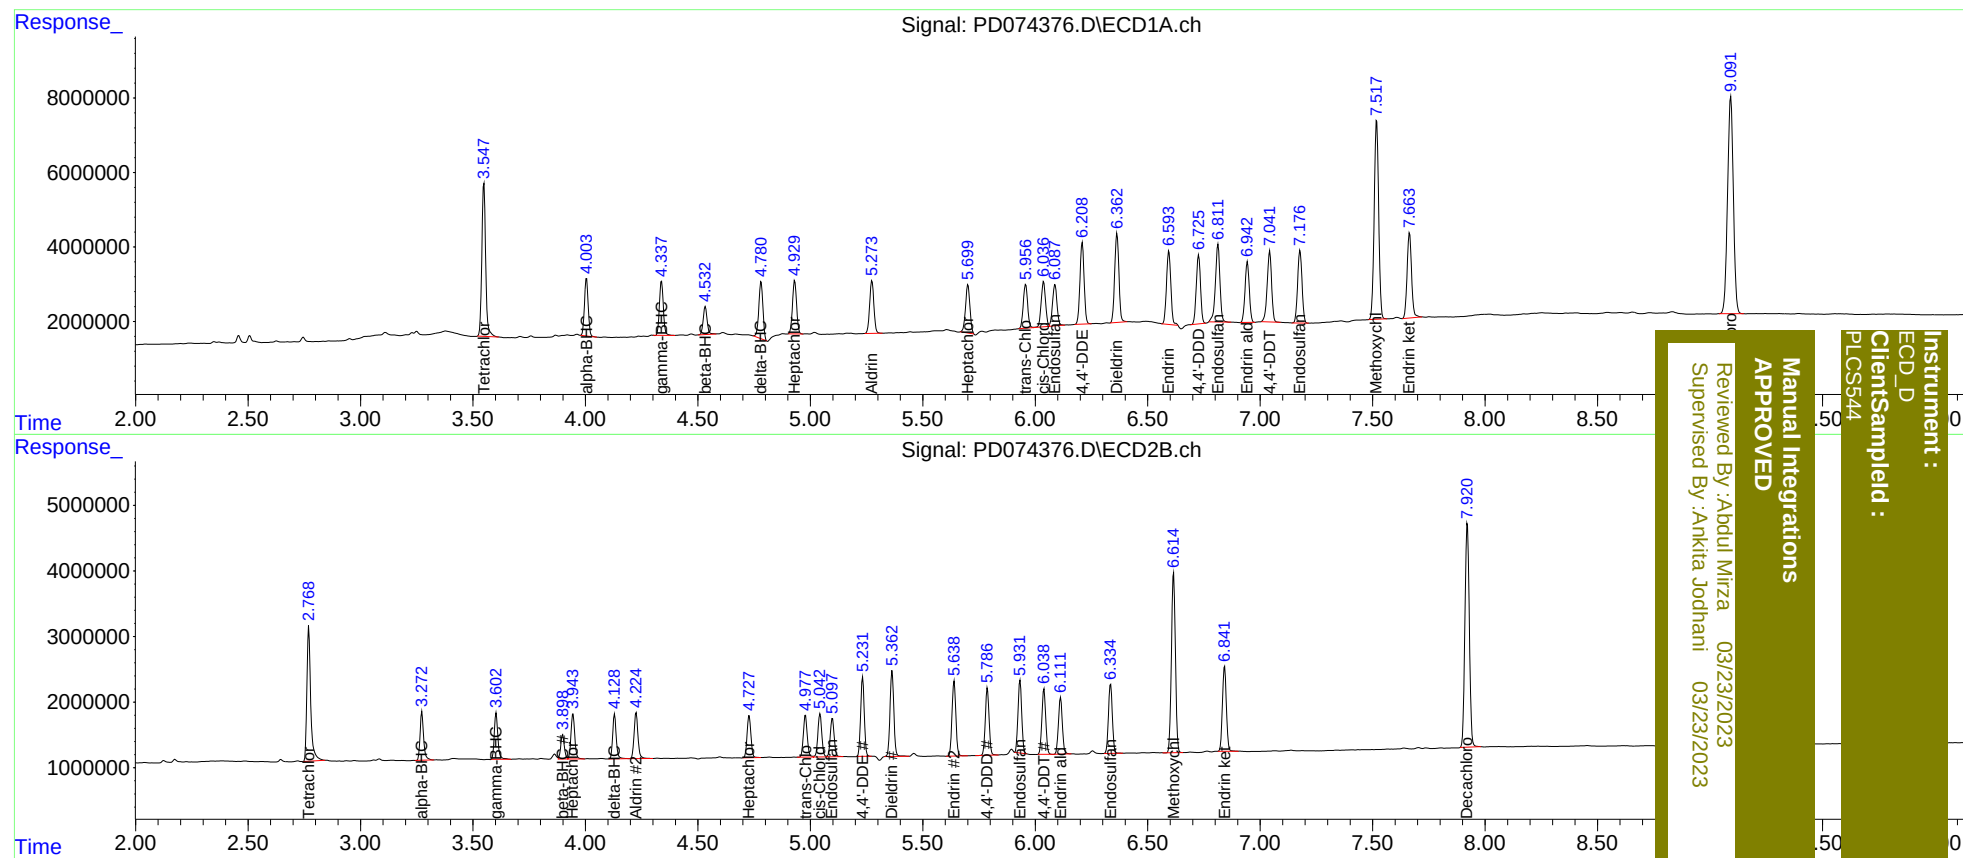

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/23/2023
Supervised By: Ankita Jodhani 03/23/2023

Instrument :
ECD_D
Client Sampled :
PLCS544