

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032323\
 Data File : PD074403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 17:45
 Operator : AR\AJ
 Sample : PB151608BS
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS608

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/23/2023
 Supervised By :Ankita Jodhani 03/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 21:24:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.771	48062592	23967202	19.346	19.050
27)	SA Decachlor...	9.093	7.922	107.0E6	46406740	39.098	38.756
Target Compounds							
2)	A alpha-BHC	4.005	3.274	17920233	8142389	4.592	4.556
3)	MA gamma-BHC...	4.339	3.604	16946081	7722463	4.591	4.521
4)	MA Heptachlor	4.931	3.945	17630559	7988190	4.657	4.818
5)	MB Aldrin	5.274	4.226	18354319	8369714	5.022	4.888
6)	B beta-BHC	4.534	3.900	8438289	4018767	4.991	4.960
7)	B delta-BHC	4.782	4.130	19067067	7237201	5.240	4.092
8)	B Heptachlo...	5.701	4.729	18395818	7615062	5.603	4.807
9)	A Endosulfan I	6.088	5.099	15563821	6963093	5.217	4.966
10)	B trans-Chl...	5.957	4.979	16109010	7679206	5.021	4.964
11)	B cis-Chlor...	6.037	5.043	16683019	7961977	5.091	5.033
12)	B 4,4'-DDE	6.209	5.233	28477145	13569853	9.507	9.342
13)	MA Dieldrin	6.364	5.364	31961172	15545346	10.075	10.027
14)	MA Endrin	6.594	5.640	26960429	13570627	10.231	10.088
15)	B Endosulfa...	6.811	5.932	28743609	13305555	10.414m	9.896m
16)	A 4,4'-DDD	6.727	5.788	24339764	11988030	10.299	10.182
17)	MA 4,4'-DDT	7.042	6.040	25205472	11407473	10.044	9.106
18)	B Endrin al...	6.943	6.113	21901429	10604193	9.724	9.646
19)	B Endosulfa...	7.178	6.336	26933923	12744690	10.341	10.125
20)	A Methoxychlor	7.518	6.616	72194303	33581258	52.586	54.596
21)	B Endrin ke...	7.664	6.843	32928124	15586799	11.106	10.244

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032323\
Data File : PD074403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 17:45
Operator : AR\AJ
Sample : PB151608BS
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 21:24:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

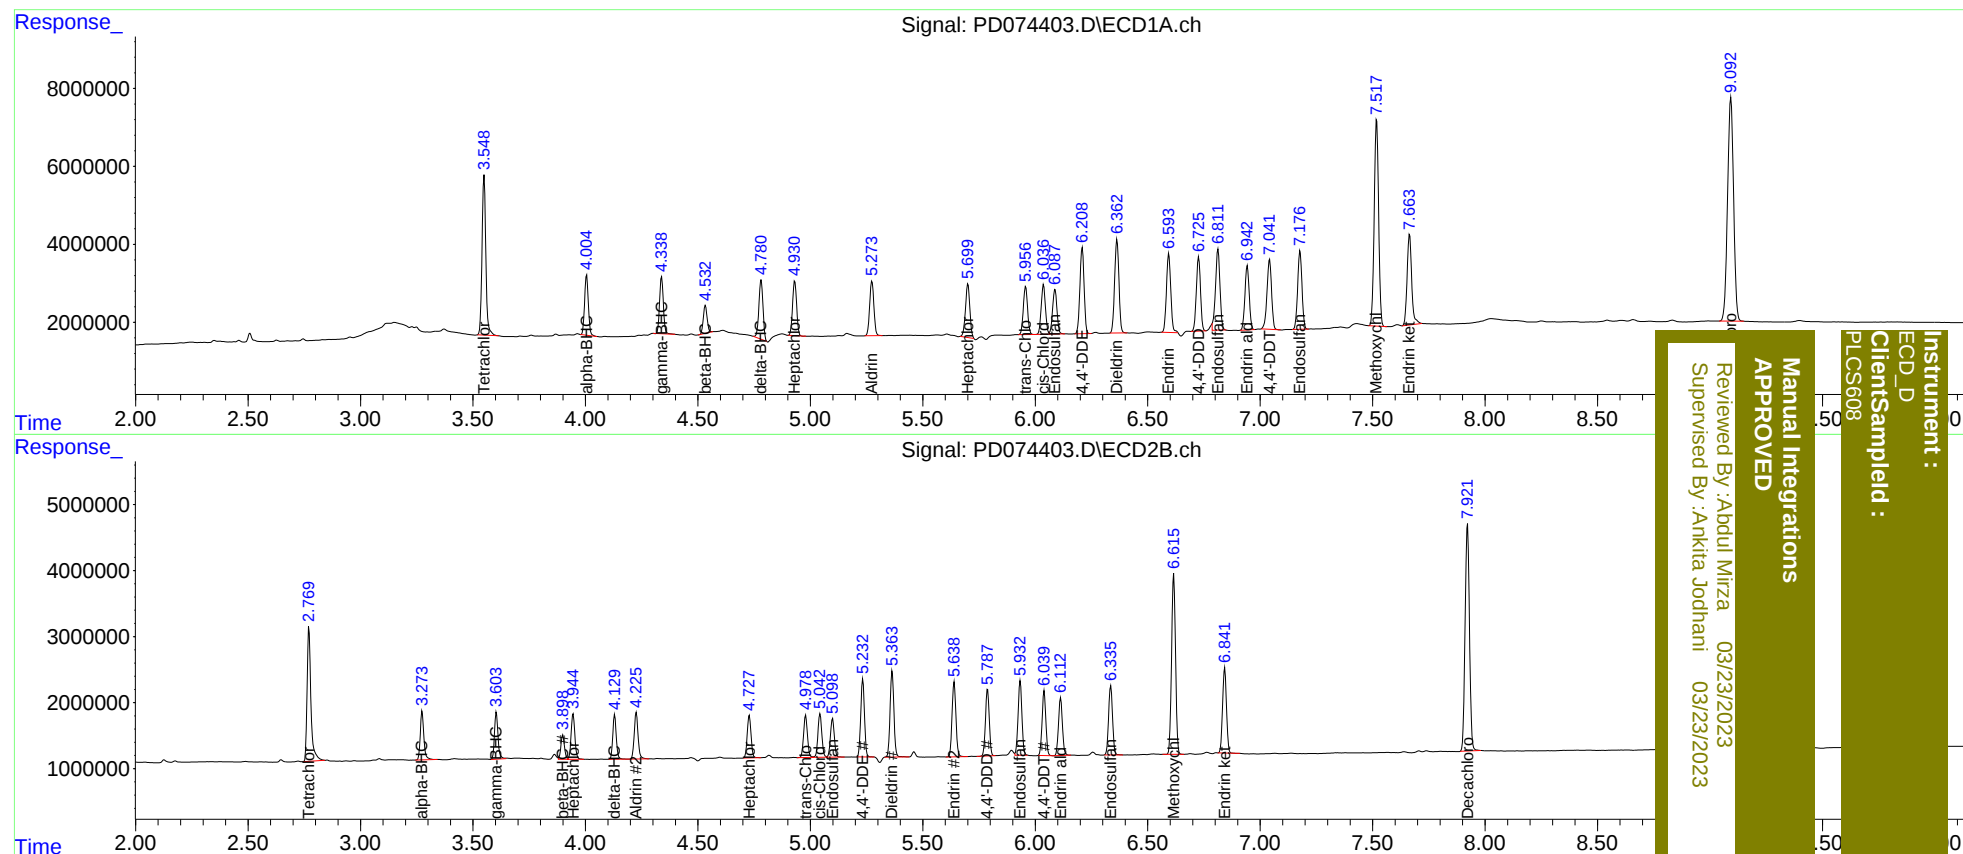

Instrument :
ECD_D
ClientSampled :
PLCS608

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 03/23/2023
Supervised By: Ankita Jodhani 03/23/2023