

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052062.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 11:50
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:28:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


6) B	beta-BHC	0.000	4.935f	0 27992262	N.D.	1.520
10) B	trans-Chl...	0.000	6.131	0 53792882	N.D.	1.604


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052062.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 11:50
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:28:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

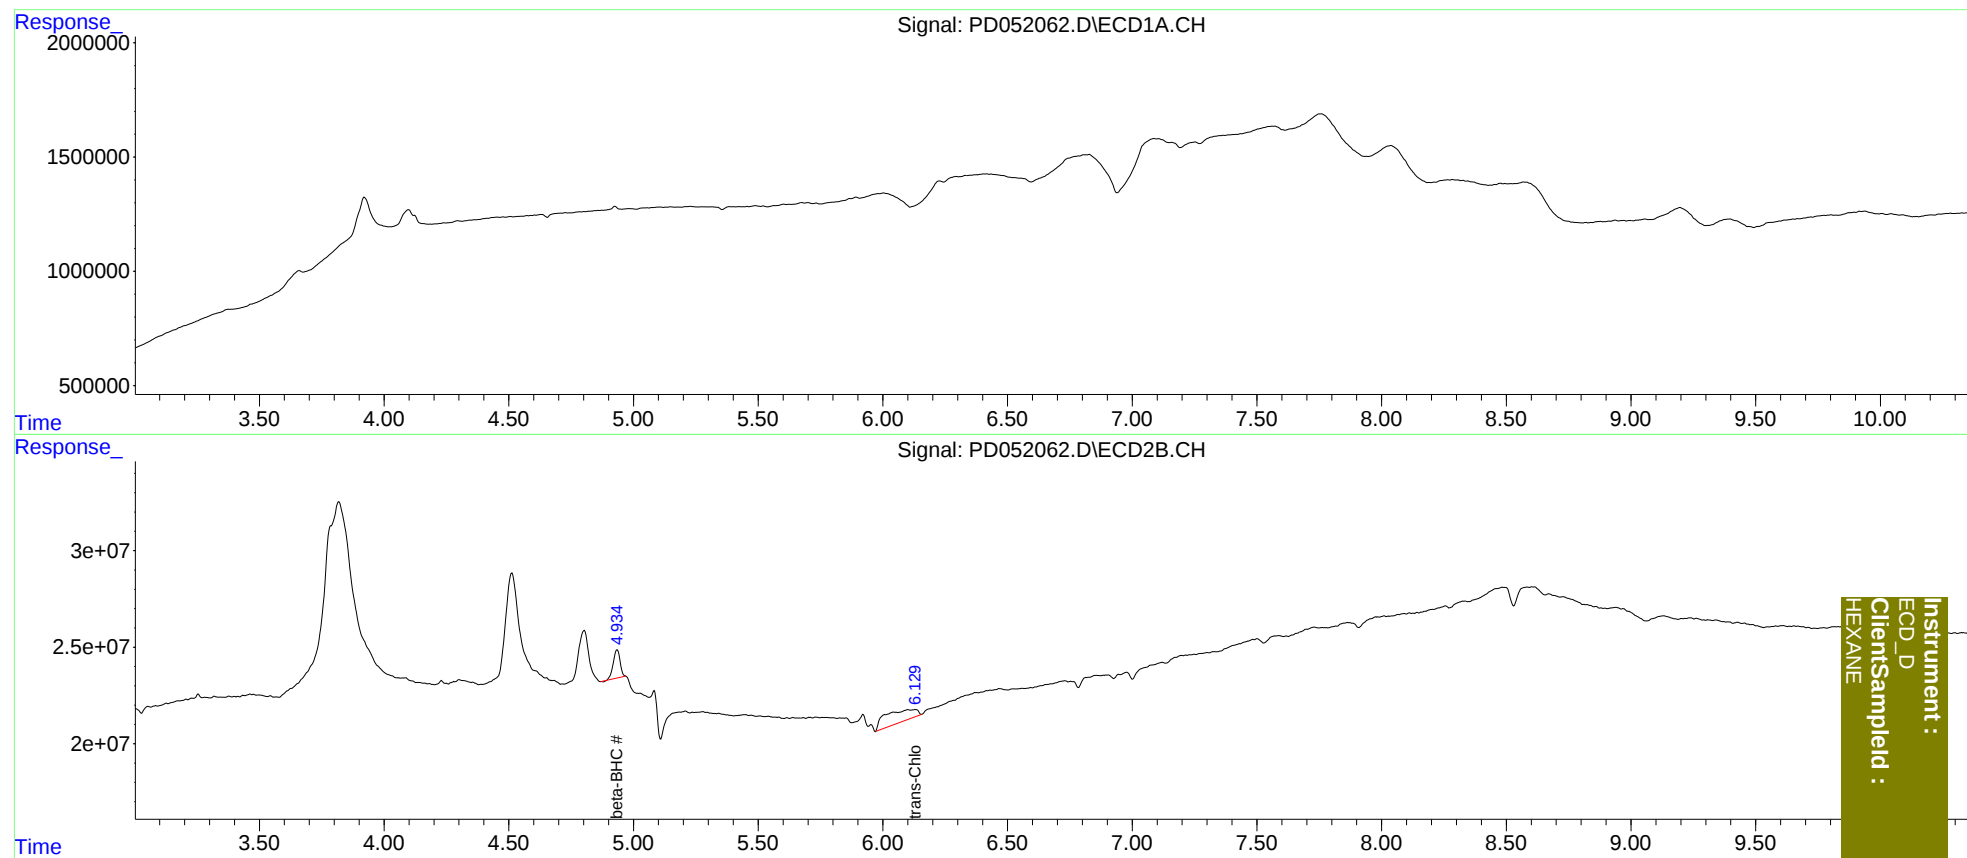


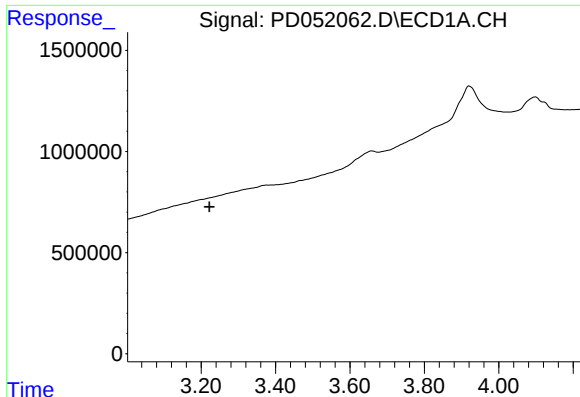

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

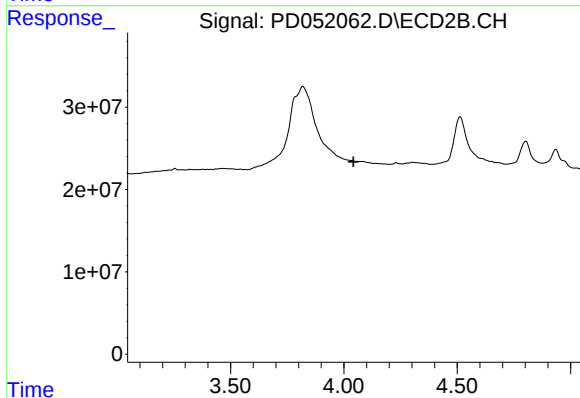


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.043 min
Response: 0
Conc: N.D.

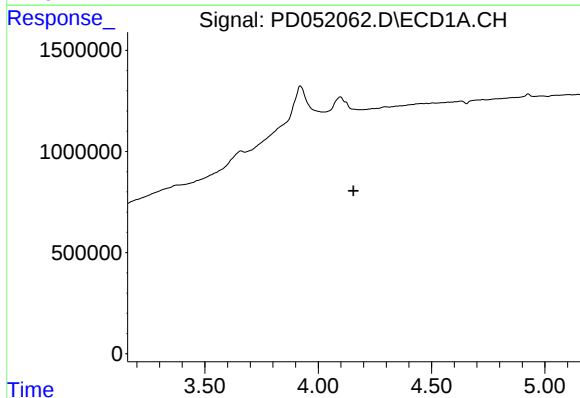


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.156 min
Response: 0
Conc: N.D.

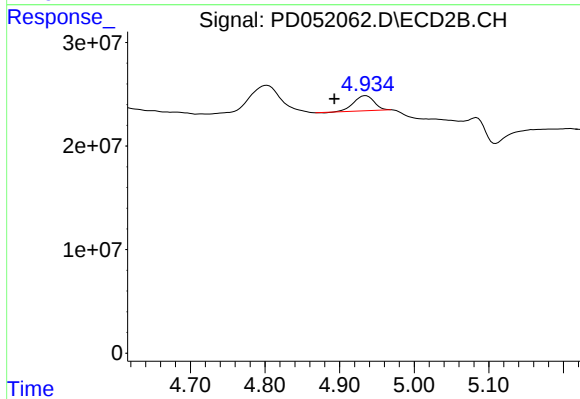

#6 beta-BHC


R.T.: 4.935 min
Delta R.T.: 0.042 min
Response: 27992262
Conc: 1.52 ng/ml

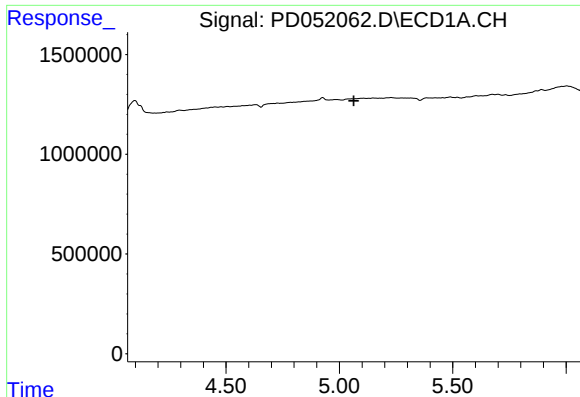

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

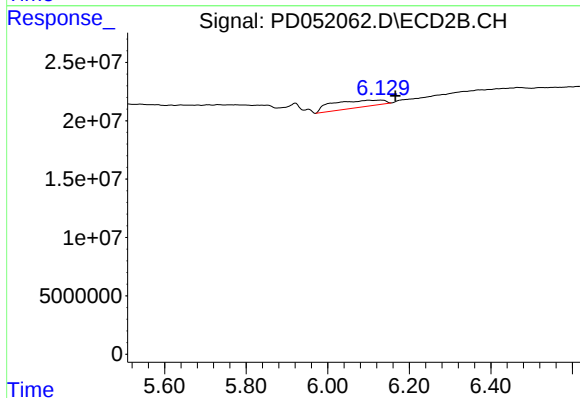


#10 trans-Chlordane

R.T.: 6.131 min
Delta R.T.: -0.034 min
Response: 53792882
Conc: 1.60 ng/ml

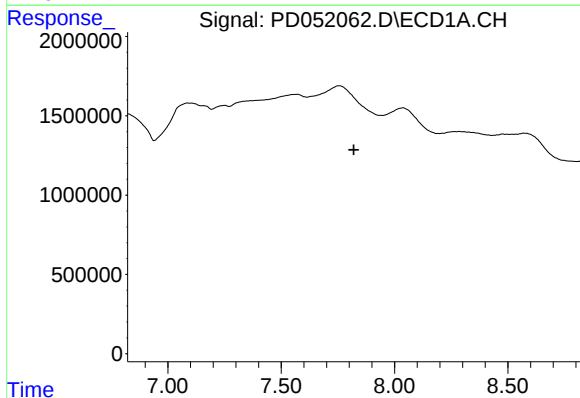

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.820 min
Response: 0
Conc: N.D.

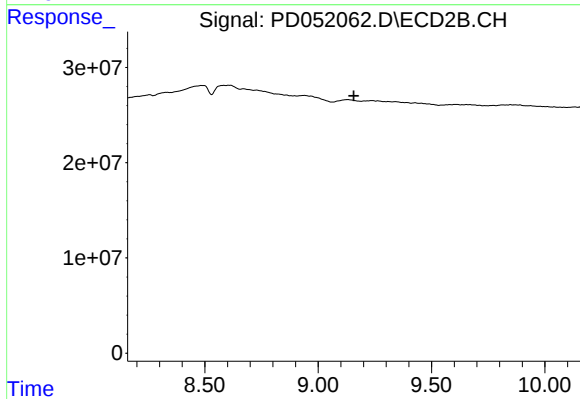

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.157 min
Response: 0
Conc: N.D.