

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052074.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 14:40
 Operator : AJ\SJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:07:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:07:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	28150733	604.4E6	20.000	20.000
27)	SA Decachlor...	7.821	9.156	42289260	598.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.642	4.435	44571080	900.7E6	20.000	20.000
3)	MA gamma-BHC...	3.910	4.723	44328953	818.1E6	20.000	20.000
4)	MA Heptachlor	4.188	5.236	43819280	828.9E6	20.000	20.000
9)	A Endosulfan I	5.168	6.290	39497366	628.2E6	20.000	20.000
13)	MA Dieldrin	5.404	6.548	89915170	1226.9E6	40.000	40.000
14)	MA Endrin	5.651	6.767	77107879	921.8E6	40.000	40.000
16)	A 4,4'-DDD	5.792	6.887	70185339	909.9E6	40.000	40.000
17)	MA 4,4'-DDT	6.022	7.187	69535865	771.1E6	40.000	40.000
20)	A Methoxychlor	6.568	7.646	189.8E6	1871.8E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052074.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 14:40
Operator : AJ\SJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:07:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:07:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

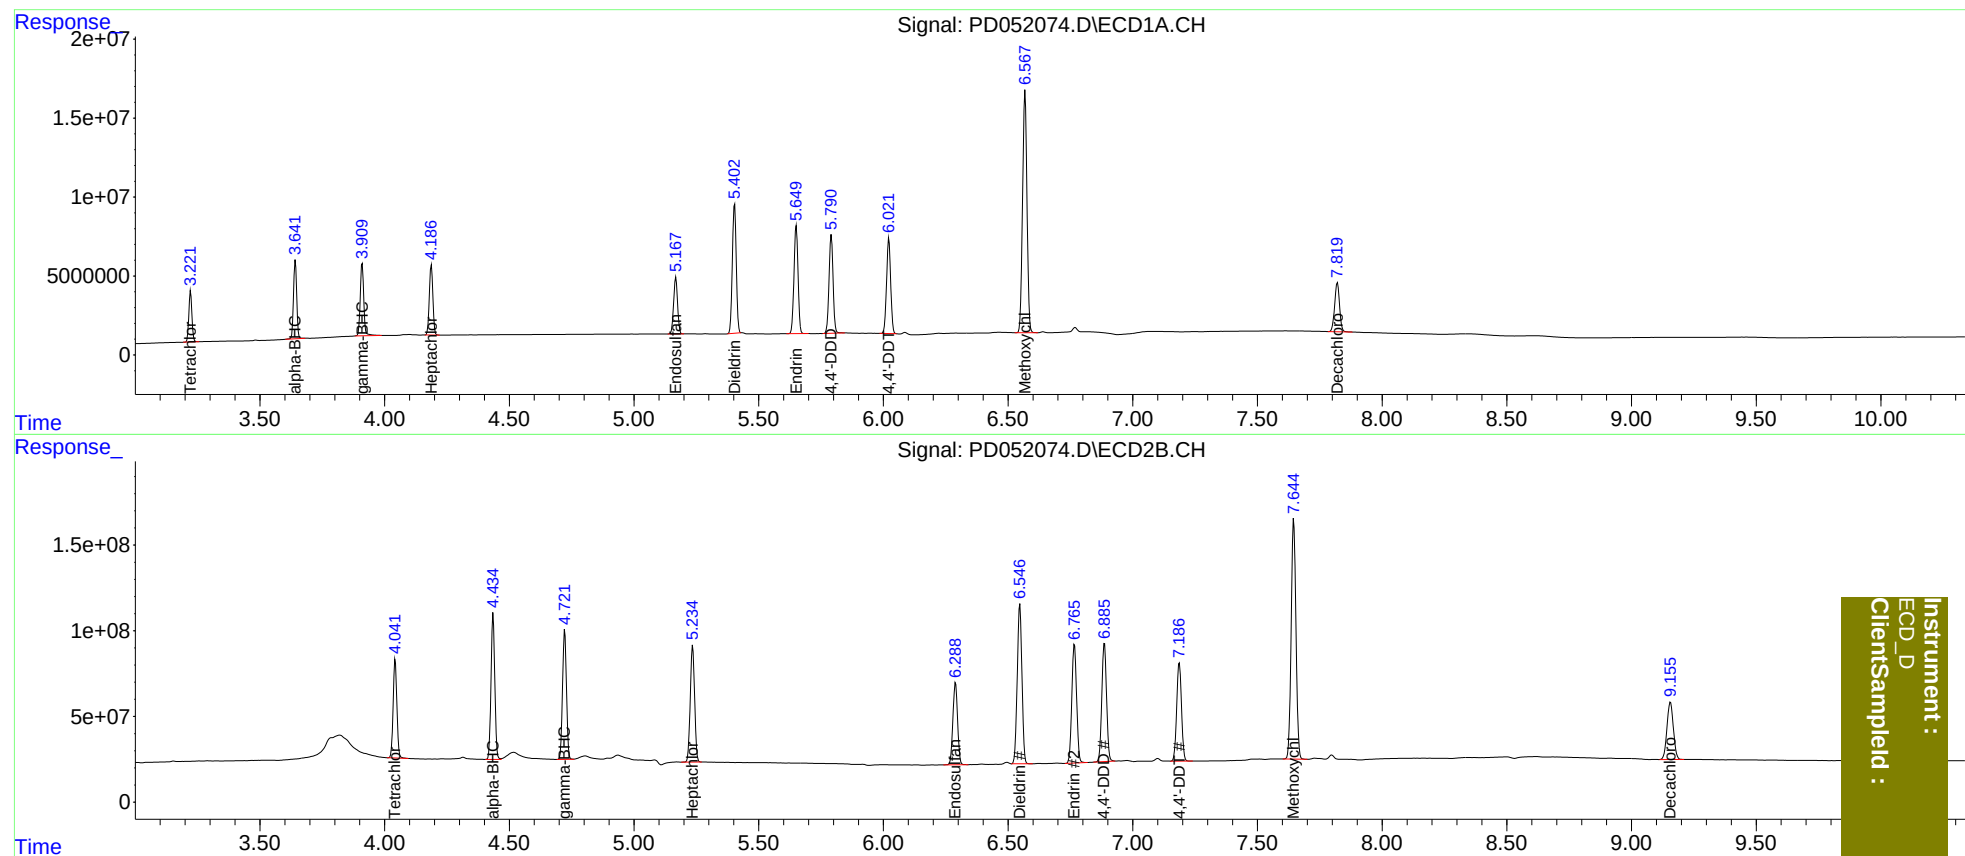


Instrument :
ECD_D
ClientSampled :

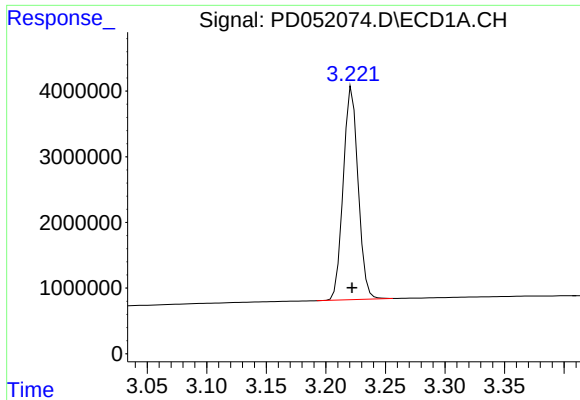

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 28150733
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

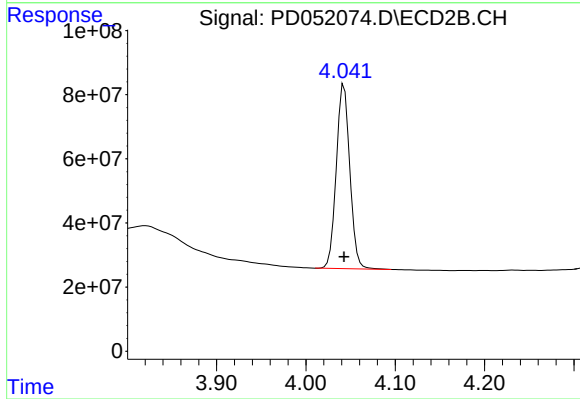


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 604358567
Conc: 20.00 ng/ml

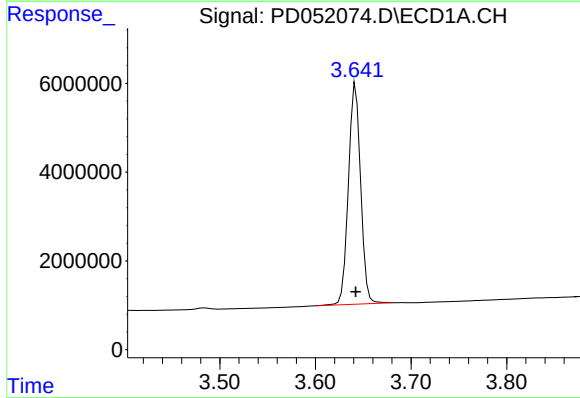


#2 alpha-BHC

R.T.: 3.642 min
Delta R.T.: 0.000 min
Response: 44571080
Conc: 20.00 ng/ml

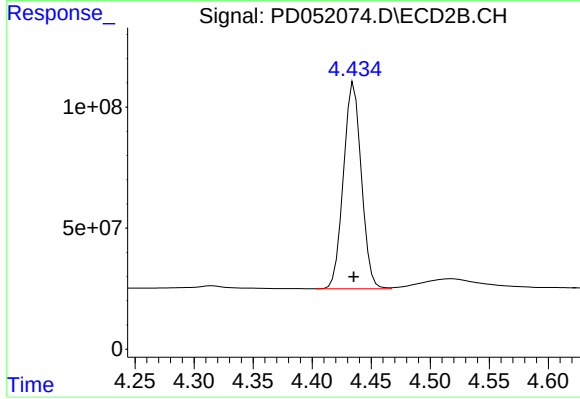

#2 alpha-BHC


R.T.: 4.435 min
Delta R.T.: 0.000 min
Response: 900706992
Conc: 20.00 ng/ml

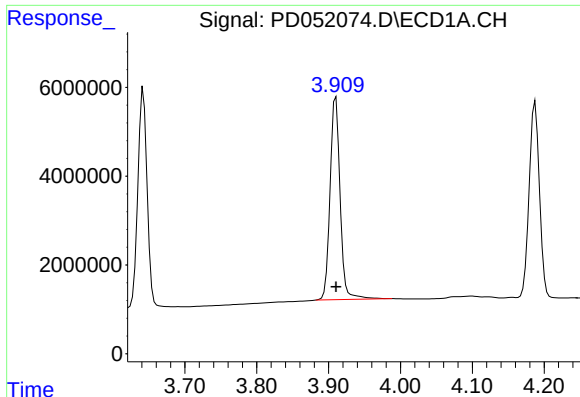

#3 gamma-BHC (Lindane)


R.T.: 3.910 min
Delta R.T.: 0.000 min
Response: 44328953
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

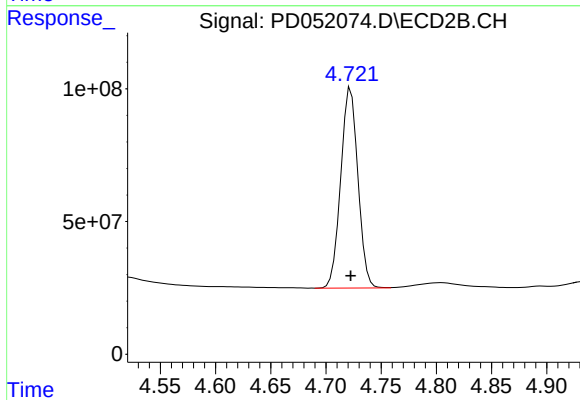


#3 gamma-BHC (Lindane)

R.T.: 4.723 min
Delta R.T.: 0.000 min
Response: 818084980
Conc: 20.00 ng/ml

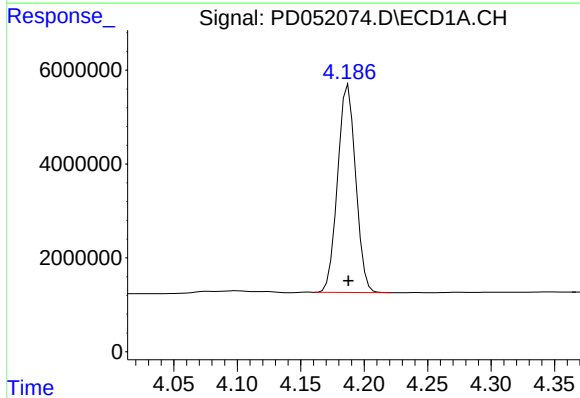


#4 Heptachlor

R.T.: 4.188 min
Delta R.T.: 0.000 min
Response: 43819280
Conc: 20.00 ng/ml

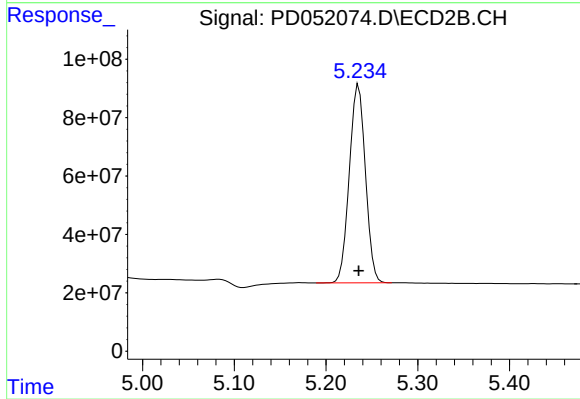

#4 Heptachlor


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 828897329
Conc: 20.00 ng/ml

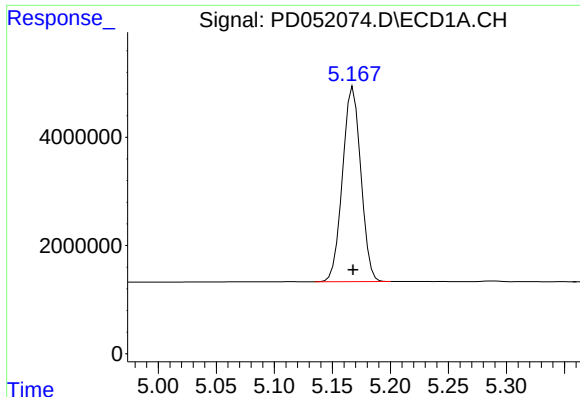

#9 Endosulfan I


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 39497366
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

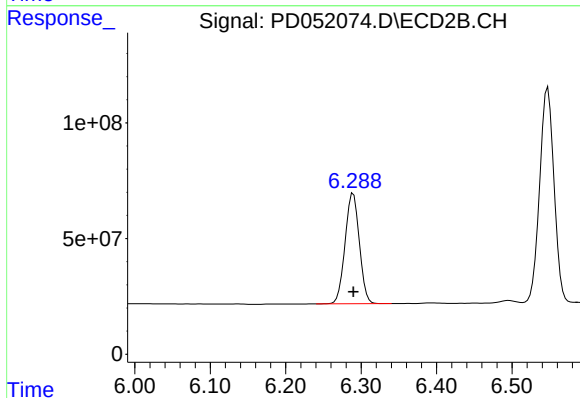


#9 Endosulfan I

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 628225770
Conc: 20.00 ng/ml

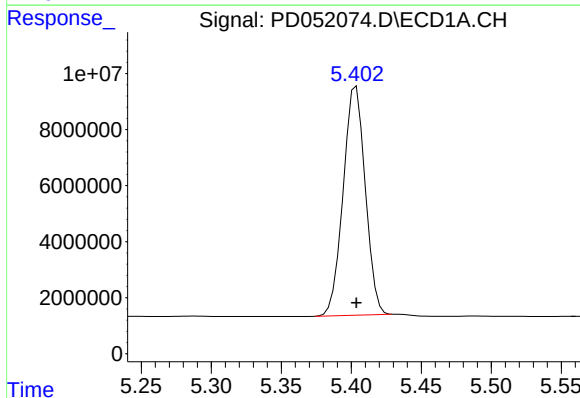


#13 Dieldrin

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 89915170
Conc: 40.00 ng/ml

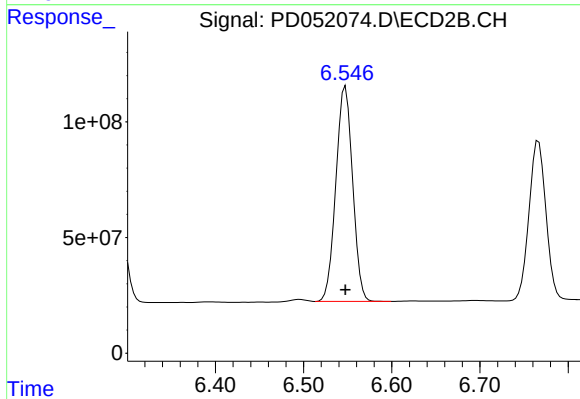

#13 Dieldrin


R.T.: 6.548 min
Delta R.T.: 0.000 min
Response: 1226859509
Conc: 40.00 ng/ml

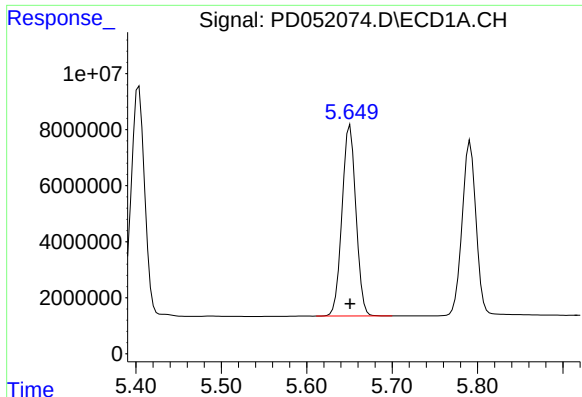

#14 Endrin


R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 77107879
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

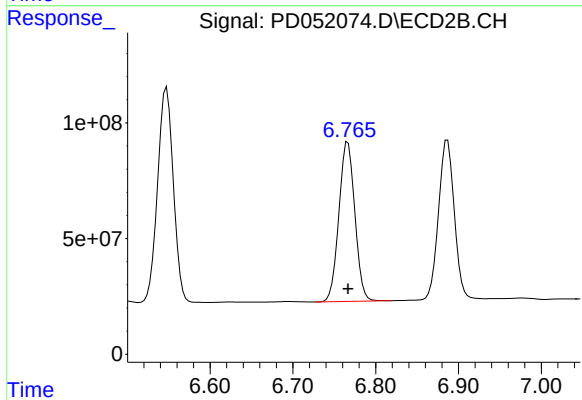


#14 Endrin

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 921838566
Conc: 40.00 ng/ml

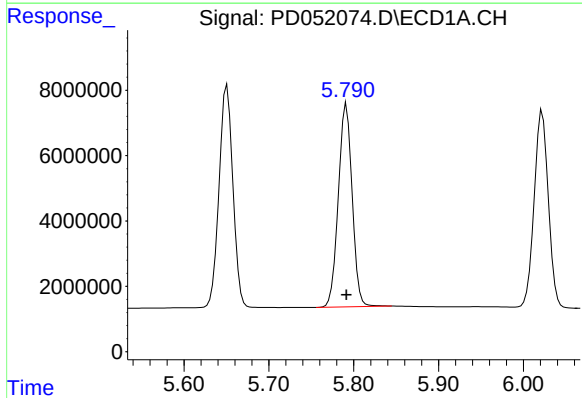


#16 4,4'-DDD

R.T.: 5.792 min
Delta R.T.: 0.000 min
Response: 70185339
Conc: 40.00 ng/ml

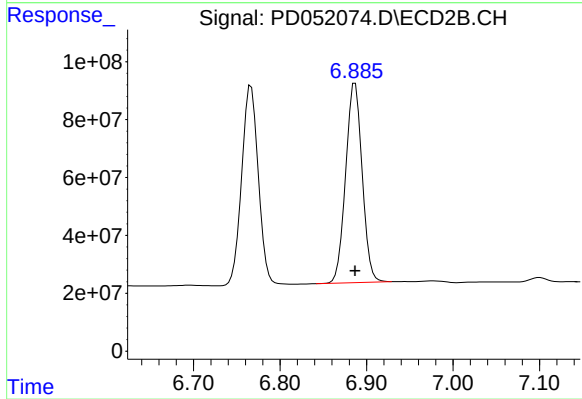

#16 4,4'-DDD


R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 909931765
Conc: 40.00 ng/ml

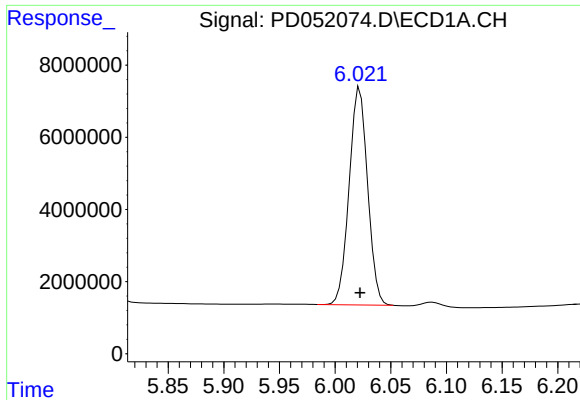

#17 4,4'-DDT


R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 69535865
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

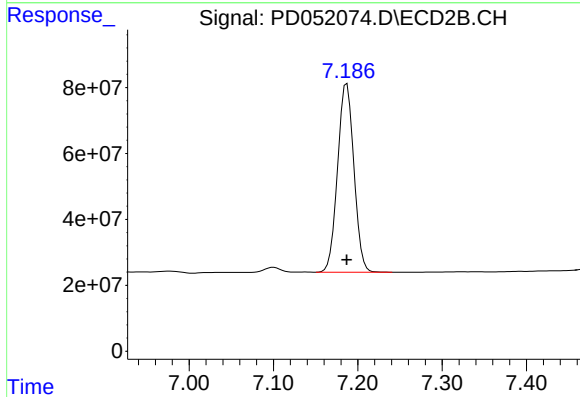


#17 4,4'-DDT

R.T.: 7.187 min
Delta R.T.: 0.000 min
Response: 771078850
Conc: 40.00 ng/ml

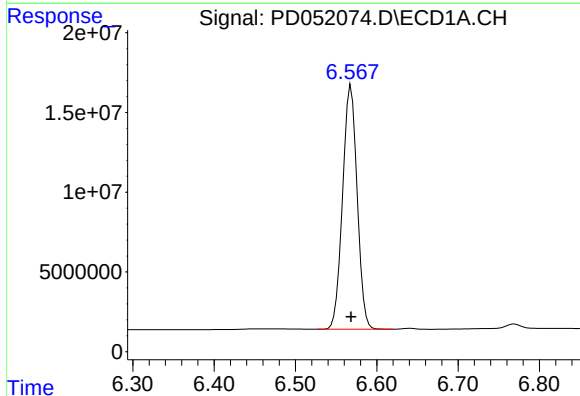


#20 Methoxychlor

R.T.: 6.568 min
Delta R.T.: 0.000 min
Response: 189842836
Conc: 200.00 ng/ml

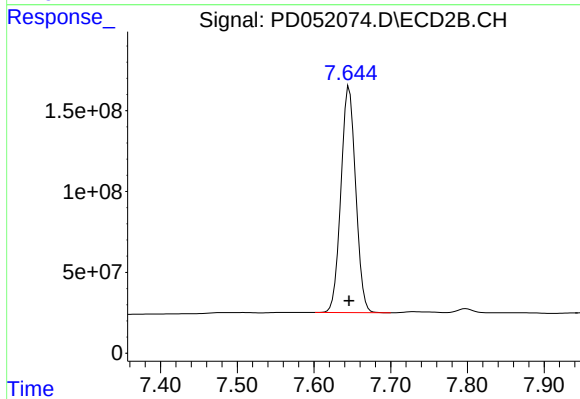

#20 Methoxychlor


R.T.: 7.646 min
Delta R.T.: 0.000 min
Response: 1871783397
Conc: 200.00 ng/ml

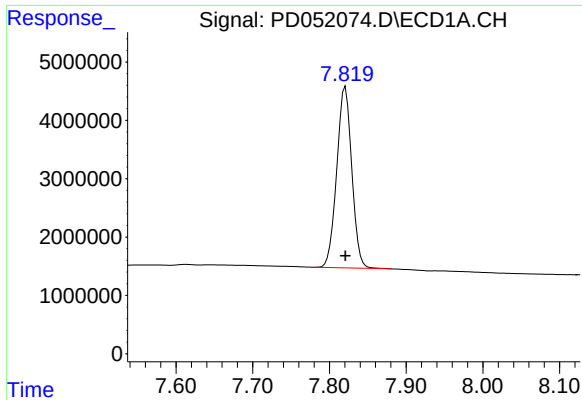

#27 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.000 min
Response: 42289260
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

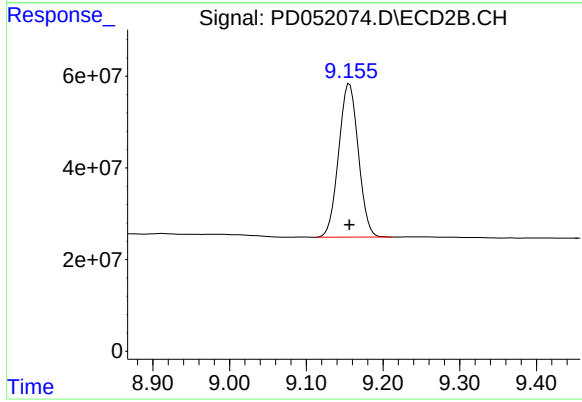

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 598719294
Conc: 40.00 ng/ml