

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052084.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 17:02
 Operator : AJ\SJ
 Sample : K2031-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5Y0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:29:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	29148436	582.5E6	20.732	19.605
27)	SA Decachlor...	7.820	9.157	26931888	408.8E6	25.596	27.739
Target Compounds							
2)	A alpha-BHC	0.000	4.404f	0	20138773	N.D.	0.452
3)	MA gamma-BHC...	3.923	4.719	21214993	293.5E6	9.235	7.290
4)	MA Heptachlor	0.000	5.213	0	70879488	N.D.	1.739
5)	MB Aldrin	4.444f	0.000	13903786	0	6.670	N.D. #
6)	B beta-BHC	4.126f	4.938f	2755907	50579285	2.912	2.746
7)	B delta-BHC	0.000	5.087f	0	806.2E6	N.D.	21.898
8)	B Heptachlo...	0.000	5.912	0	30370490	N.D.	0.911
10)	B trans-Chl...	0.000	6.147	0	187.1E6	N.D.	5.578


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052084.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 17:02
Operator : AJ\SJ
Sample : K2031-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:29:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

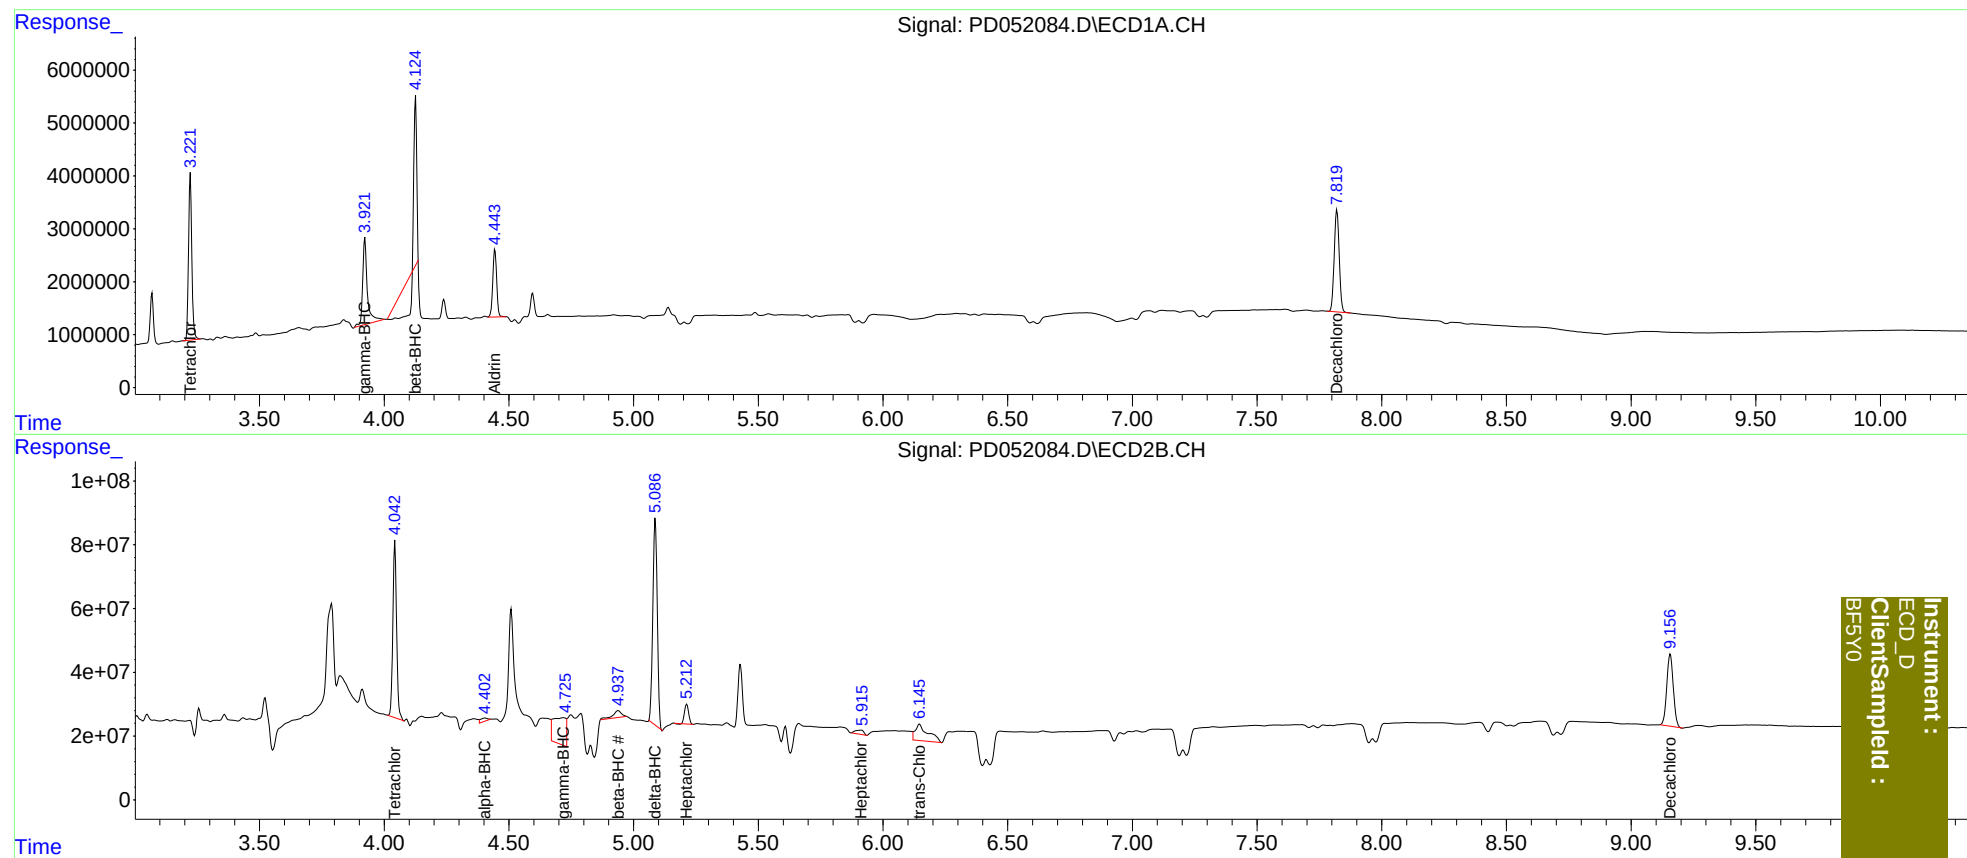


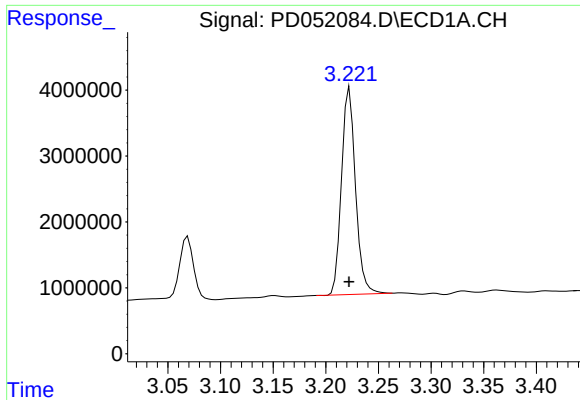

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 29148436
Conc: 20.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5Y0

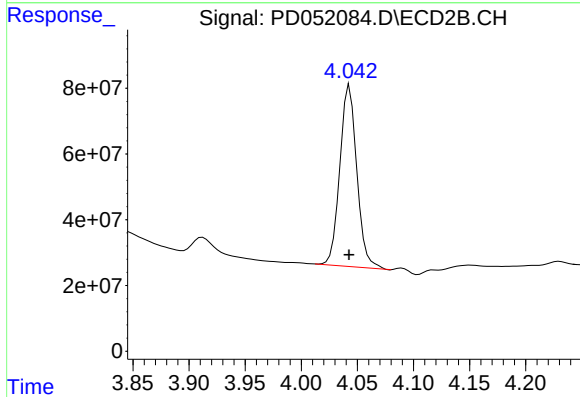


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 582493360
Conc: 19.61 ng/ml

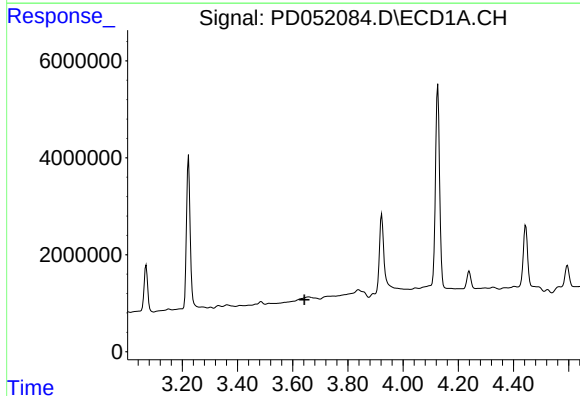


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.642 min
Response: 0
Conc: N.D.

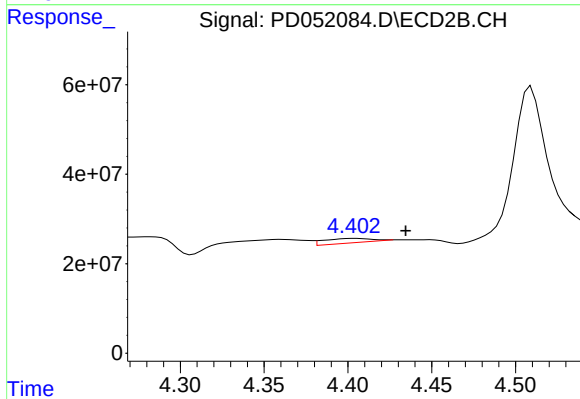

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: -0.030 min
Response: 20138773
Conc: 0.45 ng/ml

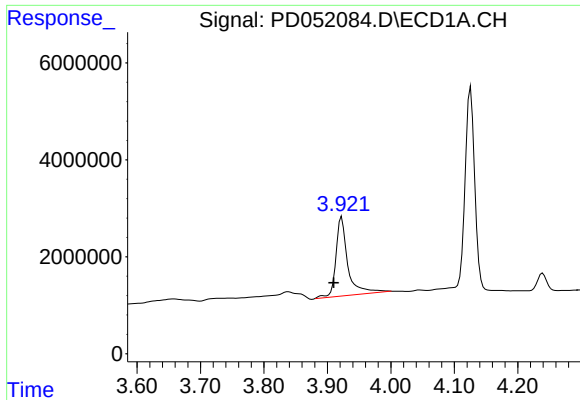

#3 gamma-BHC (Lindane)


R.T.: 3.923 min
Delta R.T.: 0.012 min
Response: 21214993
Conc: 9.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5Y0

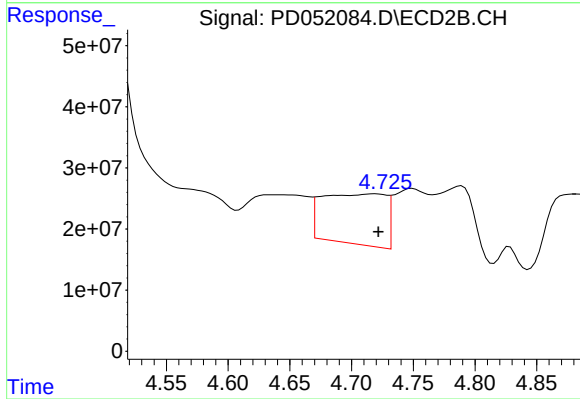


#3 gamma-BHC (Lindane)

R.T.: 4.719 min
Delta R.T.: -0.003 min
Response: 293495898
Conc: 7.29 ng/ml

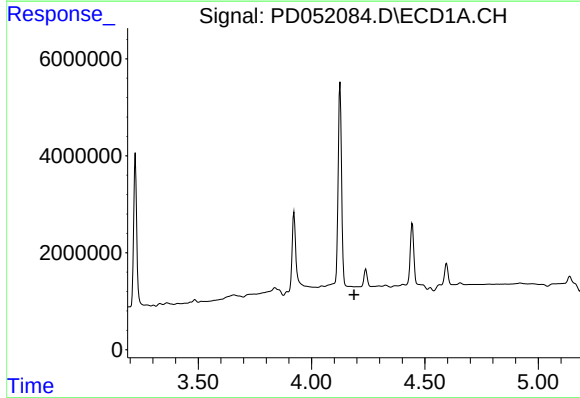


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

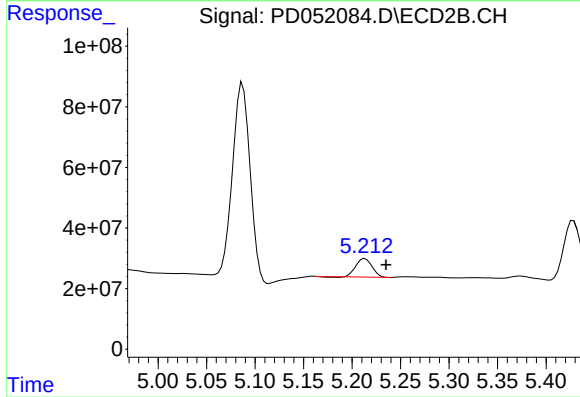

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: -0.022 min
Response: 70879488
Conc: 1.74 ng/ml

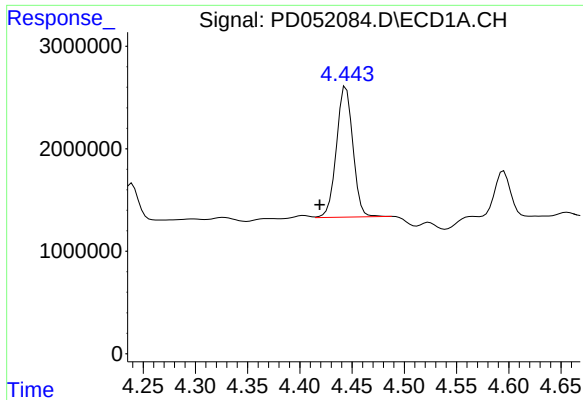

#5 Aldrin


R.T.: 4.444 min
Delta R.T.: 0.025 min
Response: 13903786
Conc: 6.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5Y0

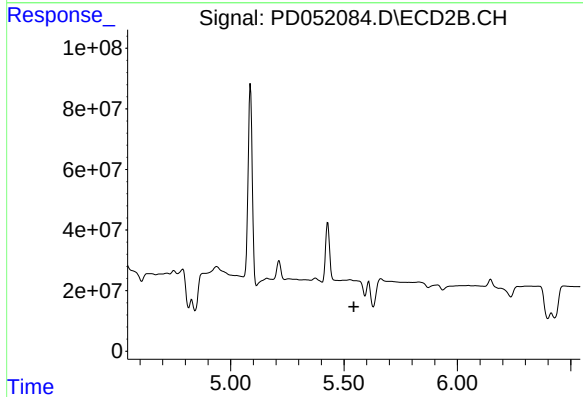


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.543 min
Response: 0
Conc: N.D.

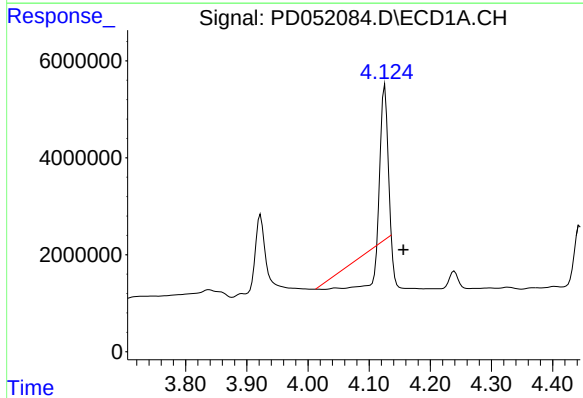


#6 beta-BHC

R.T.: 4.126 min
Delta R.T.: -0.030 min
Response: 2755907
Conc: 2.91 ng/ml

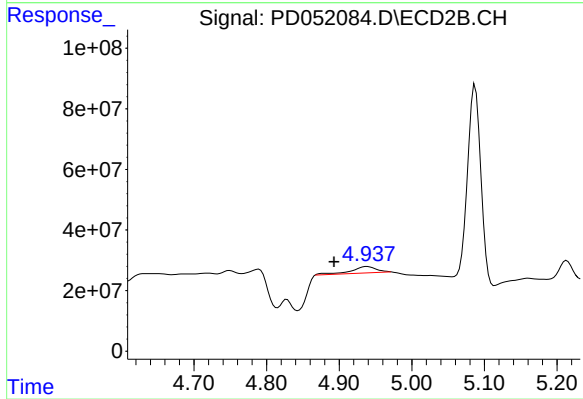

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.045 min
Response: 50579285
Conc: 2.75 ng/ml

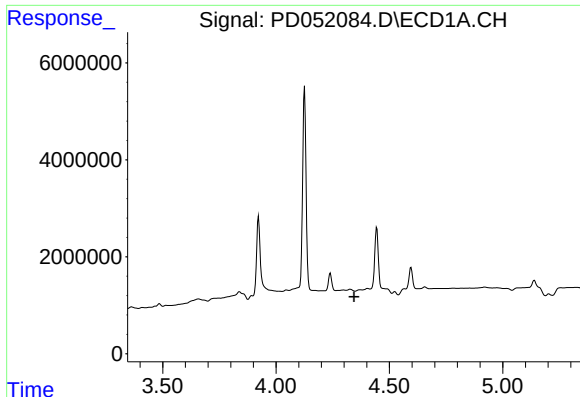

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5Y0

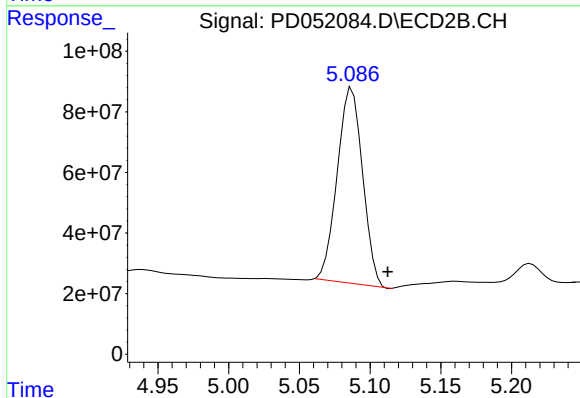


#7 delta-BHC

R.T.: 5.087 min
Delta R.T.: -0.025 min
Response: 806185521
Conc: 21.90 ng/ml

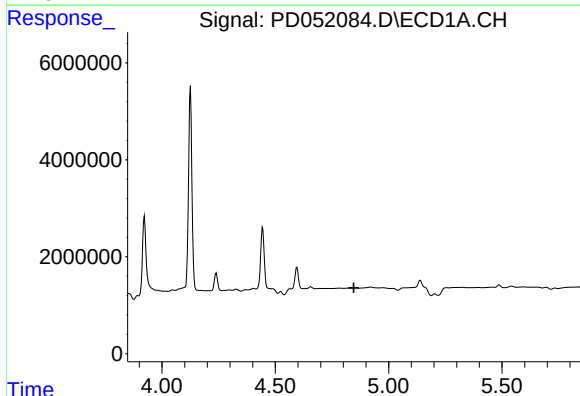


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.847 min
Response: 0
Conc: N.D.

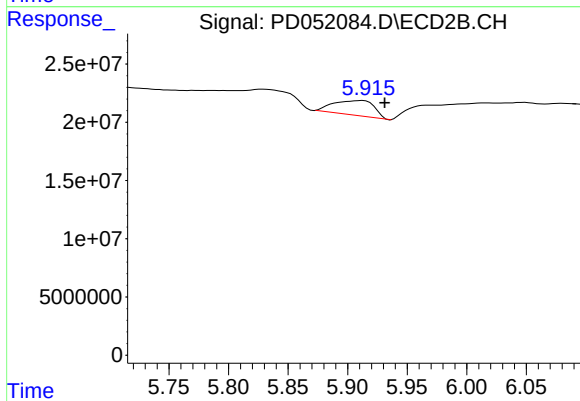

#8 Heptachlor epoxide


R.T.: 5.912 min
Delta R.T.: -0.019 min
Response: 30370490
Conc: 0.91 ng/ml

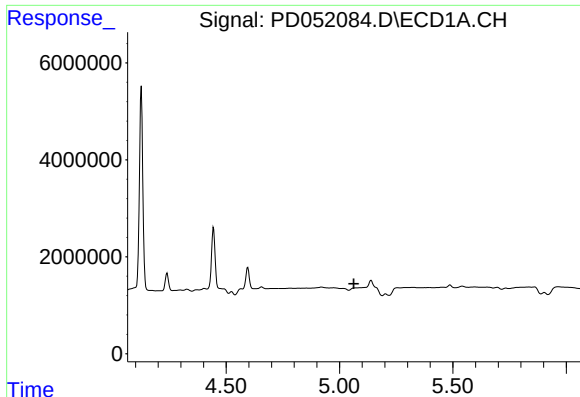

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5Y0

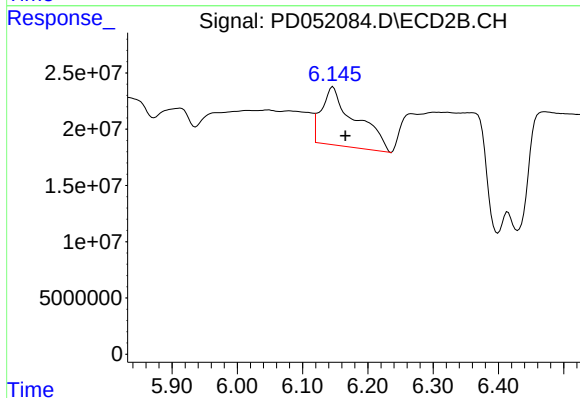


#10 trans-Chlordane

R.T.: 6.147 min
Delta R.T.: -0.019 min
Response: 187067641
Conc: 5.58 ng/ml

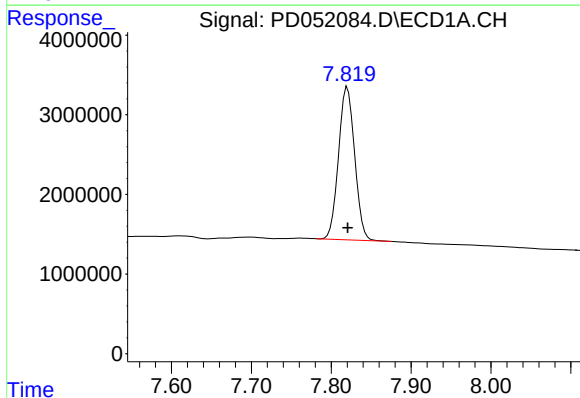

#27 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: 0.000 min
Response: 26931888
Conc: 25.60 ng/ml

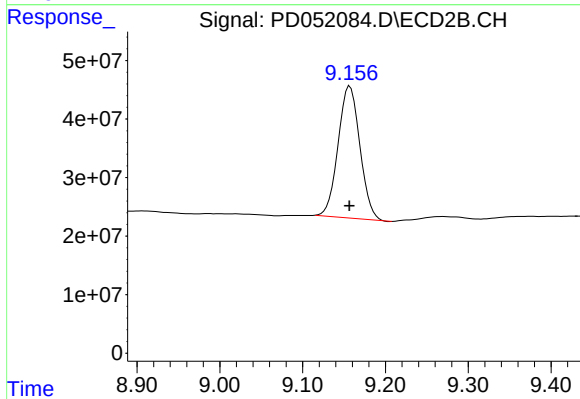

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 408822785
Conc: 27.74 ng/ml