

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 18:55
 Operator : AJ\SJ
 Sample : K2065-19
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5L8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:31:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	18143607	391.4E6	12.905	13.172
27)	SA Decachlor...	7.821	9.156	22424095	335.4E6	21.312	22.759
Target Compounds							
2)	A alpha-BHC	0.000	4.406f	0	27629765	N.D.	0.621
6)	B beta-BHC	0.000	4.940f	0	38175078	N.D.	2.073
7)	B delta-BHC	0.000	5.083f	0	50393633	N.D.	1.369
8)	B Heptachlo...	0.000	5.911	0	47285913	N.D.	1.419
10)	B trans-Chl...	0.000	6.160	0	29485810	N.D.	0.879
15)	B Endosulfa...	0.000	6.960	0	22524369	N.D.	0.954

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 18:55
Operator : AJ\SJ
Sample : K2065-19
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:31:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

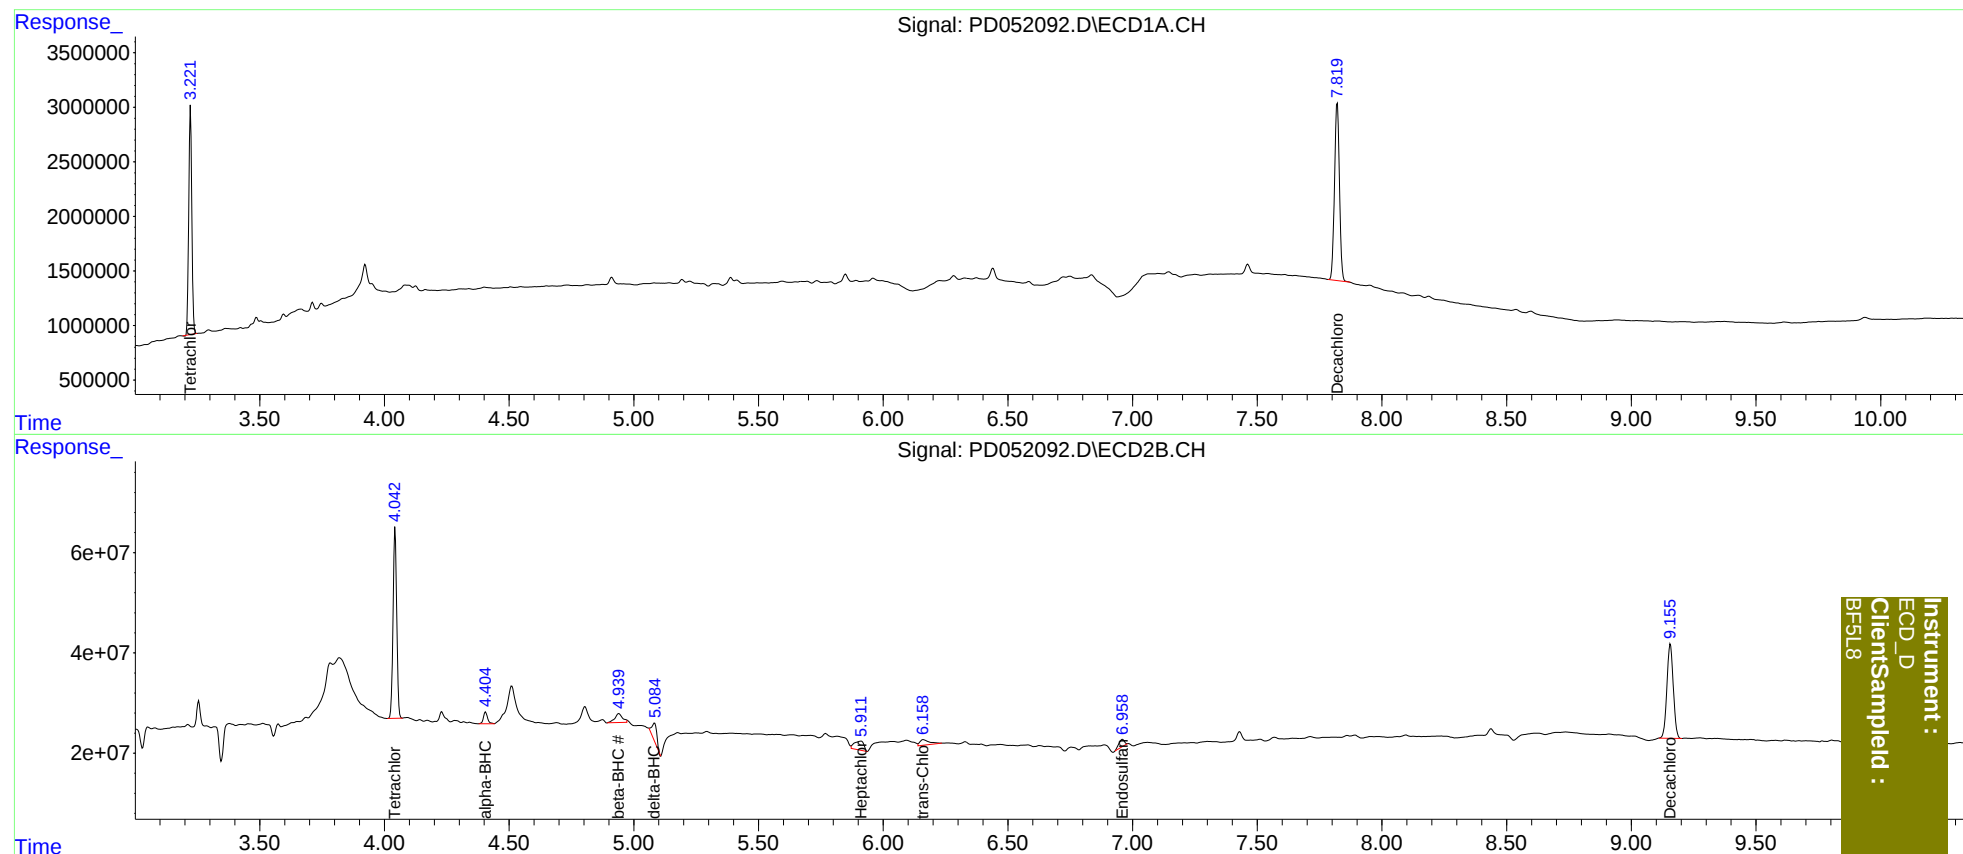


Instrument :
ECD_D
ClientSampleId :
BF5L8

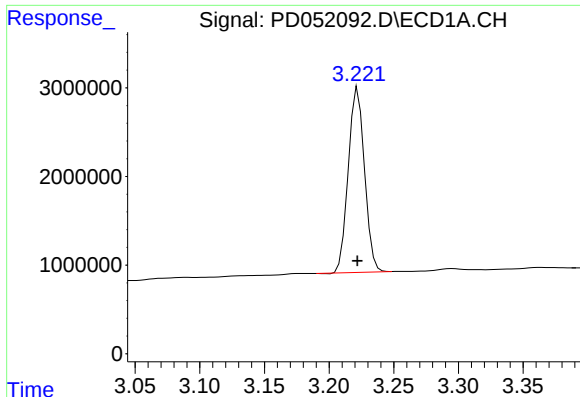

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 18143607
Conc: 12.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L8

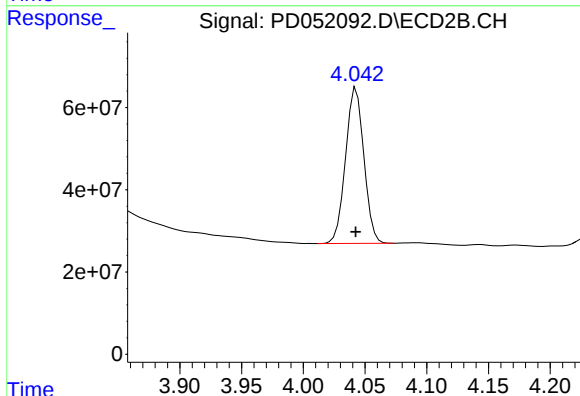


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 391366719
Conc: 13.17 ng/ml

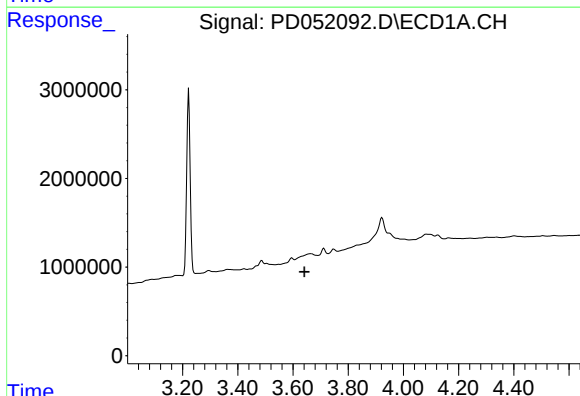


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.642 min
Response: 0
Conc: N.D.

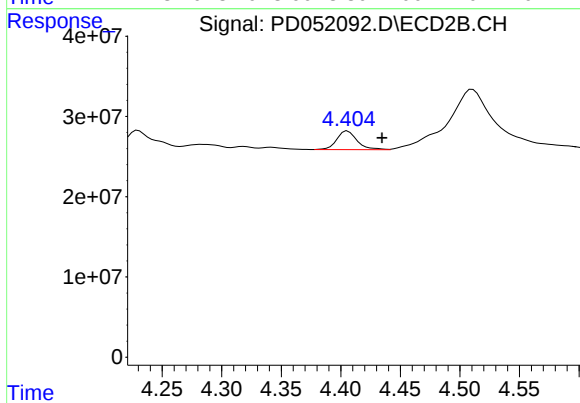

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: -0.029 min
Response: 27629765
Conc: 0.62 ng/ml

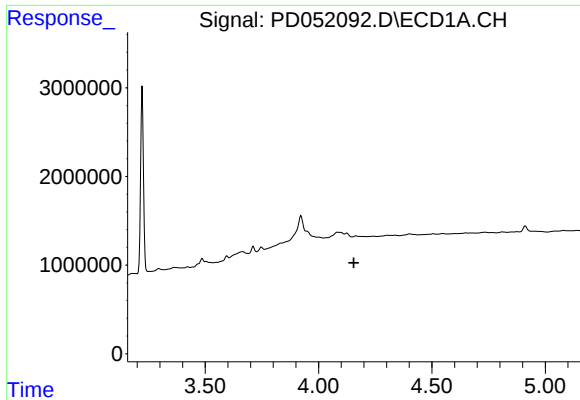

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.156 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L8

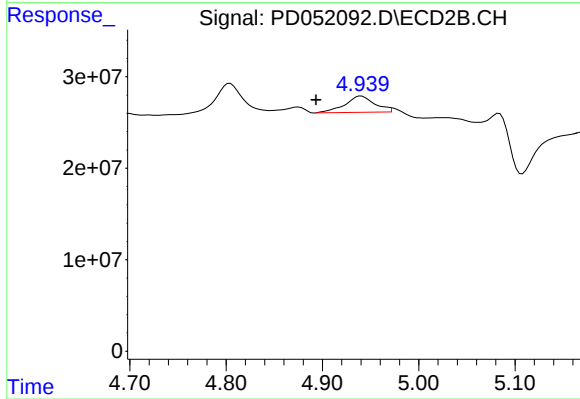


#6 beta-BHC

R.T.: 4.940 min
Delta R.T.: 0.047 min
Response: 38175078
Conc: 2.07 ng/ml

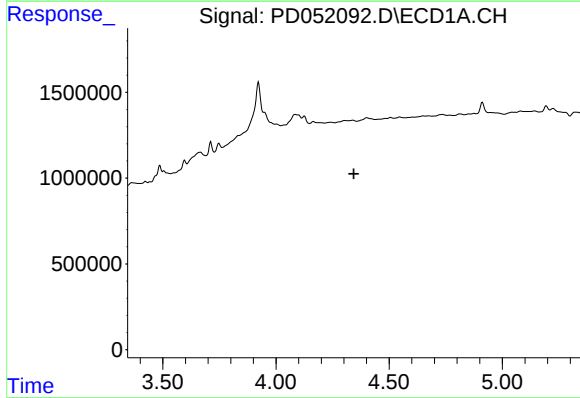


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.344 min
Response: 0
Conc: N.D.

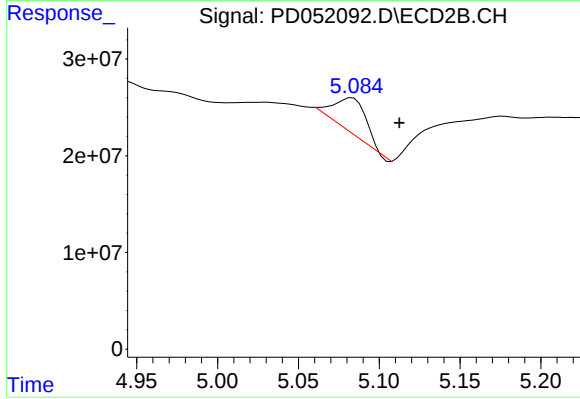

#7 delta-BHC


R.T.: 5.083 min
Delta R.T.: -0.029 min
Response: 50393633
Conc: 1.37 ng/ml

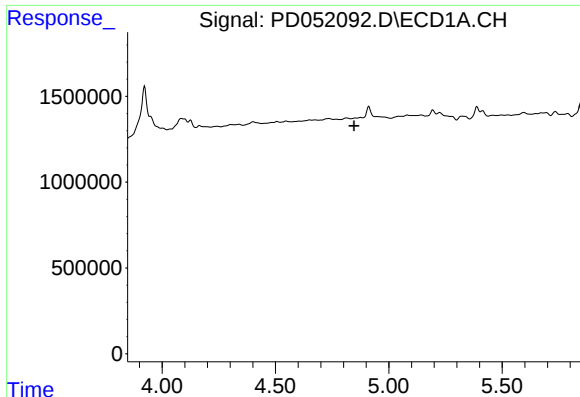

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L8

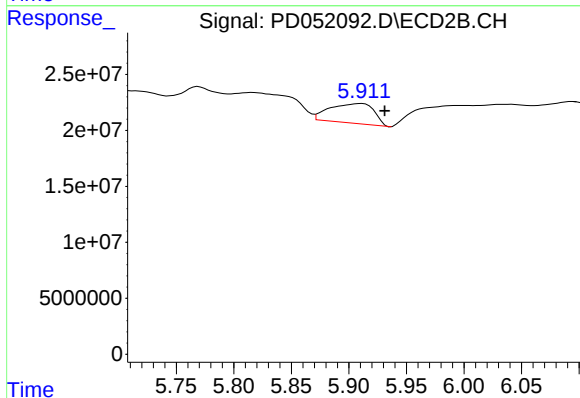


#8 Heptachlor epoxide

R.T.: 5.911 min
Delta R.T.: -0.020 min
Response: 47285913
Conc: 1.42 ng/ml

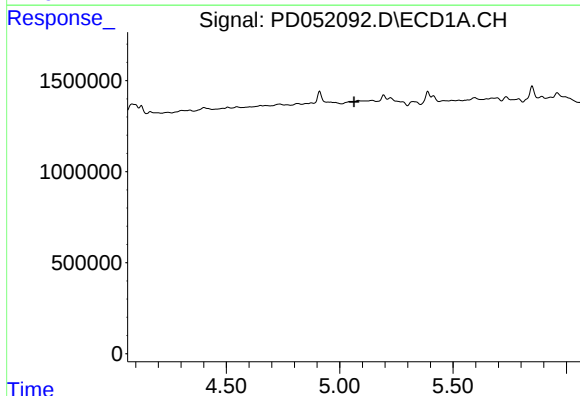


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

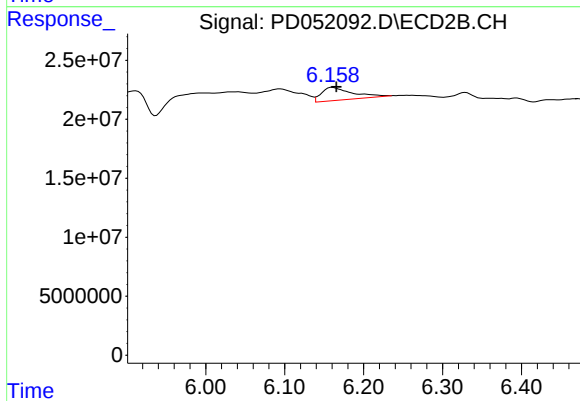

#10 trans-Chlordane


R.T.: 6.160 min
Delta R.T.: -0.005 min
Response: 29485810
Conc: 0.88 ng/ml

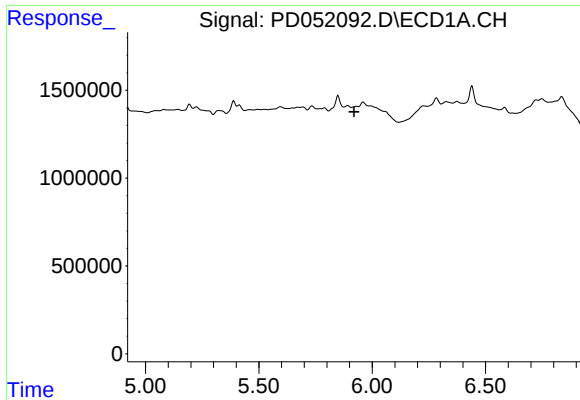

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L8

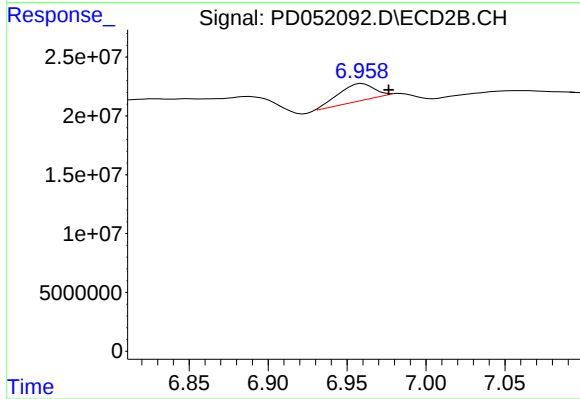


#15 Endosulfan II

R.T.: 6.960 min
Delta R.T.: -0.017 min
Response: 22524369
Conc: 0.95 ng/ml

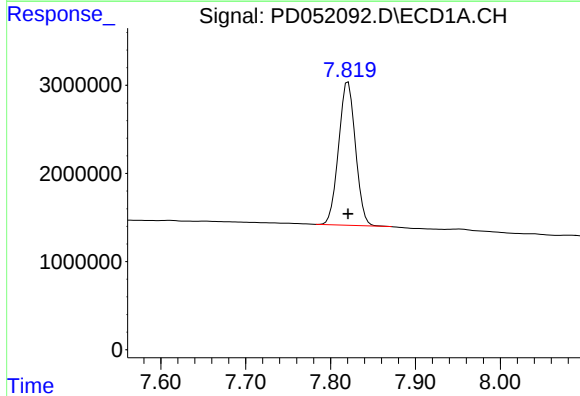

#27 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.000 min
Response: 22424095
Conc: 21.31 ng/ml

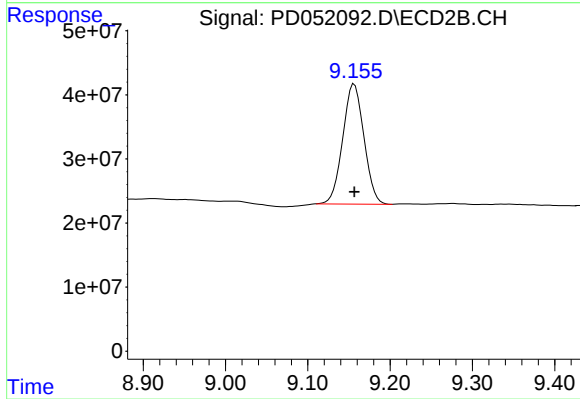

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 335423986
Conc: 22.76 ng/ml