

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052093.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 19:09
 Operator : AJ\SJ
 Sample : K2065-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:31:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	19136658	403.3E6	13.611	13.575
27)	SA Decachlor...	7.819	9.157	27191677	397.3E6	25.843	26.957
Target Compounds							
2)	A alpha-BHC	0.000	4.408f	0	28409246	N.D.	0.638
3)	MA gamma-BHC...	3.921	0.000	4997878	0	2.176	N.D. #
6)	B beta-BHC	0.000	4.937f	0	48344322	N.D.	2.625
7)	B delta-BHC	0.000	5.083f	0	58900253	N.D.	1.600
8)	B Heptachlo...	0.000	5.911	0	71066456	N.D.	2.132
9)	A Endosulfan I	0.000	6.241f	0	15868569	N.D.	0.513
10)	B trans-Chl...	0.000	6.165	0	50552723	N.D.	1.507
11)	B cis-Chlor...	0.000	6.241	0	15868569	N.D.	0.495
15)	B Endosulfa...	0.000	6.985	0	22160816	N.D.	0.938
17)	MA 4,4'-DDT	0.000	7.232f	0	6838779	N.D.	0.368
25)	Toxaphene-4	0.000	7.232	0	6838779	N.D.	12.940


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052093.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 19:09
Operator : AJ\SJ
Sample : K2065-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:31:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

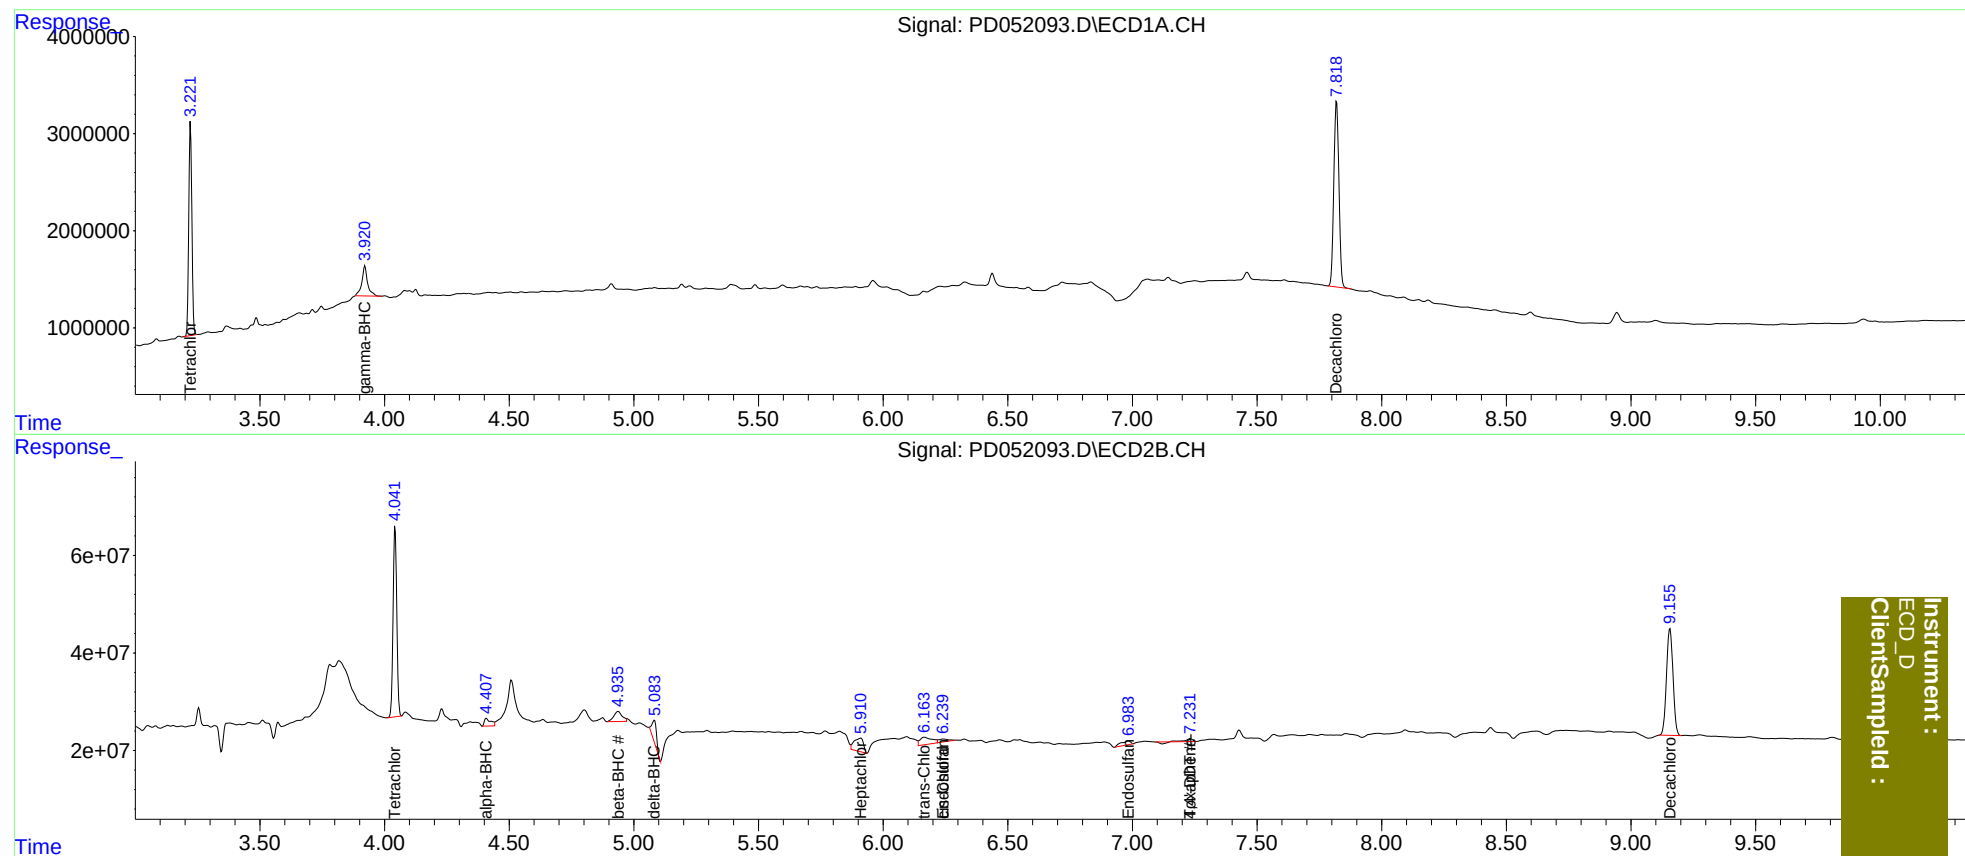


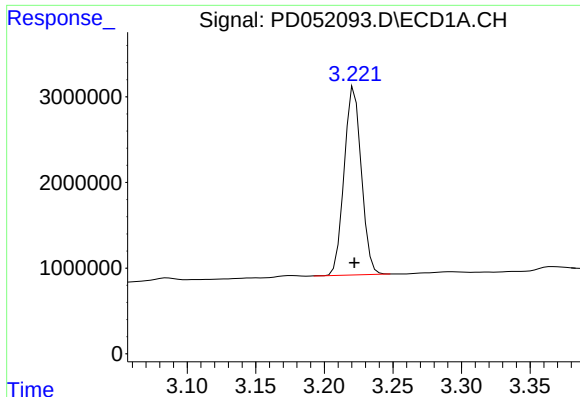

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 19136658
Conc: 13.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

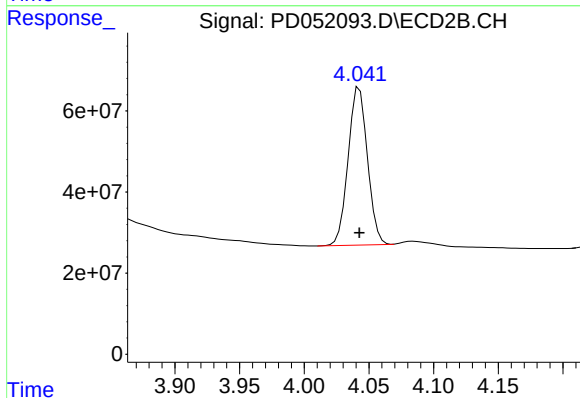


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 403323355
Conc: 13.57 ng/ml

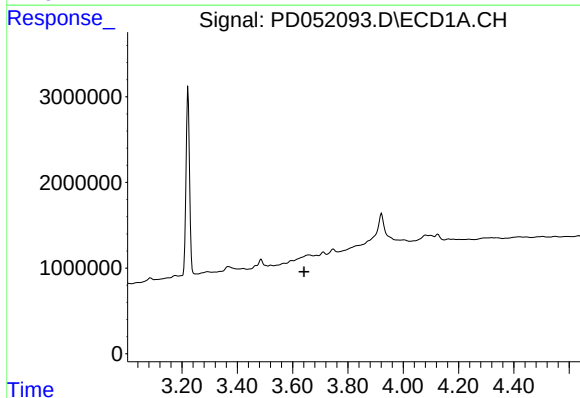


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.642 min
Response: 0
Conc: N.D.

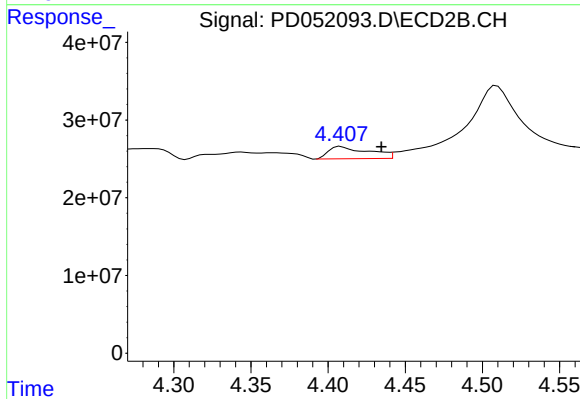

#2 alpha-BHC

R.T.: 4.408 min
Delta R.T.: -0.026 min
Response: 28409246
Conc: 0.64 ng/ml

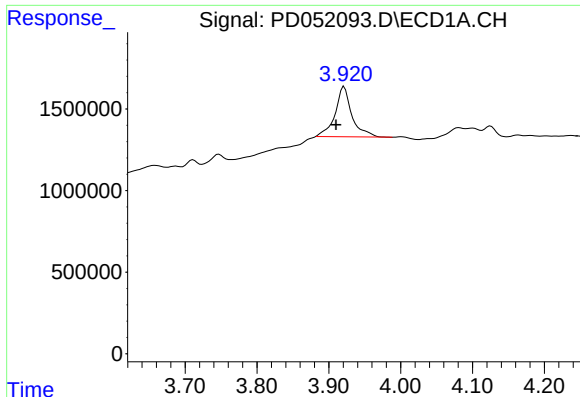

#3 gamma-BHC (Lindane)


R.T.: 3.921 min

Delta R.T.: 0.011 min

Response: 4997878

Conc: 2.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

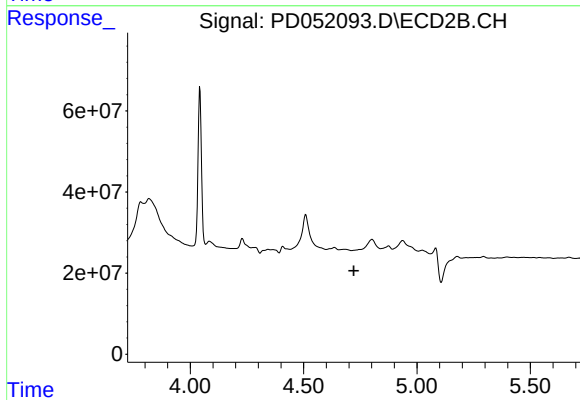


#3 gamma-BHC (Lindane)

R.T.: 0.000 min

Exp R.T. : 4.722 min

Response: 0

Conc: N.D.

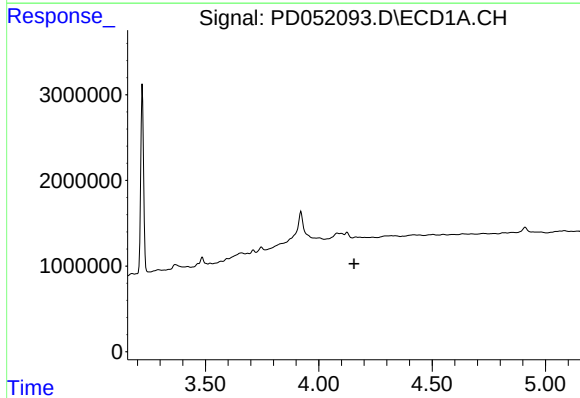


#6 beta-BHC

R.T.: 0.000 min

Exp R.T. : 4.156 min

Response: 0

Conc: N.D.

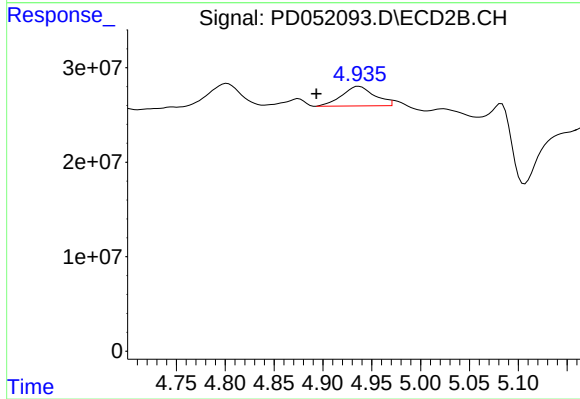


#6 beta-BHC

R.T.: 4.937 min

Delta R.T.: 0.044 min

Response: 48344322


Conc: 2.62 ng/ml

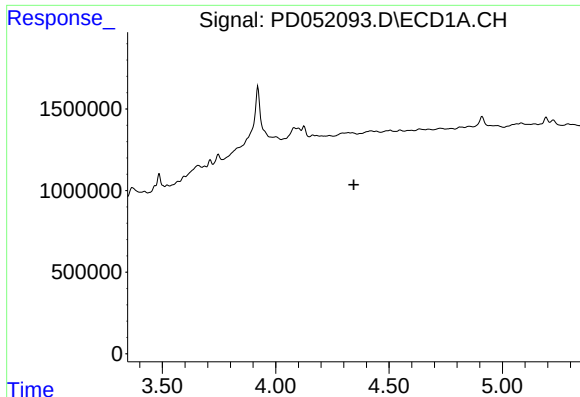

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

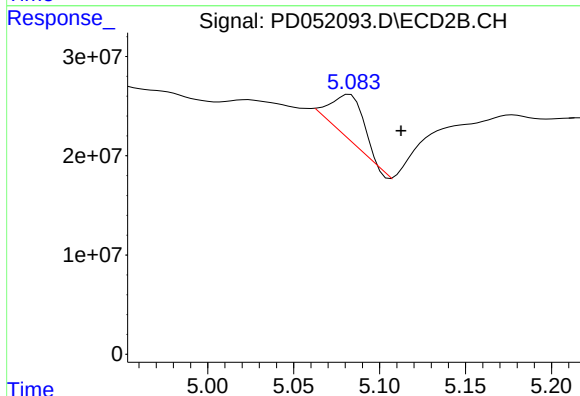


#7 delta-BHC

R.T.: 5.083 min
Delta R.T.: -0.030 min
Response: 58900253
Conc: 1.60 ng/ml

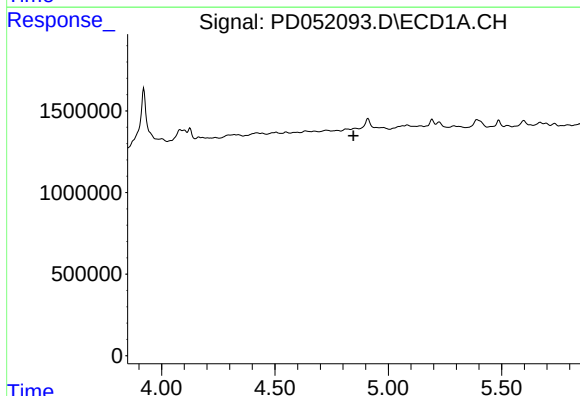


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.847 min
Response: 0
Conc: N.D.

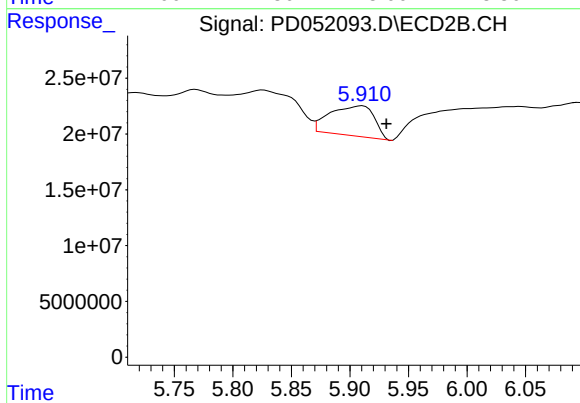

#8 Heptachlor epoxide


R.T.: 5.911 min
Delta R.T.: -0.020 min
Response: 71066456
Conc: 2.13 ng/ml

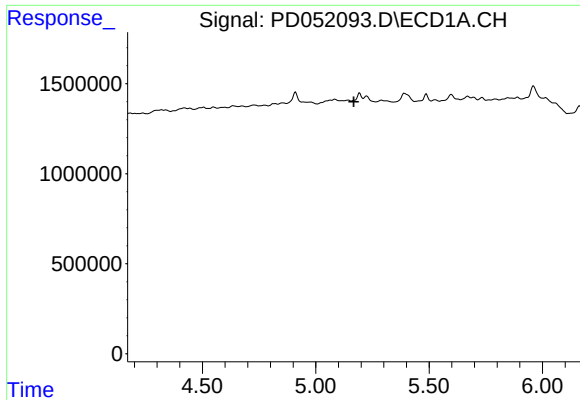

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

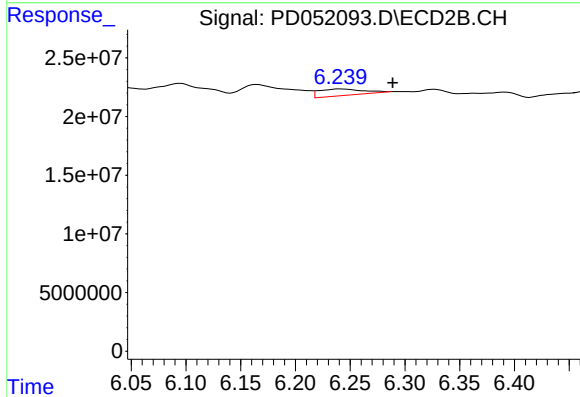


#9 Endosulfan I

R.T.: 6.241 min
Delta R.T.: -0.048 min
Response: 15868569
Conc: 0.51 ng/ml

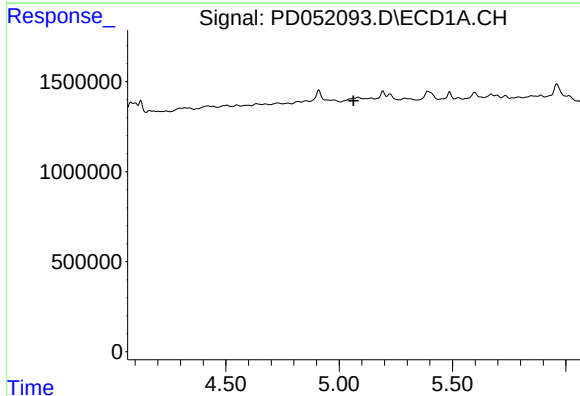


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

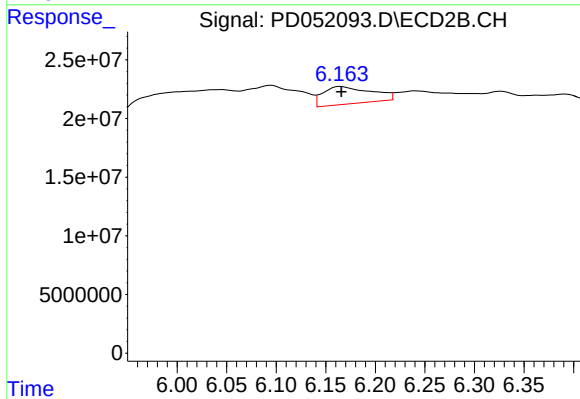

#10 trans-Chlordane


R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 50552723
Conc: 1.51 ng/ml

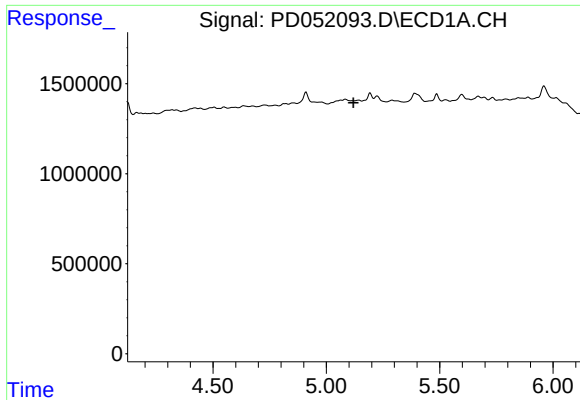

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.120 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

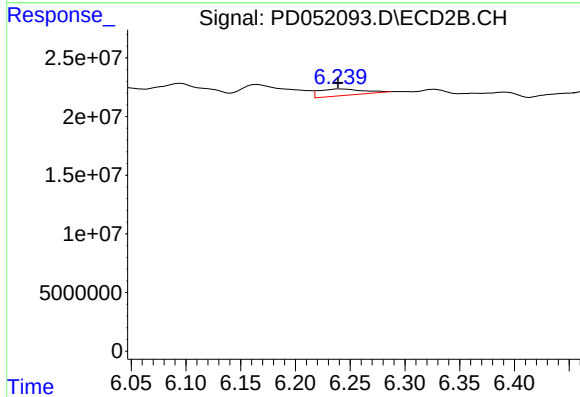


#11 cis-Chlordane

R.T.: 6.241 min
Delta R.T.: 0.002 min
Response: 15868569
Conc: 0.49 ng/ml

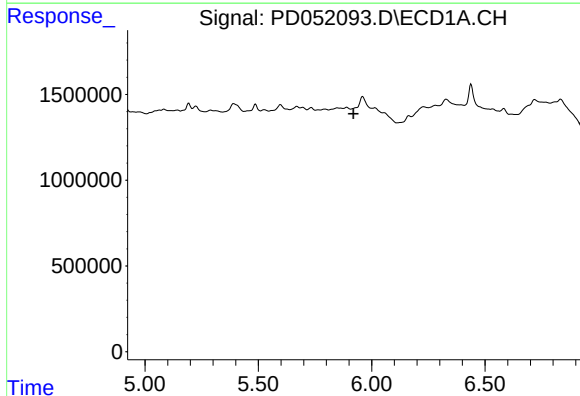


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

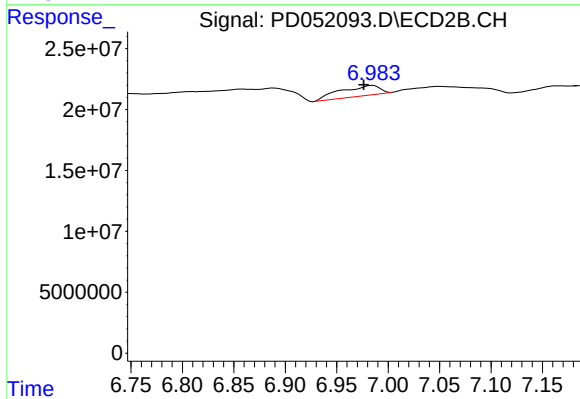

#15 Endosulfan II


R.T.: 6.985 min
Delta R.T.: 0.009 min
Response: 22160816
Conc: 0.94 ng/ml

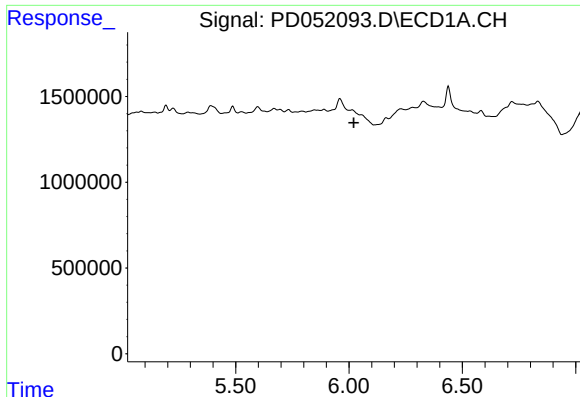

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

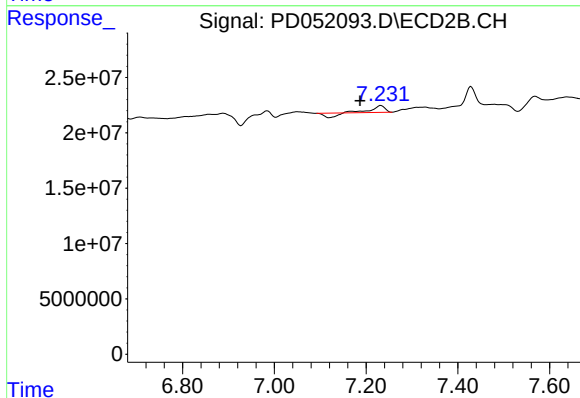


#17 4,4'-DDT

R.T.: 7.232 min
Delta R.T.: 0.045 min
Response: 6838779
Conc: 0.37 ng/ml

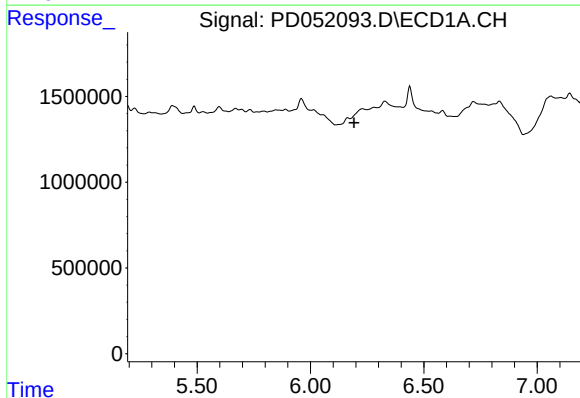


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 6.192 min
Response: 0
Conc: N.D.

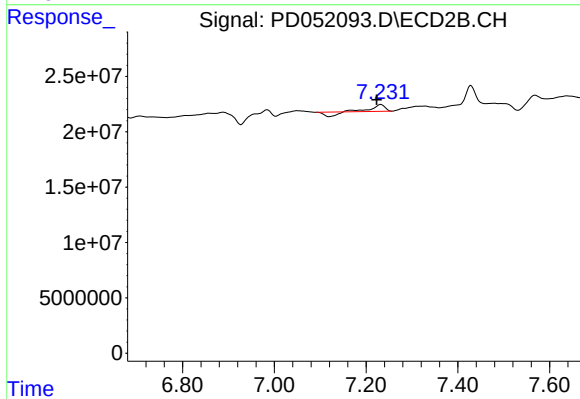

#25 Toxaphene-4


R.T.: 7.232 min
Delta R.T.: 0.009 min
Response: 6838779
Conc: 12.94 ng/ml

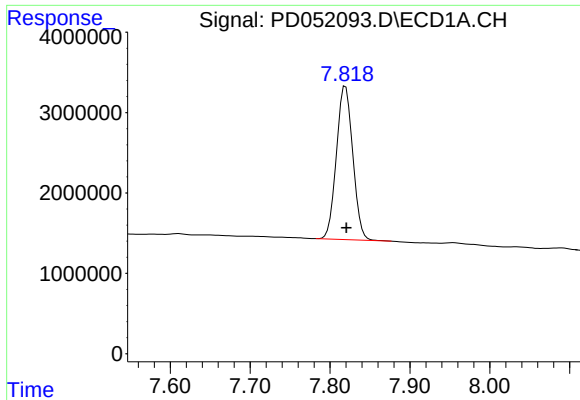

#27 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: -0.001 min
Response: 27191677
Conc: 25.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

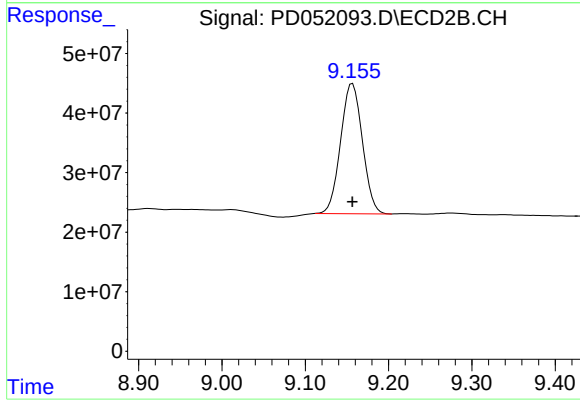

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 397294045
Conc: 26.96 ng/ml