

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052096.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 19:52
 Operator : AJ\SJ
 Sample : K2065-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5L4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:31:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	22351990	465.9E6	15.898	15.681
27)	SA Decachlor...	7.821	9.156	28908417	465.5E6	27.474	31.582
Target Compounds							
2)	A alpha-BHC	0.000	4.406f	0 45240575	N.D.	1.016	
3)	MA gamma-BHC...	3.922	0.000	9148265	0 3.982	N.D.	#
6)	B beta-BHC	0.000	4.938f	0 35579895	N.D.	1.932	
8)	B Heptachlo...	0.000	5.911	0 52647687	N.D.	1.579	
9)	A Endosulfan I	0.000	6.257	0 36429038	N.D.	1.177	
10)	B trans-Chl...	0.000	6.181	0 35057108	N.D.	1.045	
11)	B cis-Chlor...	0.000	6.257	0 36429038	N.D.	1.136	
15)	B Endosulfa...	0.000	6.942	0 6928301	N.D.	0.293	
16)	A 4,4'-DDD	0.000	6.942f	0 6928301	N.D.	0.310	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052096.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 19:52
Operator : AJ\SJ
Sample : K2065-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:31:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

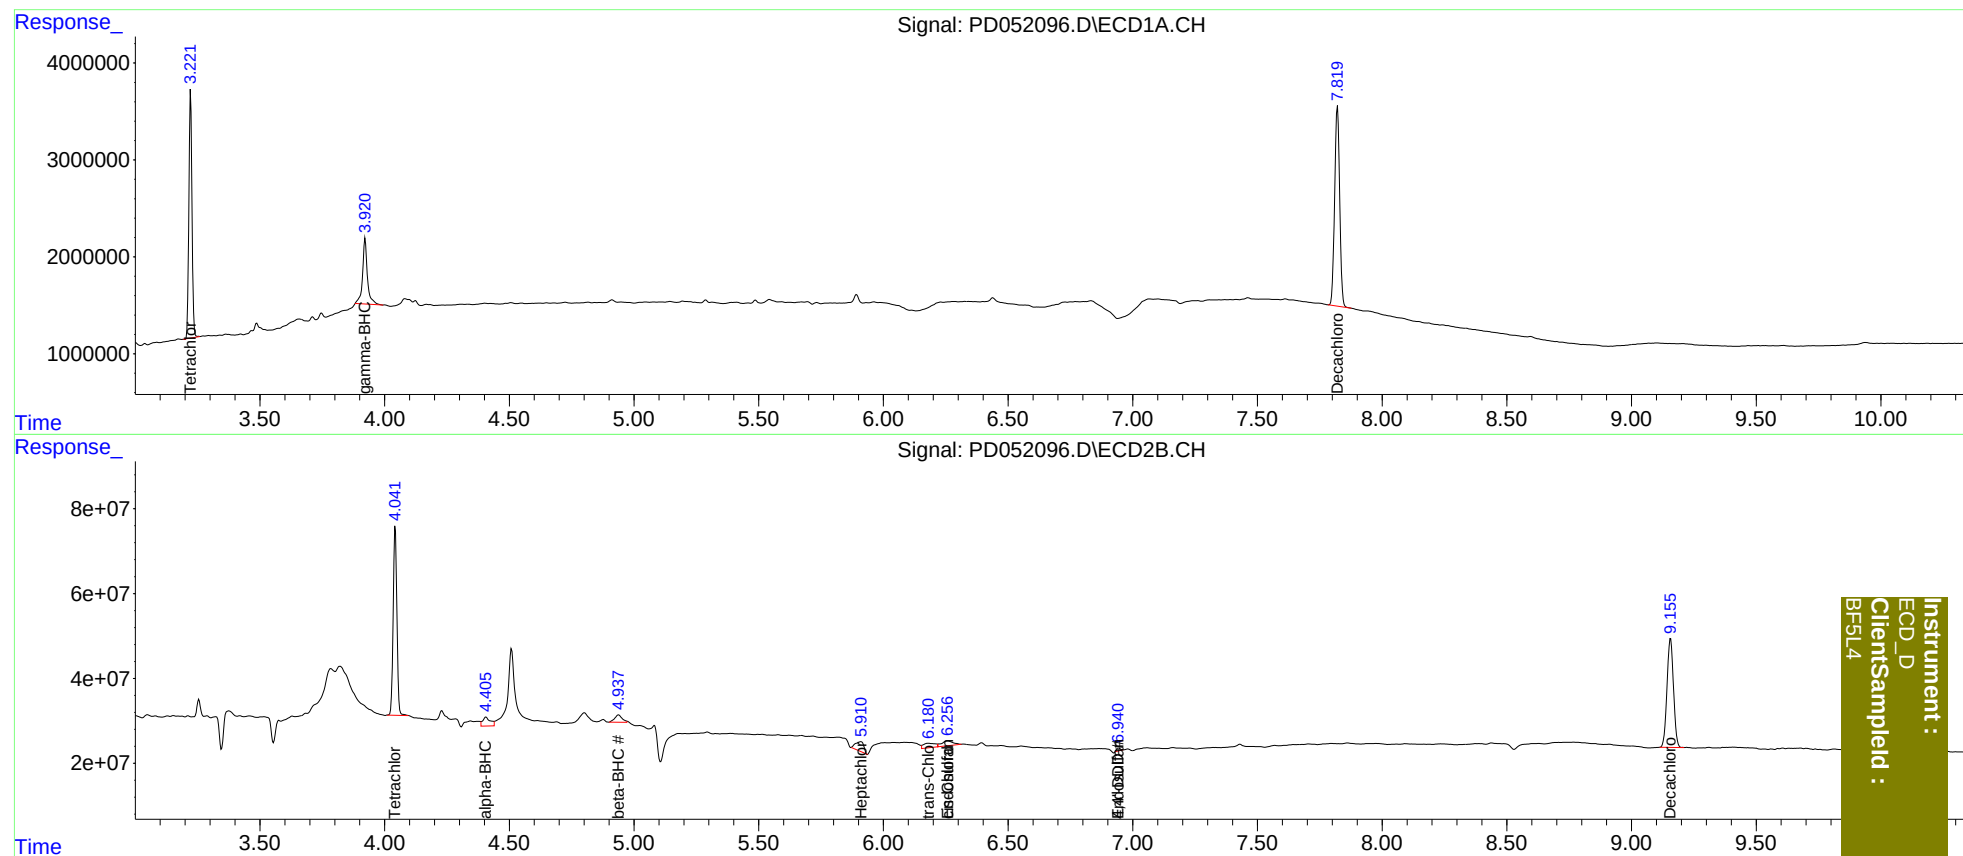


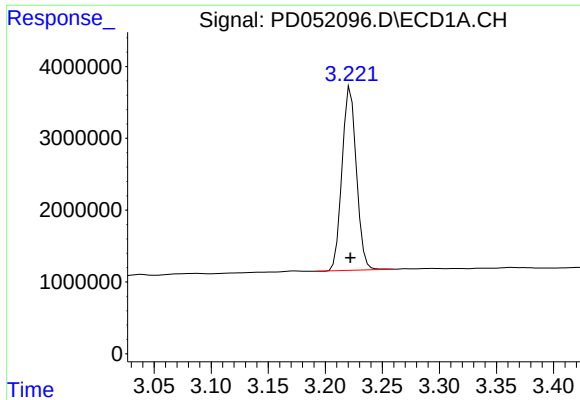

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 22351990
Conc: 15.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L4

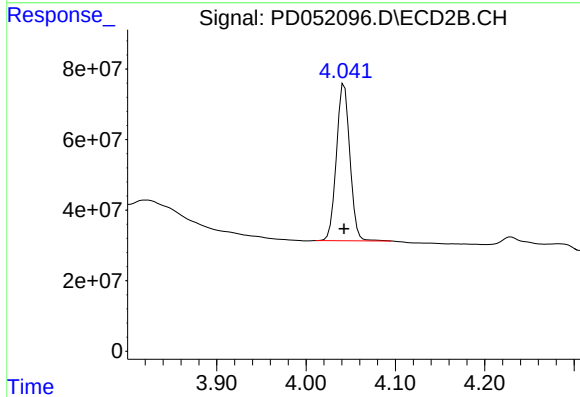


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 465910247
Conc: 15.68 ng/ml

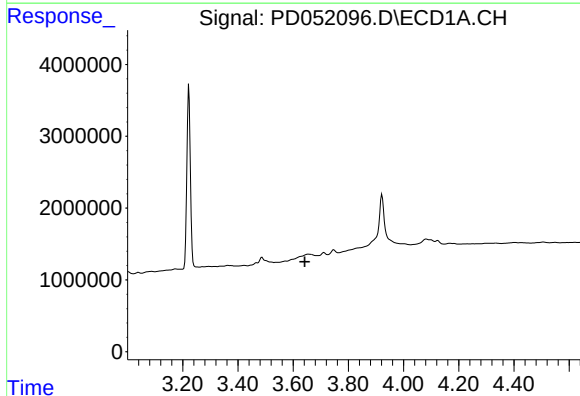


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.642 min
Response: 0
Conc: N.D.

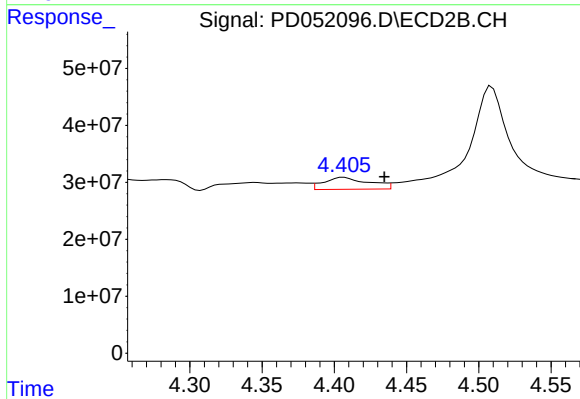

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: -0.028 min
Response: 45240575
Conc: 1.02 ng/ml

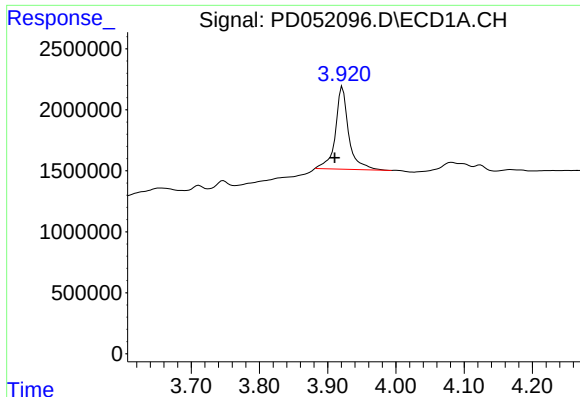

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.012 min
Response: 9148265
Conc: 3.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L4

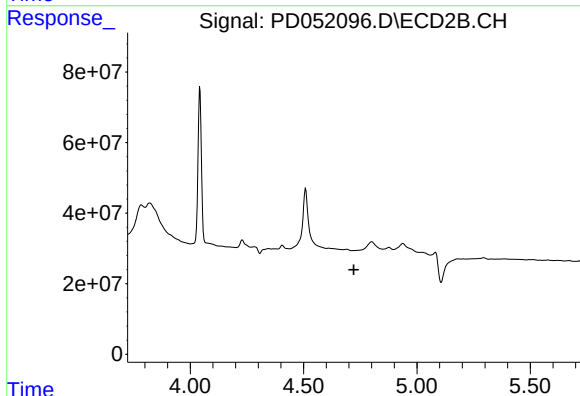


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

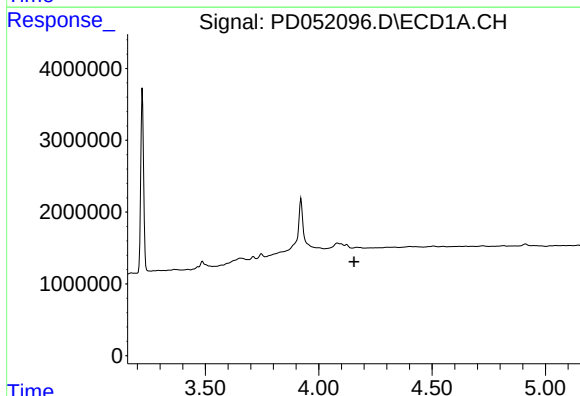


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.156 min
Response: 0
Conc: N.D.

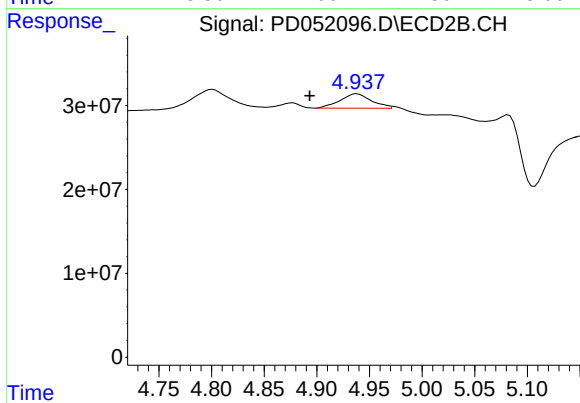

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.045 min
Response: 35579895
Conc: 1.93 ng/ml

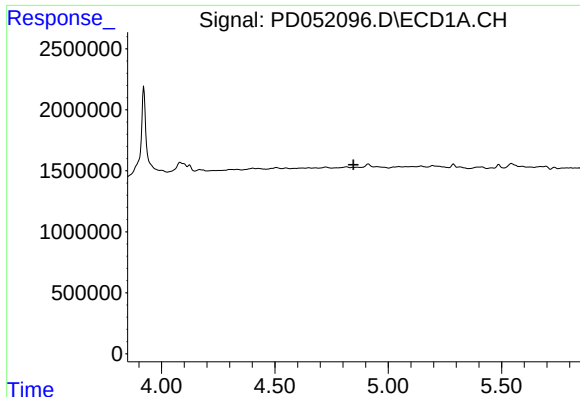

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L4

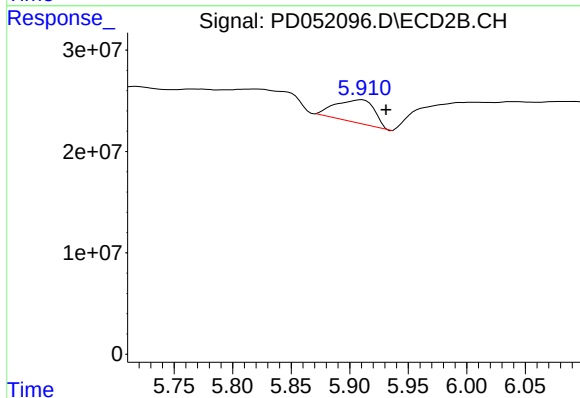


#8 Heptachlor epoxide

R.T.: 5.911 min
Delta R.T.: -0.020 min
Response: 52647687
Conc: 1.58 ng/ml

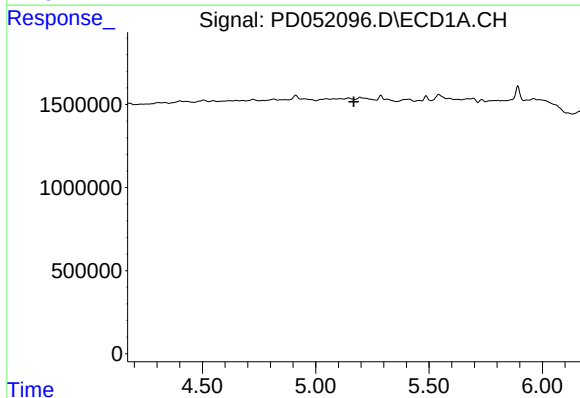


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

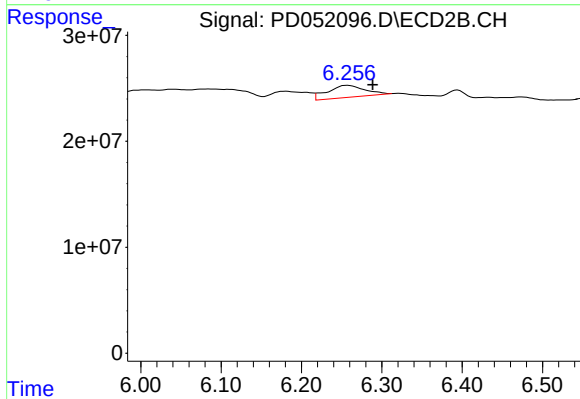

#9 Endosulfan I


R.T.: 6.257 min
Delta R.T.: -0.031 min
Response: 36429038
Conc: 1.18 ng/ml

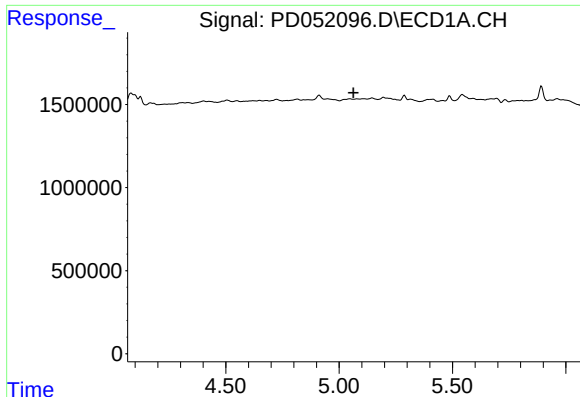

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L4

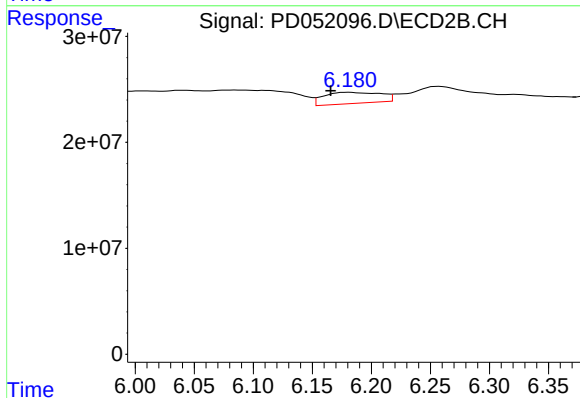


#10 trans-Chlordane

R.T.: 6.181 min
Delta R.T.: 0.015 min
Response: 35057108
Conc: 1.05 ng/ml

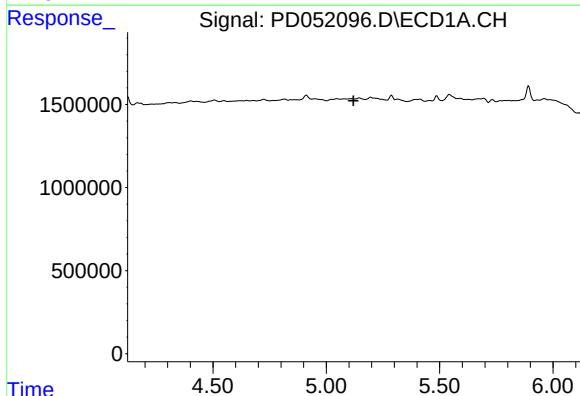


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.120 min
Response: 0
Conc: N.D.

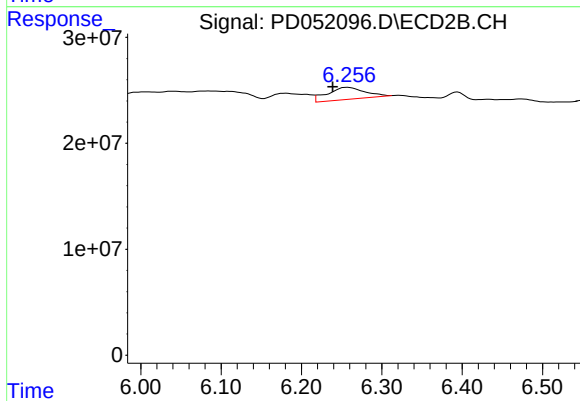

#11 cis-Chlordane


R.T.: 6.257 min
Delta R.T.: 0.018 min
Response: 36429038
Conc: 1.14 ng/ml

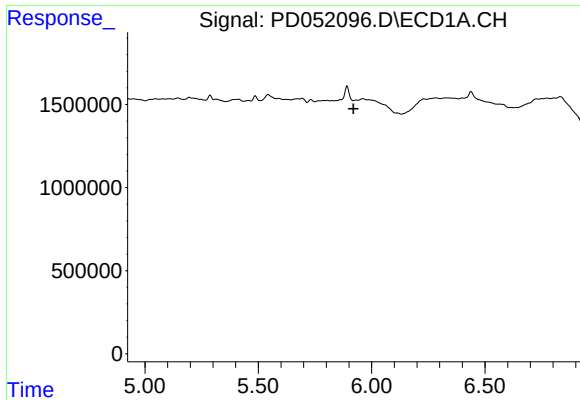

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L4

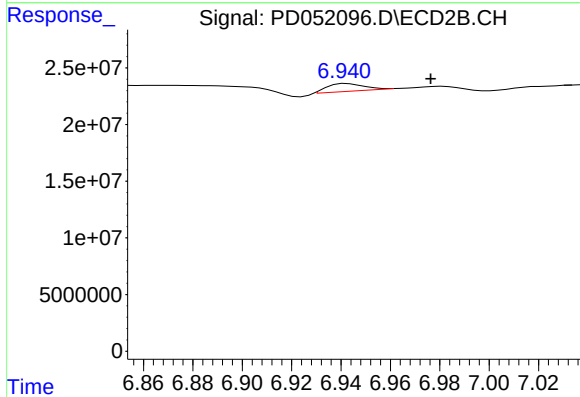


#15 Endosulfan II

R.T.: 6.942 min
Delta R.T.: -0.034 min
Response: 6928301
Conc: 0.29 ng/ml

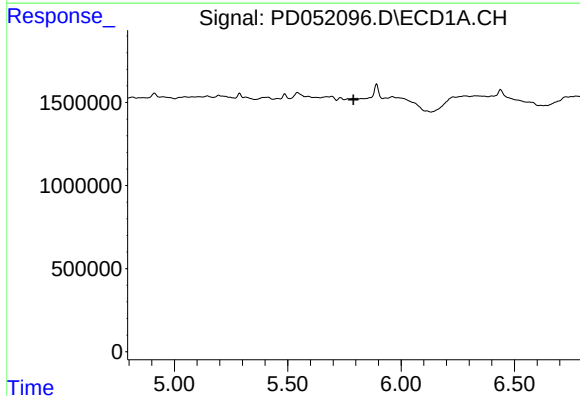


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.790 min
Response: 0
Conc: N.D.

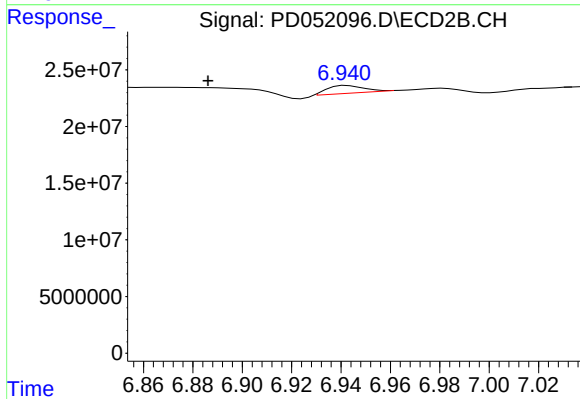

#16 4,4'-DDD


R.T.: 6.942 min
Delta R.T.: 0.056 min
Response: 6928301
Conc: 0.31 ng/ml

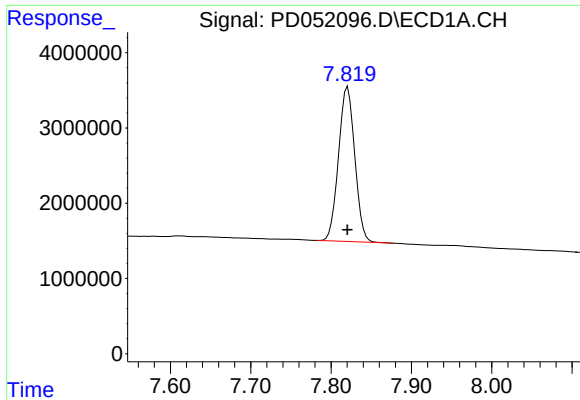

#27 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.000 min
Response: 28908417
Conc: 27.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L4

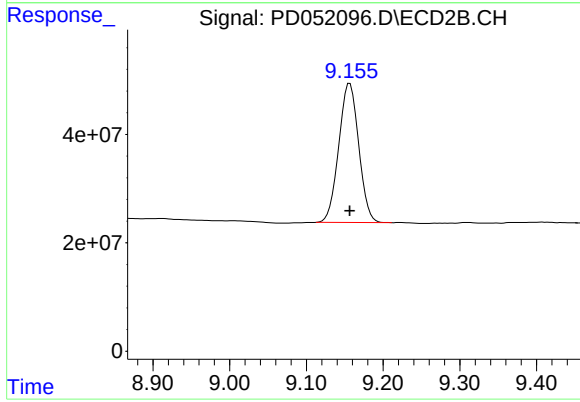

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 465458919
Conc: 31.58 ng/ml