

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052100.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2019 20:49
 Operator : AJ\SJ
 Sample : K2044-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5W6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:32:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.043	21438586	468.0E6	15.248	15.751
27)	SA Decachlor...	7.821	9.156	25628944	408.5E6	24.357	27.719
Target Compounds							
2)	A alpha-BHC	0.000	4.406f	0	47388384	N.D.	1.064
3)	MA gamma-BHC...	3.922	0.000	14273796	0	6.214	N.D. #
6)	B beta-BHC	0.000	4.938f	0	6219954	N.D.	0.338
7)	B delta-BHC	0.000	5.082f	0	57511477	N.D.	1.562
8)	B Heptachlo...	0.000	5.910	0	50386772	N.D.	1.512
10)	B trans-Chl...	0.000	6.175	0	25363033	N.D.	0.756
11)	B cis-Chlor...	0.000	6.175f	0	25363033	N.D.	0.791
15)	B Endosulfa...	0.000	6.971	0	34290797	N.D.	1.452
19)	B Endosulfa...	0.000	7.303	0	13109862	N.D.	0.630


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052100.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2019 20:49
Operator : AJ\SJ
Sample : K2044-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:32:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

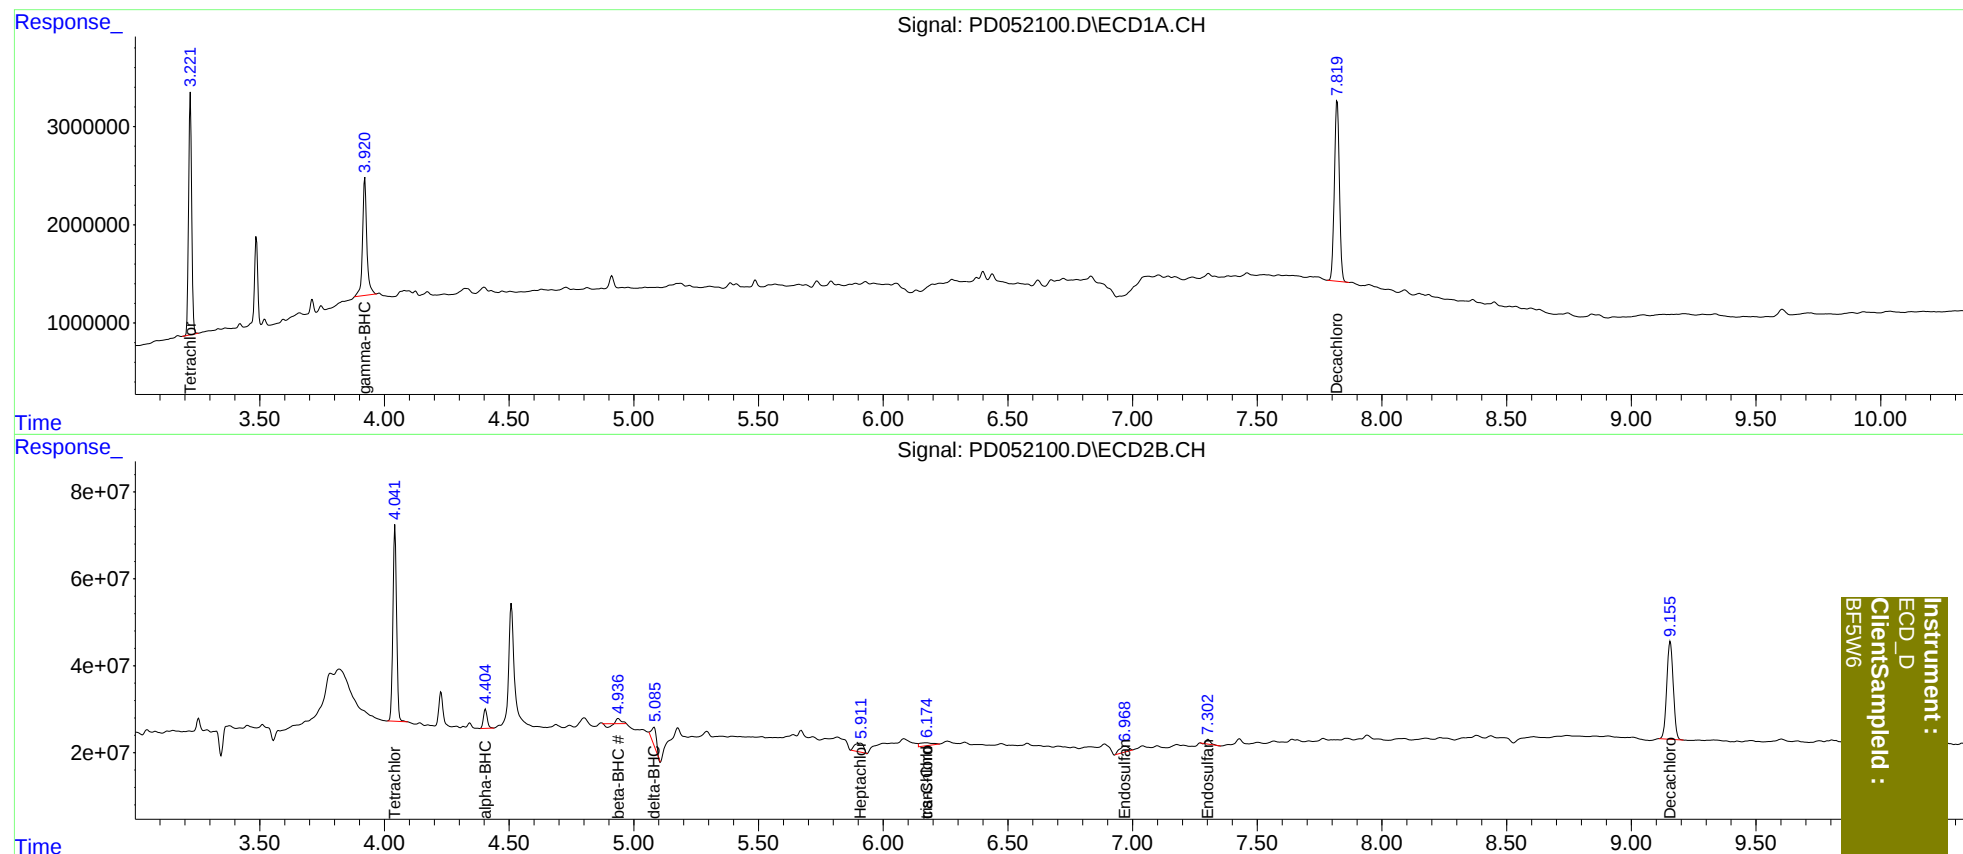


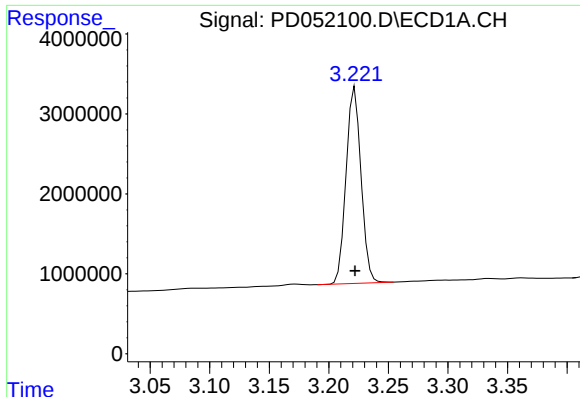

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 21438586
Conc: 15.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5W6

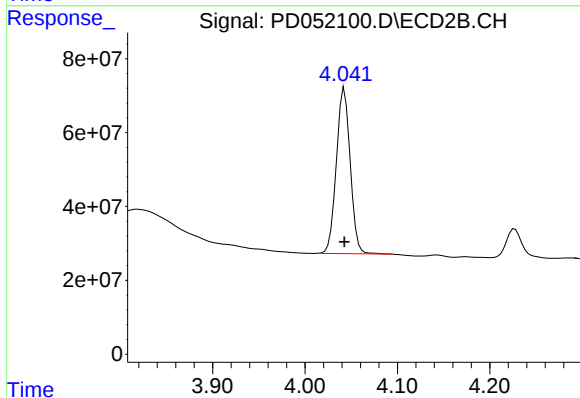


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 467969112
Conc: 15.75 ng/ml

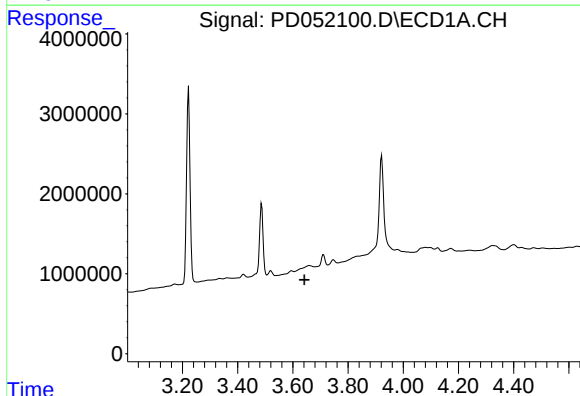


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.642 min
Response: 0
Conc: N.D.

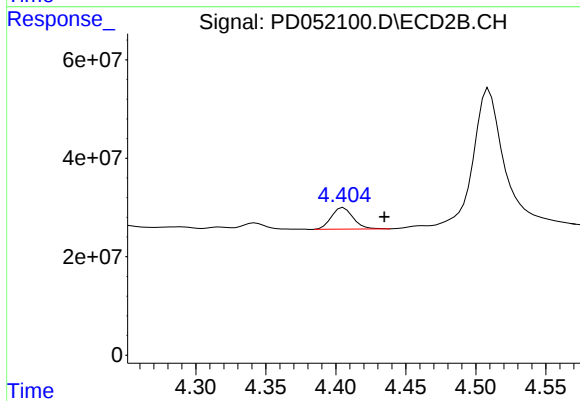

#2 alpha-BHC


R.T.: 4.406 min
Delta R.T.: -0.029 min
Response: 47388384
Conc: 1.06 ng/ml

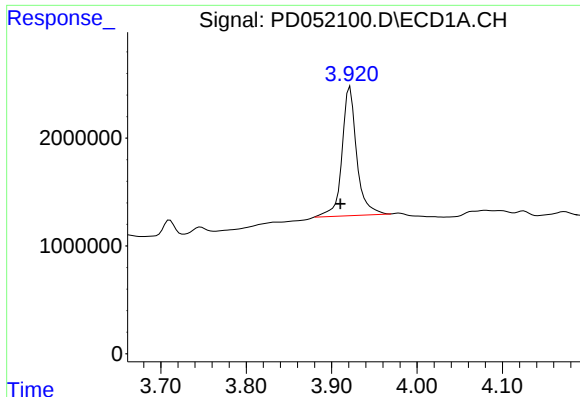

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.011 min
Response: 14273796
Conc: 6.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5W6

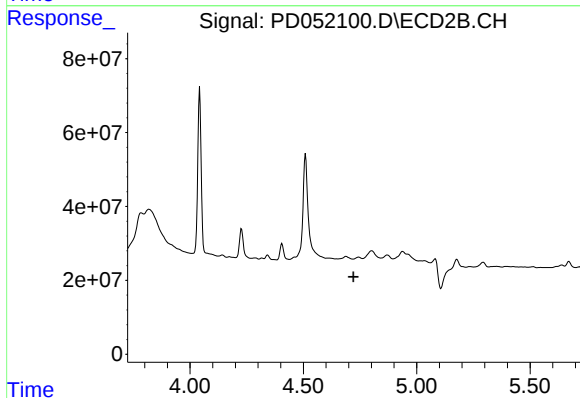


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

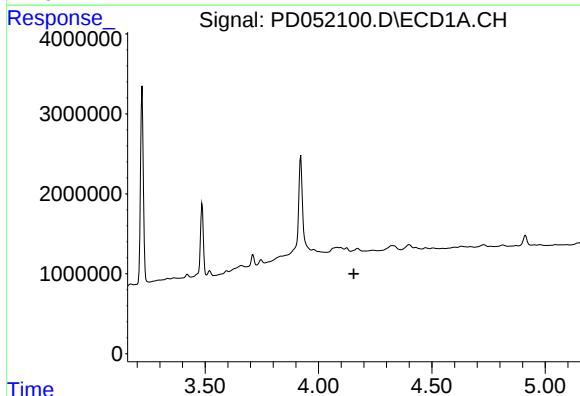


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.156 min
Response: 0
Conc: N.D.

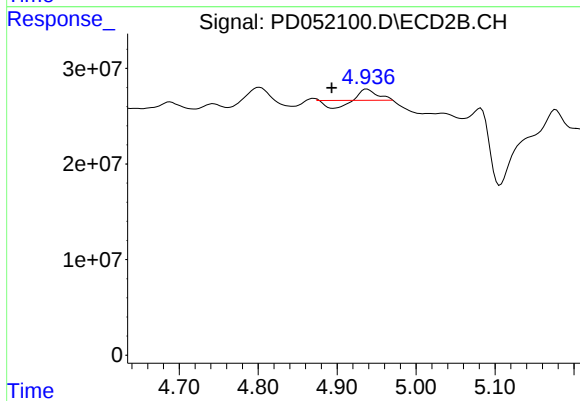

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.045 min
Response: 6219954
Conc: 0.34 ng/ml

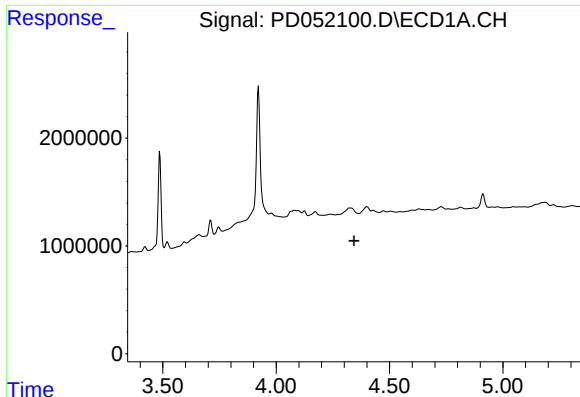

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6

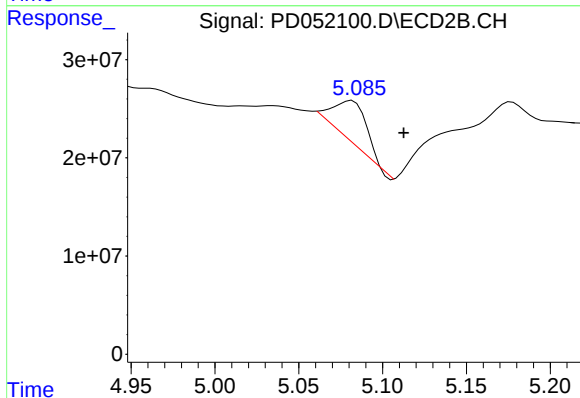


#7 delta-BHC

R.T.: 5.082 min
Delta R.T.: -0.031 min
Response: 57511477
Conc: 1.56 ng/ml

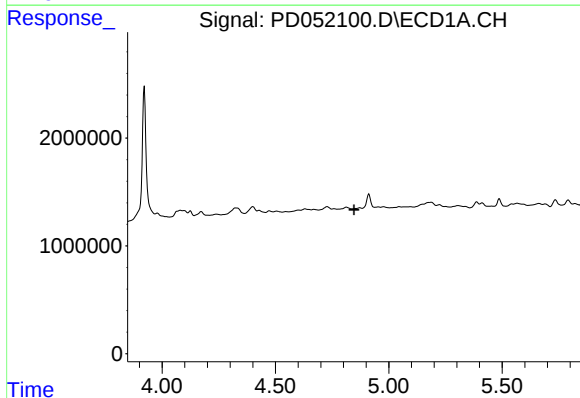


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.847 min
Response: 0
Conc: N.D.

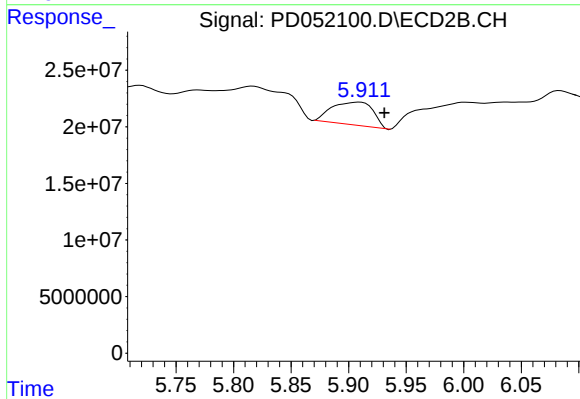

#8 Heptachlor epoxide


R.T.: 5.910 min
Delta R.T.: -0.021 min
Response: 50386772
Conc: 1.51 ng/ml

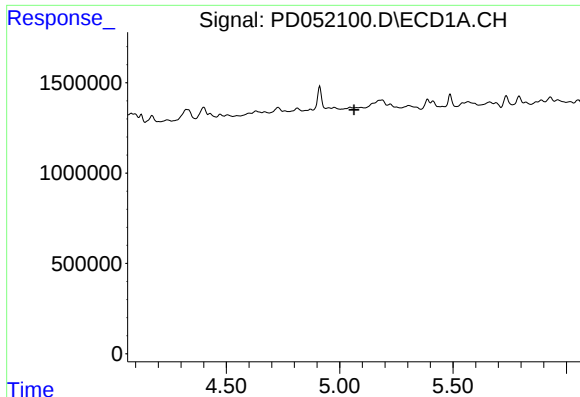

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6

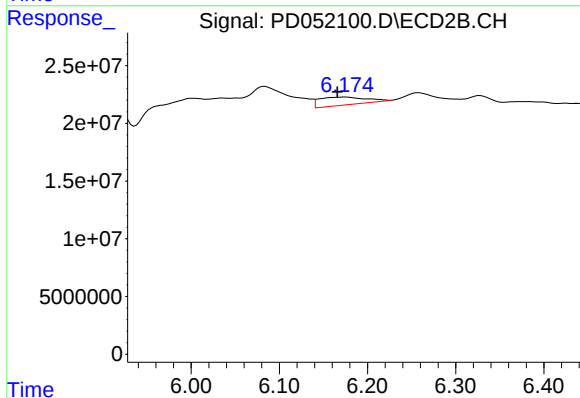


#10 trans-Chlordane

R.T.: 6.175 min
Delta R.T.: 0.010 min
Response: 25363033
Conc: 0.76 ng/ml

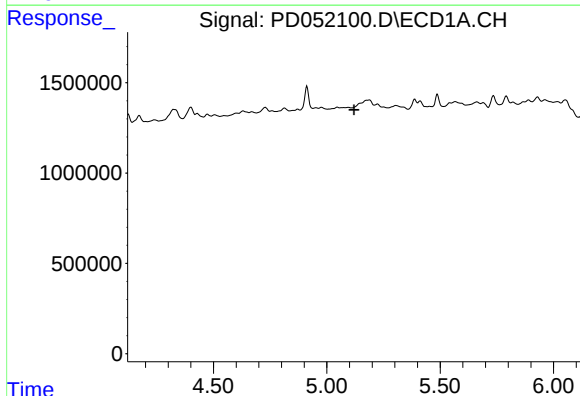


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.120 min
Response: 0
Conc: N.D.

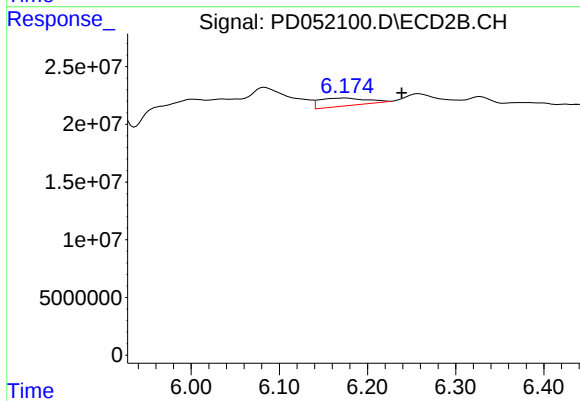

#11 cis-Chlordane


R.T.: 6.175 min
Delta R.T.: -0.064 min
Response: 25363033
Conc: 0.79 ng/ml

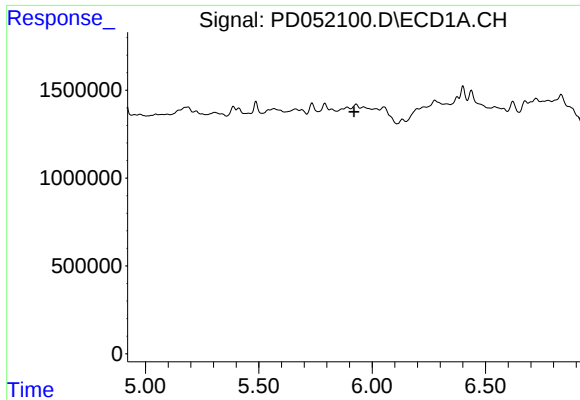

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6

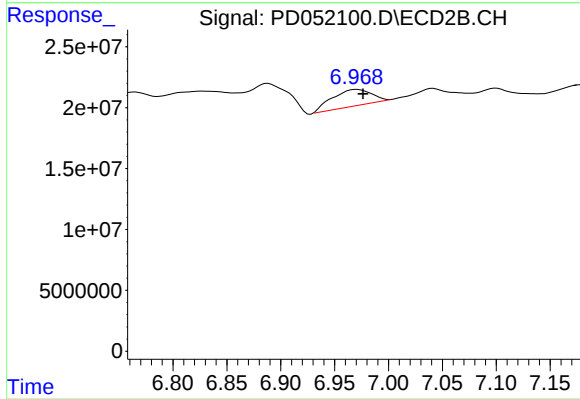


#15 Endosulfan II

R.T.: 6.971 min
Delta R.T.: -0.006 min
Response: 34290797
Conc: 1.45 ng/ml

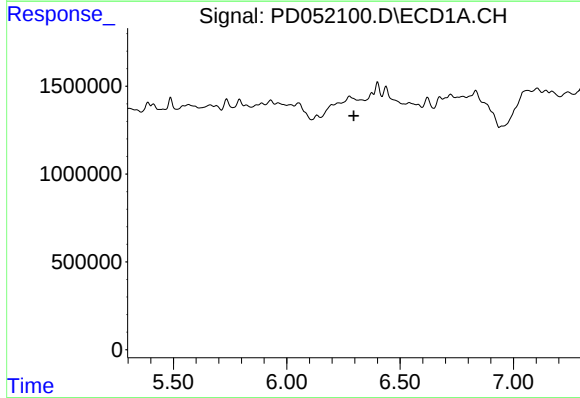


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.295 min
Response: 0
Conc: N.D.

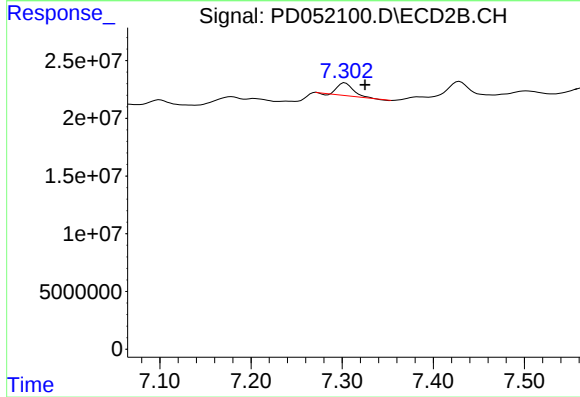

#19 Endosulfan Sulfate


R.T.: 7.303 min
Delta R.T.: -0.022 min
Response: 13109862
Conc: 0.63 ng/ml

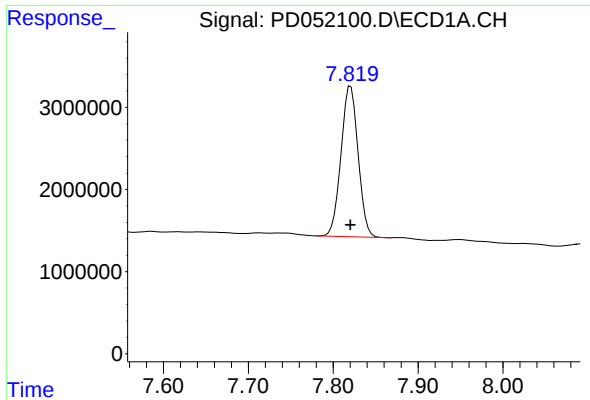

#27 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.000 min
Response: 25628944
Conc: 24.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5W6

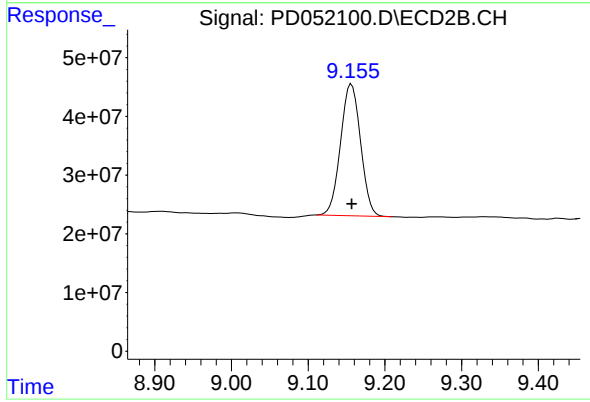

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 408526228
Conc: 27.72 ng/ml