

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
 Data File : PD052116.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2019 4:08
 Operator : AJ\SJ
 Sample : K2065-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 08:34:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 08:23:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	24186756	426.2E6	17.203	14.344
27)	SA Decachlor...	7.821	9.156	38044806	307.9E6	36.157	20.890 #
Target Compounds							
2)	A alpha-BHC	0.000	4.407f	0	44779817	N.D.	1.006
3)	MA gamma-BHC...	3.920	4.688f	5506129	19899954	2.397	0.494 #
6)	B beta-BHC	0.000	4.939f	0	25464205	N.D.	1.383
7)	B delta-BHC	0.000	5.082f	0	52590691	N.D.	1.428
8)	B Heptachlo...	0.000	5.913	0	61886541	N.D.	1.857
9)	A Endosulfan I	0.000	6.245f	0	133.5E6	N.D.	4.313
10)	B trans-Chl...	0.000	6.141	0	114.1E6	N.D.	3.404
11)	B cis-Chlor...	0.000	6.245	0	133.5E6	N.D.	4.161

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032419\
Data File : PD052116.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2019 4:08
Operator : AJ\SJ
Sample : K2065-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 08:34:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032419CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 08:23:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

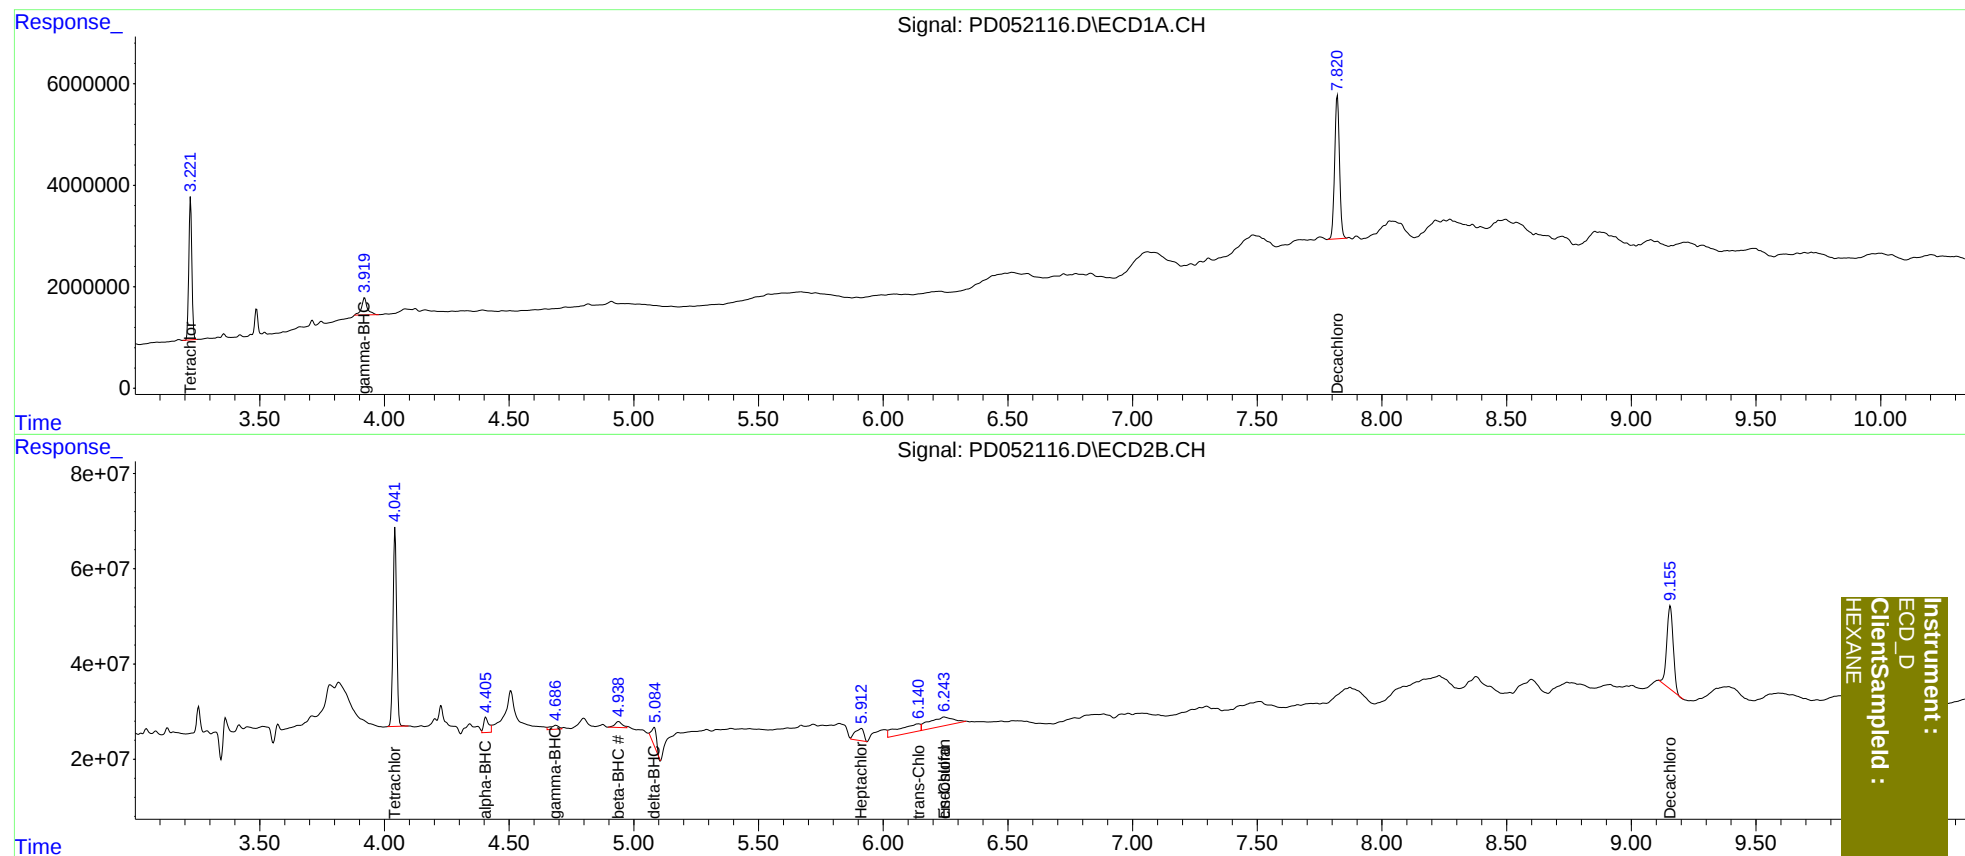


Instrument :
ECD_D
ClientSampled :
HEXANE

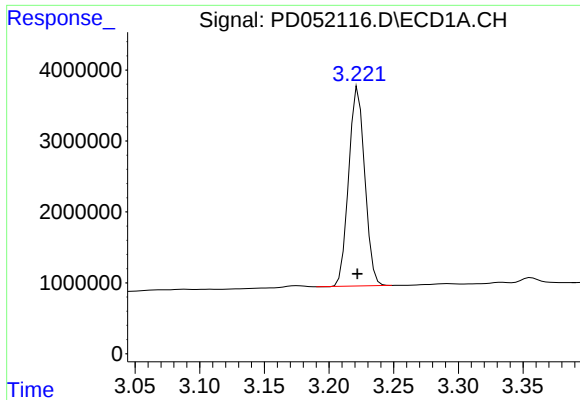

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 24186756
Conc: 17.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

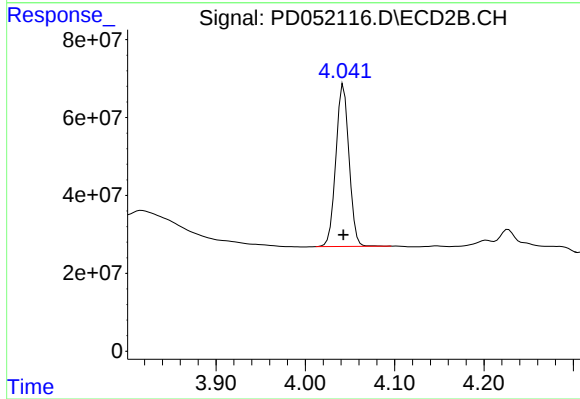


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 426179352
Conc: 14.34 ng/ml

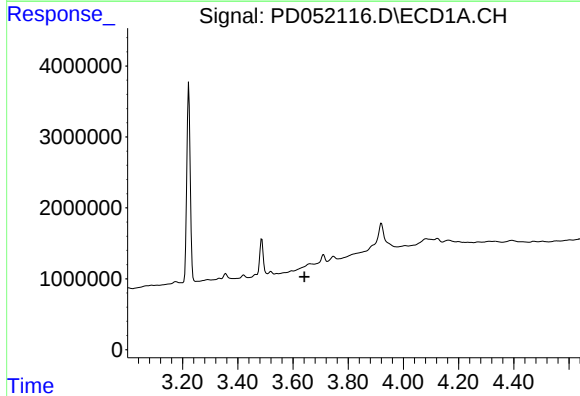


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.642 min
Response: 0
Conc: N.D.

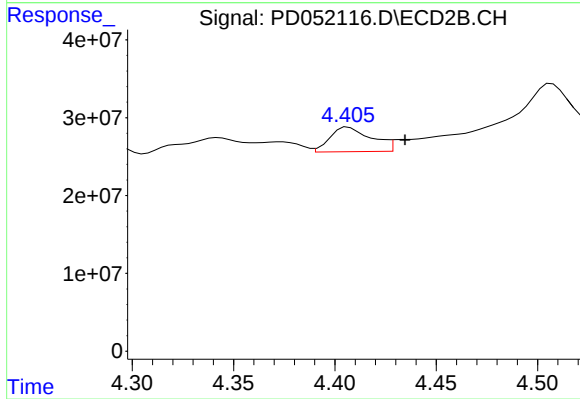

#2 alpha-BHC


R.T.: 4.407 min
Delta R.T.: -0.028 min
Response: 44779817
Conc: 1.01 ng/ml

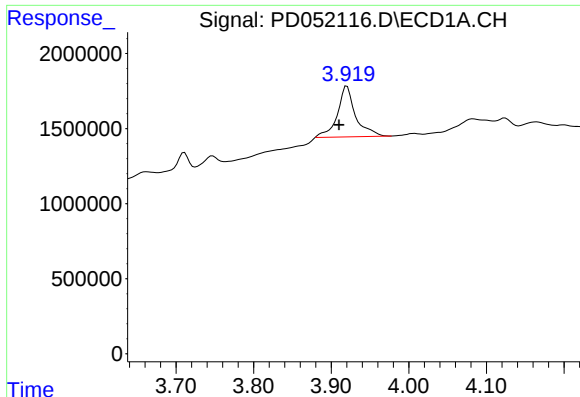

#3 gamma-BHC (Lindane)


R.T.: 3.920 min
Delta R.T.: 0.010 min
Response: 5506129
Conc: 2.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

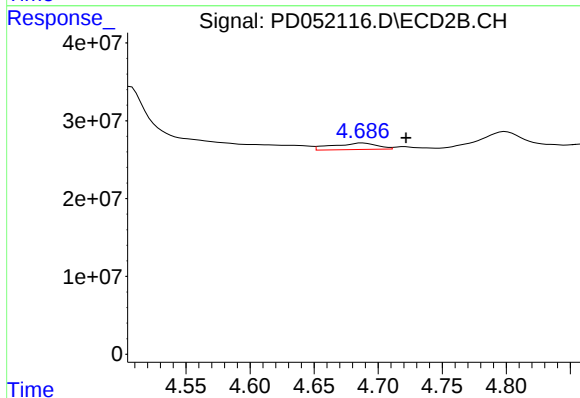


#3 gamma-BHC (Lindane)

R.T.: 4.688 min
Delta R.T.: -0.034 min
Response: 19899954
Conc: 0.49 ng/ml

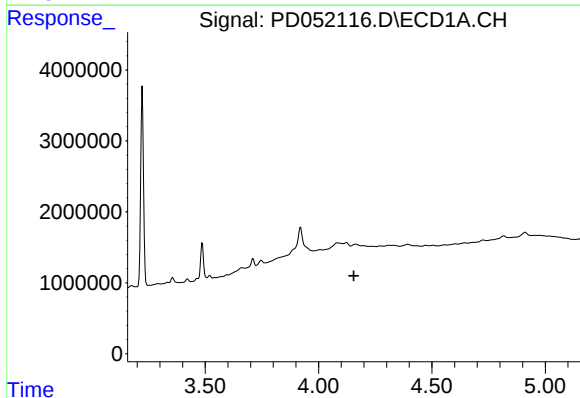


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.156 min
Response: 0
Conc: N.D.

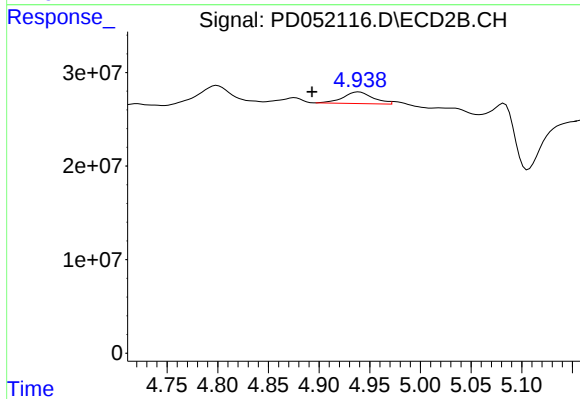

#6 beta-BHC


R.T.: 4.939 min
Delta R.T.: 0.046 min
Response: 25464205
Conc: 1.38 ng/ml

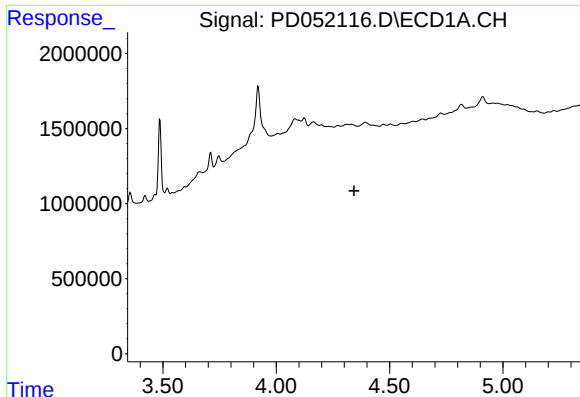

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

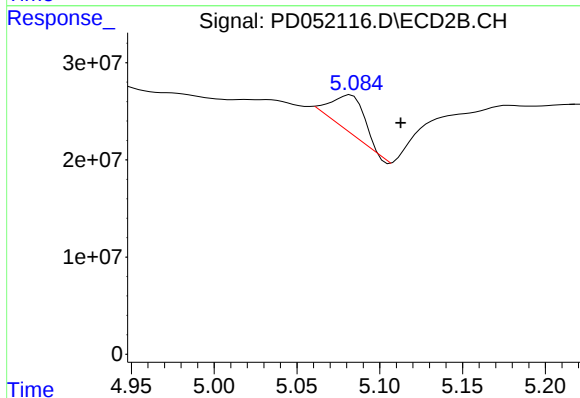


#7 delta-BHC

R.T.: 5.082 min
Delta R.T.: -0.030 min
Response: 52590691
Conc: 1.43 ng/ml

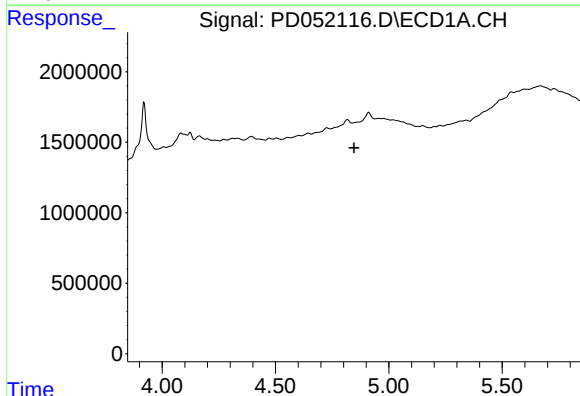


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.847 min
Response: 0
Conc: N.D.

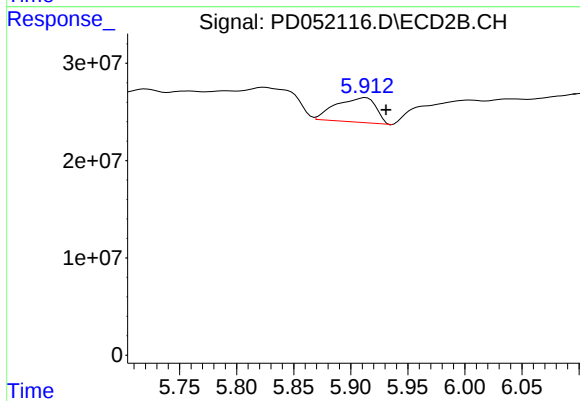

#8 Heptachlor epoxide


R.T.: 5.913 min
Delta R.T.: -0.018 min
Response: 61886541
Conc: 1.86 ng/ml

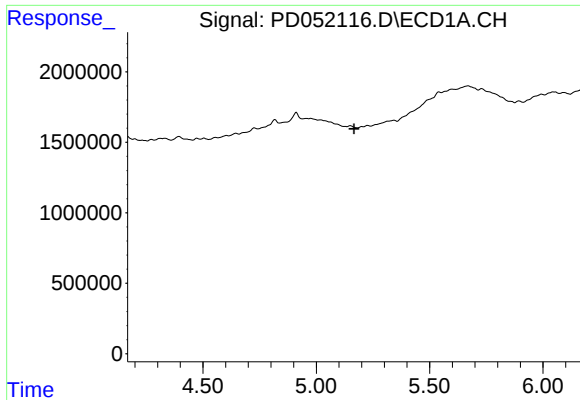

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

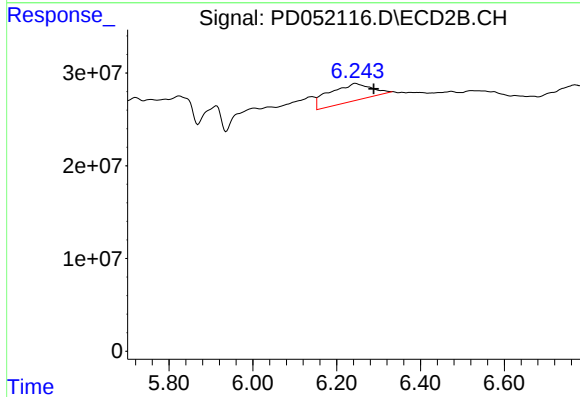


#9 Endosulfan I

R.T.: 6.245 min
Delta R.T.: -0.044 min
Response: 133456106
Conc: 4.31 ng/ml

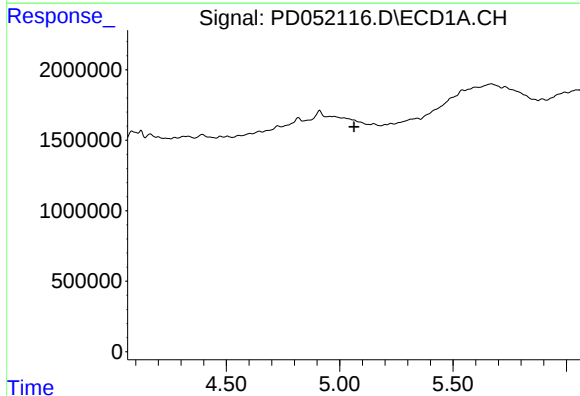


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

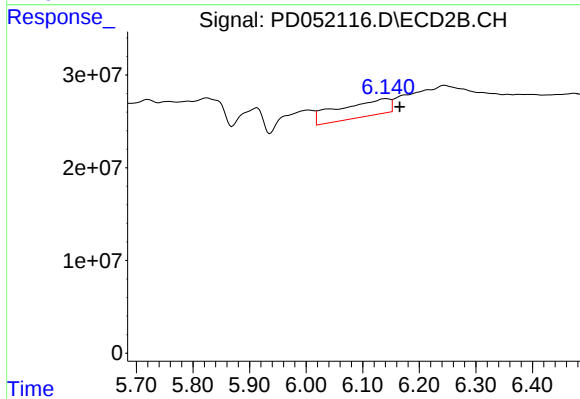

#10 trans-Chlordane


R.T.: 6.141 min
Delta R.T.: -0.025 min
Response: 114139619
Conc: 3.40 ng/ml

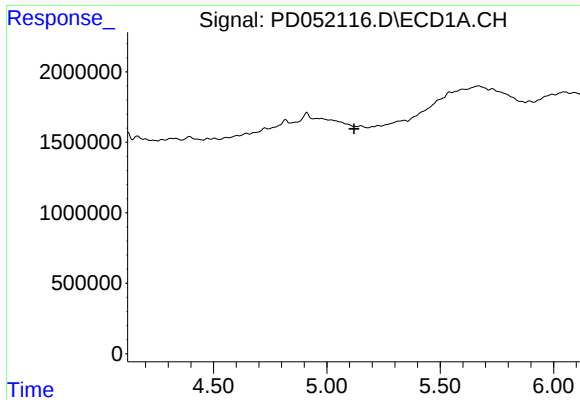

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.120 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

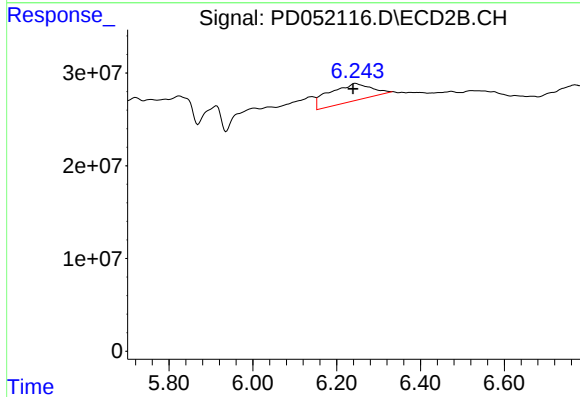


#11 cis-Chlordane

R.T.: 6.245 min
Delta R.T.: 0.006 min
Response: 133456106
Conc: 4.16 ng/ml

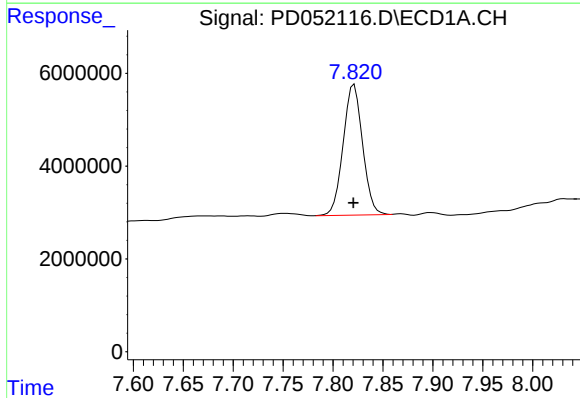

#27 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.000 min
Response: 38044806
Conc: 36.16 ng/ml

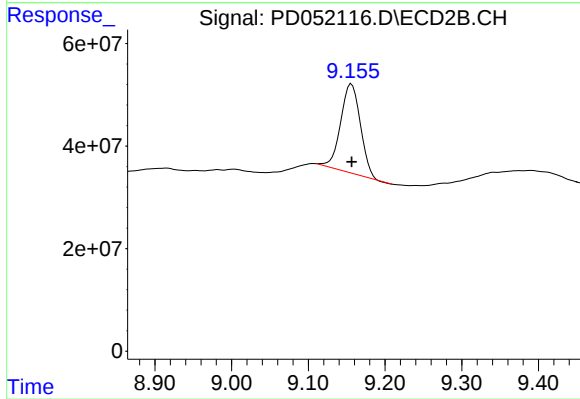

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 307868762
Conc: 20.89 ng/ml