

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032423\
 Data File : PD074422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 03:18
 Operator : AR\AJ
 Sample : 50/100 PEST/PCB/SPIKE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 50/100 PEST/PCB/SPIKE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/24/2023
 Supervised By : Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:18:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


2) A	alpha-BHC	4.007	3.275	206.4E6	93367607	52.886	52.246
3) MA	gamma-BHC...	4.340	3.605	184.1E6	84631009	49.867	49.549
4) MA	Heptachlor	4.933	3.946	184.0E6	81718225	48.590	49.285
5) MB	Aldrin	5.276	4.227	190.9E6	88392502	52.235	51.627
6) B	beta-BHC	4.533	3.901	76060658	37991634	44.992m	46.894
7) B	delta-BHC	4.784	4.131	182.9E6	87438126	50.259	49.435
8) B	Heptachlo...	5.703	4.730	160.6E6	76689232	48.904	48.409
9) A	Endosulfan I	6.090	5.101	150.0E6	70527051	50.290	50.298
10) B	trans-Chl...	5.960	4.980	161.0E6	77714800	50.174	50.235
11) B	cis-Chlor...	6.040	5.045	162.0E6	77193990	49.443	48.800
12) B	4,4'-DDE	6.212	5.235	317.8E6	150.3E6	106.095	103.478
13) MA	Dieldrin	6.367	5.366	347.3E6	165.0E6	109.487	106.422
14) MA	Endrin	6.597	5.642	273.7E6	137.3E6	103.869	102.043
15) B	Endosulfa...	6.815	5.935	282.1E6	134.5E6	102.189	100.027
16) A	4,4'-DDD	6.730	5.789	260.4E6	127.0E6	110.195	107.857
17) MA	4,4'-DDT	7.044	6.041	274.4E6	126.0E6	109.331	100.595
18) B	Endrin al...	6.946	6.115	210.7E6	101.9E6	93.553	92.683
19) B	Endosulfa...	7.181	6.338	263.2E6	125.0E6	101.069	99.318
20) A	Methoxychlor	7.521	6.618	709.9E6	298.4E6	517.082	485.196
21) B	Endrin ke...	7.667	6.844	314.1E6	155.9E6	105.934	102.477

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032423\
Data File : PD074422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 03:18
Operator : AR\AJ
Sample : 50/100 PEST/PCB/SPIKE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:18:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

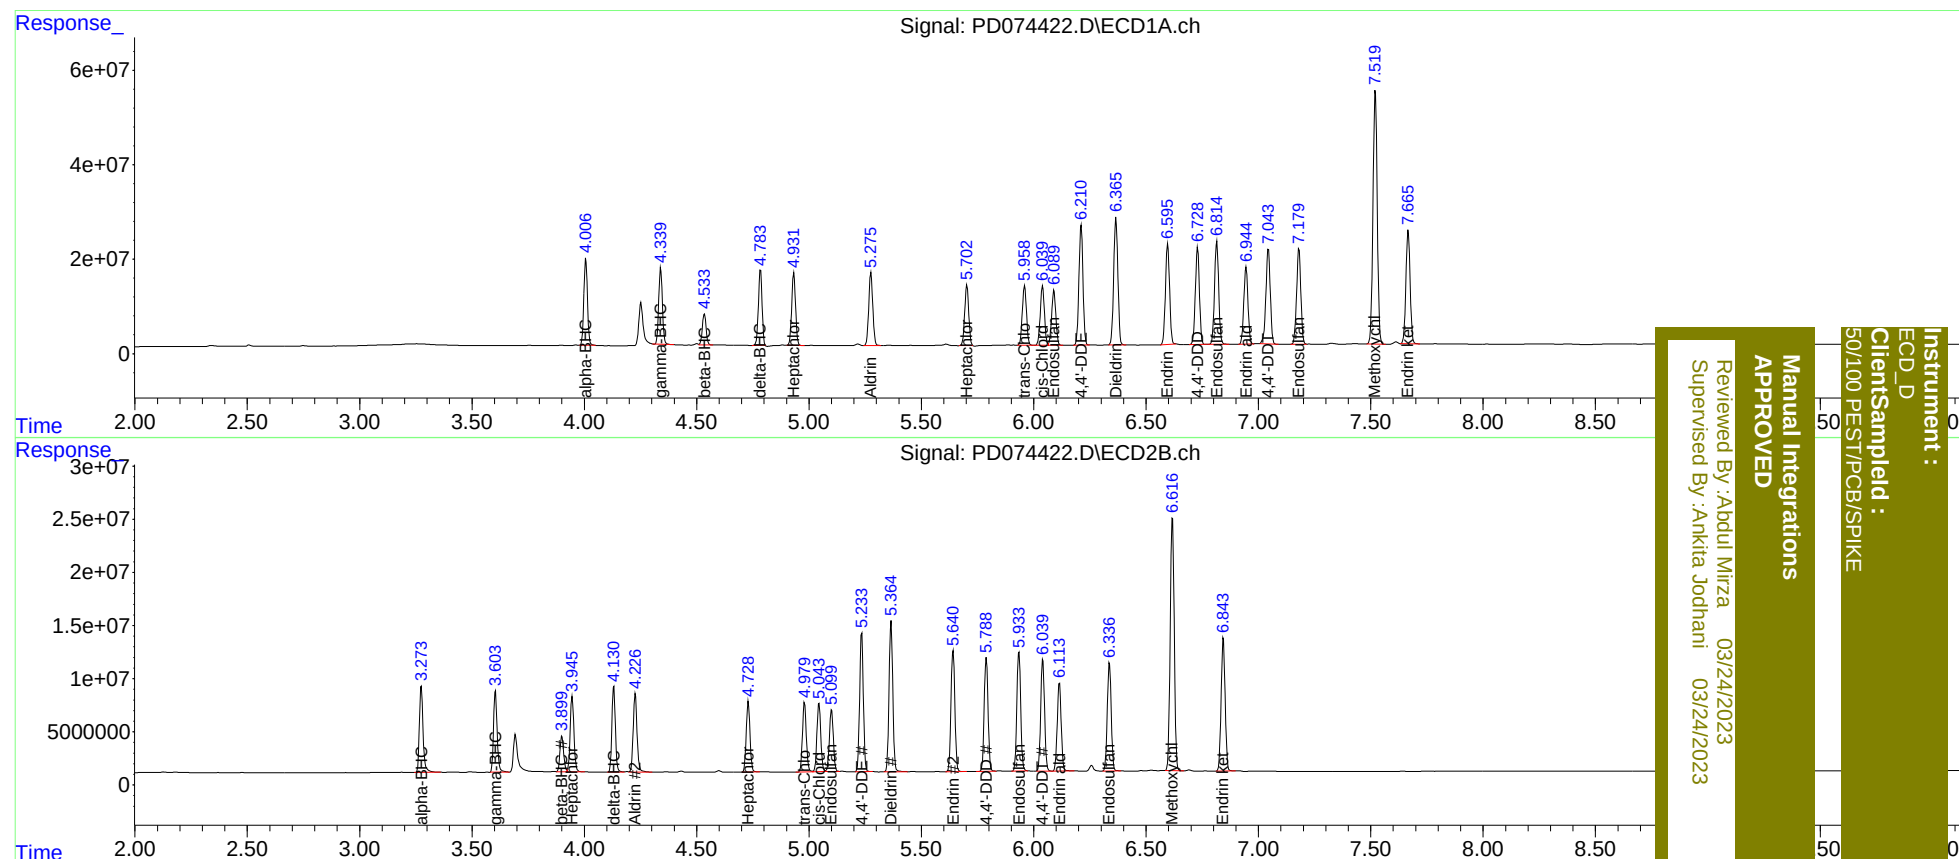

Reviewed By: Abdul Mirza 03/24/2023
Supervised By: Ankita Jodhani 03/24/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
50/100 PEST/PCB/SPIKE