

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032423\
 Data File : PD074447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 08:56
 Operator : AR\AJ
 Sample : 01992-21MS
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EYGC8MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/24/2023
 Supervised By :Ankita Jodhani 03/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 09:16:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	35444982	17644931	14.267	14.025
27)	SA Decachlor...	9.094	7.923	70374321	30276878	25.713	25.286
Target Compounds							
2)	A alpha-BHC	4.006	3.274	211.0E6	95888146	54.080	53.656
3)	MA gamma-BHC...	4.340	3.604	195.3E6	87962769	52.910	51.500
4)	MA Heptachlor	4.932	3.946	190.5E6	85940158	50.307	51.831
5)	MB Aldrin	5.275	4.227	198.0E6	91537968	54.181	53.464
6)	B beta-BHC	4.534	3.900	82354370	38959668	48.715	48.089
7)	B delta-BHC	4.783	4.131	169.9E6	81409513	46.686	46.027
8)	B Heptachlo...	5.700	4.729	171.0E6	80268065	52.099m	50.669
9)	A Endosulfan I	6.089	5.100	157.5E6	74667001	52.800	53.251
10)	B trans-Chl...	5.958	4.980	169.3E6	82073095	52.756	53.052
11)	B cis-Chlor...	6.039	5.044	170.7E6	81574777	52.106	51.569
12)	B 4,4'-DDE	6.210	5.234	336.4E6	158.4E6	112.322	109.044
13)	MA Dieldrin	6.365	5.365	362.9E6	170.9E6	114.396	110.260
14)	MA Endrin	6.596	5.641	288.3E6	143.9E6	109.383	106.956
15)	B Endosulfa...	6.814	5.934	296.0E6	139.4E6	107.236	103.648
16)	A 4,4'-DDD	6.728	5.789	275.6E6	129.8E6	116.617	110.207
17)	MA 4,4'-DDT	7.043	6.041	279.2E6	128.8E6	111.263	102.845
18)	B Endrin al...	6.944	6.114	217.9E6	104.8E6	96.745	95.308
19)	B Endosulfa...	7.179	6.337	268.4E6	125.2E6	103.046	99.465
20)	A Methoxychlor	7.519	6.617	739.1E6	310.4E6	538.327	504.667
21)	B Endrin ke...	7.665	6.844	334.0E6	160.3E6	112.656	105.363

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032423\
Data File : PD074447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 08:56
Operator : AR\AJ
Sample : 01992-21MS
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 09:16:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

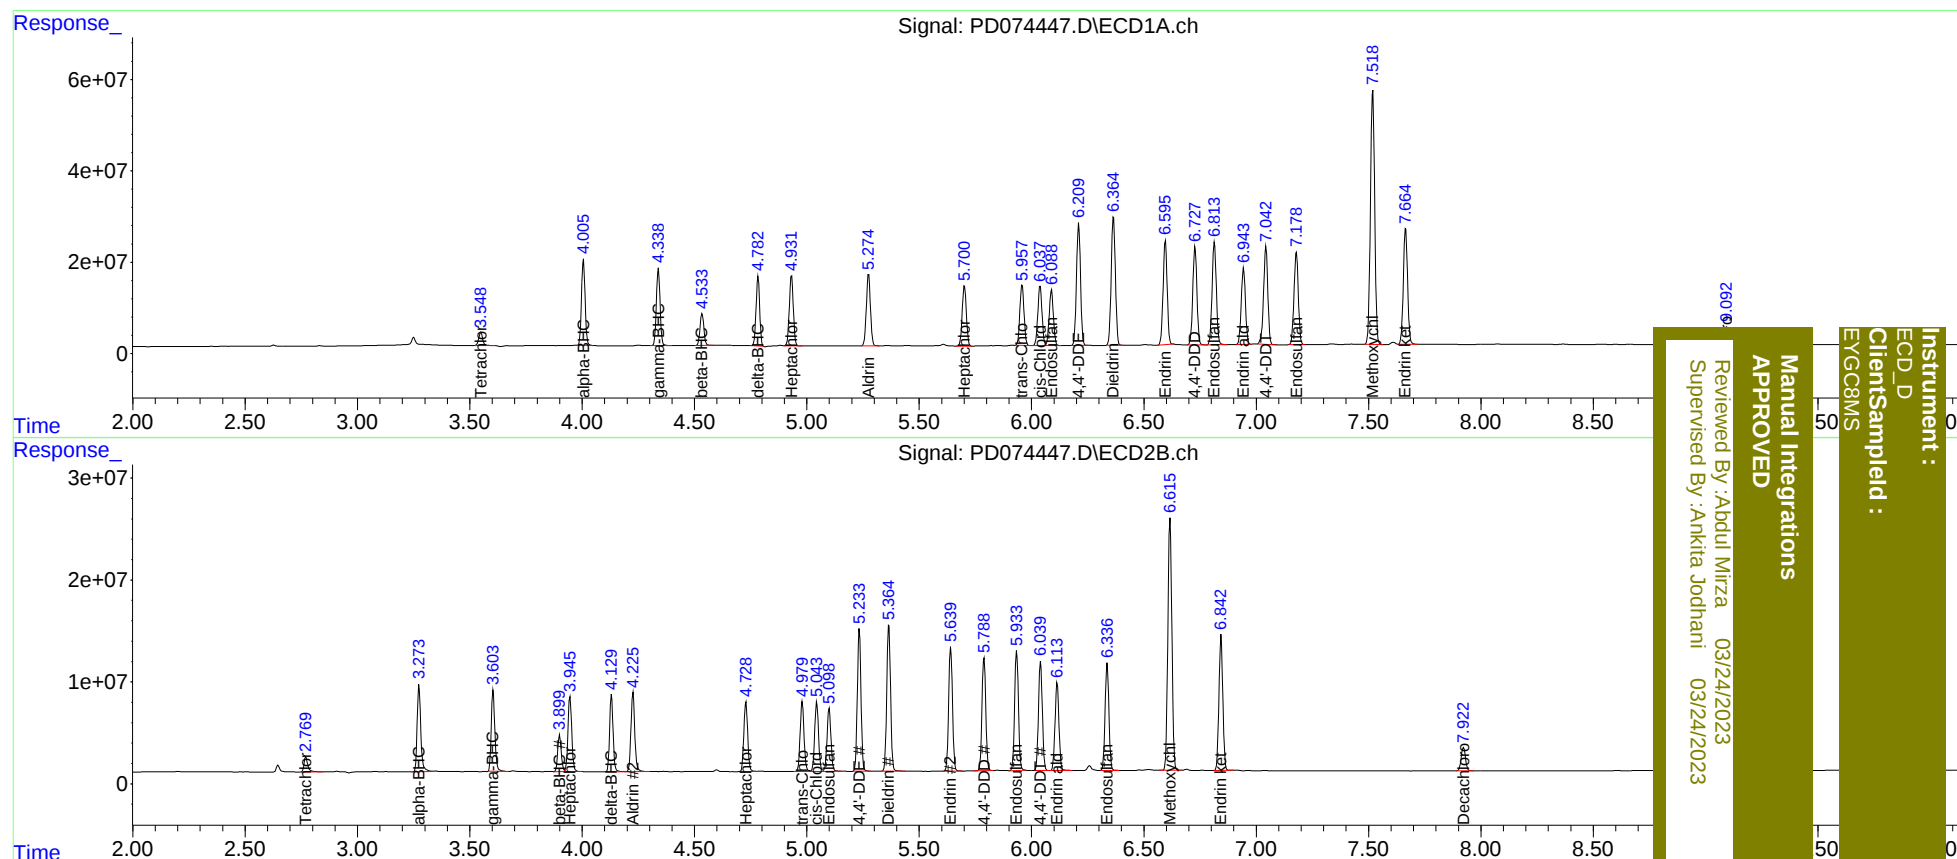

Instrument :
ECD_D
ClientSampled :
EYGC8MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 03/24/2023
Supervised By: Ankita Jodhani 03/24/2023