

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032519\
 Data File : PD052113.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2019 12:27
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 07:51:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	0.000	4.931f	0 28235692	N.D.	1.539
8) B	Heptachlo...	0.000	5.921	0 31309871	N.D.	0.919
10) B	trans-Chl...	0.000	6.132	0 24969296	N.D.	0.735
14) MA	Endrin	0.000	6.758	0 13750743	N.D.	0.597
20) A	Methoxychlor	0.000	7.585f	0 25537230	N.D.	2.745


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032519\
Data File : PD052113.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2019 12:27
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 07:51:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

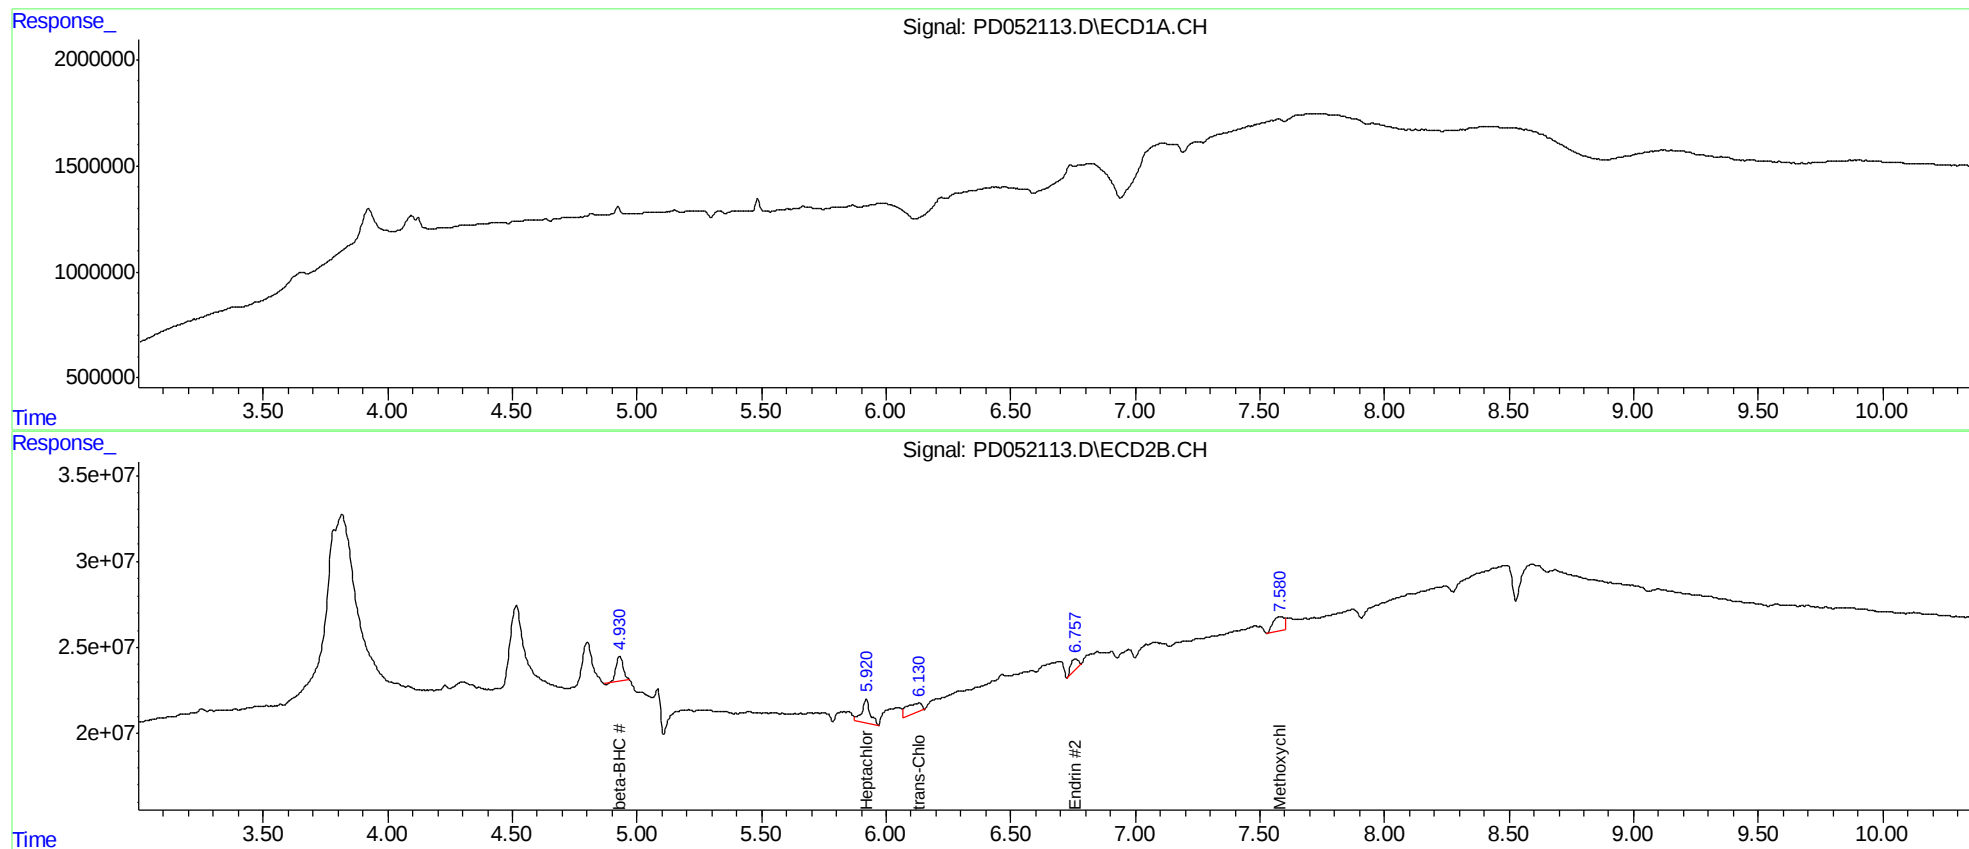


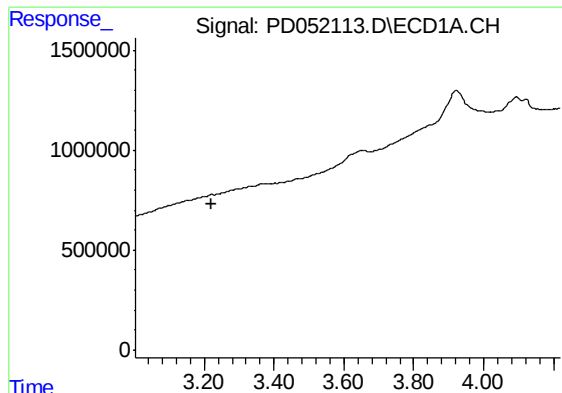

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

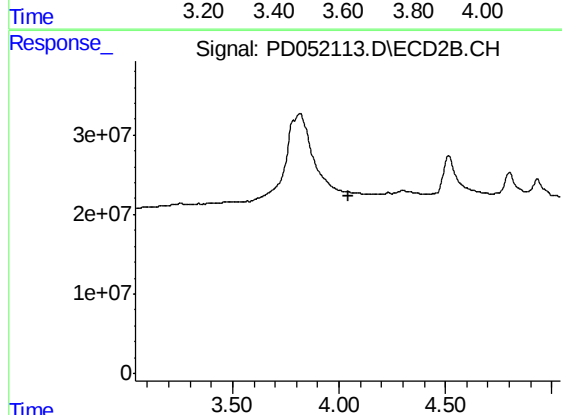


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.043 min
Response: 0
Conc: N.D.

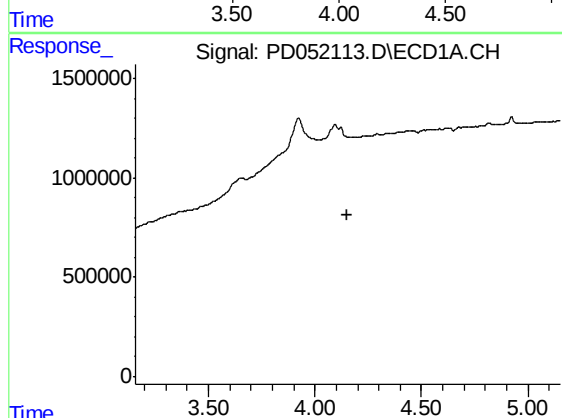


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

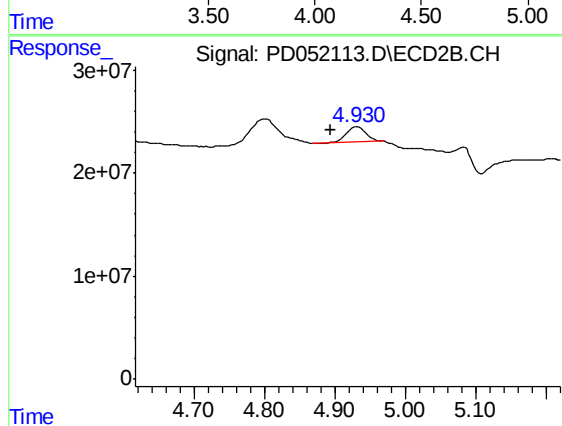

#6 beta-BHC


R.T.: 4.931 min
Delta R.T.: 0.038 min
Response: 28235692
Conc: 1.54 ng/ml

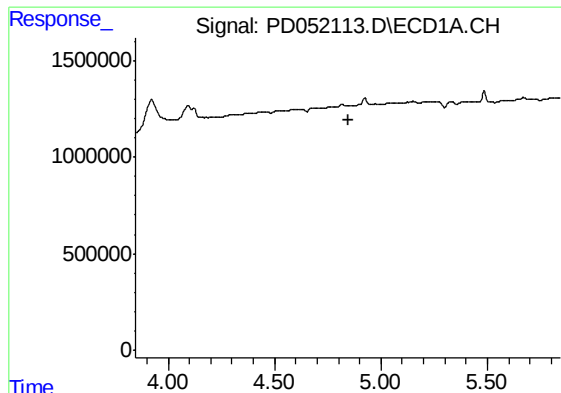

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

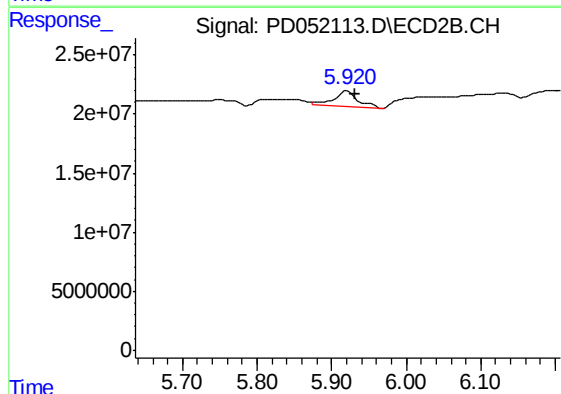


#8 Heptachlor epoxide

R.T.: 5.921 min
Delta R.T.: -0.009 min
Response: 31309871
Conc: 0.92 ng/ml

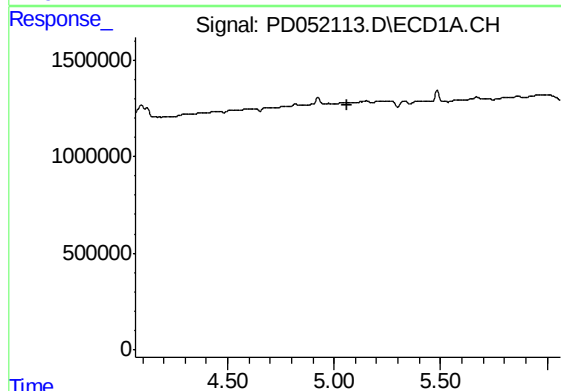


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

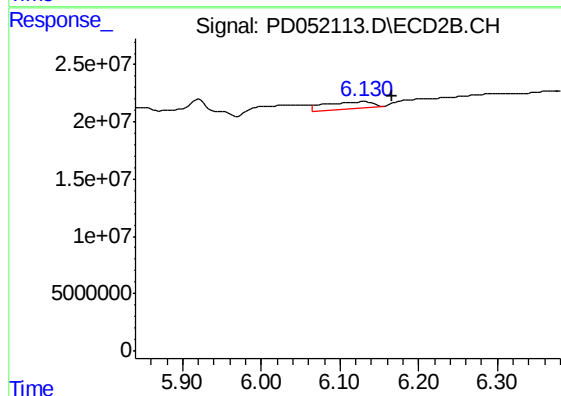

#10 trans-Chlordane


R.T.: 6.132 min
Delta R.T.: -0.034 min
Response: 24969296
Conc: 0.74 ng/ml

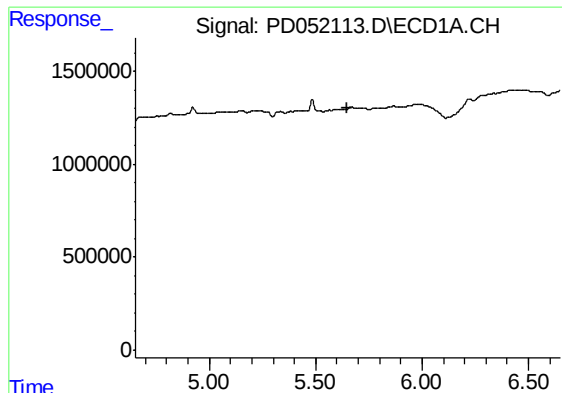

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

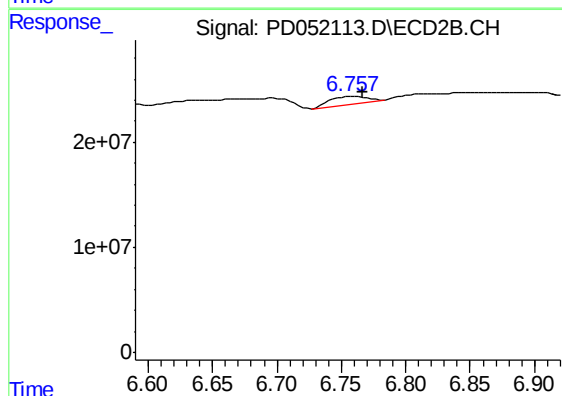


#14 Endrin

R.T.: 6.758 min
Delta R.T.: -0.008 min
Response: 13750743
Conc: 0.60 ng/ml

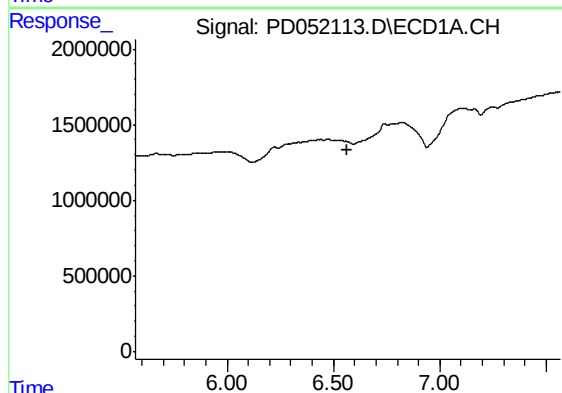


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.567 min
Response: 0
Conc: N.D.

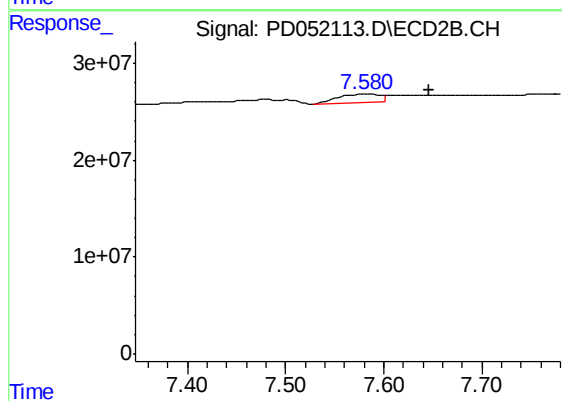

#20 Methoxychlor


R.T.: 7.585 min
Delta R.T.: -0.061 min
Response: 25537230
Conc: 2.75 ng/ml

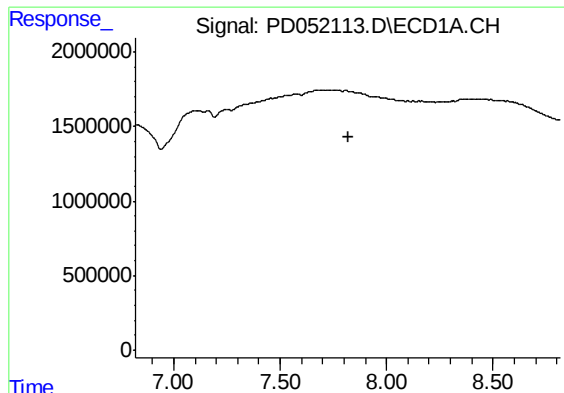

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

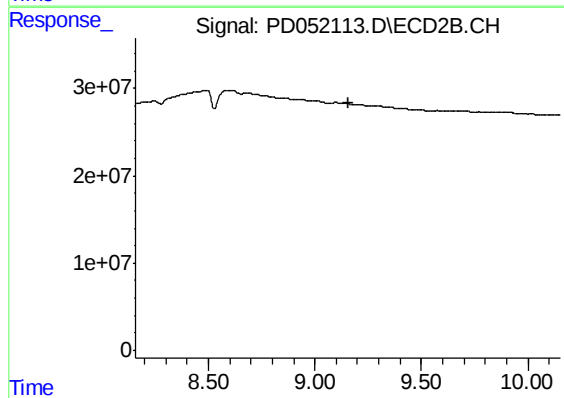

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.156 min
Response: 0
Conc: N.D.