

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032519\
 Data File : PD052140.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2019 20:07
 Operator : AJ\SJ
 Sample : K2065-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5L7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 07:53:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	20300656	382.2E6	14.302	13.136
27)	SA Decachlor...	7.819	9.155	37727678	367.4E6	24.094	23.801
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0	115.1E6	N.D.	2.633
6)	B beta-BHC	0.000	4.936f	0	9725255	N.D.	0.530
7)	B delta-BHC	0.000	5.081f	0	49305671	N.D.	1.243
8)	B Heptachlo...	0.000	5.918	0	123.4E6	N.D.	3.621
9)	A Endosulfan I	0.000	6.252f	0	18282684	N.D.	0.583
10)	B trans-Chl...	0.000	6.156	0	93904968	N.D.	2.765
11)	B cis-Chlor...	0.000	6.252	0	18282684	N.D.	0.563
14)	MA Endrin	0.000	6.758	0	46851174	N.D.	2.035
15)	B Endosulfa...	0.000	6.985	0	28532189	N.D.	1.125


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032519\
Data File : PD052140.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2019 20:07
Operator : AJ\SJ
Sample : K2065-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF5L7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 07:53:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

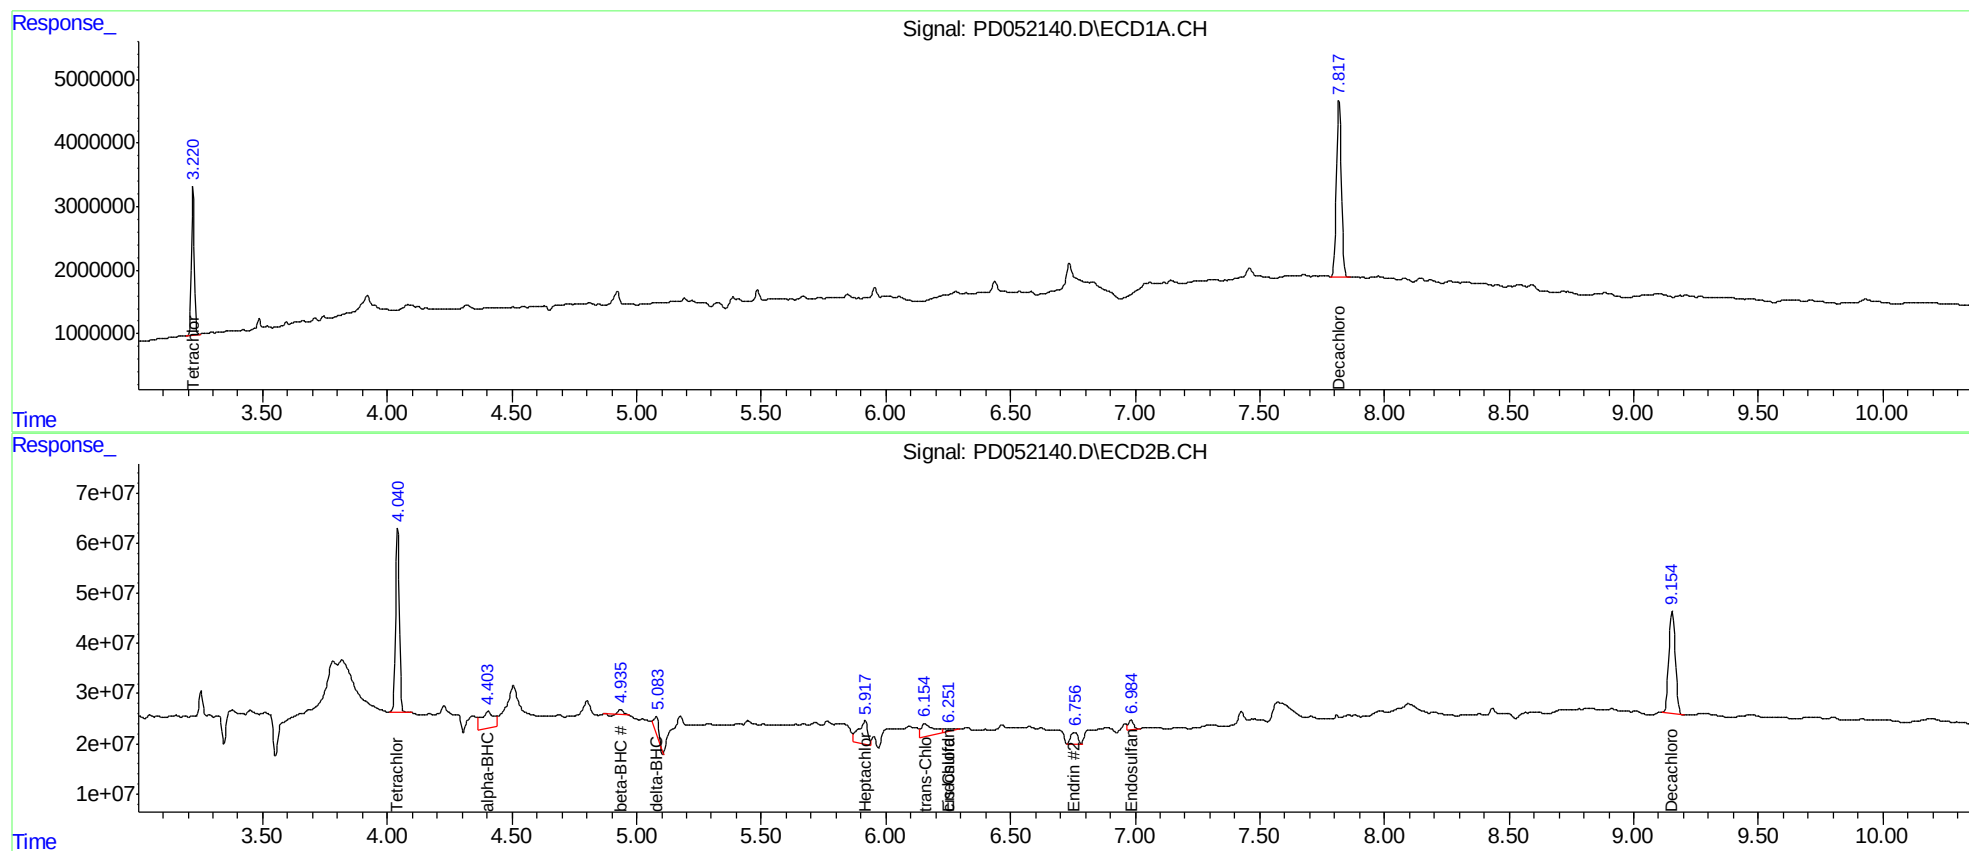


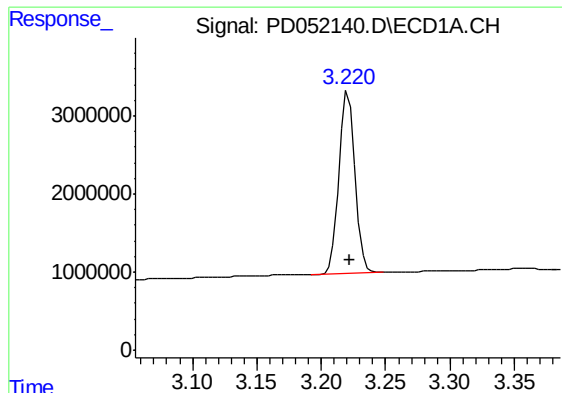

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 20300656
Conc: 14.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L7

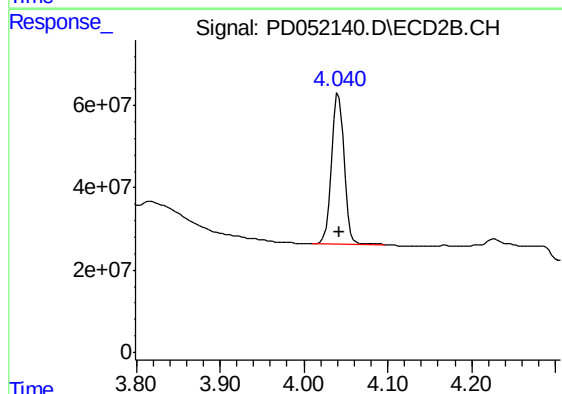


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 382220124
Conc: 13.14 ng/ml

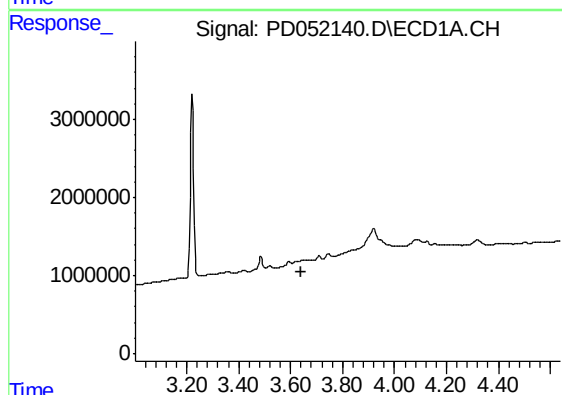


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

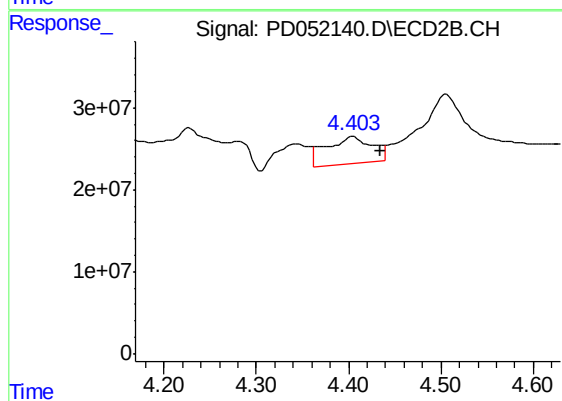

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 115132047
Conc: 2.63 ng/ml

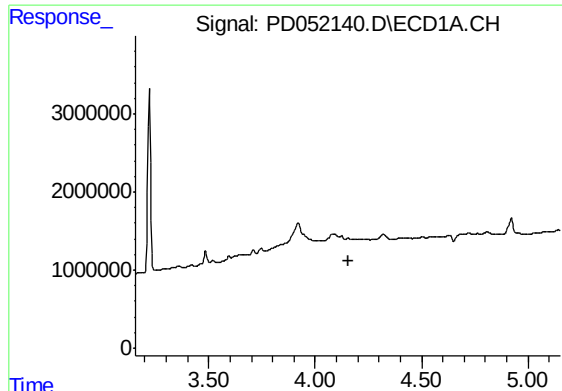

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L7

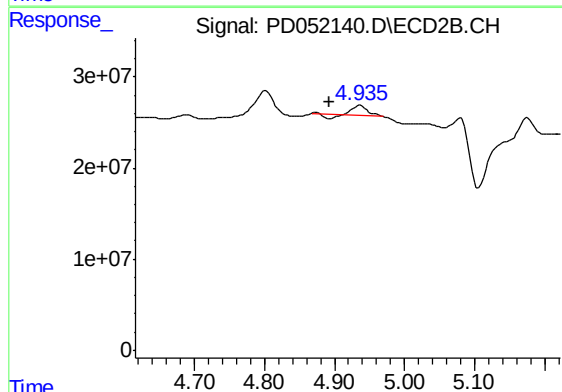


#6 beta-BHC

R.T.: 4.936 min
Delta R.T.: 0.043 min
Response: 9725255
Conc: 0.53 ng/ml

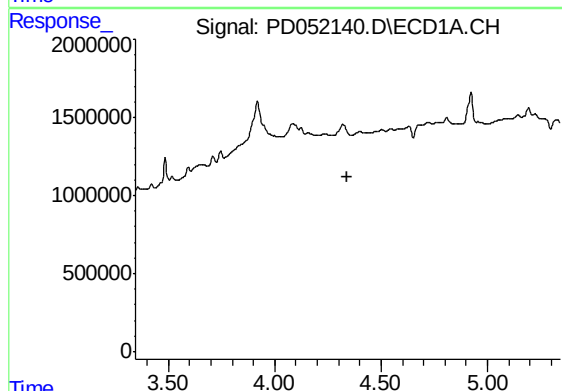


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

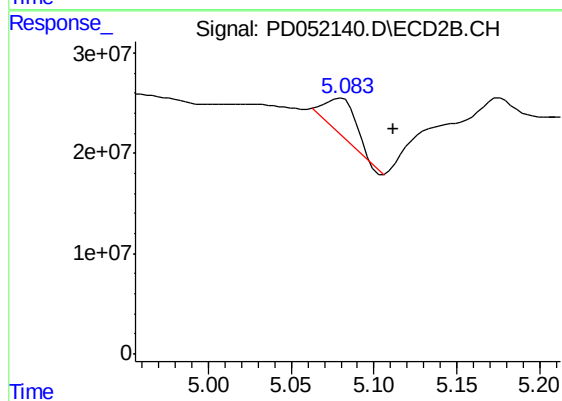

#7 delta-BHC


R.T.: 5.081 min
Delta R.T.: -0.031 min
Response: 49305671
Conc: 1.24 ng/ml

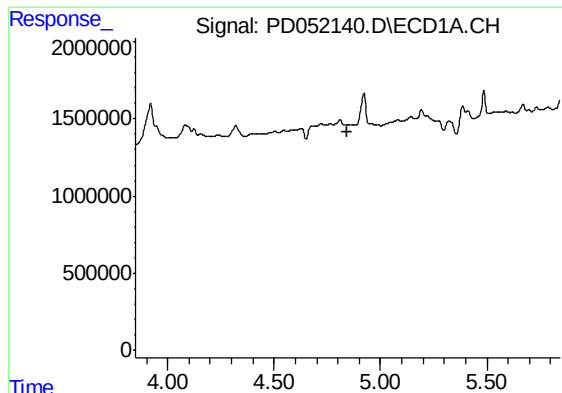

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L7

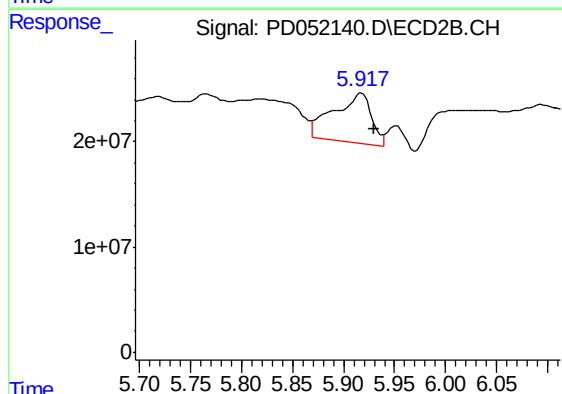


#8 Heptachlor epoxide

R.T.: 5.918 min
Delta R.T.: -0.012 min
Response: 123350249
Conc: 3.62 ng/ml

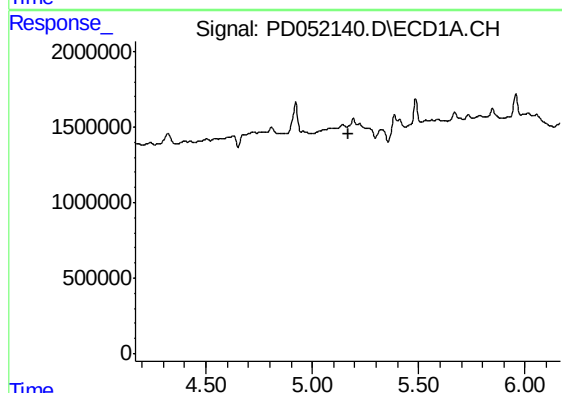


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

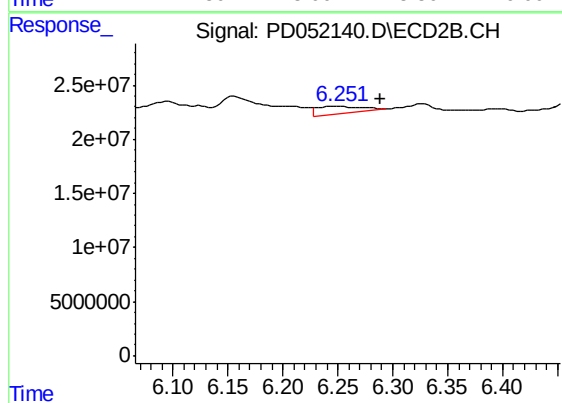

#9 Endosulfan I


R.T.: 6.252 min
Delta R.T.: -0.037 min
Response: 18282684
Conc: 0.58 ng/ml

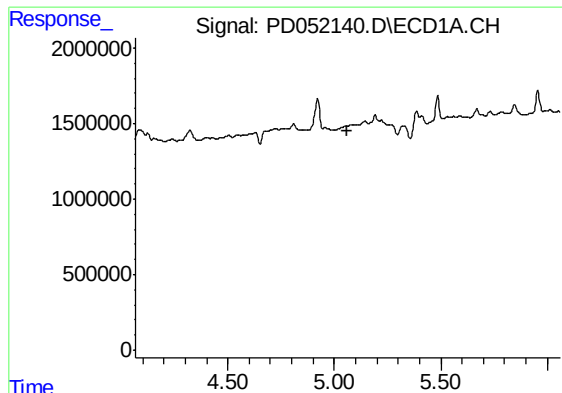

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L7

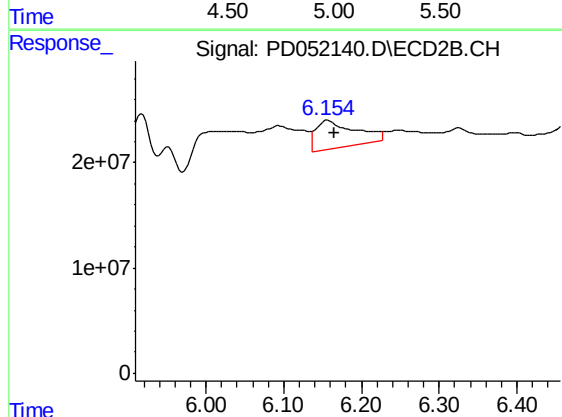


#10 trans-Chlordane

R.T.: 6.156 min
Delta R.T.: -0.010 min
Response: 93904968
Conc: 2.77 ng/ml

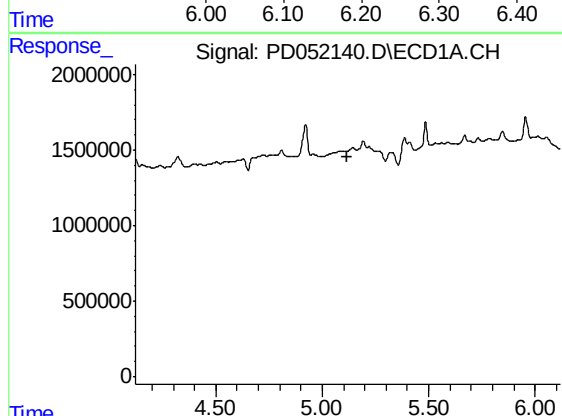


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

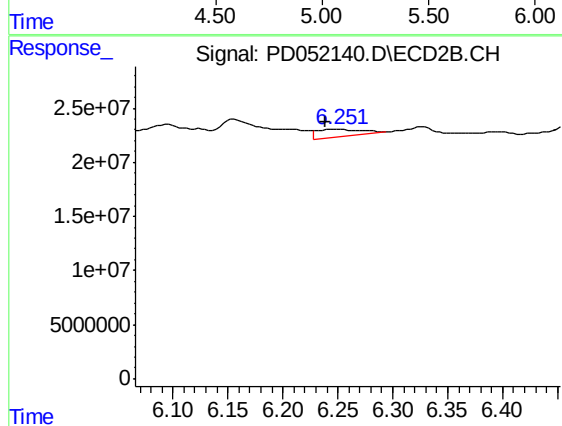

#11 cis-Chlordane


R.T.: 6.252 min
Delta R.T.: 0.014 min
Response: 18282684
Conc: 0.56 ng/ml

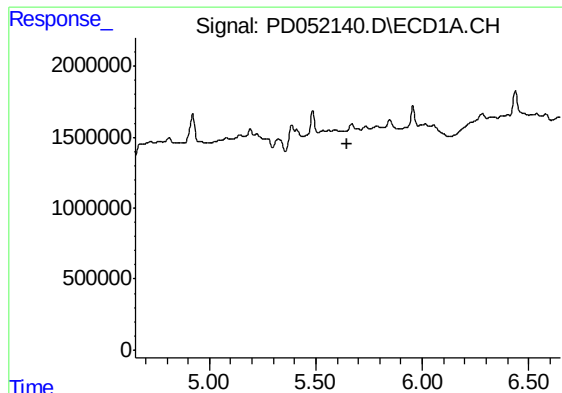

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5L7

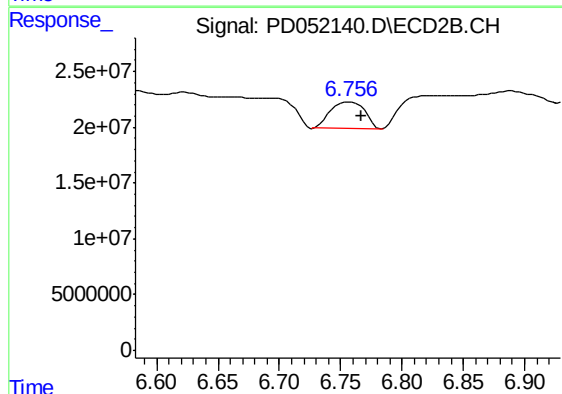


#14 Endrin

R.T.: 6.758 min
Delta R.T.: -0.009 min
Response: 46851174
Conc: 2.04 ng/ml

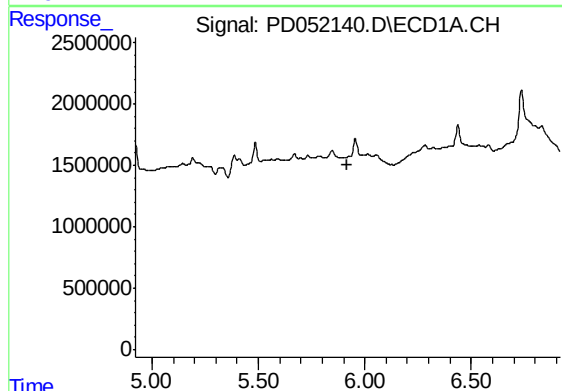


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

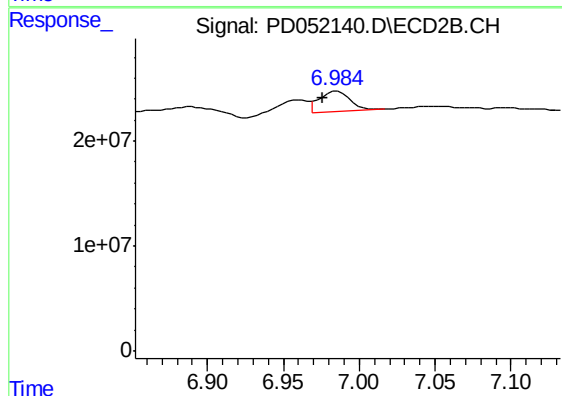

#15 Endosulfan II


R.T.: 6.985 min
Delta R.T.: 0.009 min
Response: 28532189
Conc: 1.13 ng/ml

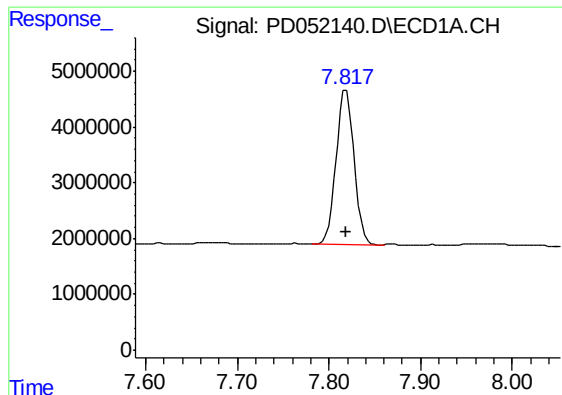

#27 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 37727678
Conc: 24.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5L7

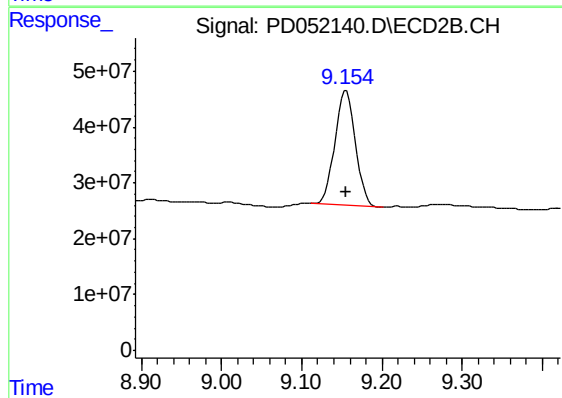

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 367408354
Conc: 23.80 ng/ml