

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032522\
 Data File : PD068752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 11:48
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 16:35:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.172	27959665	241.5E6	23.028	25.261
28)	SA Decachlor...	8.202	9.365	30345397	145.9E6	24.019	25.738
Target Compounds							
9)	A Endosulfan I	5.496	6.448	15933167	123.3E6	11.387	13.144
10)	B gamma-Chl...	5.384	6.322	17412238	136.1E6	11.479	13.206
12)	B 4,4'-DDE	5.609	6.547	30441775	229.4E6	22.252	24.752
13)	MA Dieldrin	5.740	6.707	32756458	244.9E6	22.434	25.214
19)	B Endosulfa...	6.654	7.481	27065965	174.0E6	21.165	23.660
20)	A Methoxychlor	6.916	7.794	69346553	384.1E6	100.063	105.379
21)	B Endrin ke...	7.147	7.955	33034996	194.8E6	22.440	25.146



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032522\
Data File : PD068752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 11:48
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 16:35:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

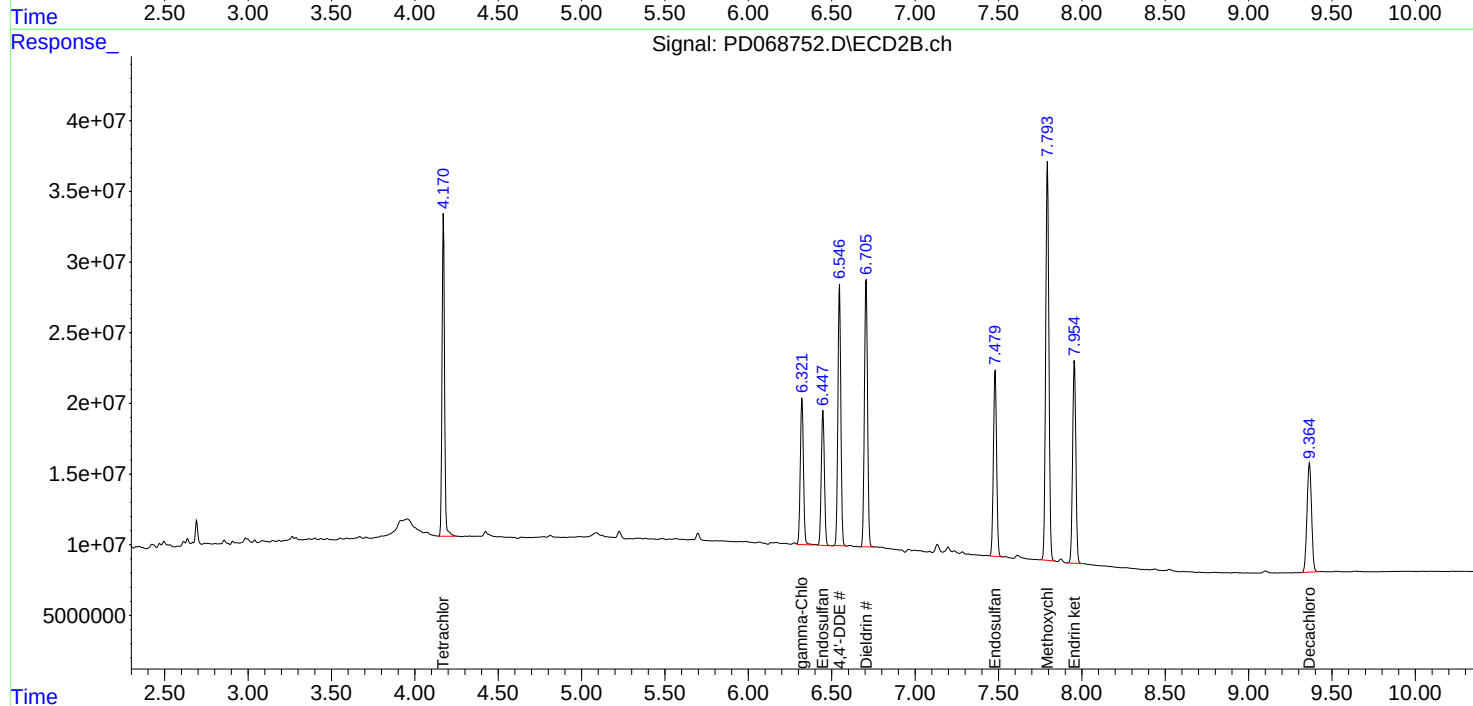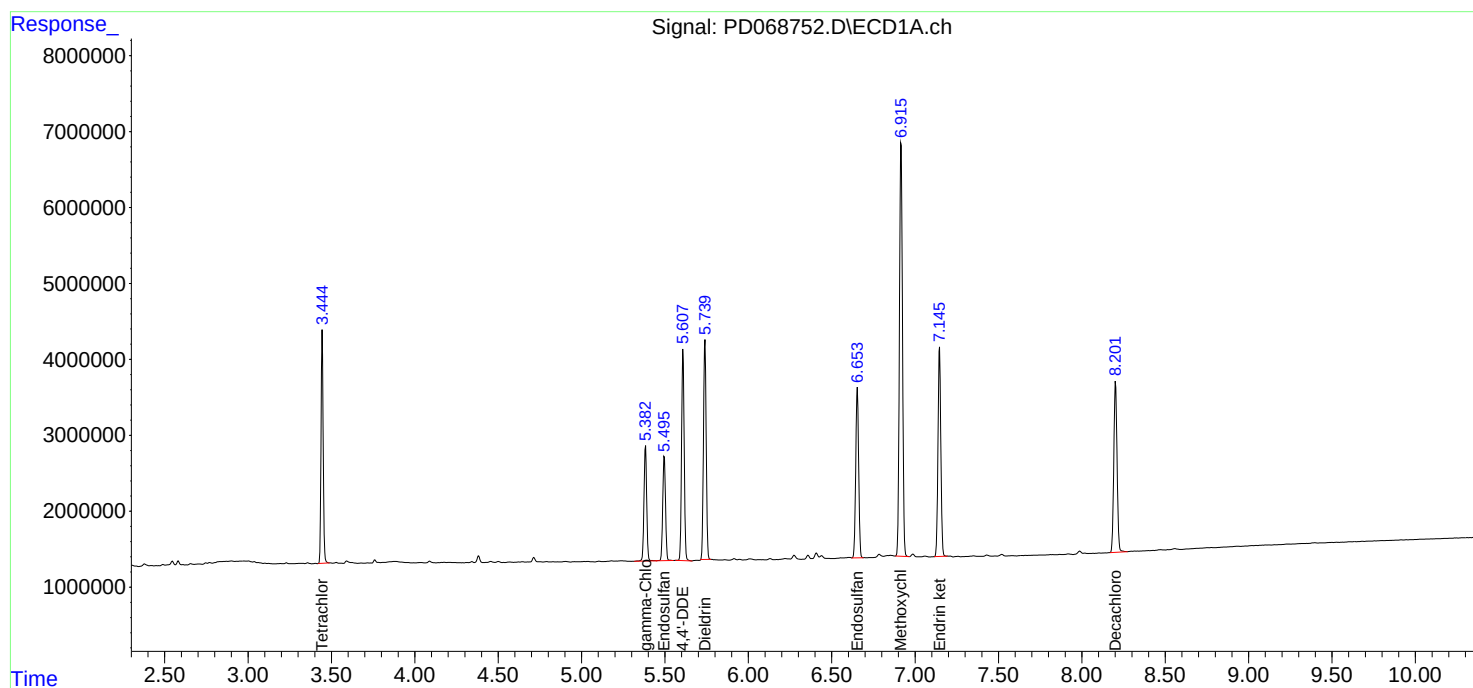


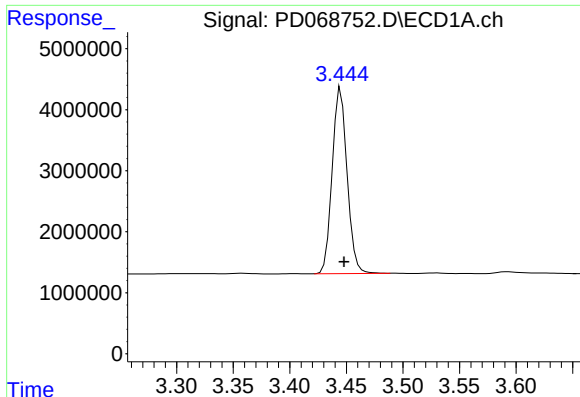

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: -0.003 min
Response: 27959665
Conc: 23.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

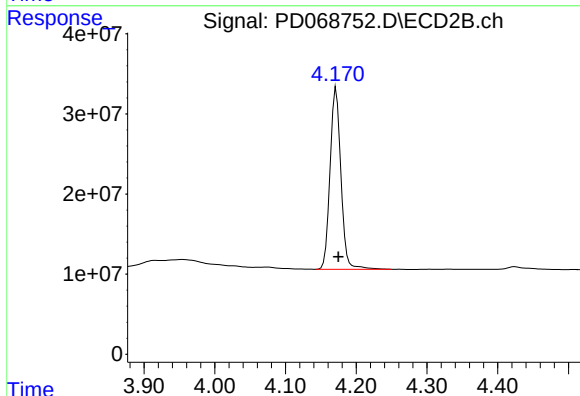


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.003 min
Response: 241513942
Conc: 25.26 ng/ml

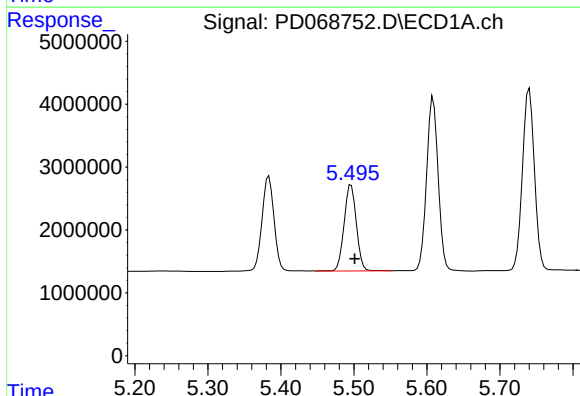


#9 Endosulfan I

R.T.: 5.496 min
Delta R.T.: -0.005 min
Response: 15933167
Conc: 11.39 ng/ml

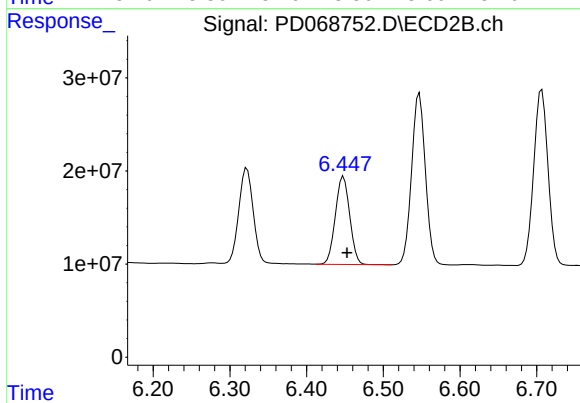

#9 Endosulfan I


R.T.: 6.448 min
Delta R.T.: -0.005 min
Response: 123269478
Conc: 13.14 ng/ml

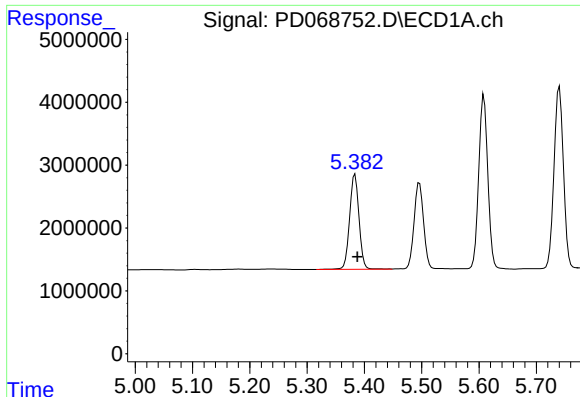

#10 gamma-Chlordane


R.T.: 5.384 min
Delta R.T.: -0.005 min
Response: 17412238
Conc: 11.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

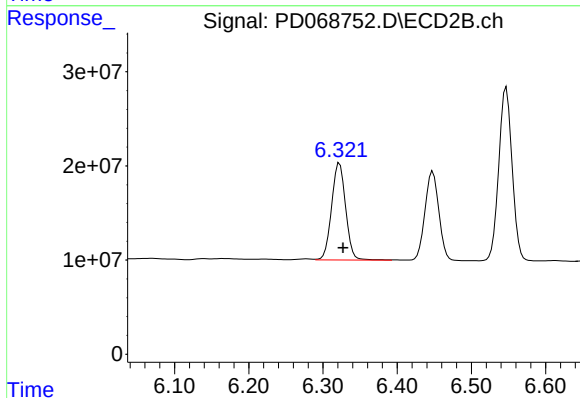


#10 gamma-Chlordane

R.T.: 6.322 min
Delta R.T.: -0.005 min
Response: 136121293
Conc: 13.21 ng/ml

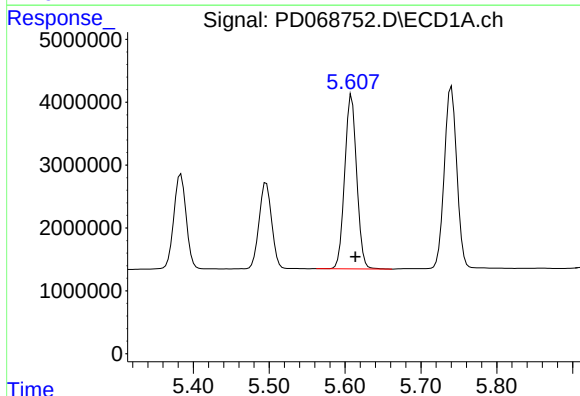


#12 4,4'-DDE

R.T.: 5.609 min
Delta R.T.: -0.005 min
Response: 30441775
Conc: 22.25 ng/ml

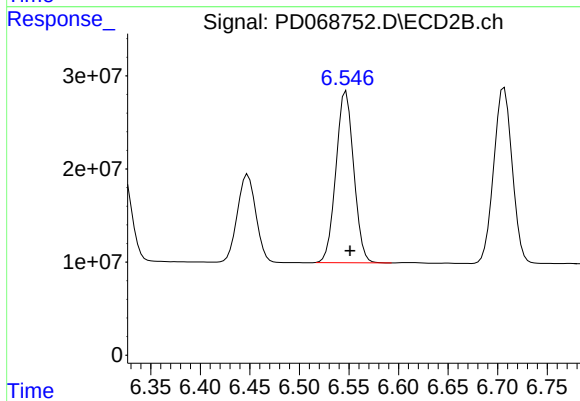

#12 4,4'-DDE


R.T.: 6.547 min
Delta R.T.: -0.004 min
Response: 229374838
Conc: 24.75 ng/ml

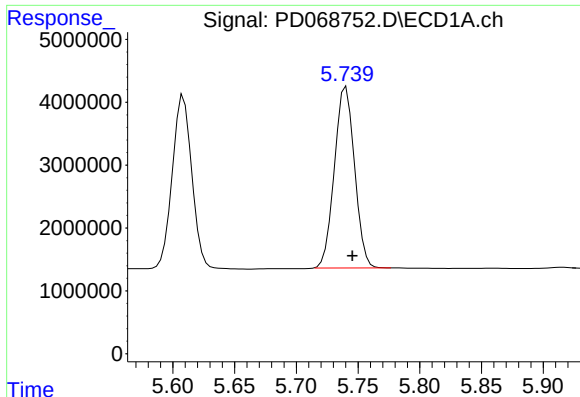

#13 Dieldrin


R.T.: 5.740 min
Delta R.T.: -0.005 min
Response: 32756458
Conc: 22.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

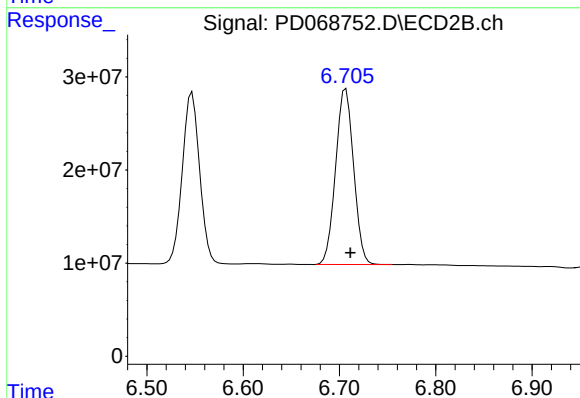


#13 Dieldrin

R.T.: 6.707 min
Delta R.T.: -0.005 min
Response: 244909301
Conc: 25.21 ng/ml

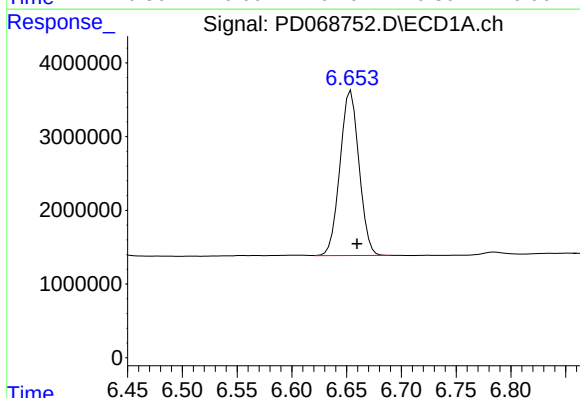


#19 Endosulfan Sulfate

R.T.: 6.654 min
Delta R.T.: -0.006 min
Response: 27065965
Conc: 21.16 ng/ml

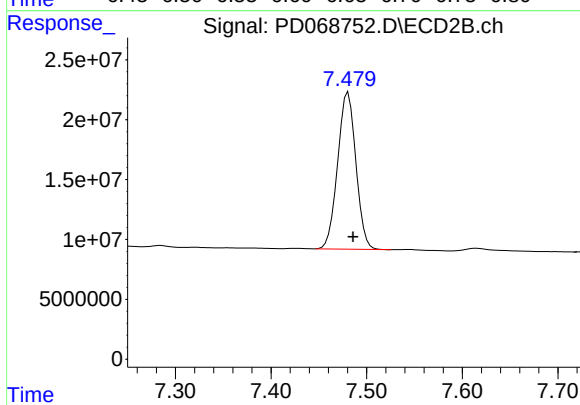

#19 Endosulfan Sulfate


R.T.: 7.481 min
Delta R.T.: -0.005 min
Response: 174019274
Conc: 23.66 ng/ml

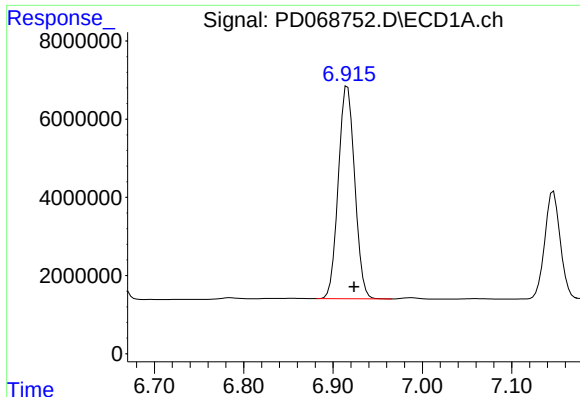

#20 Methoxychlor


R.T.: 6.916 min
Delta R.T.: -0.007 min
Response: 69346553
Conc: 100.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

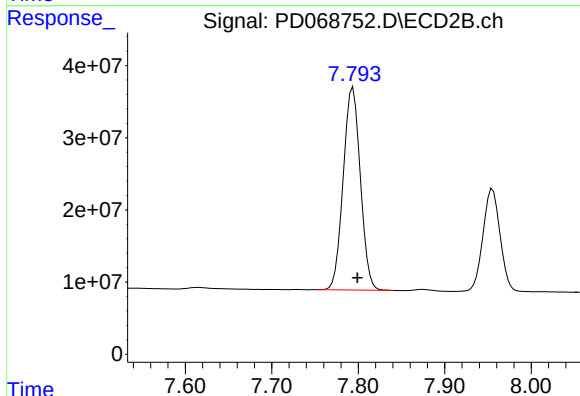


#20 Methoxychlor

R.T.: 7.794 min
Delta R.T.: -0.005 min
Response: 384137887
Conc: 105.38 ng/ml

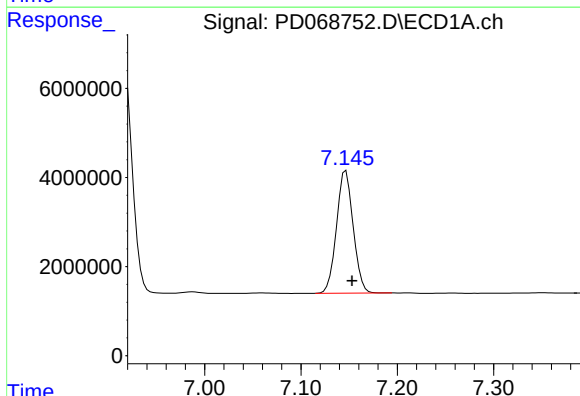


#21 Endrin ketone

R.T.: 7.147 min
Delta R.T.: -0.006 min
Response: 33034996
Conc: 22.44 ng/ml

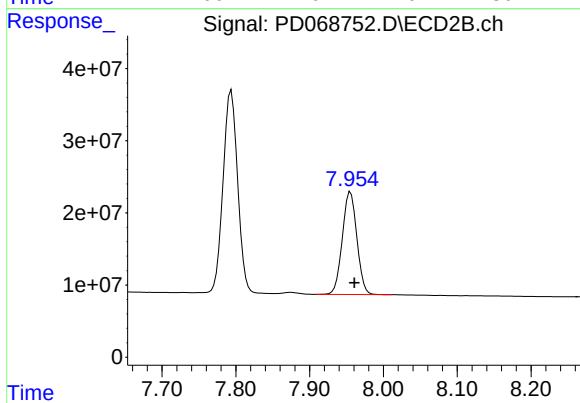

#21 Endrin ketone


R.T.: 7.955 min
Delta R.T.: -0.005 min
Response: 194846967
Conc: 25.15 ng/ml

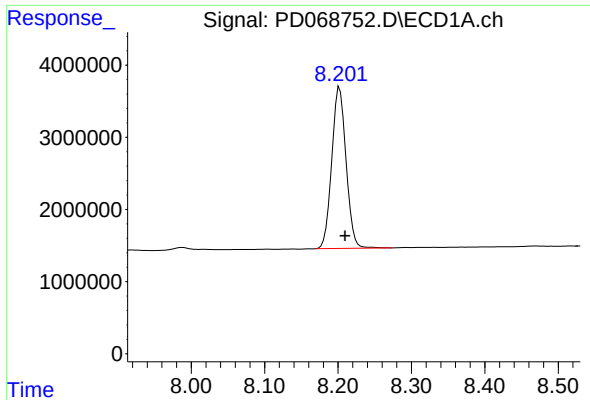

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.007 min
Response: 30345397
Conc: 24.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

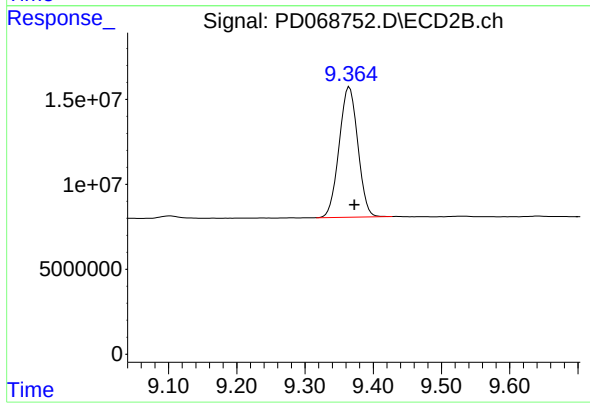

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: -0.007 min
Response: 145851150
Conc: 25.74 ng/ml