

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032523\
 Data File : PD074464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 14:16
 Operator : AR\AJ
 Sample : 01993-04MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EYGC6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/27/2023
 Supervised By : Ankita Jodhani 03/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 22:52:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.549	2.770	44271755	22451696	17.820	17.846
2) SA Decachlor...	9.093	7.922	86809009	37864240	31.717	31.622
Target Compounds						
2) A alpha-BHC	4.006	3.274	196.3E6	87923618	50.301	49.199
3) MA gamma-BHC...	4.339	3.604	179.0E6	79938314	48.492	46.802
4) MA Heptachlor	4.931	3.945	172.6E6	77433647	45.593	46.700
5) MB Aldrin	5.275	4.226	181.2E6	83077145	49.591	48.522
6) B beta-BHC	4.532	3.899	77819358	35355197	46.032m	43.640
7) B delta-BHC	4.783	4.130	175.5E6	83277036	48.229	47.082
8) B Heptachlo...	5.702	4.729	153.5E6	71873172	46.768	45.369
9) A Endosulfan I	6.089	5.099	142.9E6	66830646	47.906	47.662
10) B trans-Chl...	5.958	4.979	153.2E6	73050770	47.750	47.220
11) B cis-Chlor...	6.038	5.044	154.9E6	76164499	47.276	48.149
12) B 4,4'-DDE	6.210	5.234	303.1E6	140.6E6	101.174	96.775
13) MA Dieldrin	6.364	5.364	329.8E6	153.0E6	103.971	98.683
14) MA Endrin	6.595	5.640	259.2E6	127.9E6	98.368	95.089
15) B Endosulfa...	6.813	5.934	268.1E6	124.9E6	97.135	92.862
16) A 4,4'-DDD	6.727	5.788	251.7E6	116.1E6	106.522	98.641
17) MA 4,4'-DDT	7.043	6.040	251.9E6	116.6E6	100.386	93.066
18) B Endrin al...	6.944	6.114	197.9E6	93049582	87.840	84.646
19) B Endosulfa...	7.179	6.336	250.6E6	115.4E6	96.202	91.652
20) A Methoxychlor	7.518	6.616	661.2E6	277.7E6	481.649	451.409
21) B Endrin ke...	7.665	6.843	302.7E6	142.9E6	102.092	93.928

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032523\
Data File : PD074464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 14:16
Operator : AR\AJ
Sample : 01993-04MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 22:52:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

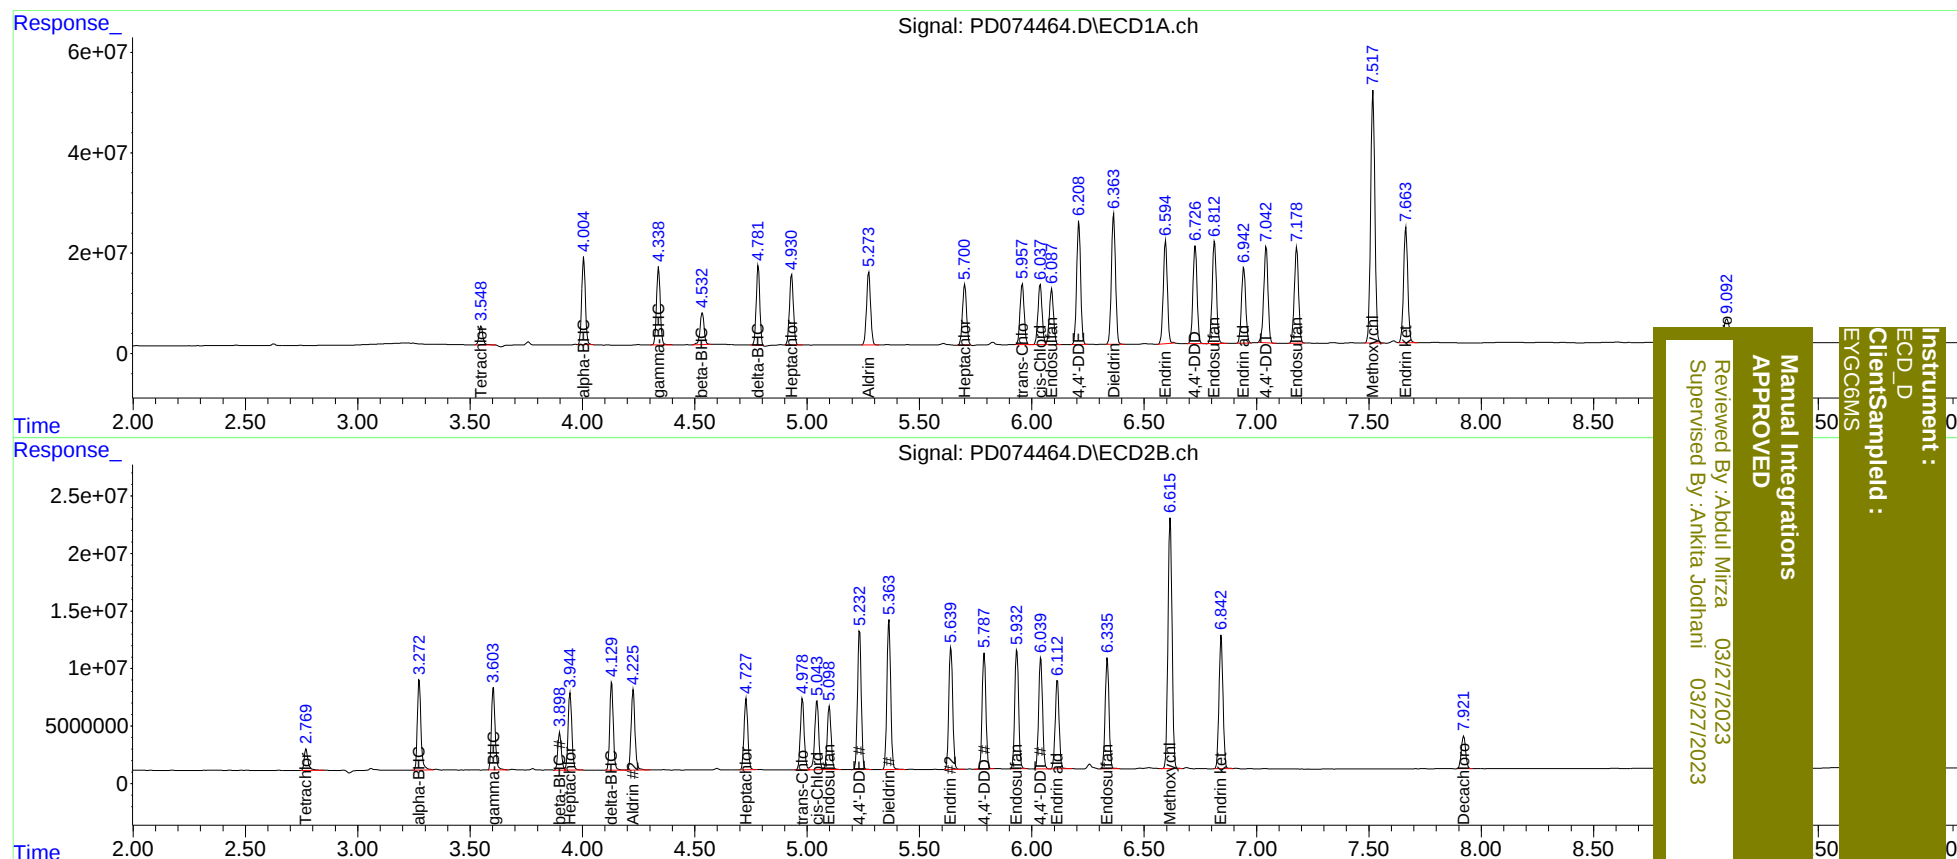

26066
Reviewed By: Abdul Miza 03/27/2023
Supervised By: Ankita Jodhani 03/27/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EYGC6MS