

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032523\
 Data File : PD074465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 14:30
 Operator : AR\AJ
 Sample : 01993-05MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EYGC6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/27/2023
 Supervised By :Ankita Jodhani 03/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 22:52:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	44575320	22913240	17.942	18.213
27)	SA Decachlor...	9.094	7.922	87574318	38444420	31.997	32.107
Target Compounds							
2)	A alpha-BHC	4.006	3.274	200.5E6	90150440	51.393	50.445
3)	MA gamma-BHC...	4.339	3.604	182.6E6	82205510	49.481	48.129
4)	MA Heptachlor	4.932	3.946	175.5E6	79335998	46.355	47.848
5)	MB Aldrin	5.275	4.227	184.6E6	85038530	50.499	49.668
6)	B beta-BHC	4.533	3.900	80223962	36159691	47.454m	44.633
7)	B delta-BHC	4.783	4.131	178.2E6	85337834	48.969	48.248
8)	B Heptachlo...	5.702	4.729	155.9E6	73318494	47.479	46.282
9)	A Endosulfan I	6.089	5.100	145.6E6	68361753	48.795	48.754
10)	B trans-Chl...	5.959	4.980	156.2E6	74711957	48.673	48.294
11)	B cis-Chlor...	6.038	5.044	157.9E6	77873630	48.193	49.229
12)	B 4,4'-DDE	6.210	5.234	308.5E6	144.0E6	103.003	99.103
13)	MA Dieldrin	6.365	5.365	335.4E6	156.5E6	105.735	100.945
14)	MA Endrin	6.595	5.641	262.8E6	130.7E6	99.737	97.117
15)	B Endosulfa...	6.814	5.934	272.6E6	127.3E6	98.759	94.720
16)	A 4,4'-DDD	6.728	5.789	255.7E6	118.7E6	108.196	100.803
17)	MA 4,4'-DDT	7.043	6.041	256.4E6	119.3E6	102.179	95.226
18)	B Endrin al...	6.944	6.114	200.0E6	94768662	88.801	86.209
19)	B Endosulfa...	7.180	6.337	254.5E6	117.8E6	97.725	93.558
20)	A Methoxychlor	7.519	6.616	672.2E6	282.1E6	489.630	458.711
21)	B Endrin ke...	7.666	6.843	307.8E6	145.7E6	103.806	95.745

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032523\
Data File : PD074465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 14:30
Operator : AR\AJ
Sample : 01993-05MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 22:52:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

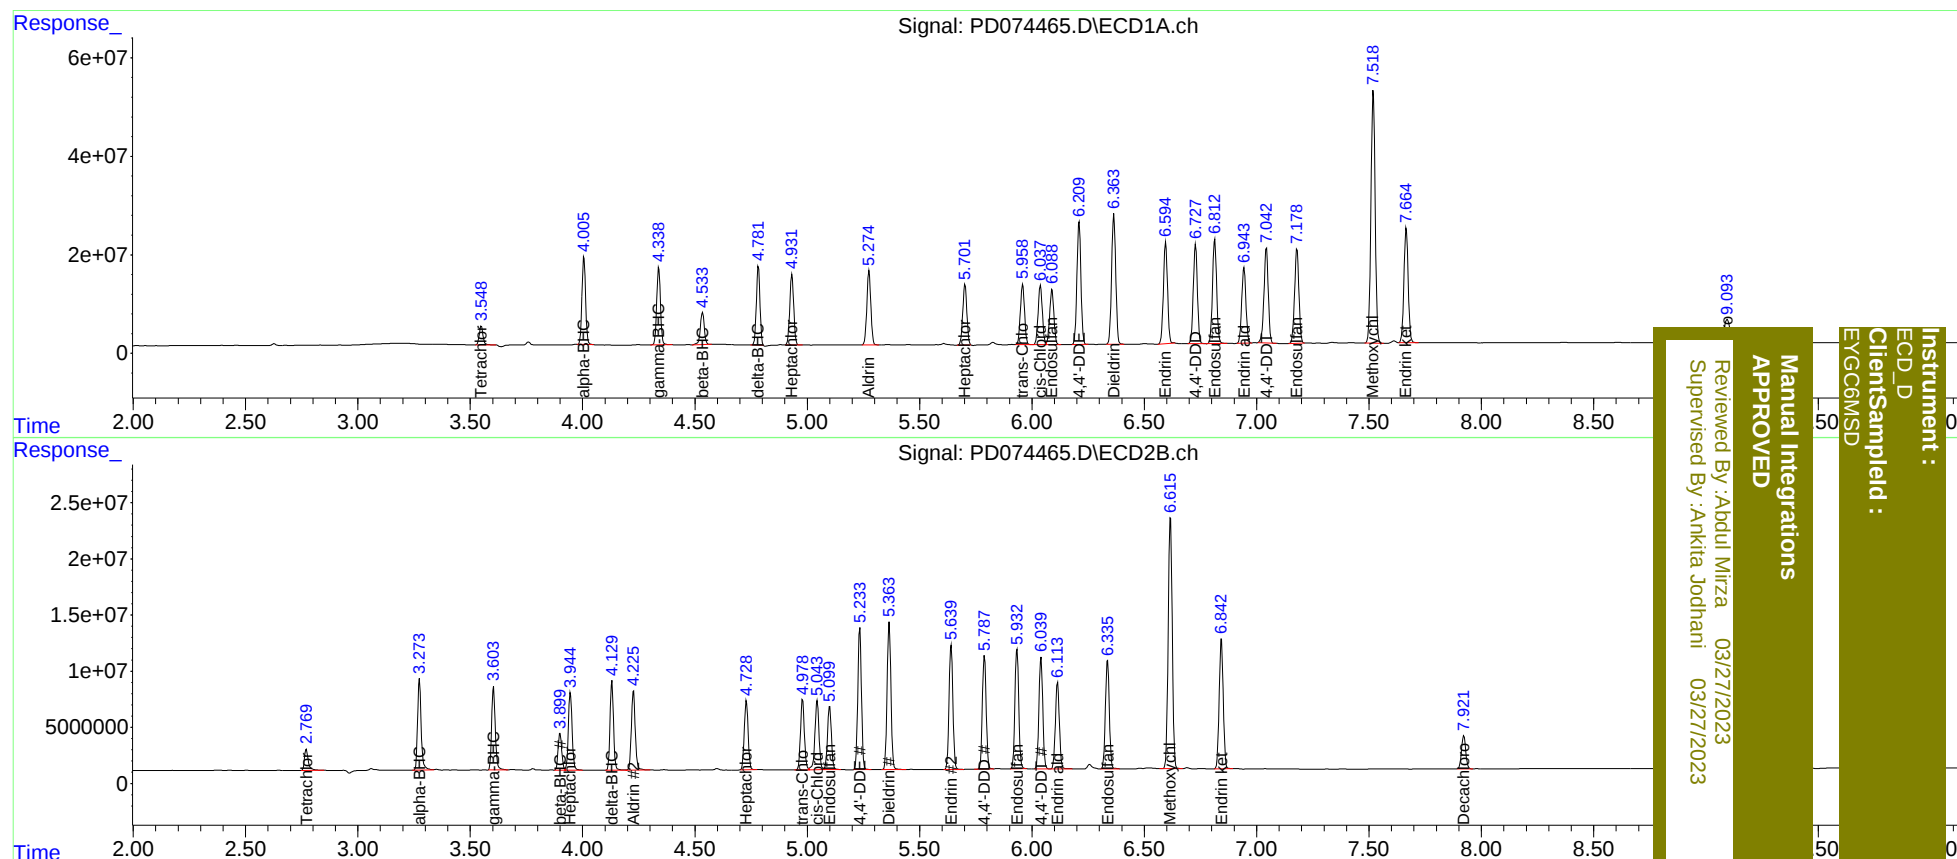

Instrument :
ECD_D
ClientSampled :
EYGC6MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 03/27/2023
Supervised By: Ankita Jodhani 03/27/2023