

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032523\
 Data File : PD074459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 13:09
 Operator : AR\AJ
 Sample : PB151643BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS643

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/27/2023
 Supervised By :Ankita Jodhani 03/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 22:50:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 14 03:05:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.770	48830657	24137350	19.655	19.185
27)	SA Decachlor...	9.099	7.925	101.8E6	44270354	37.200	36.972
Target Compounds							
2)	A alpha-BHC	4.007	3.273	17873206	8159927	4.580	4.566
3)	MA gamma-BHC...	4.339	3.604	17193788	7771847	4.658m	4.550
4)	MA Heptachlor	4.933	3.945	18231395	8156655	4.816	4.919
5)	MB Aldrin	5.275	4.226	18766561	8448651	5.135m	4.935
6)	B beta-BHC	4.534	3.900	9286069	4442117	5.493m	5.483
7)	B delta-BHC	4.784	4.131	20249732	7202317	5.565	4.072 #
8)	B Heptachlo...	5.704	4.729	16999908	7570655	5.178	4.779
9)	A Endosulfan I	6.091	5.100	15699825	6980767	5.263	4.979
10)	B trans-Chl...	5.961	4.980	16631868	7627789	5.184	4.931
11)	B cis-Chlor...	6.041	5.045	17143952	7775883	5.232	4.916
12)	B 4,4'-DDE	6.213	5.234	29356359	13598508	9.801	9.362
13)	MA Dieldrin	6.368	5.365	32846544	15034735	10.354	9.698
14)	MA Endrin	6.598	5.641	24269995	12494114	9.210	9.287
15)	B Endosulfa...	6.817	5.934	30296059	13440354	10.976	9.997m
16)	A 4,4'-DDD	6.731	5.790	25677586	12365840	10.865	10.503
17)	MA 4,4'-DDT	7.046	6.042	23702656	10631314	9.446	8.486
18)	B Endrin al...	6.947	6.115	22325555	10634383	9.912	9.674
19)	B Endosulfa...	7.182	6.338	26905766	12591020	10.330	10.002
20)	A Methoxychlor	7.523	6.618	67024757	30767559	48.821	50.022
21)	B Endrin ke...	7.669	6.845	32433370	16019115	10.939	10.528

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032523\
Data File : PD074459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 13:09
Operator : AR\AJ
Sample : PB151643BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 22:50:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031323CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 14 03:05:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

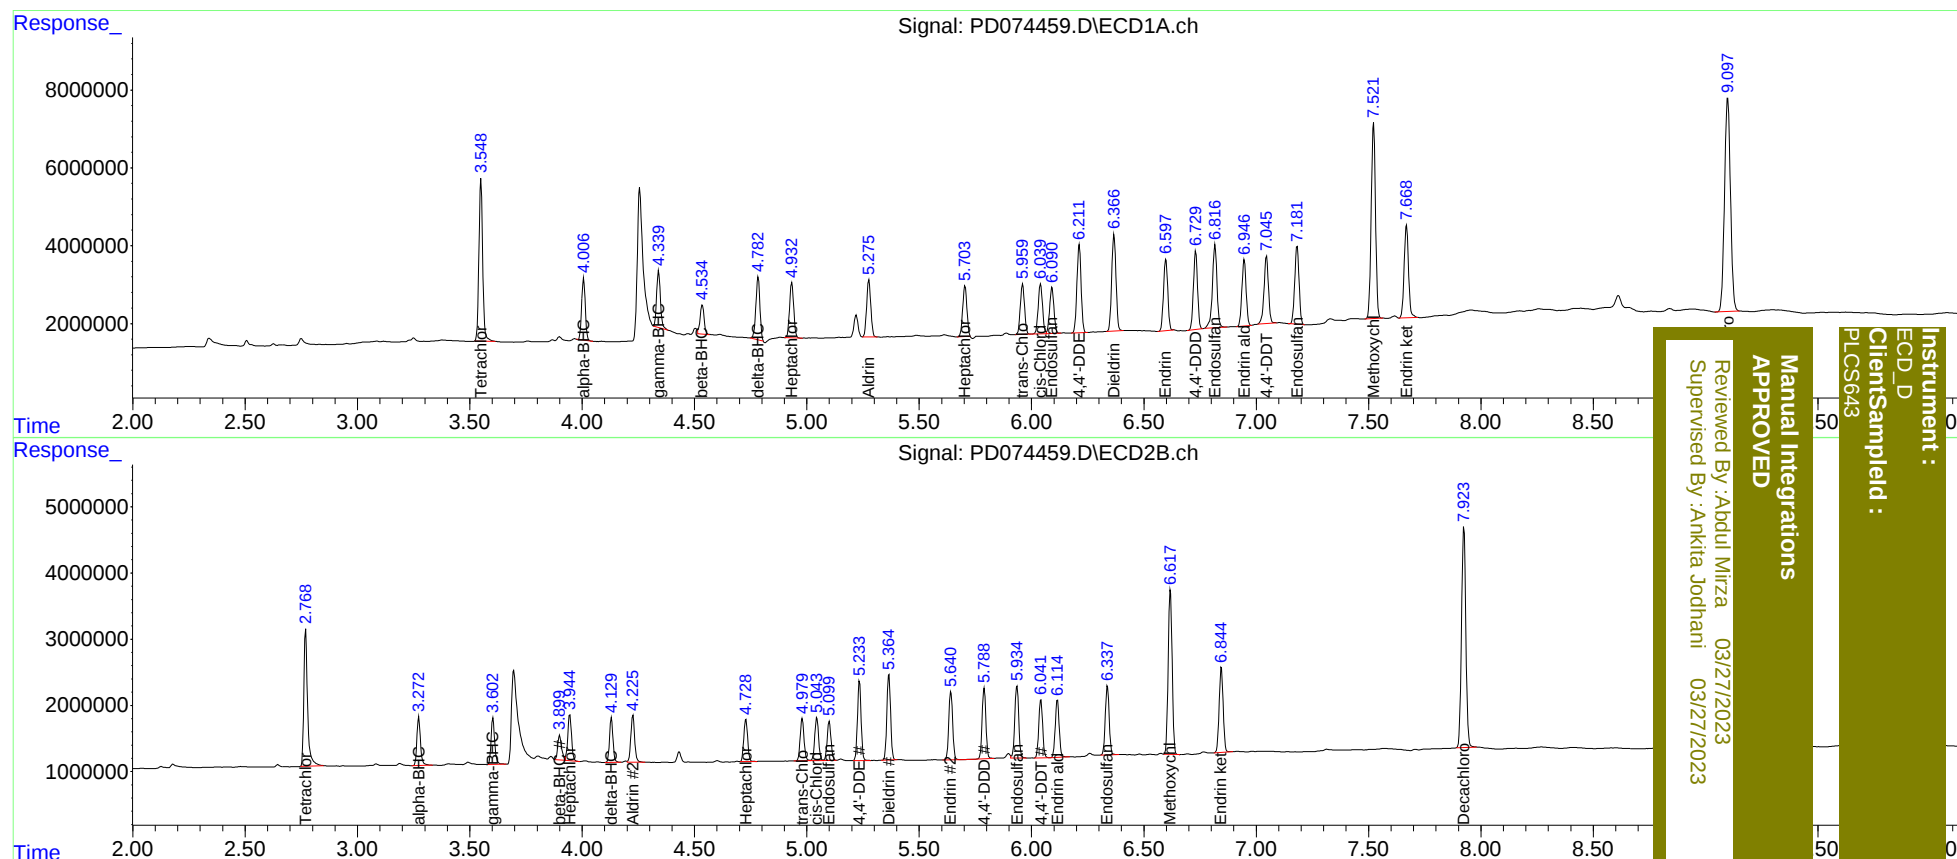

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/27/2023
Supervised By: Ankita Jodhani 03/27/2023

Instrument :
ECD_D
Client Sampled :
PLCS643