

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032619\
 Data File : PD052145.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 7:23
 Operator : AJ\SJ
 Sample : PIBLK47
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 08:01:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.041	34869962	739.5E6	24.566	25.416
27)	SA Decachlor...	7.820	9.156	67822690	716.8E6	43.313	46.436
Target Compounds							
8)	B Heptachlo...	0.000	5.922	0 96156816	N.D.	2.823	
9)	A Endosulfan I	0.000	6.236f	0 22893603	N.D.	0.730	
10)	B trans-Chl...	0.000	6.206f	0 39055942	N.D.	1.150	
11)	B cis-Chlor...	0.000	6.236	0 22893603	N.D.	0.705	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032619\
Data File : PD052145.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 7:23
Operator : AJ\SJ
Sample : PIBLK47
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 08:01:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

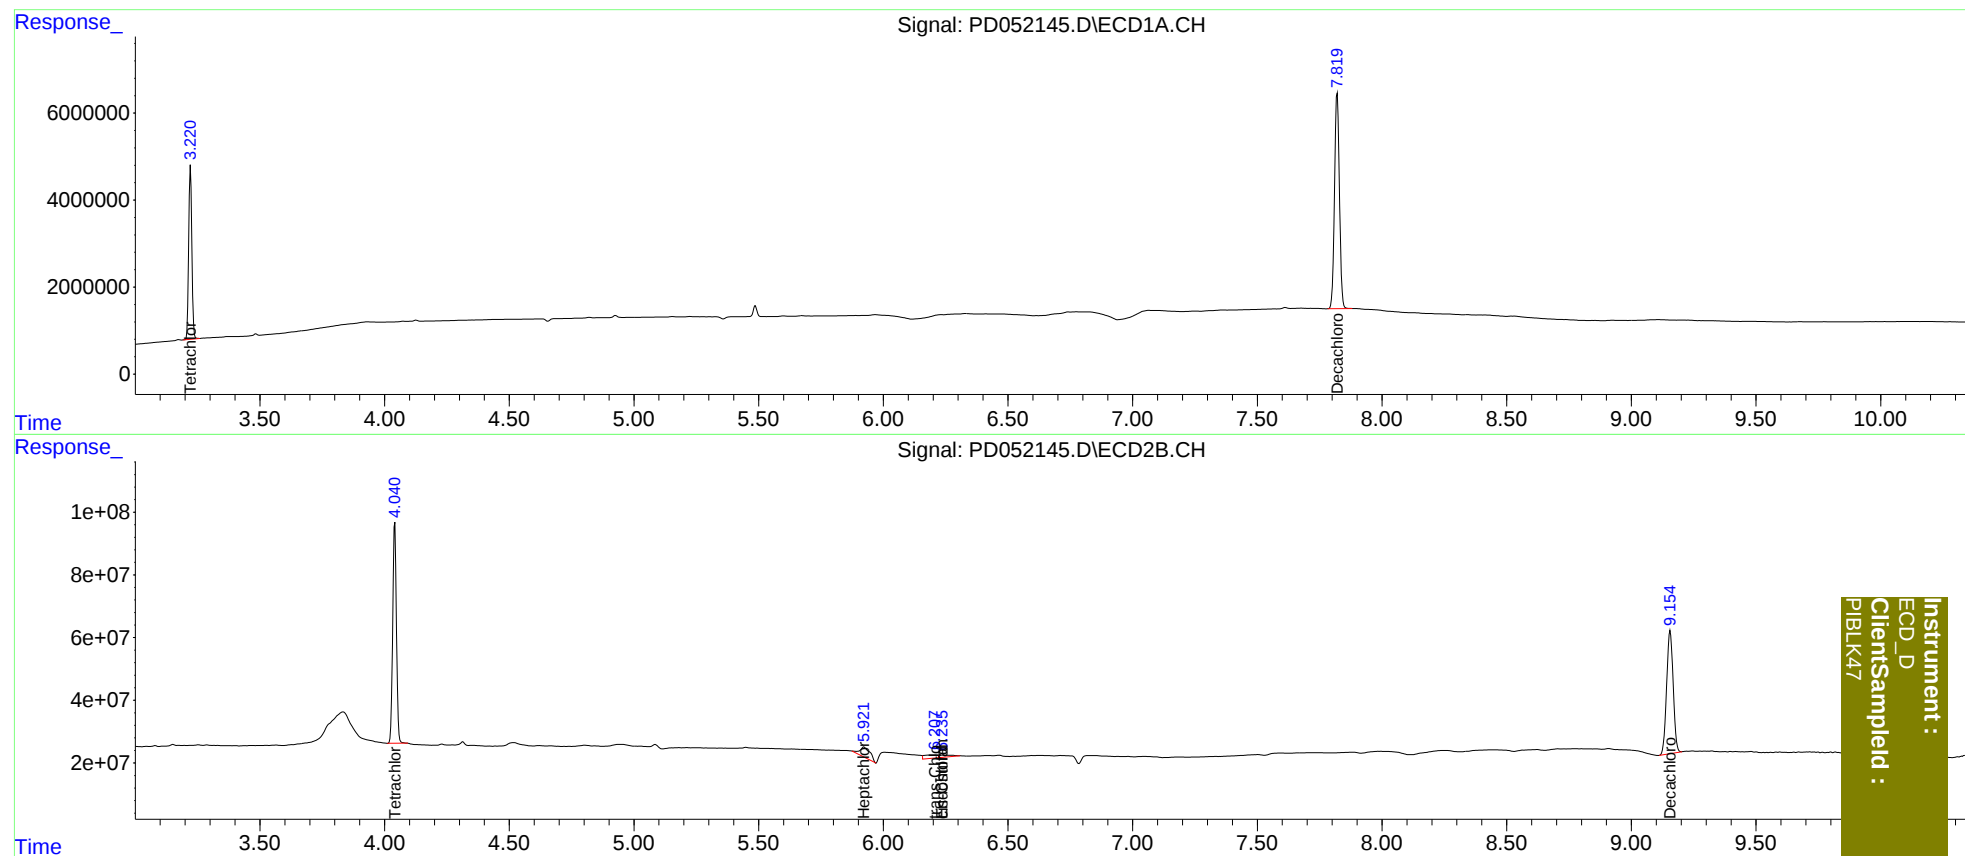


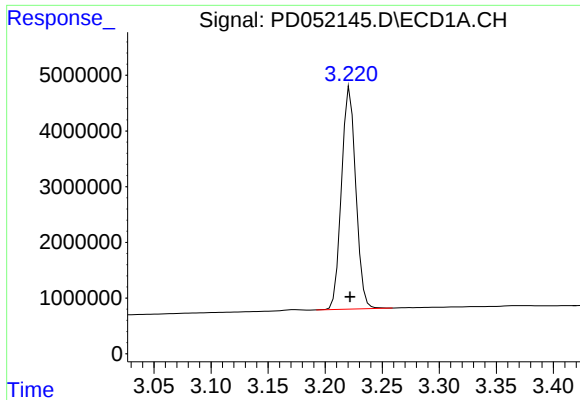

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 34869962
Conc: 24.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK47

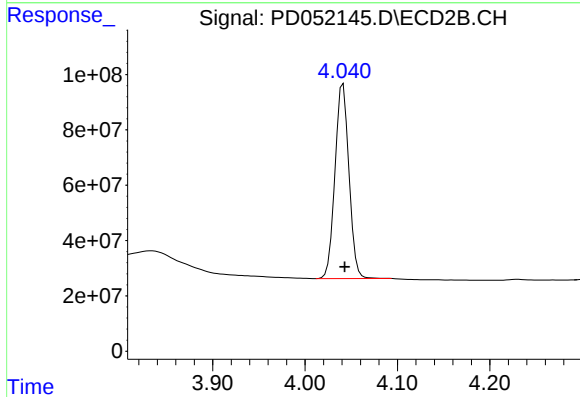


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 739523664
Conc: 25.42 ng/ml

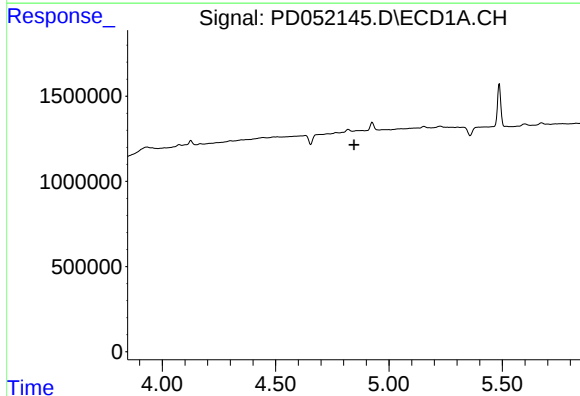


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

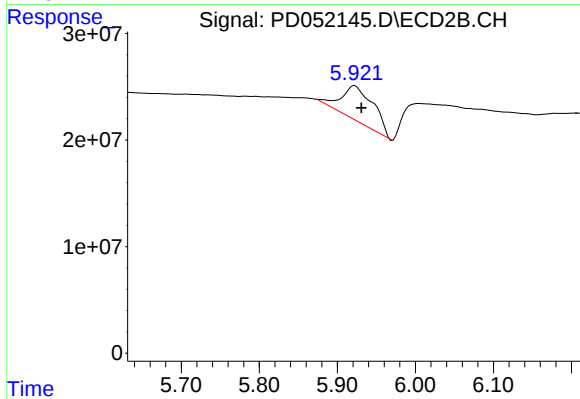

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 96156816
Conc: 2.82 ng/ml

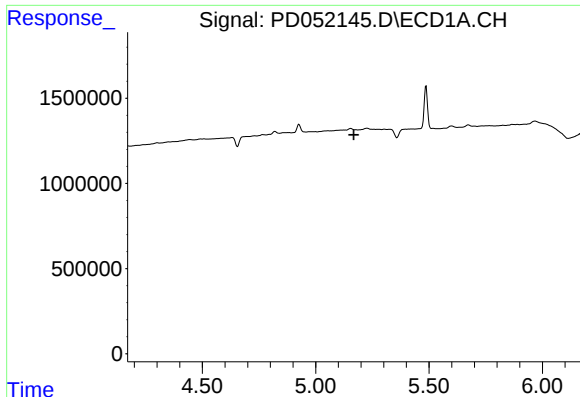

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK47

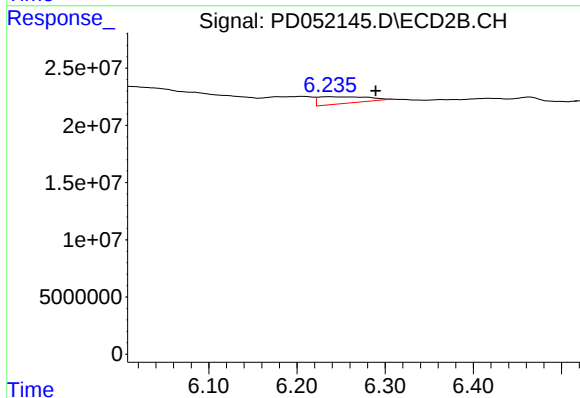


#9 Endosulfan I

R.T.: 6.236 min
Delta R.T.: -0.053 min
Response: 22893603
Conc: 0.73 ng/ml

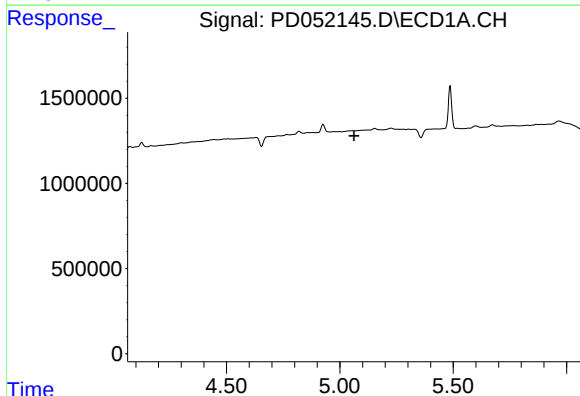


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

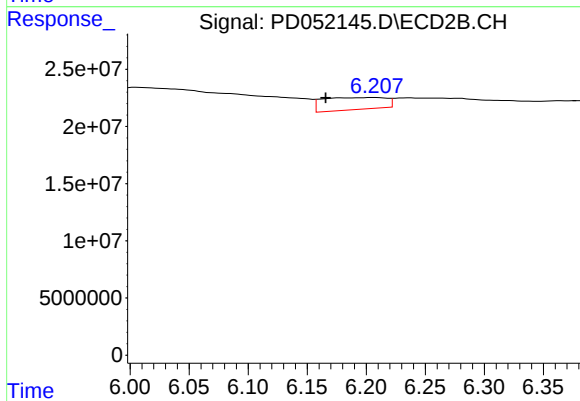

#10 trans-Chlordane


R.T.: 6.206 min
Delta R.T.: 0.040 min
Response: 39055942
Conc: 1.15 ng/ml

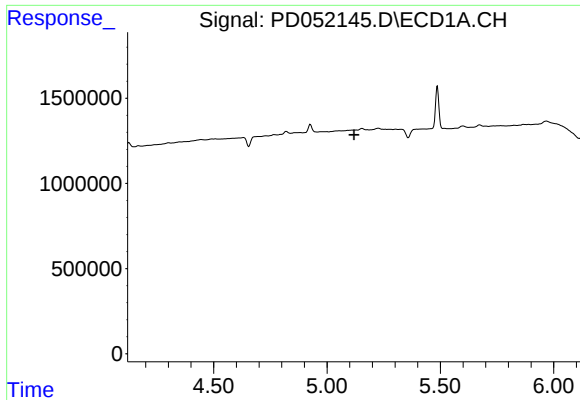

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK47

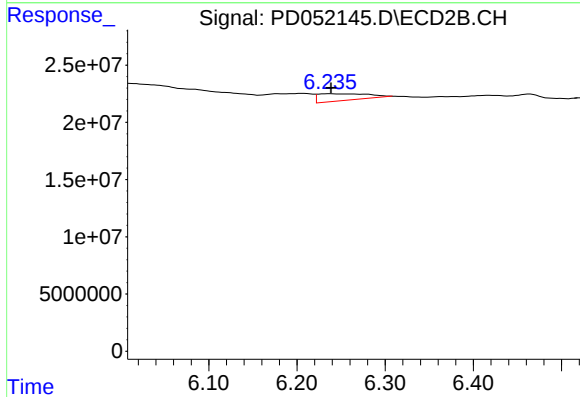


#11 cis-Chlordane

R.T.: 6.236 min
Delta R.T.: -0.002 min
Response: 22893603
Conc: 0.71 ng/ml

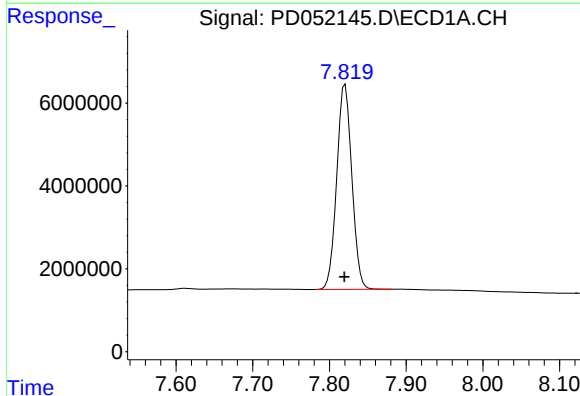

#27 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: 0.001 min
Response: 67822690
Conc: 43.31 ng/ml

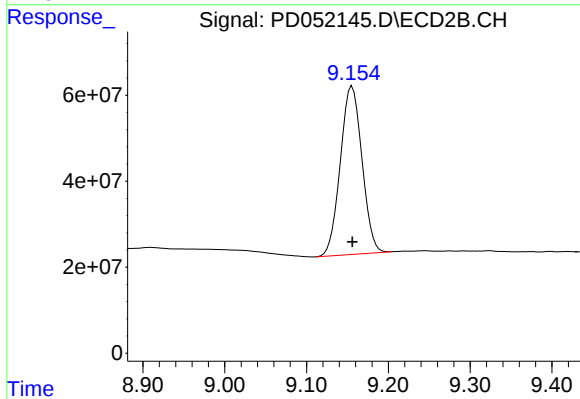

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 716820178
Conc: 46.44 ng/ml