

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032619\
 Data File : PD052148.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 8:19
 Operator : AJ\SJ
 Sample : K2044-10RE
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5W6RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 08:02:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	23253270	477.1E6	16.382	16.398
27)	SA Decachlor...	7.819	9.155	35321398	400.1E6	22.557	25.919
Target Compounds							
2)	A alpha-BHC	0.000	4.404f	0 45640948	N.D.	1.044	
3)	MA gamma-BHC...	3.921	4.689f	14414433	15324876	6.433	0.386 #
7)	B delta-BHC	0.000	5.080f	0 48743252	N.D.	1.229	
8)	B Heptachlo...	0.000	5.910	0 47882409	N.D.	1.406	
9)	A Endosulfan I	0.000	6.252f	0 23922840	N.D.	0.763	
10)	B trans-Chl...	0.000	6.203f	0 50575513	N.D.	1.489	
11)	B cis-Chlor...	0.000	6.252	0 23922840	N.D.	0.737	
14)	MA Endrin	0.000	6.829f	0 31183430	N.D.	1.355	
15)	B Endosulfa...	0.000	6.969	0 27763618	N.D.	1.095	
16)	A 4,4'-DDD	0.000	6.829f	0 31183430	N.D.	1.310	
19)	B Endosulfa...	0.000	7.300	0 12427381	N.D.	0.553	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032619\
Data File : PD052148.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 8:19
Operator : AJ\SJ
Sample : K2044-10RE
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 08:02:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

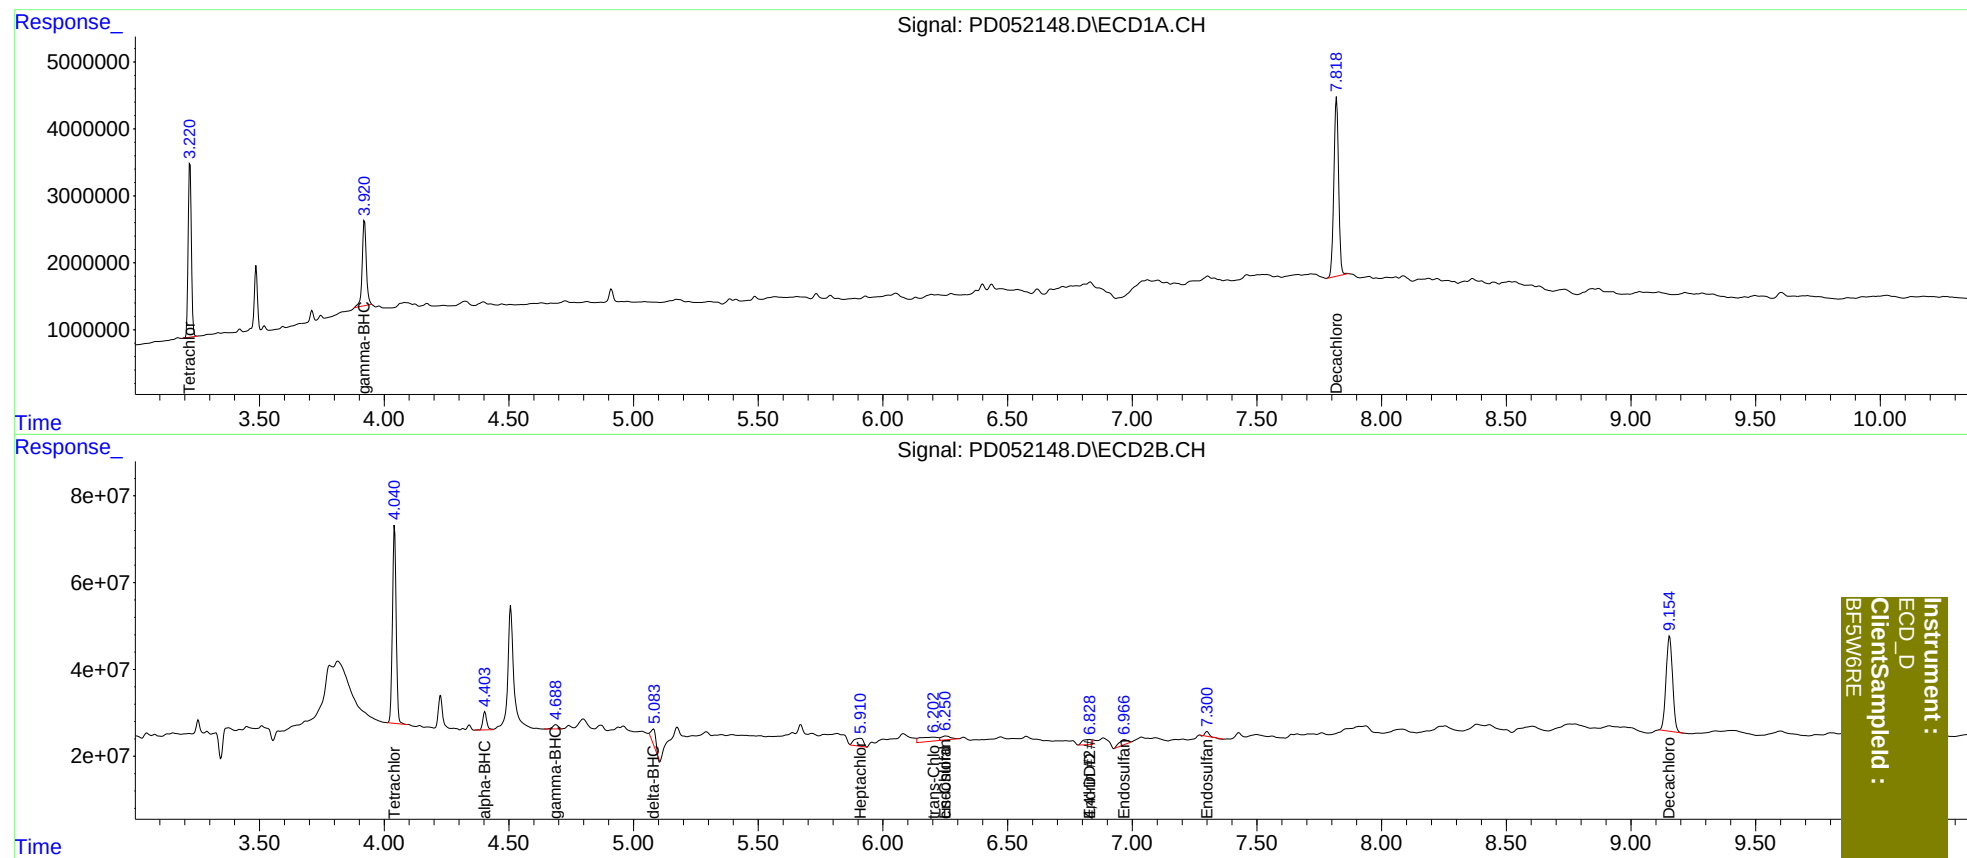


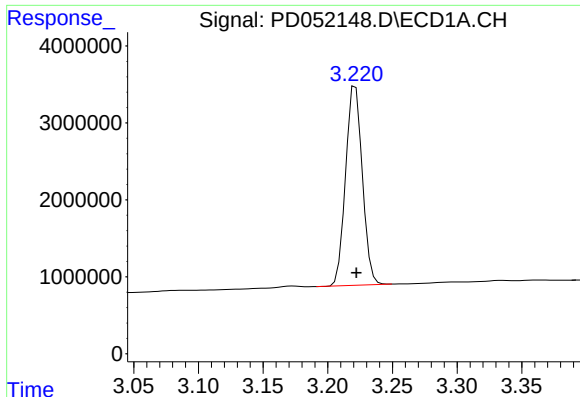

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 23253270
Conc: 16.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

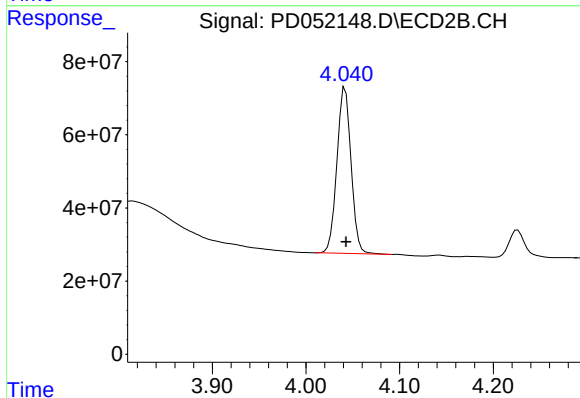


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 477142532
Conc: 16.40 ng/ml

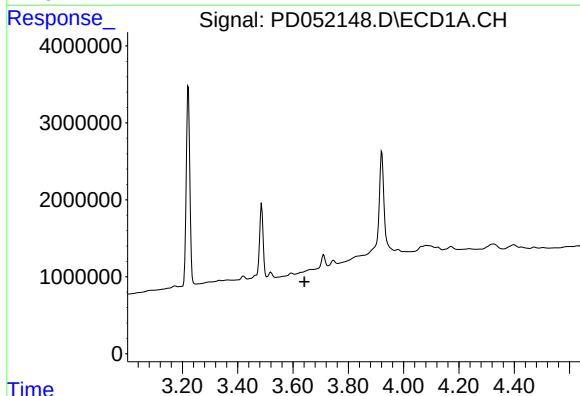


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

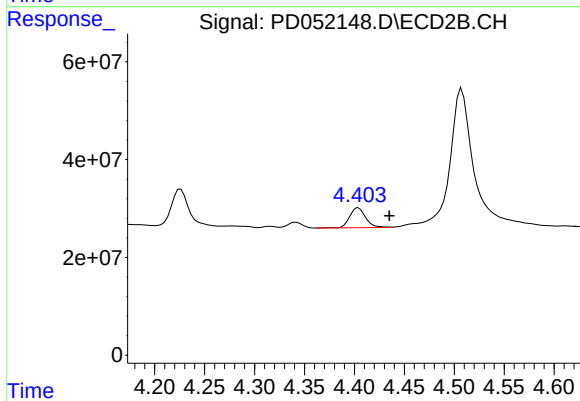

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: -0.031 min
Response: 45640948
Conc: 1.04 ng/ml

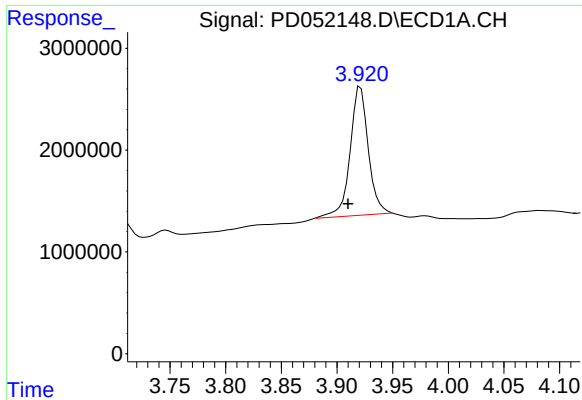

#3 gamma-BHC (Lindane)


R.T.: 3.921 min
Delta R.T.: 0.011 min
Response: 14414433
Conc: 6.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

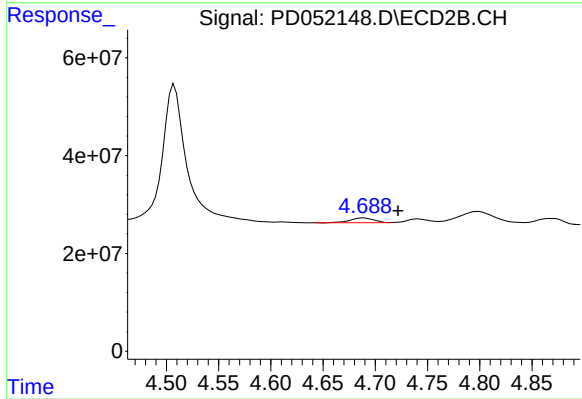


#3 gamma-BHC (Lindane)

R.T.: 4.689 min
Delta R.T.: -0.033 min
Response: 15324876
Conc: 0.39 ng/ml

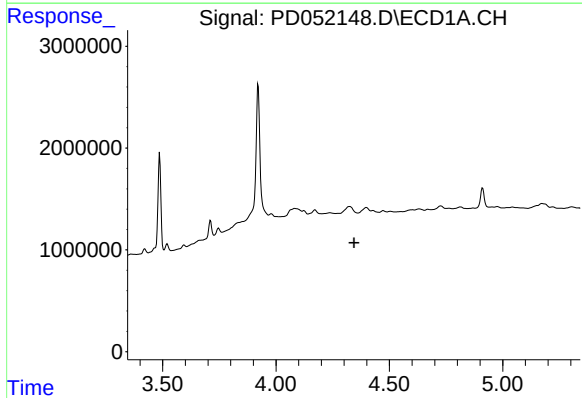


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.344 min
Response: 0
Conc: N.D.

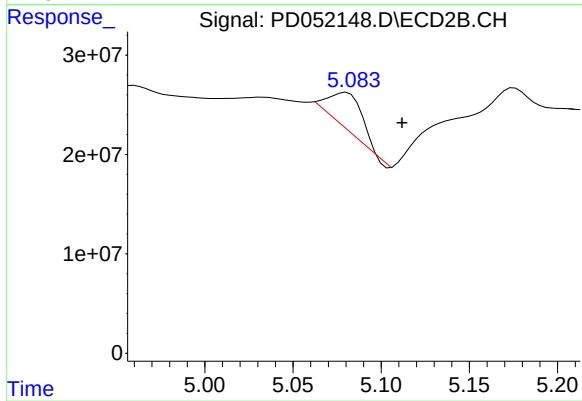

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: -0.031 min
Response: 48743252
Conc: 1.23 ng/ml

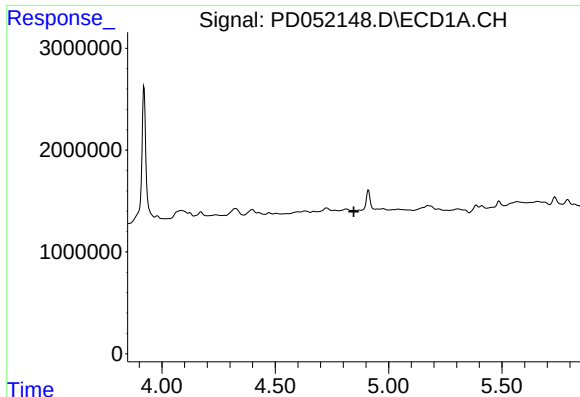

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

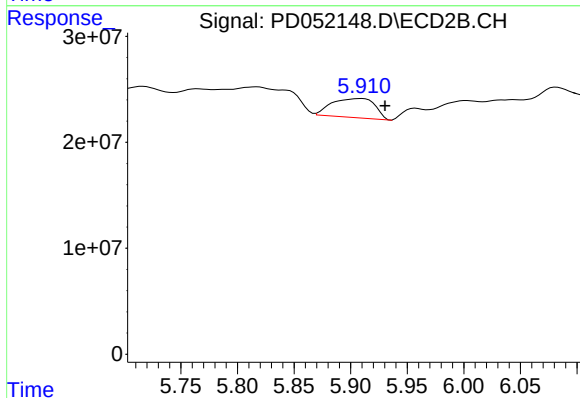


#8 Heptachlor epoxide

R.T.: 5.910 min
Delta R.T.: -0.020 min
Response: 47882409
Conc: 1.41 ng/ml

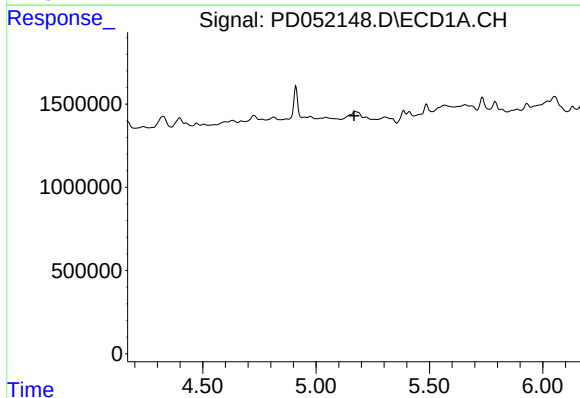


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

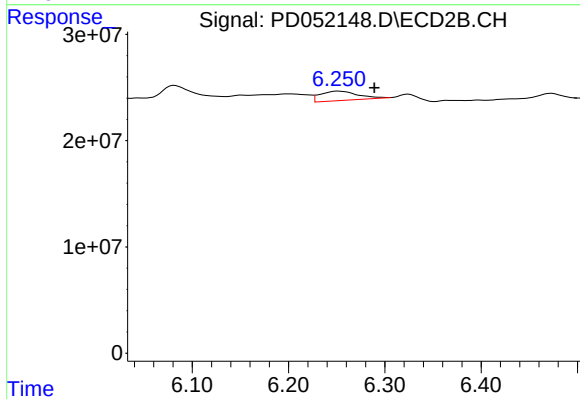

#9 Endosulfan I

R.T.: 6.252 min
Delta R.T.: -0.038 min
Response: 23922840
Conc: 0.76 ng/ml

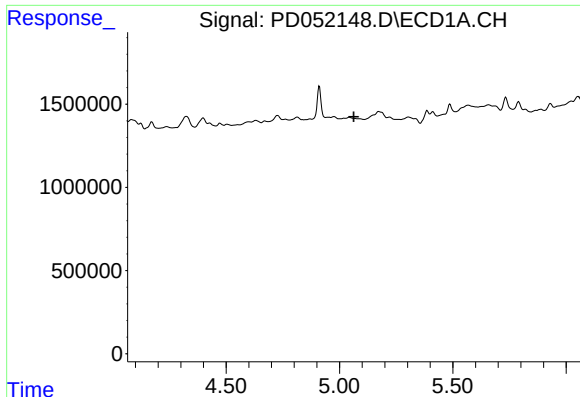

#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

#10 trans-Chlordane


R.T.: 6.203 min
Delta R.T.: 0.037 min
Response: 50575513
Conc: 1.49 ng/ml

#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

#11 cis-Chlordane


R.T.: 6.252 min
Delta R.T.: 0.013 min
Response: 23922840
Conc: 0.74 ng/ml

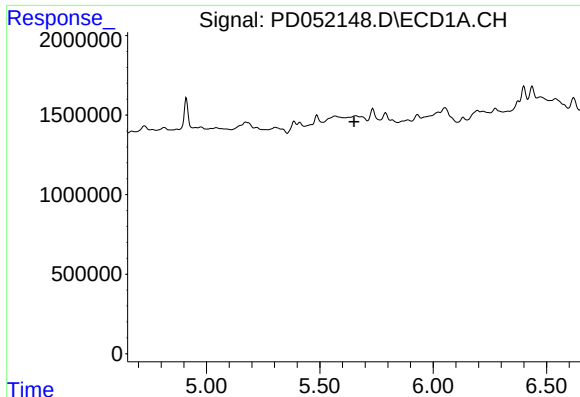

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

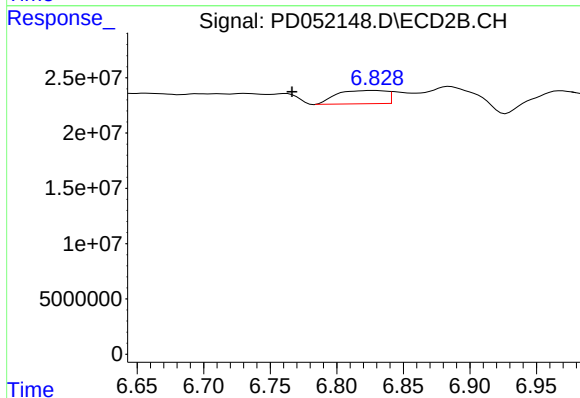


#14 Endrin

R.T.: 6.829 min
Delta R.T.: 0.063 min
Response: 31183430
Conc: 1.35 ng/ml

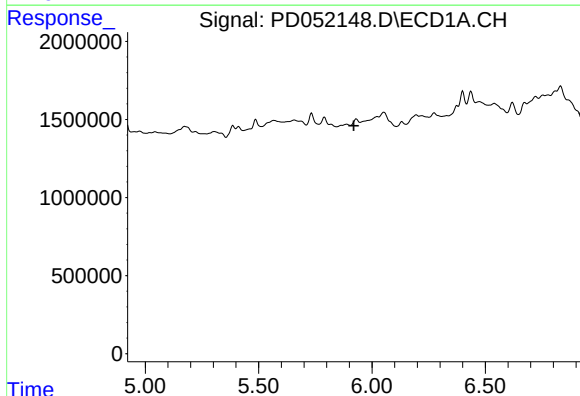


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

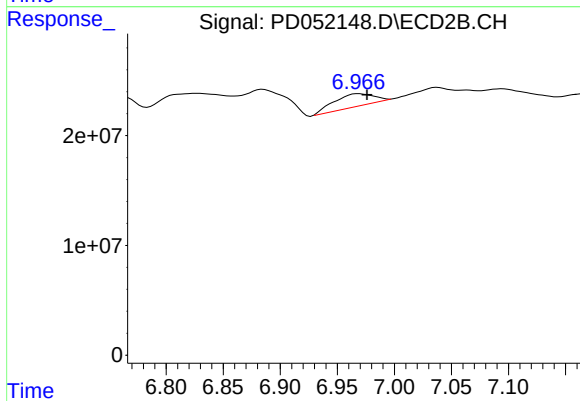

#15 Endosulfan II


R.T.: 6.969 min
Delta R.T.: -0.007 min
Response: 27763618
Conc: 1.10 ng/ml

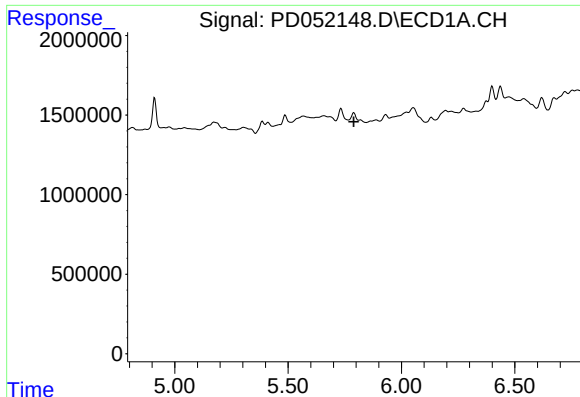

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

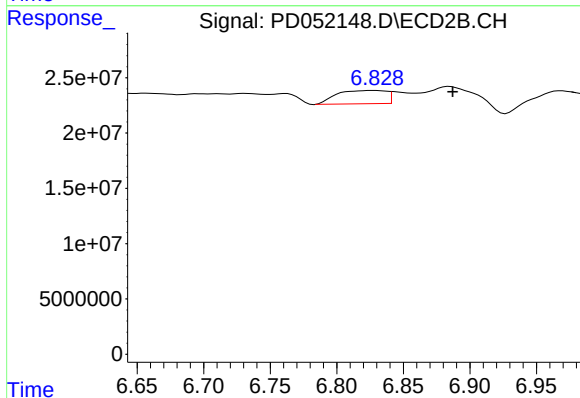


#16 4,4'-DDD

R.T.: 6.829 min
Delta R.T.: -0.058 min
Response: 31183430
Conc: 1.31 ng/ml

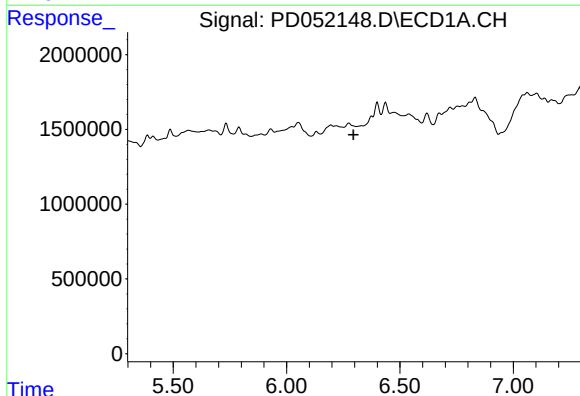


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.295 min
Response: 0
Conc: N.D.

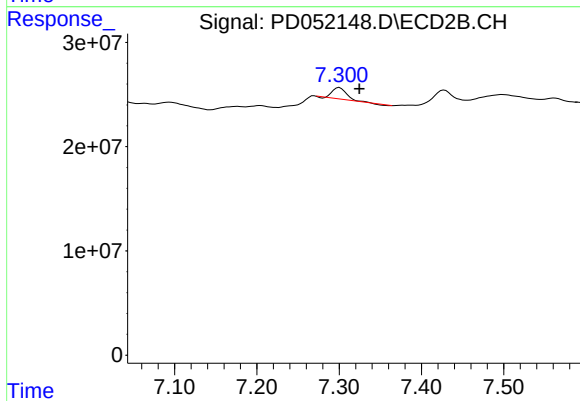

#19 Endosulfan Sulfate


R.T.: 7.300 min
Delta R.T.: -0.024 min
Response: 12427381
Conc: 0.55 ng/ml

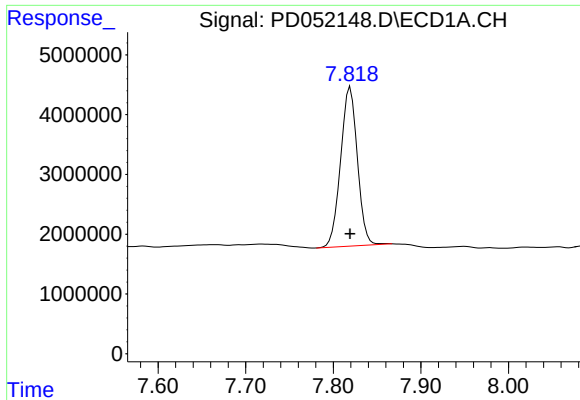

#27 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 35321398
Conc: 22.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5W6RE

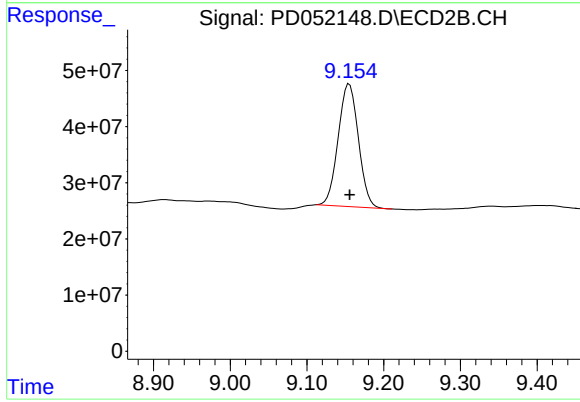

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 400102448
Conc: 25.92 ng/ml