

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
 Data File : PD068782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 19:02
 Operator : AR\AJ
 Sample : N2091-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 00:07:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	21476217	183.8E6	17.688	19.225
28)	SA Decachlor...	8.209	9.374	21972291	108.9E6	17.392	19.225
Target Compounds							
4)	MA Heptachlor	0.000	5.395	0	170587	N.D.	0.014 #
5)	MB Aldrin	4.725	5.695	259521	337298	0.162	0.029 #
6)	B beta-BHC	0.000	5.030	0	340485	N.D.	0.062 #
7)	B delta-BHC	0.000	5.232f	0	22784887	N.D.	1.895 #
8)	B Heptachlo...	0.000	6.115f	0	333647	N.D.	0.032 #
9)	A Endosulfan I	0.000	6.452	0	504850	N.D.	0.054 #
10)	B gamma-Chl...	0.000	6.303f	0	1756976	N.D.	0.170 #
21)	B Endrin ke...	0.000	7.971	0	1016868	N.D.	0.131 #
24)	Chlordane-2	0.000	5.695f	0	337298	N.D.	0.882 #
25)	Chlordane-3	0.000	6.303f	0	1756976	N.D.	1.308 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
Data File : PD068782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 19:02
Operator : AR\AJ
Sample : N2091-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 00:07:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

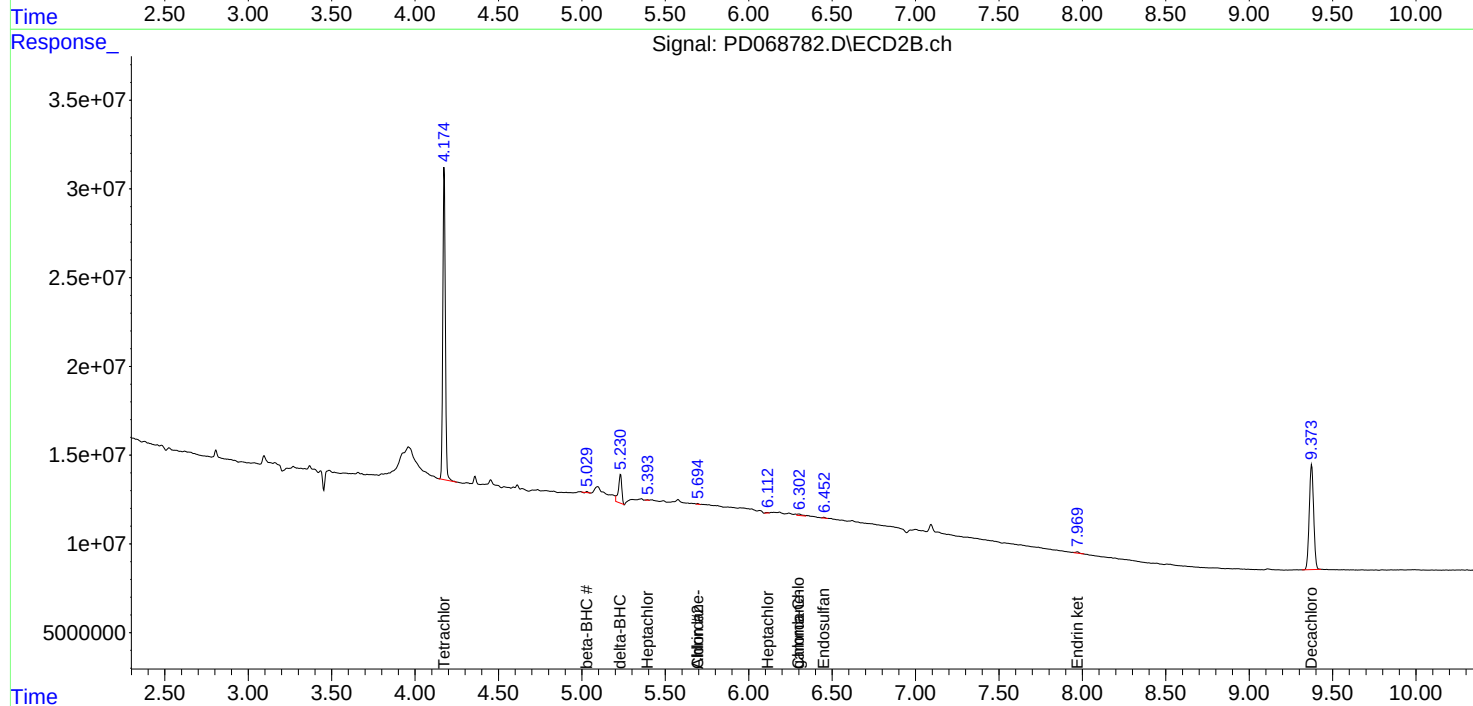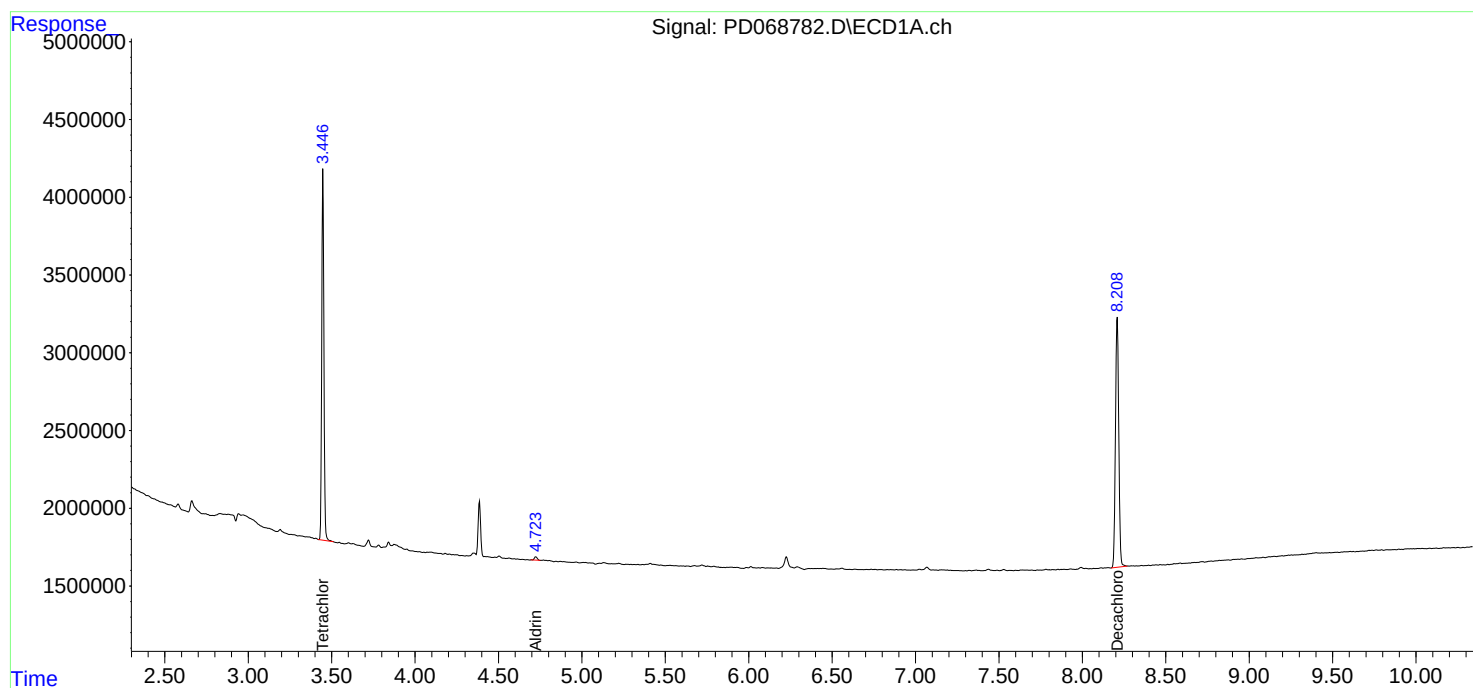


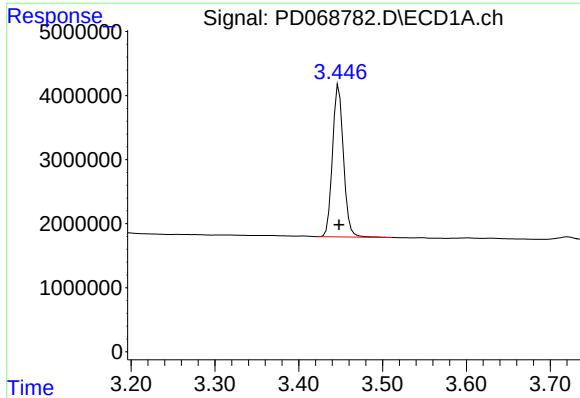

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 21476217
Conc: 17.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

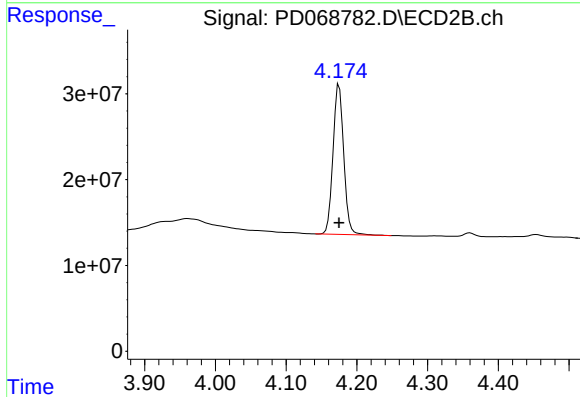


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 183804553
Conc: 19.22 ng/ml

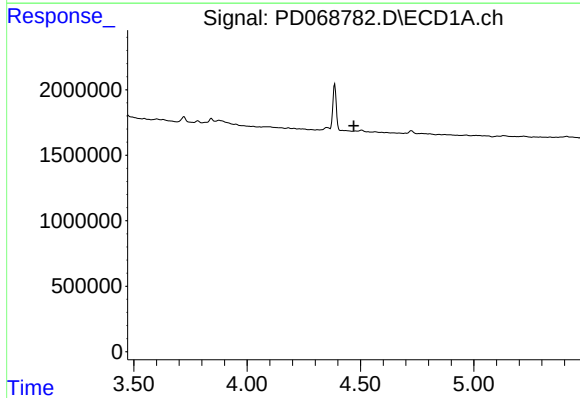


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.470 min
Response: 0
Conc: N.D.

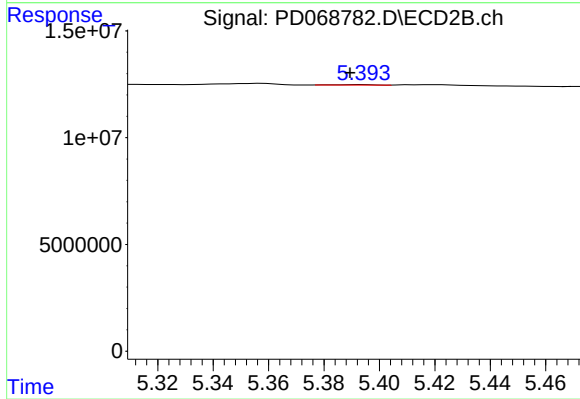

#4 Heptachlor


R.T.: 5.395 min
Delta R.T.: 0.005 min
Response: 170587
Conc: 0.01 ng/ml

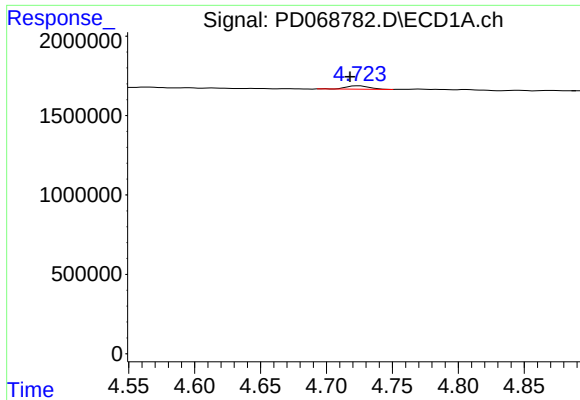

#5 Aldrin


R.T.: 4.725 min
Delta R.T.: 0.007 min
Response: 259521
Conc: 0.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

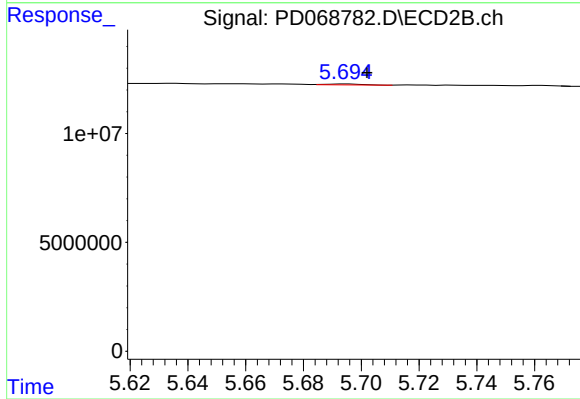


#5 Aldrin

R.T.: 5.695 min
Delta R.T.: -0.007 min
Response: 337298
Conc: 0.03 ng/ml

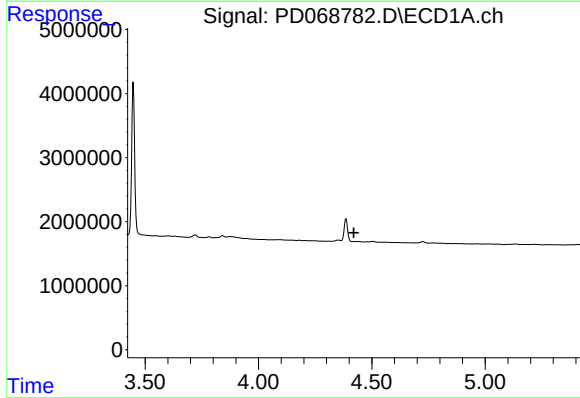


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.421 min
Response: 0
Conc: N.D.

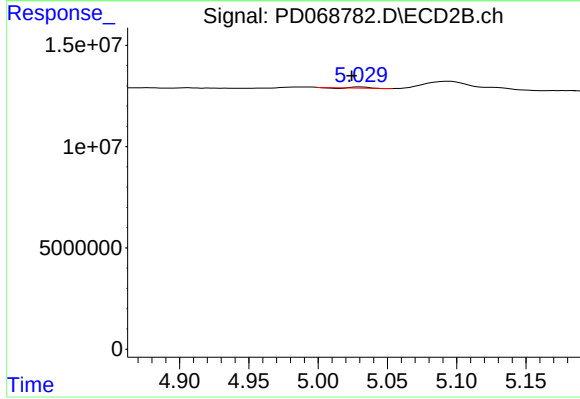

#6 beta-BHC


R.T.: 5.030 min
Delta R.T.: 0.006 min
Response: 340485
Conc: 0.06 ng/ml

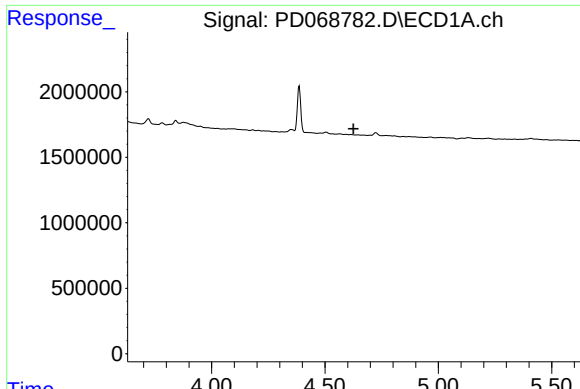

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

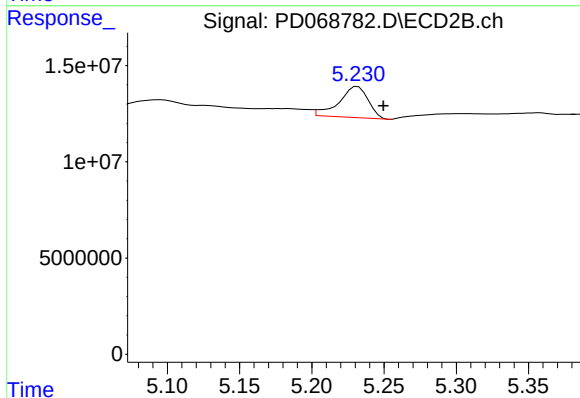


#7 delta-BHC

R.T.: 5.232 min
Delta R.T.: -0.018 min
Response: 22784887
Conc: 1.89 ng/ml

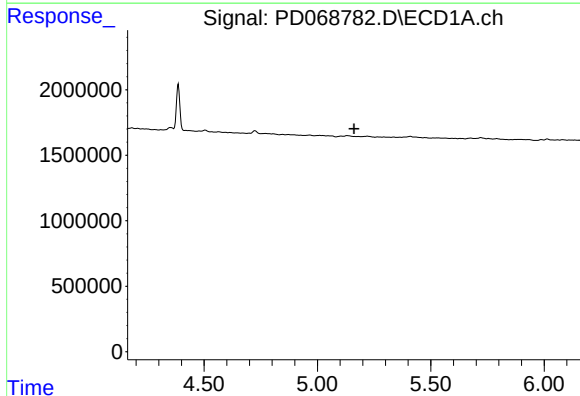


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.162 min
Response: 0
Conc: N.D.

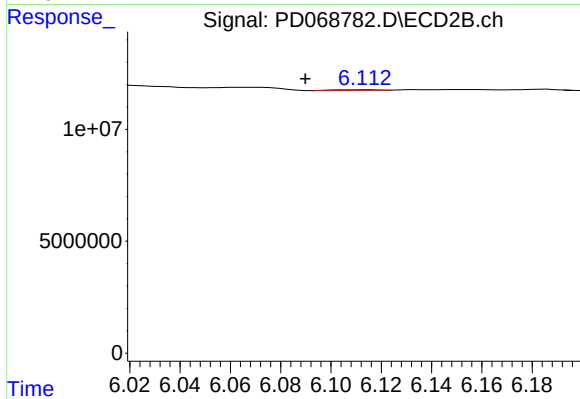

#8 Heptachlor epoxide


R.T.: 6.115 min
Delta R.T.: 0.025 min
Response: 333647
Conc: 0.03 ng/ml

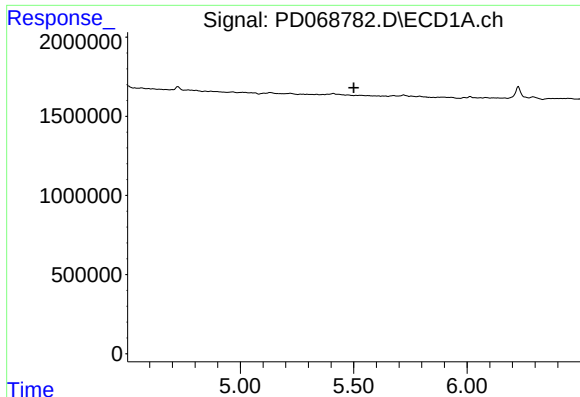

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

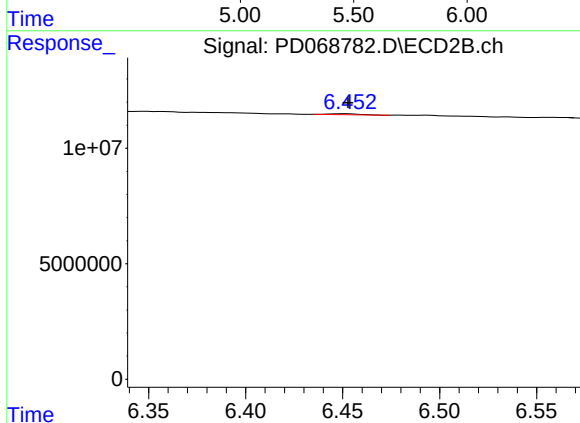


#9 Endosulfan I

R.T.: 6.452 min
Delta R.T.: -0.001 min
Response: 504850
Conc: 0.05 ng/ml

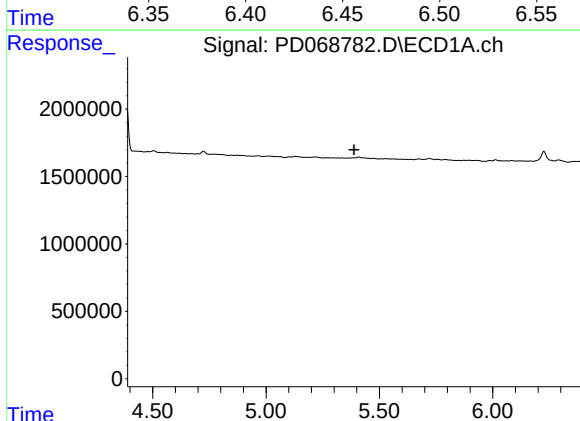


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.388 min
Response: 0
Conc: N.D.

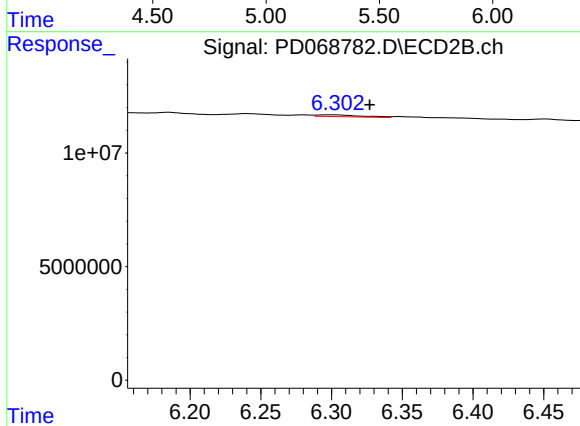

#10 gamma-Chlordane


R.T.: 6.303 min
Delta R.T.: -0.024 min
Response: 1756976
Conc: 0.17 ng/ml

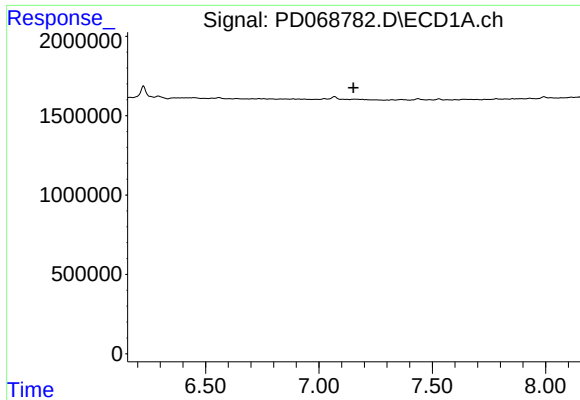

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

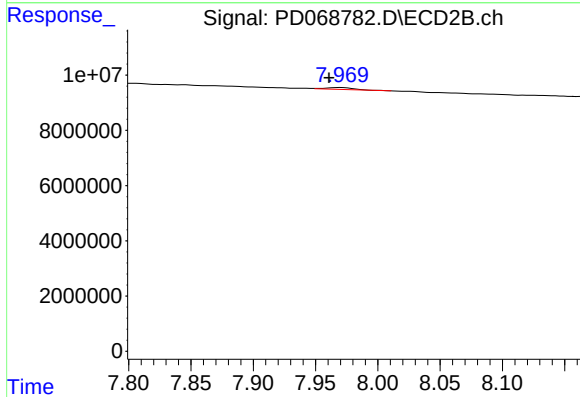


#21 Endrin ketone

R.T.: 7.971 min
Delta R.T.: 0.010 min
Response: 1016868
Conc: 0.13 ng/ml

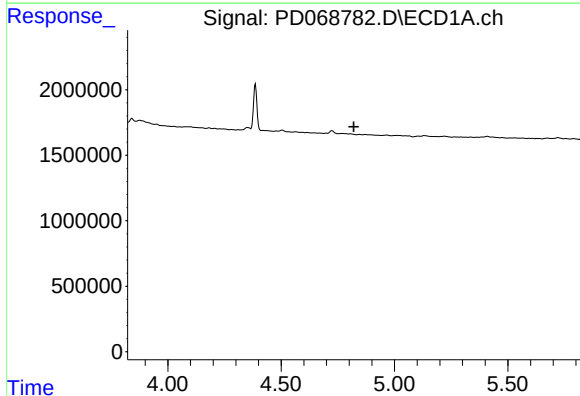


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.820 min
Response: 0
Conc: N.D.

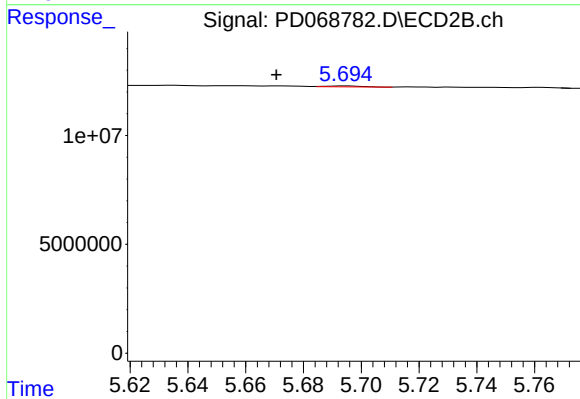

#24 Chlordane-2


R.T.: 5.695 min
Delta R.T.: 0.025 min
Response: 337298
Conc: 0.88 ng/ml

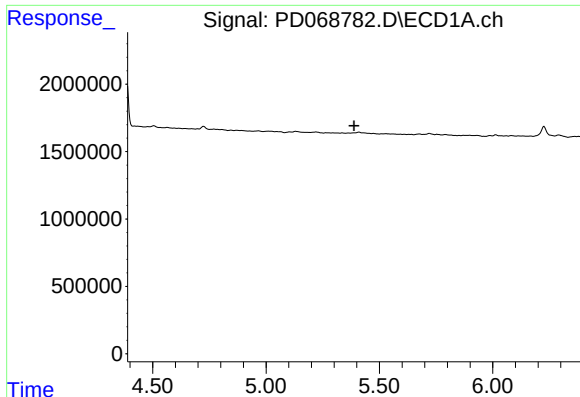

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

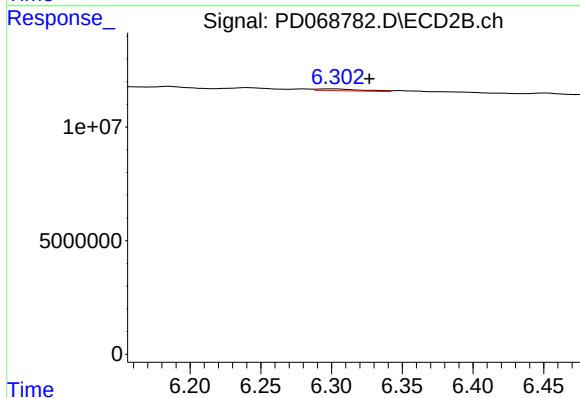


#25 Chlordane-3

R.T.: 6.303 min
Delta R.T.: -0.024 min
Response: 1756976
Conc: 1.31 ng/ml

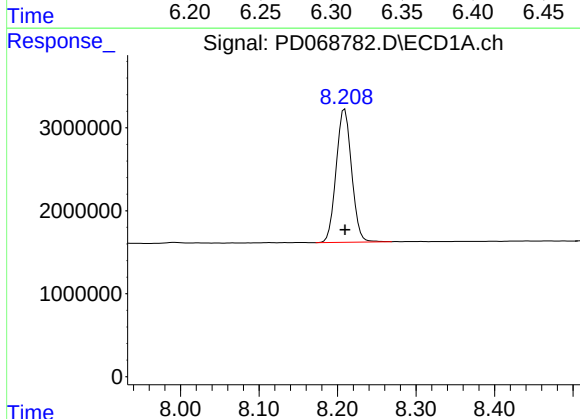

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 21972291
Conc: 17.39 ng/ml

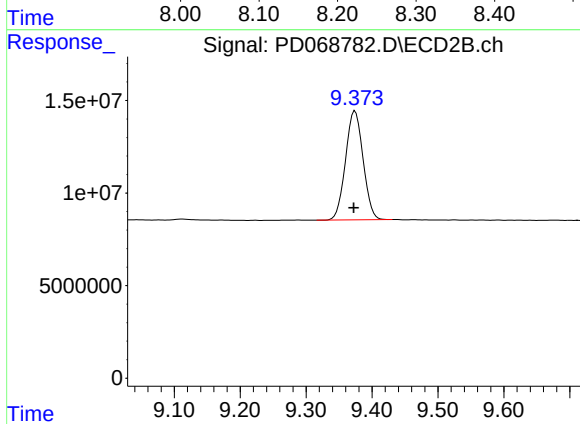

#28 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.002 min
Response: 108943725
Conc: 19.23 ng/ml