

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
 Data File : PD068783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 19:16
 Operator : AR\AJ
 Sample : N2094-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 00:08:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	21444529	183.6E6	17.662	19.199
28)	SA Decachlor...	8.209	9.375	25624996	127.5E6	20.283	22.494
Target Compounds							
2)	A alpha-BHC	0.000	4.590f	0	850733	N.D.	0.062 #
5)	MB Aldrin	4.723	0.000	218934	0	0.137	N.D. #
6)	B beta-BHC	0.000	5.028	0	338118	N.D.	0.062 #
7)	B delta-BHC	0.000	5.232f	0	17331169	N.D.	1.441 #
8)	B Heptachlo...	0.000	6.063f	0	2087295	N.D.	0.200 #
10)	B gamma-Chl...	0.000	6.300f	0	8459294	N.D.	0.821 #
14)	MA Endrin	6.013	0.000	417253	0	0.317	N.D. #
15)	B Endosulfa...	0.000	7.138	0	576756	N.D.	0.076 #
21)	B Endrin ke...	0.000	7.969	0	1150500	N.D.	0.148 #
23)	Chlordane-1	0.000	5.181f	0	6431337	N.D.	16.301 #
25)	Chlordane-3	0.000	6.300f	0	8459294	N.D.	6.296 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
Data File : PD068783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 19:16
Operator : AR\AJ
Sample : N2094-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 00:08:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

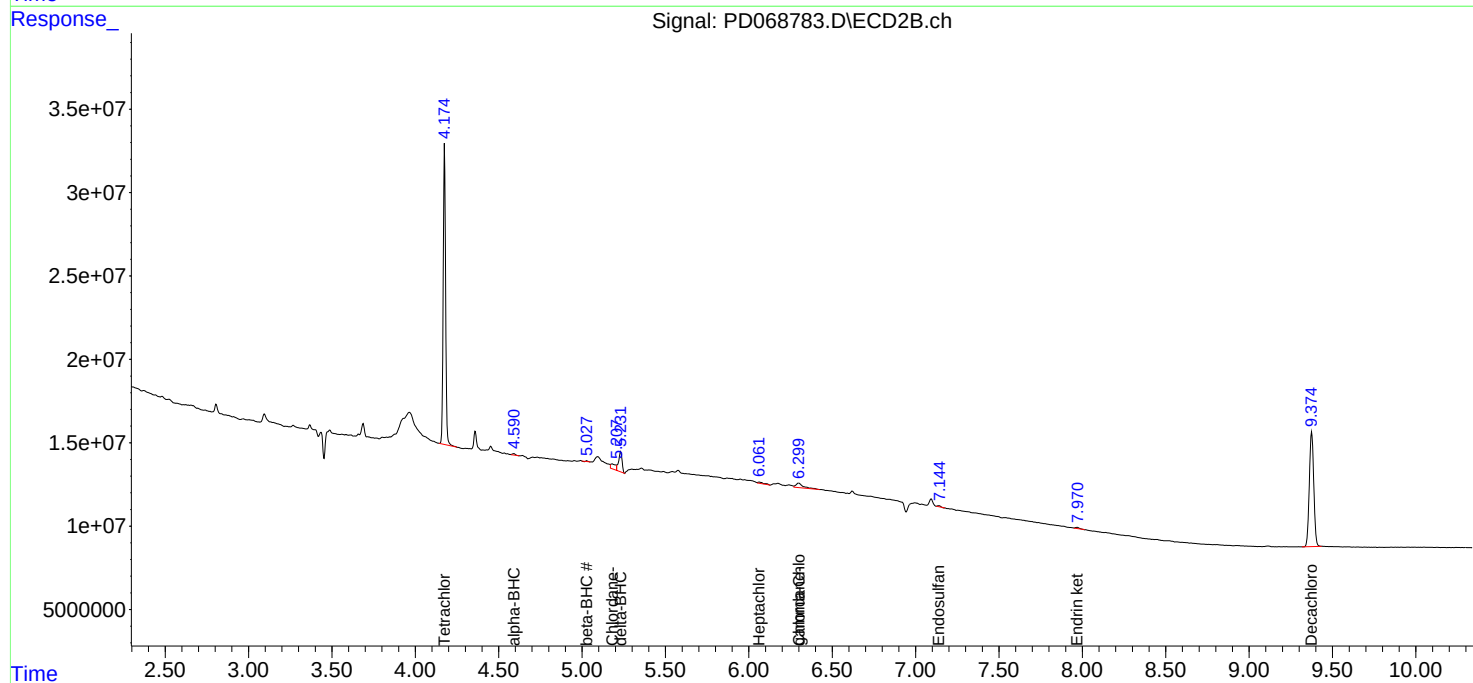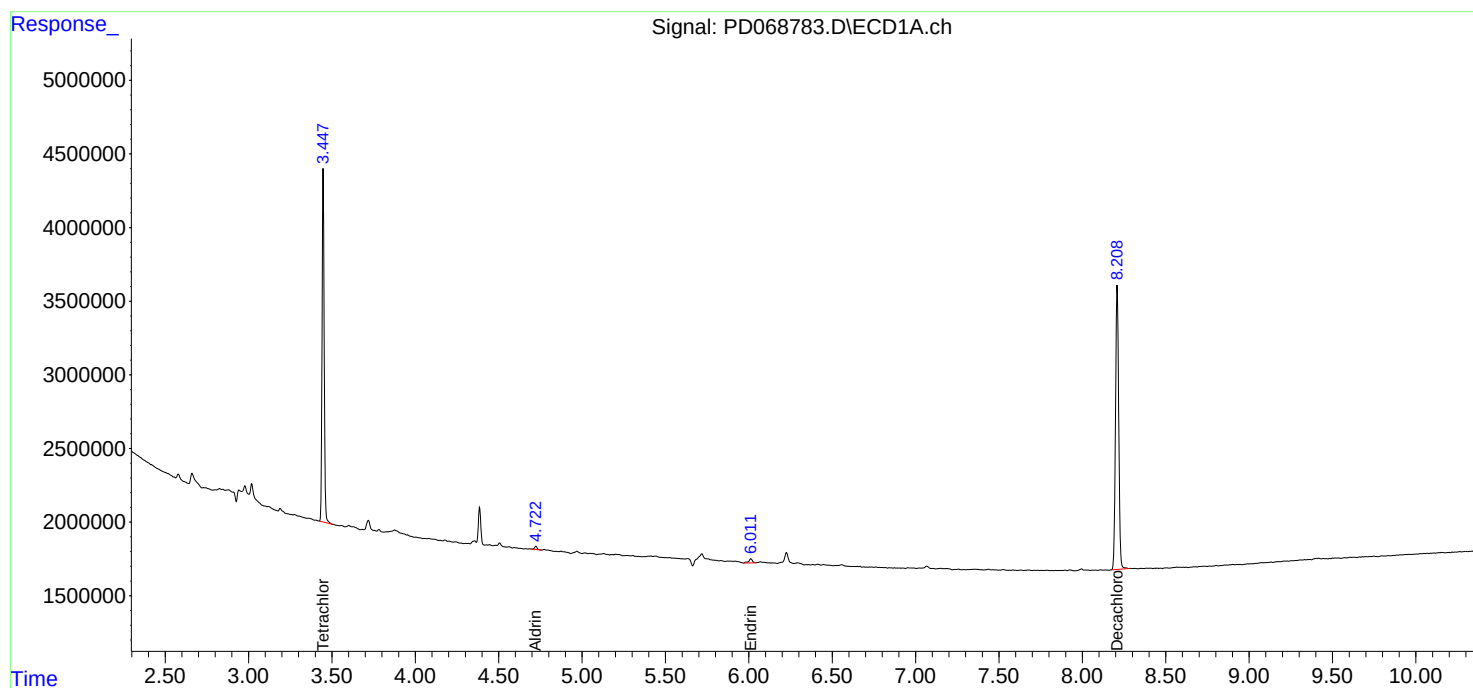


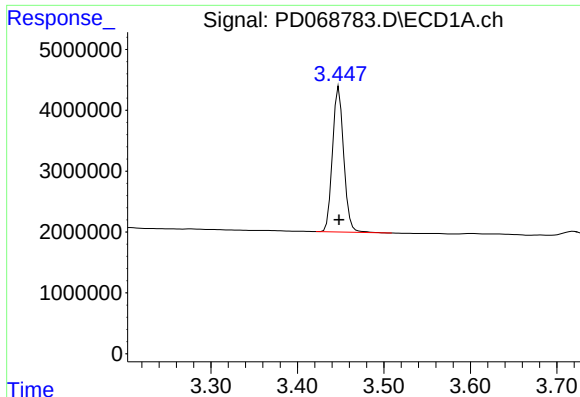

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 21444529
Conc: 17.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

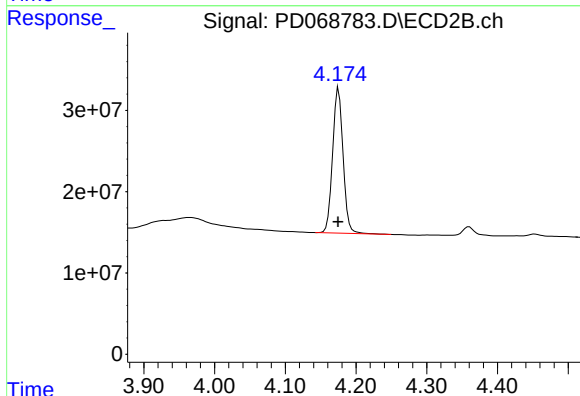


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 183552325
Conc: 19.20 ng/ml

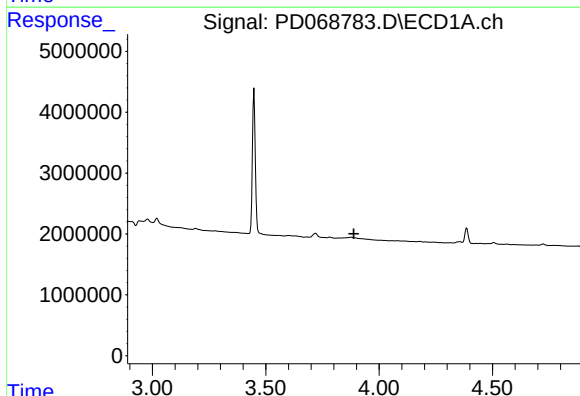


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

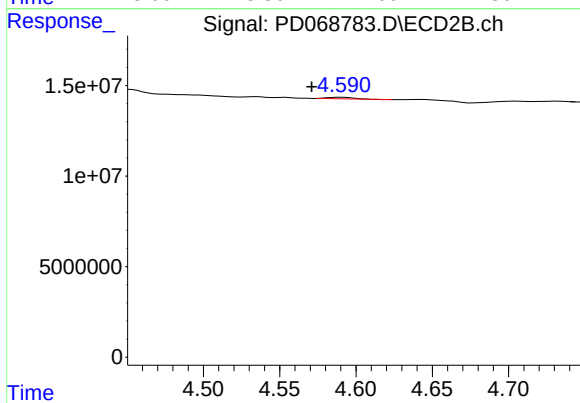

#2 alpha-BHC


R.T.: 4.590 min
Delta R.T.: 0.019 min
Response: 850733
Conc: 0.06 ng/ml

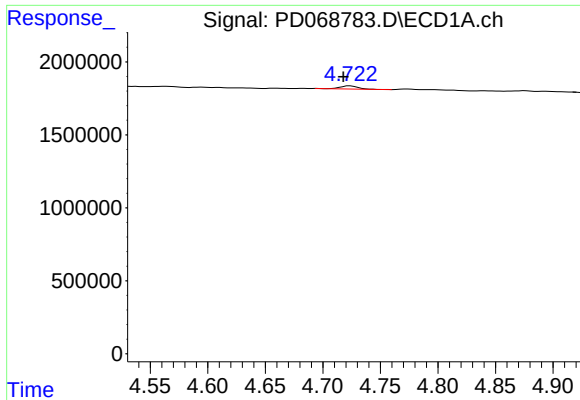

#5 Aldrin


R.T.: 4.723 min
Delta R.T.: 0.006 min
Response: 218934
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

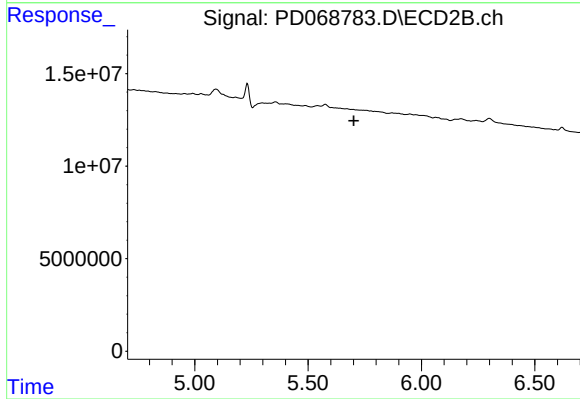


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.702 min
Response: 0
Conc: N.D.

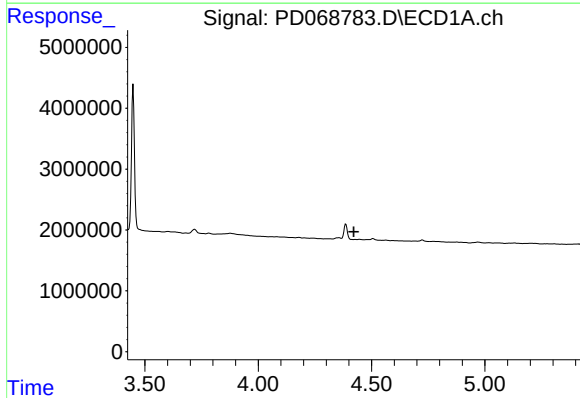


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.421 min
Response: 0
Conc: N.D.

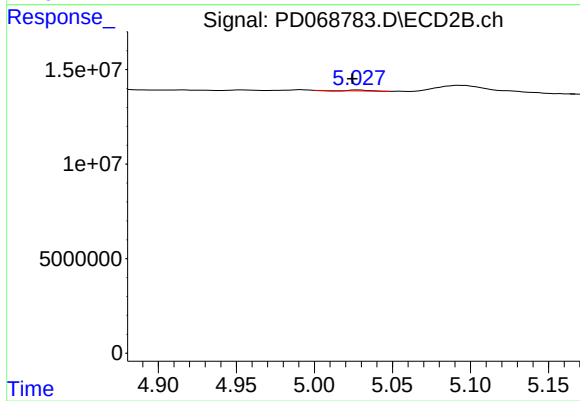

#6 beta-BHC


R.T.: 5.028 min
Delta R.T.: 0.004 min
Response: 338118
Conc: 0.06 ng/ml

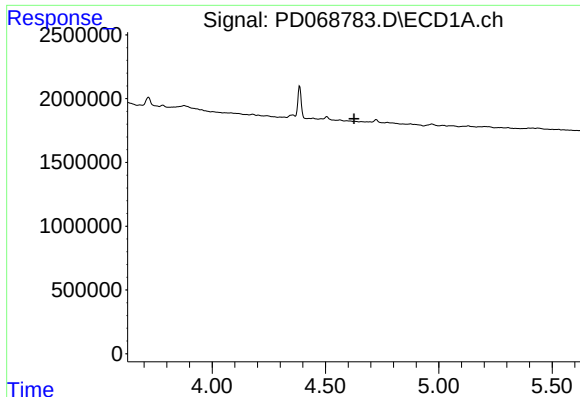

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

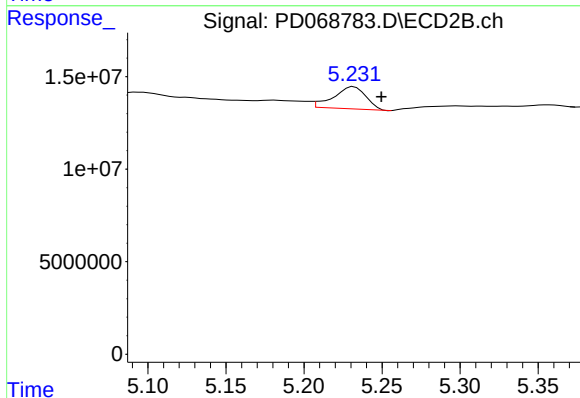


#7 delta-BHC

R.T.: 5.232 min
Delta R.T.: -0.018 min
Response: 17331169
Conc: 1.44 ng/ml

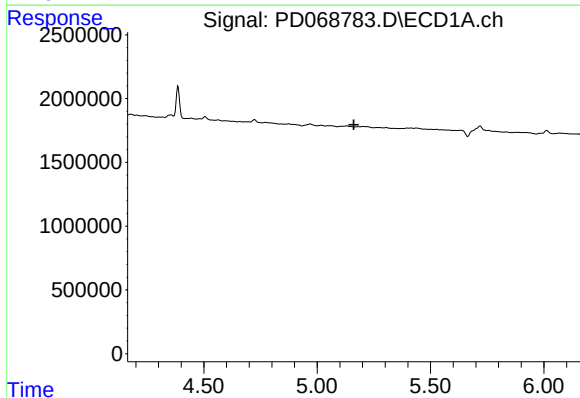


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

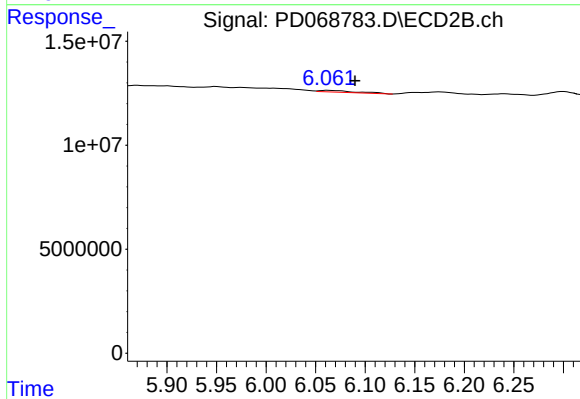

#8 Heptachlor epoxide


R.T.: 6.063 min
Delta R.T.: -0.027 min
Response: 2087295
Conc: 0.20 ng/ml

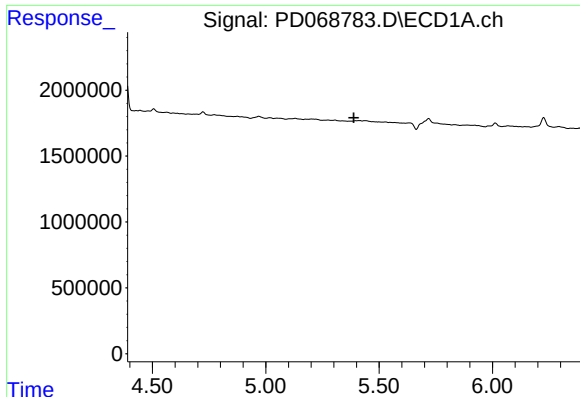

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

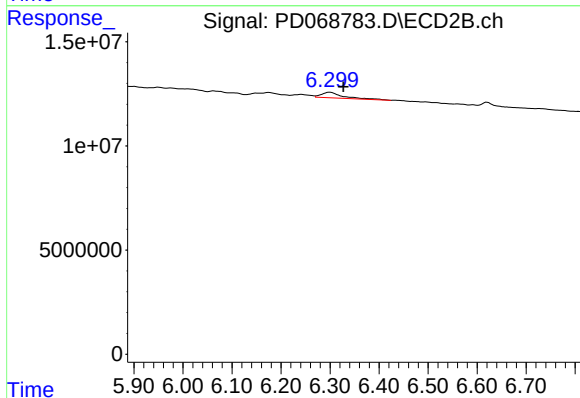


#10 gamma-Chlordane

R.T.: 6.300 min
Delta R.T.: -0.027 min
Response: 8459294
Conc: 0.82 ng/ml

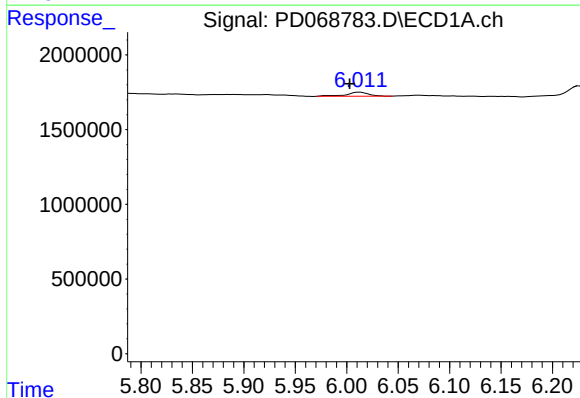


#14 Endrin

R.T.: 6.013 min
Delta R.T.: 0.009 min
Response: 417253
Conc: 0.32 ng/ml

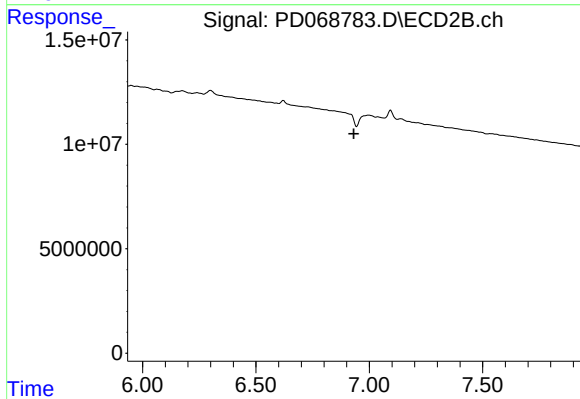

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.932 min
Response: 0
Conc: N.D.

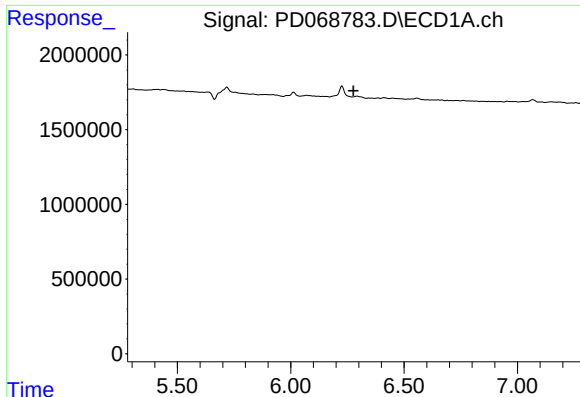

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

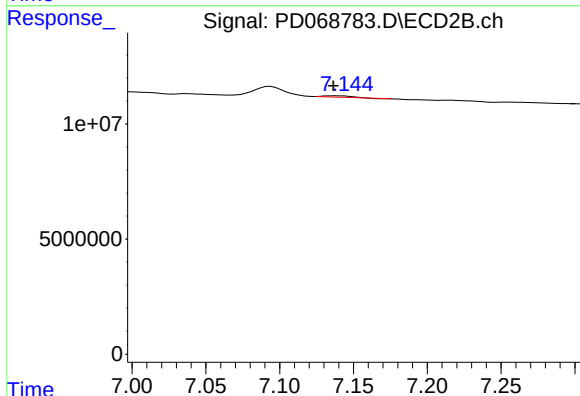


#15 Endosulfan II

R.T.: 7.138 min
Delta R.T.: 0.002 min
Response: 576756
Conc: 0.08 ng/ml

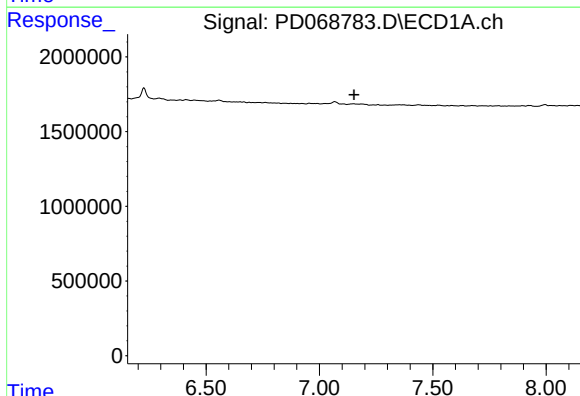


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

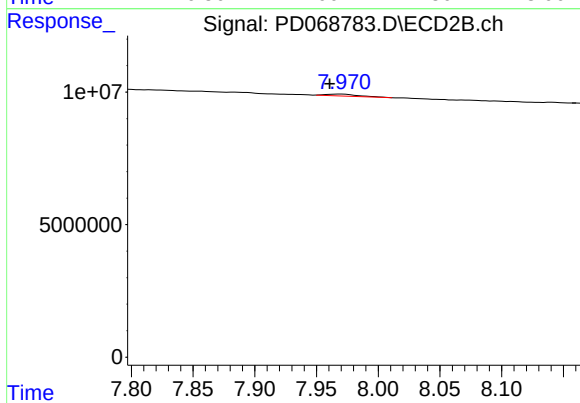

#21 Endrin ketone


R.T.: 7.969 min
Delta R.T.: 0.009 min
Response: 1150500
Conc: 0.15 ng/ml

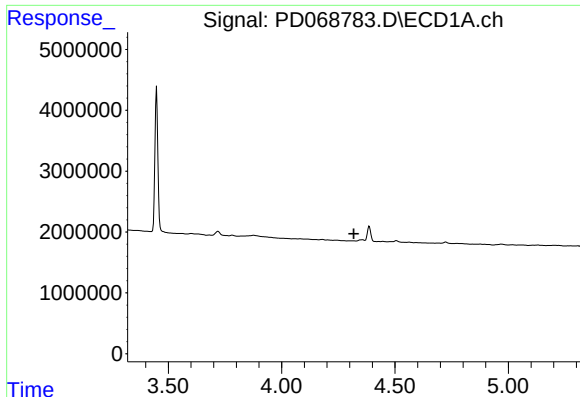

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

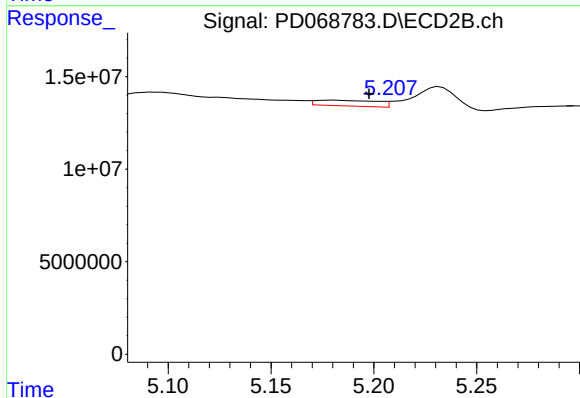


#23 Chlordane-1

R.T.: 5.181 min
Delta R.T.: -0.016 min
Response: 6431337
Conc: 16.30 ng/ml

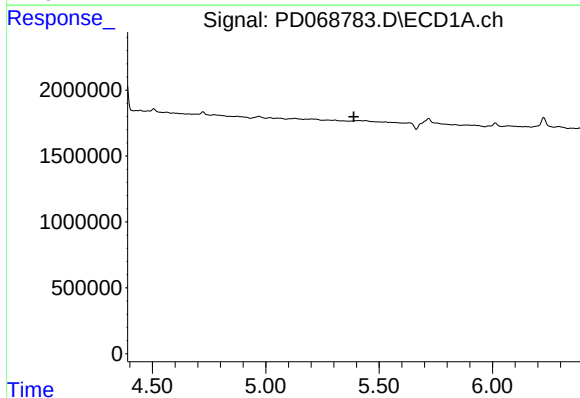


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

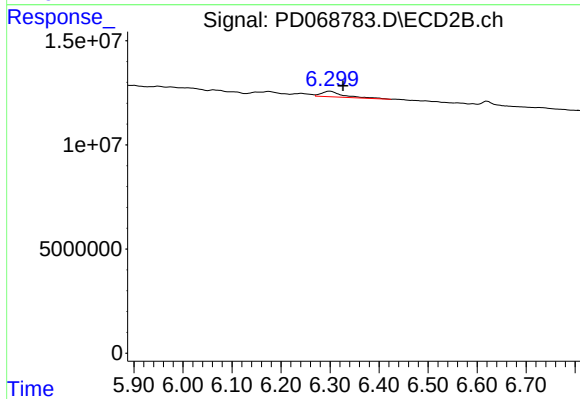

#25 Chlordane-3


R.T.: 6.300 min
Delta R.T.: -0.027 min
Response: 8459294
Conc: 6.30 ng/ml

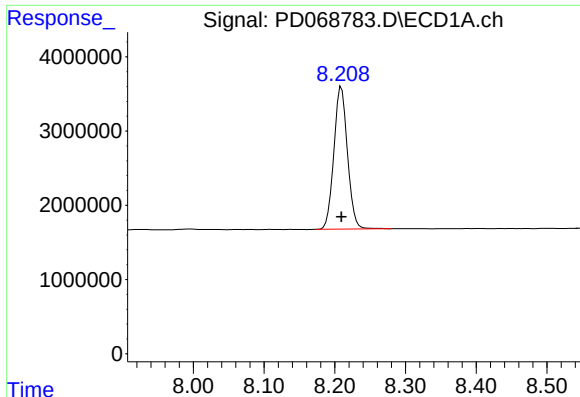

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 25624996
Conc: 20.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

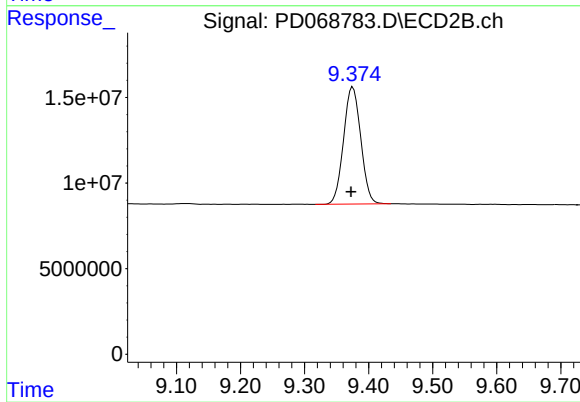

#28 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: 0.003 min
Response: 127469503
Conc: 22.49 ng/ml