

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
 Data File : PD068784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 19:30
 Operator : AR\AJ
 Sample : N2109-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 00:08:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	21513192	185.7E6	17.718	19.422
28)	SA Decachlor...	8.209	9.374	25804280	129.0E6	20.425	22.762
Target Compounds							
2)	A alpha-BHC	0.000	4.588f	0	586189	N.D.	0.043 #
5)	MB Aldrin	0.000	5.710	0	36368	N.D.	0.003 #
6)	B beta-BHC	0.000	5.029	0	528573	N.D.	0.096 #
7)	B delta-BHC	0.000	5.231f	0	16194580	N.D.	1.347 #
8)	B Heptachlo...	0.000	6.068f	0	617548	N.D.	0.059 #
10)	B gamma-Chl...	0.000	6.300f	0	1630391	N.D.	0.158 #
15)	B Endosulfa...	0.000	7.133	0	354984	N.D.	0.047 #
21)	B Endrin ke...	0.000	7.971	0	1361256	N.D.	0.176 #
22)	Mirex	0.000	8.441	0	398249	N.D.	0.073 #
23)	Chlordane-1	0.000	5.180f	0	4143830	N.D.	10.503 #
25)	Chlordane-3	0.000	6.300f	0	1630391	N.D.	1.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
Data File : PD068784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 19:30
Operator : AR\AJ
Sample : N2109-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 00:08:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

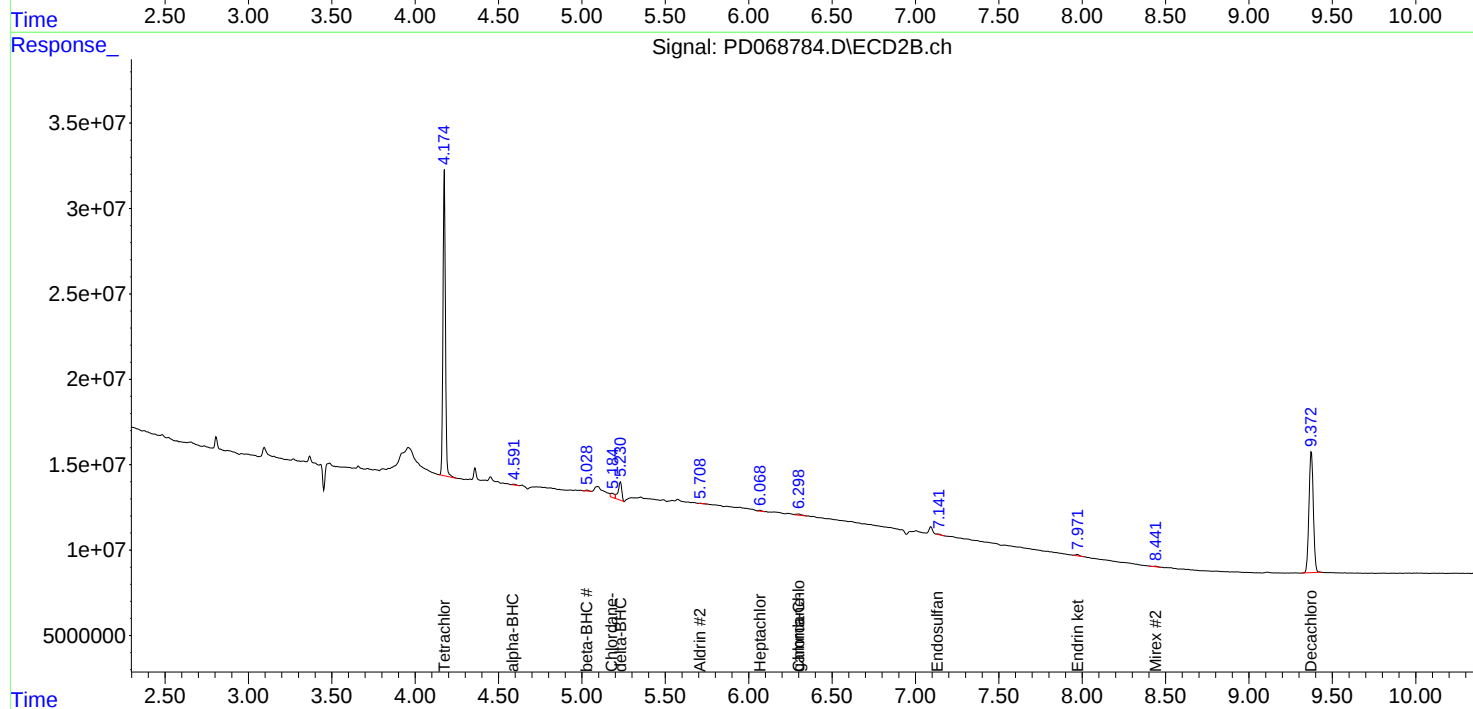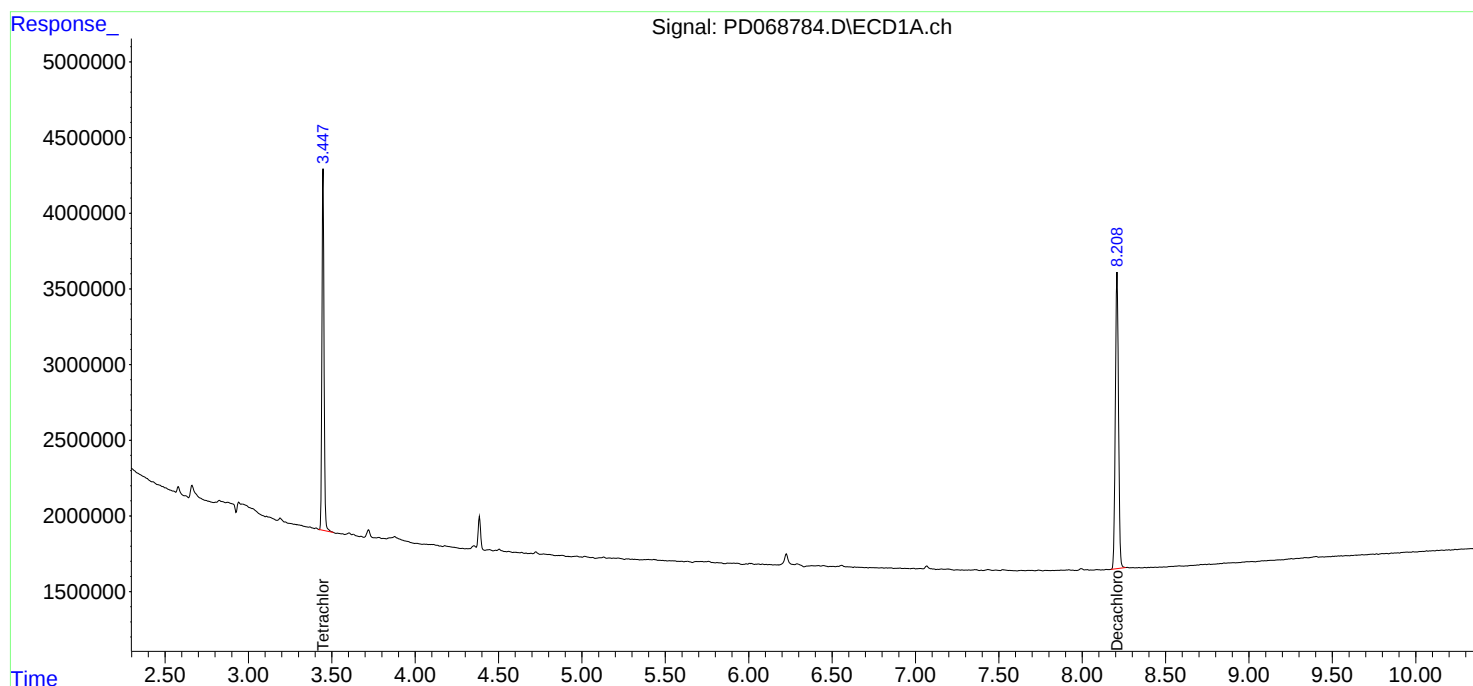


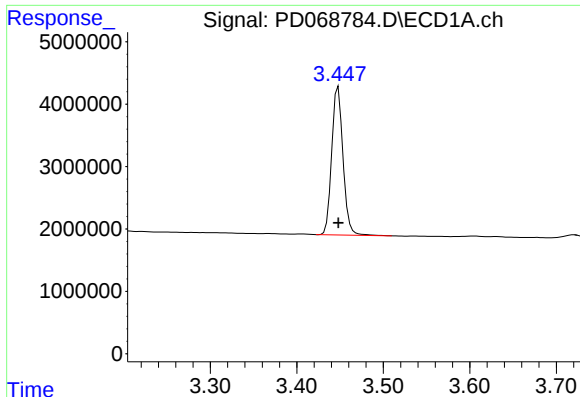

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 21513192
Conc: 17.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

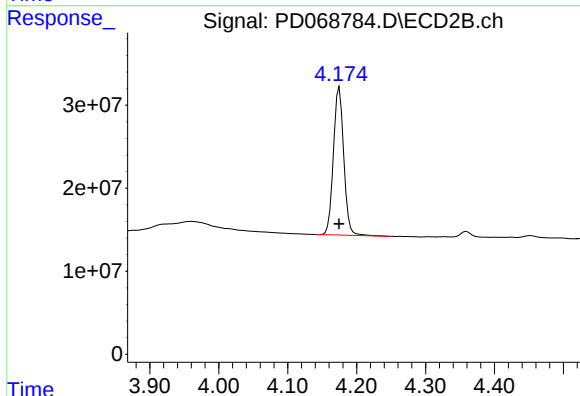


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 185684166
Conc: 19.42 ng/ml

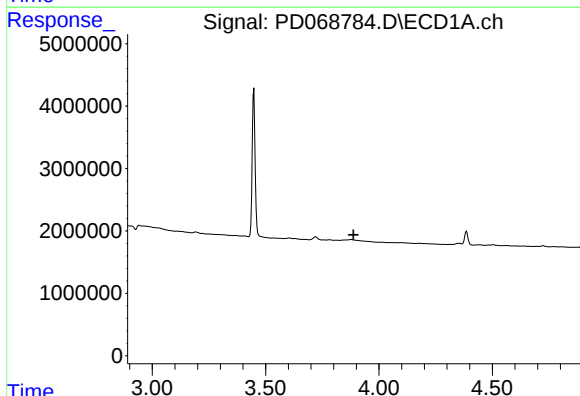


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

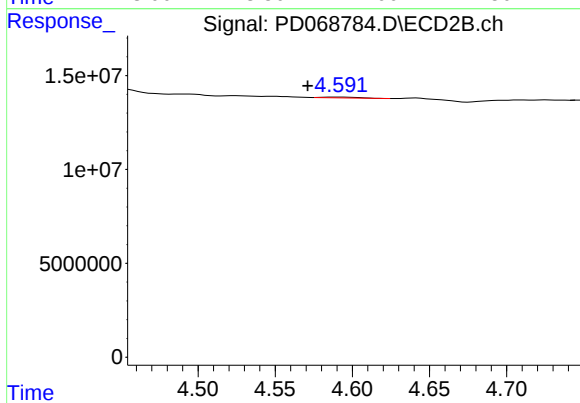

#2 alpha-BHC


R.T.: 4.588 min
Delta R.T.: 0.017 min
Response: 586189
Conc: 0.04 ng/ml

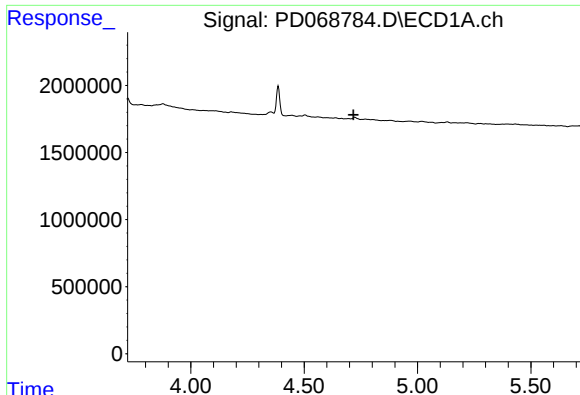

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.718 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

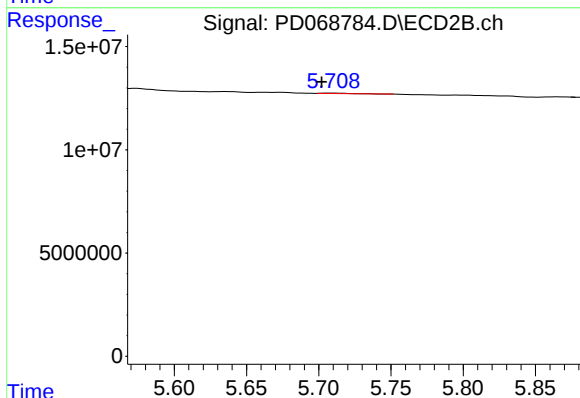


#5 Aldrin

R.T.: 5.710 min
Delta R.T.: 0.008 min
Response: 36368
Conc: 0.00 ng/ml

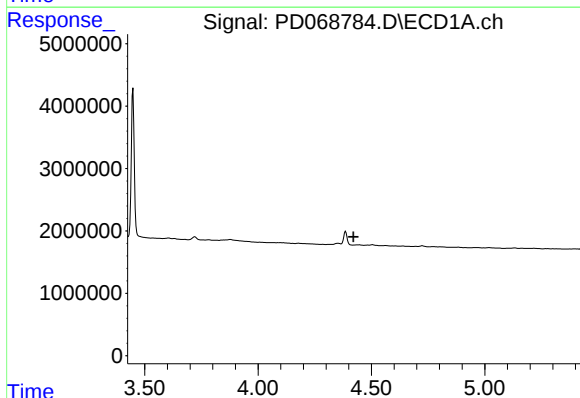


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.421 min
Response: 0
Conc: N.D.

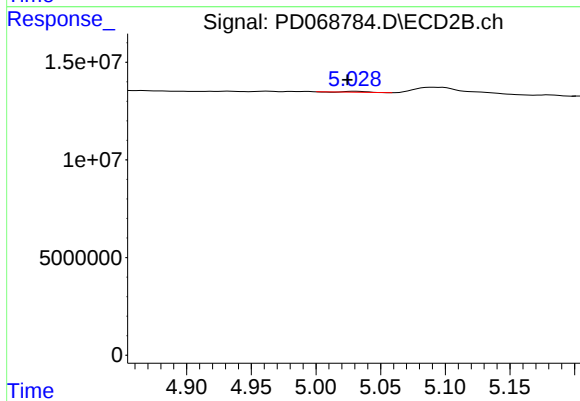

#6 beta-BHC


R.T.: 5.029 min
Delta R.T.: 0.005 min
Response: 528573
Conc: 0.10 ng/ml

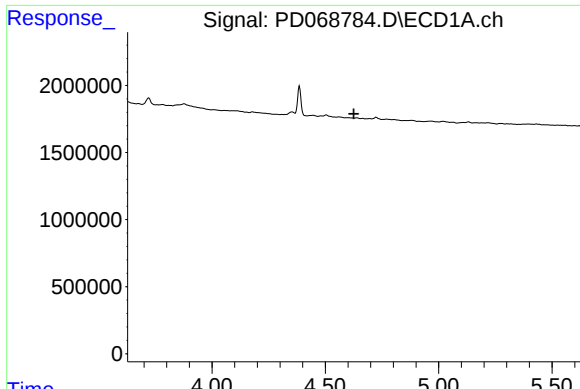

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.626 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

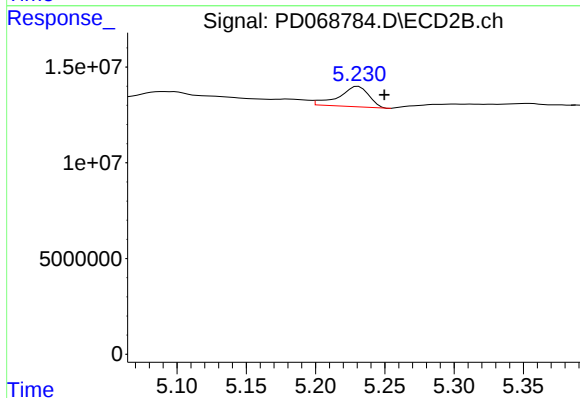


#7 delta-BHC

R.T.: 5.231 min
Delta R.T.: -0.019 min
Response: 16194580
Conc: 1.35 ng/ml

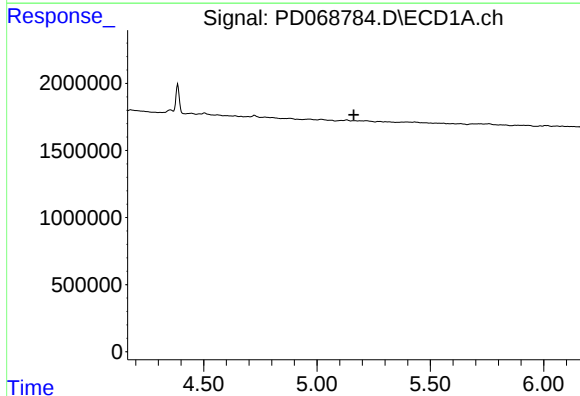


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.162 min
Response: 0
Conc: N.D.

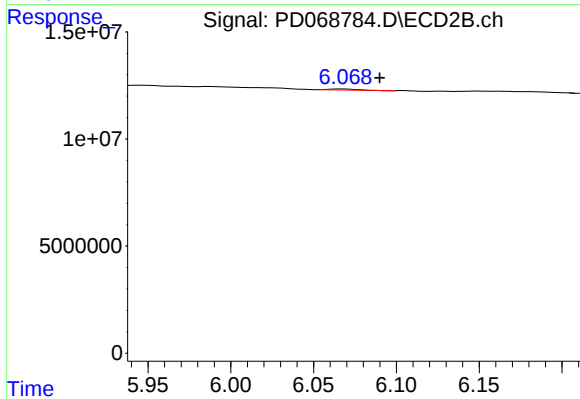

#8 Heptachlor epoxide


R.T.: 6.068 min
Delta R.T.: -0.022 min
Response: 617548
Conc: 0.06 ng/ml

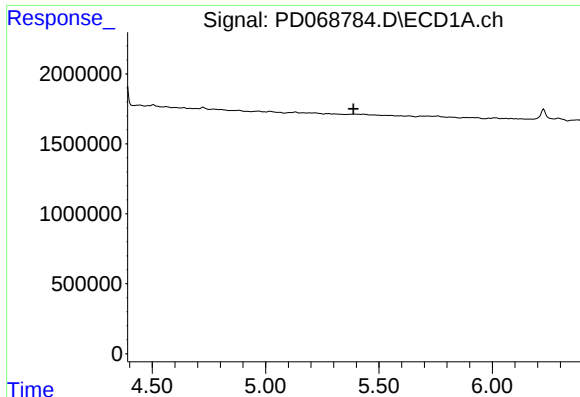

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

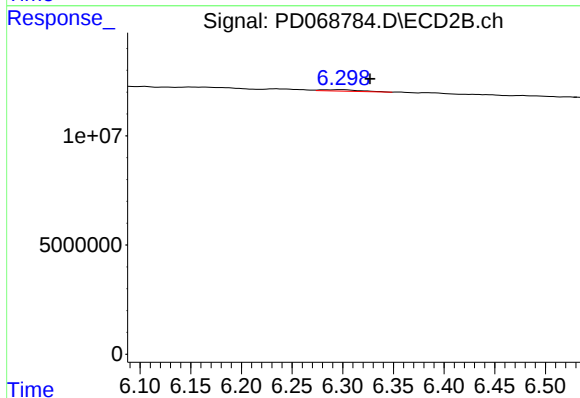


#10 gamma-Chlordane

R.T.: 6.300 min
Delta R.T.: -0.027 min
Response: 1630391
Conc: 0.16 ng/ml

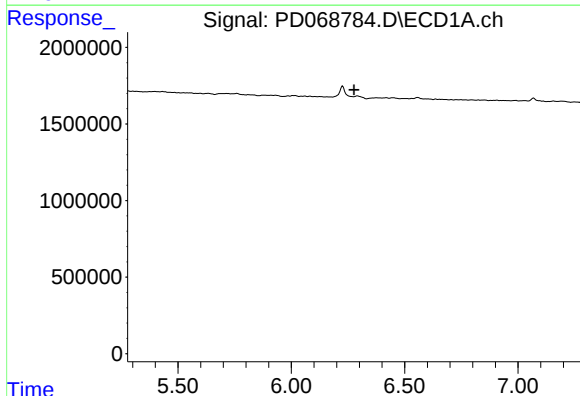


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.277 min
Response: 0
Conc: N.D.

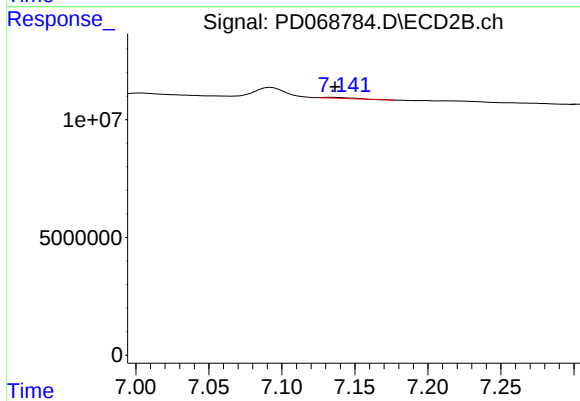

#15 Endosulfan II


R.T.: 7.133 min
Delta R.T.: -0.004 min
Response: 354984
Conc: 0.05 ng/ml

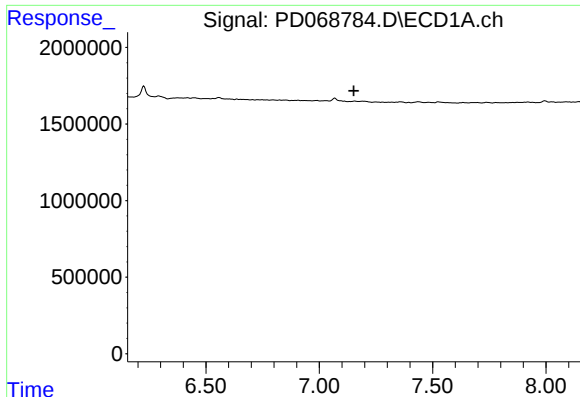

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

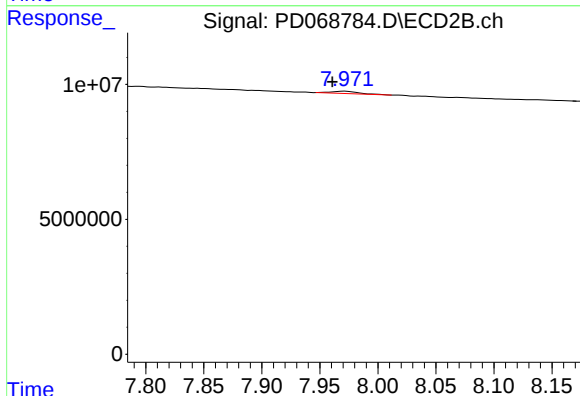


#21 Endrin ketone

R.T.: 7.971 min
Delta R.T.: 0.011 min
Response: 1361256
Conc: 0.18 ng/ml

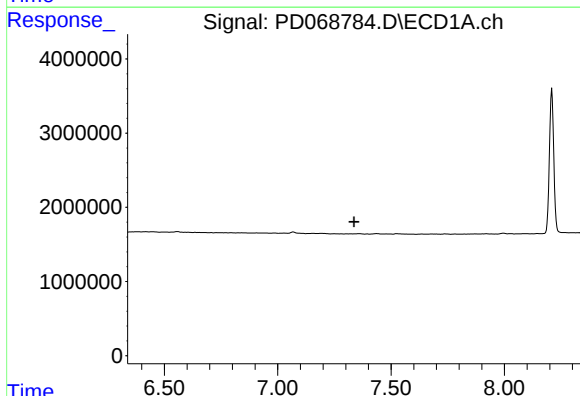


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

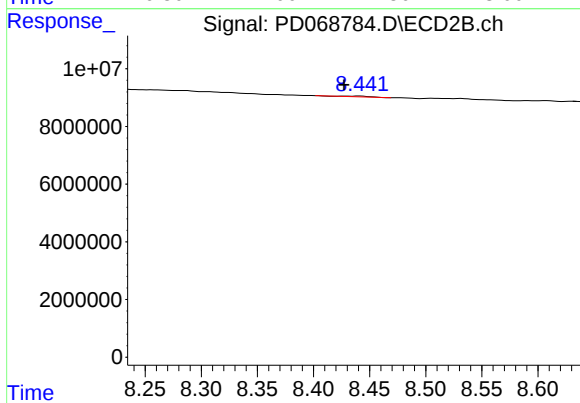

#22 Mirex


R.T.: 8.441 min
Delta R.T.: 0.014 min
Response: 398249
Conc: 0.07 ng/ml

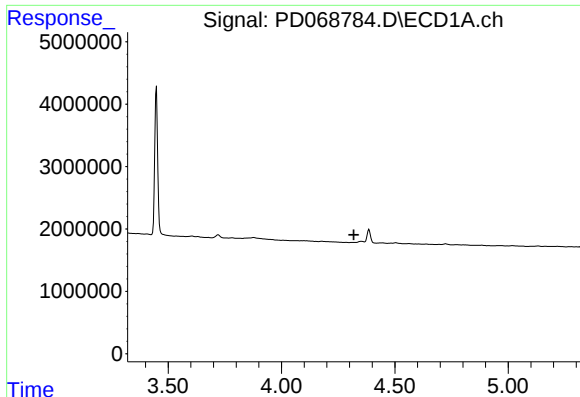

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

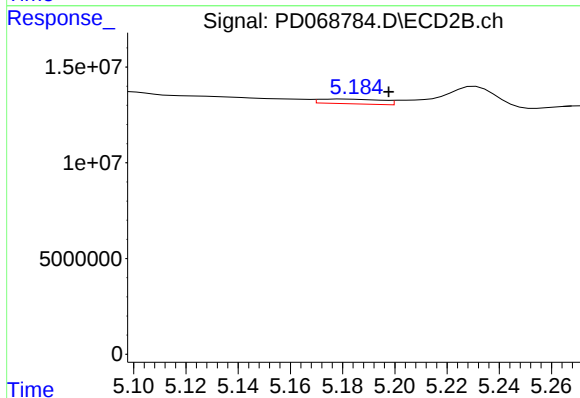


#23 Chlordane-1

R.T.: 5.180 min
Delta R.T.: -0.017 min
Response: 4143830
Conc: 10.50 ng/ml

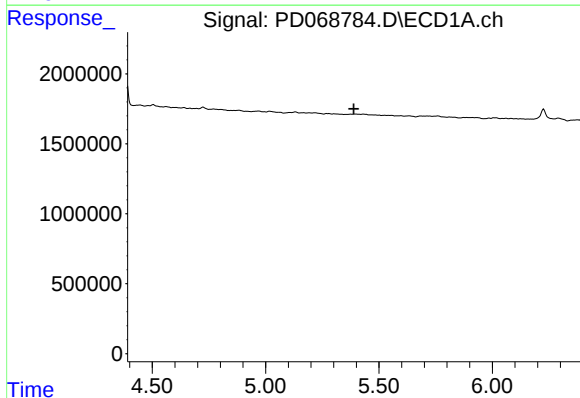


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

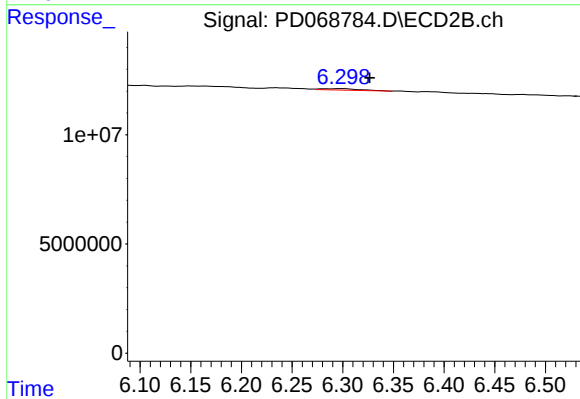

#25 Chlordane-3


R.T.: 6.300 min
Delta R.T.: -0.027 min
Response: 1630391
Conc: 1.21 ng/ml

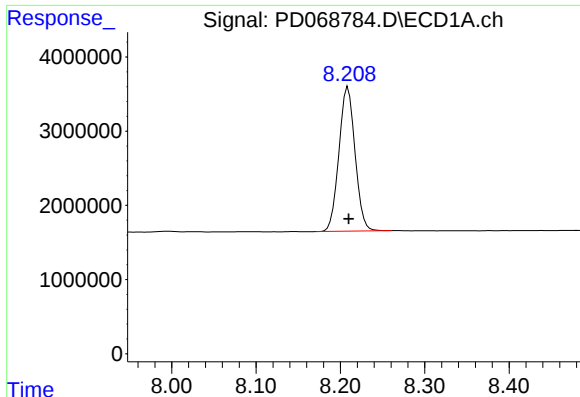

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 25804280
Conc: 20.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

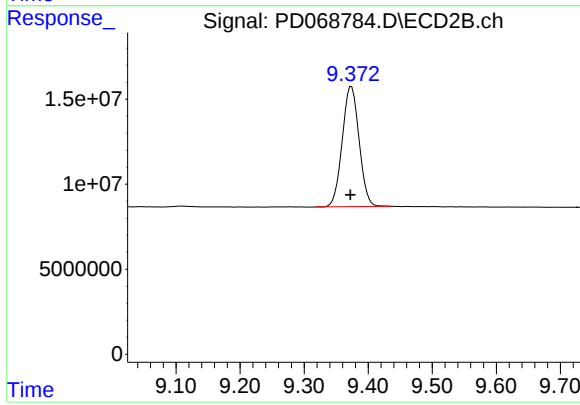

#28 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.001 min
Response: 128988521
Conc: 22.76 ng/ml