

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
 Data File : PD068785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 19:44
 Operator : AR\AJ
 Sample : PB143558TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 00:08:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.175	20118530	178.3E6	16.570	18.649
28)	SA Decachlor...	8.209	9.375	23584975	114.1E6	18.668	20.140
Target Compounds							
3)	MA gamma-BHC...	0.000	4.855	0	67662	N.D.	0.005 #
5)	MB Aldrin	0.000	5.679f	0	165184	N.D.	0.014 #
7)	B delta-BHC	0.000	5.231f	0	3632805	N.D.	0.302 #
8)	B Heptachlo...	0.000	6.087	0	378669	N.D.	0.036 #
11)	B alpha-Chl...	0.000	6.399	0	111485	N.D.	0.011 #
21)	B Endrin ke...	0.000	7.971	0	1076371	N.D.	0.139 #
23)	Chlordane-1	4.344f	5.188	158379	426959	3.732	1.082 #
24)	Chlordane-2	0.000	5.679	0	165184	N.D.	0.432 #
26)	Chlordane-4	0.000	6.399	0	111485	N.D.	0.072 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
Data File : PD068785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 19:44
Operator : AR\AJ
Sample : PB143558TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 00:08:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

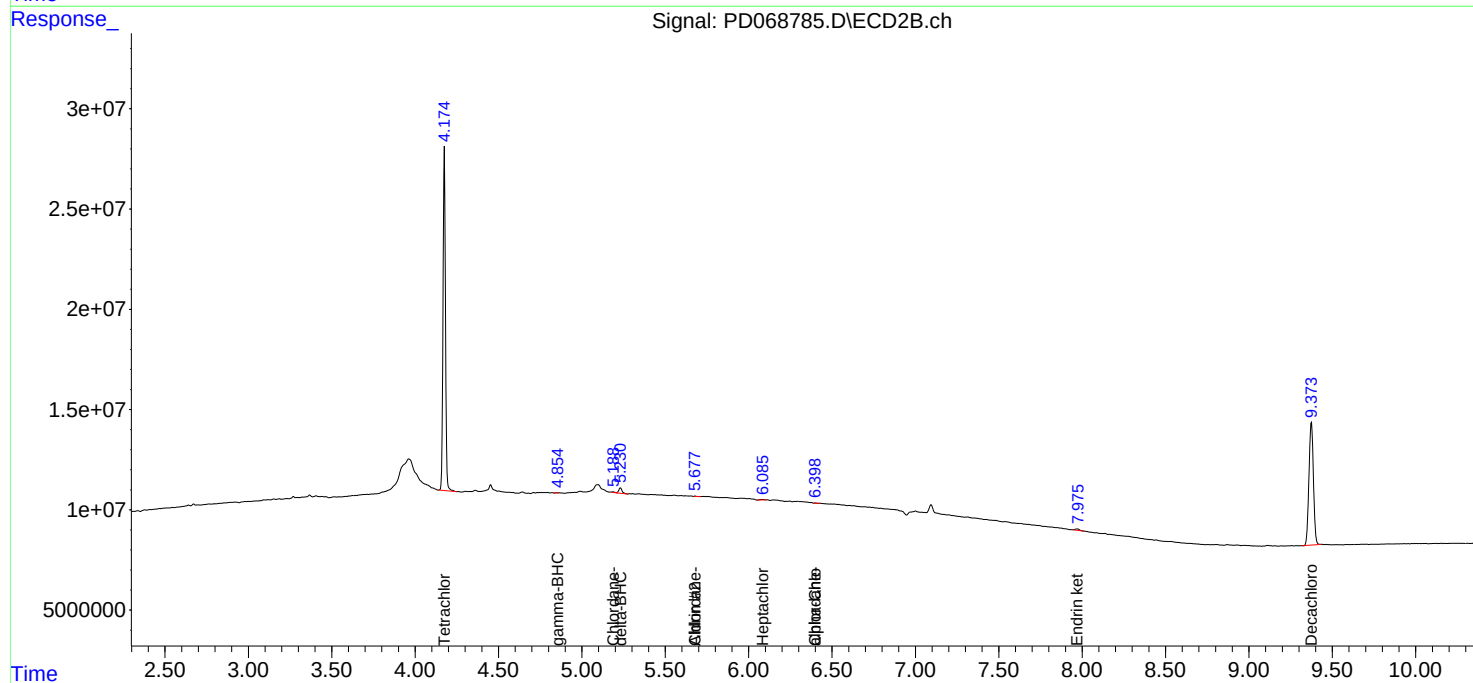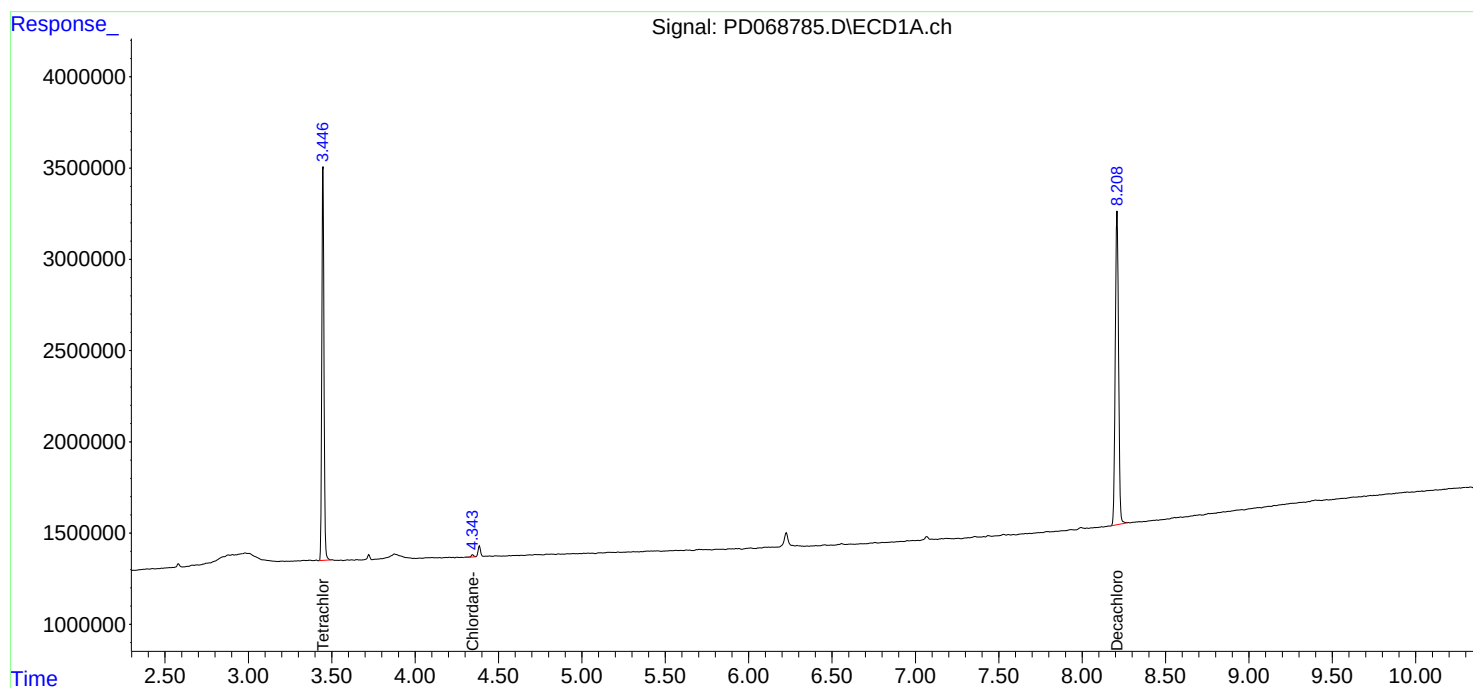


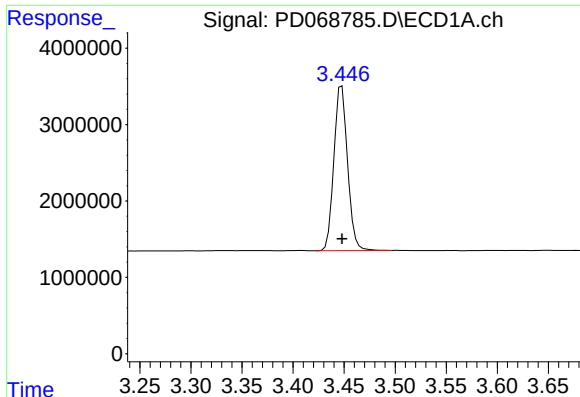

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 20118530
Conc: 16.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

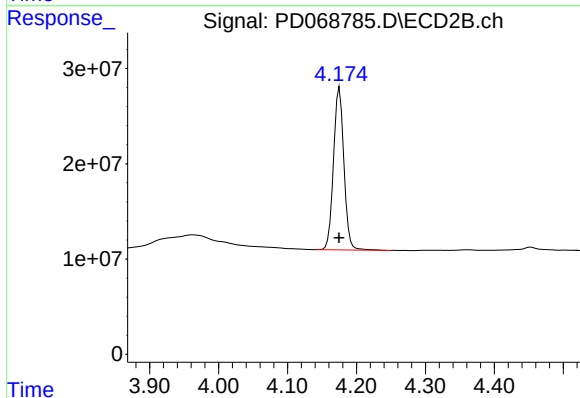


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 178295425
Conc: 18.65 ng/ml

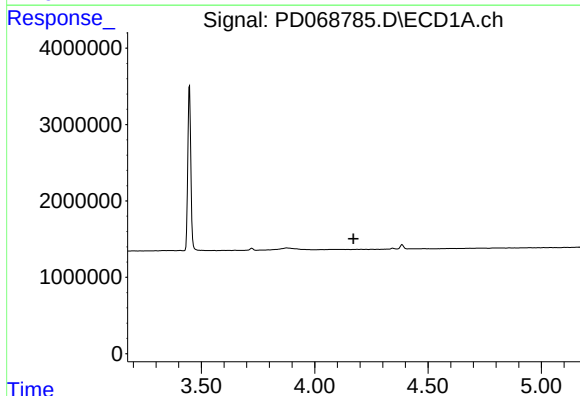


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.172 min
Response: 0
Conc: N.D.

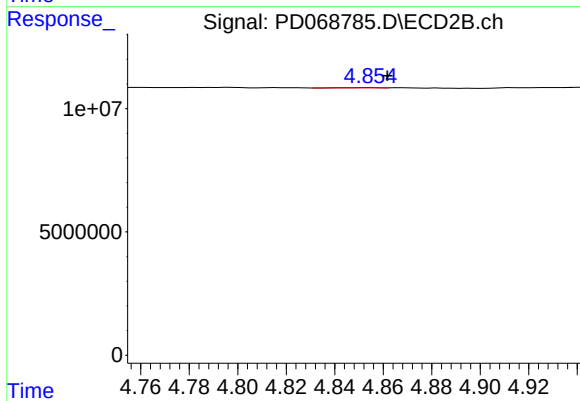

#3 gamma-BHC (Lindane)


R.T.: 4.855 min
Delta R.T.: -0.007 min
Response: 67662
Conc: 0.01 ng/ml

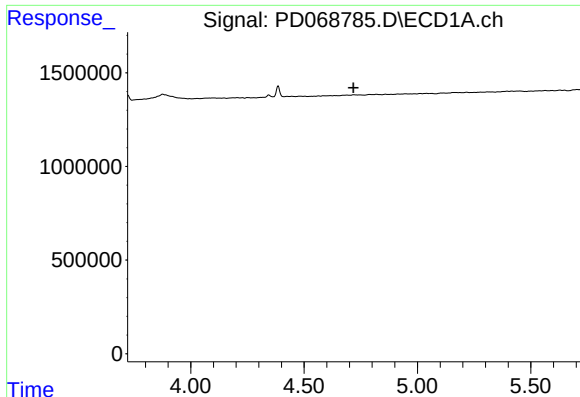

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.718 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

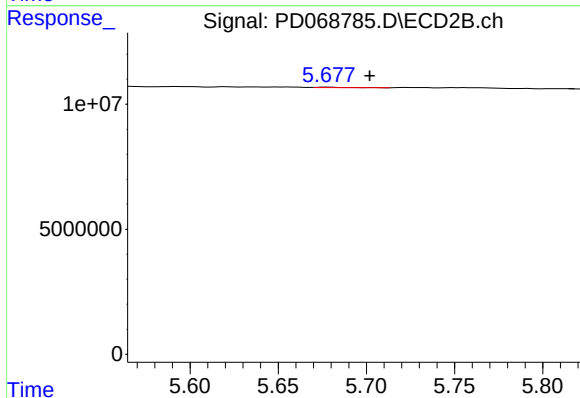


#5 Aldrin

R.T.: 5.679 min
Delta R.T.: -0.023 min
Response: 165184
Conc: 0.01 ng/ml

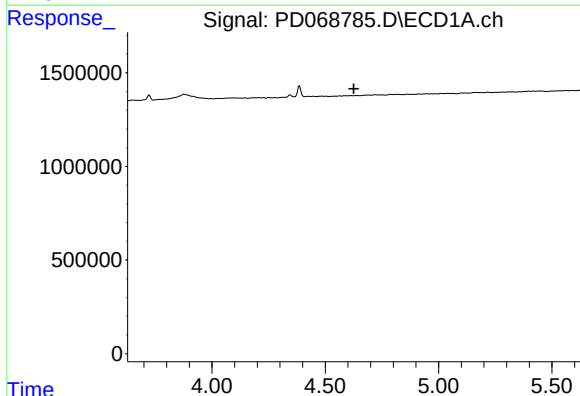


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.626 min
Response: 0
Conc: N.D.

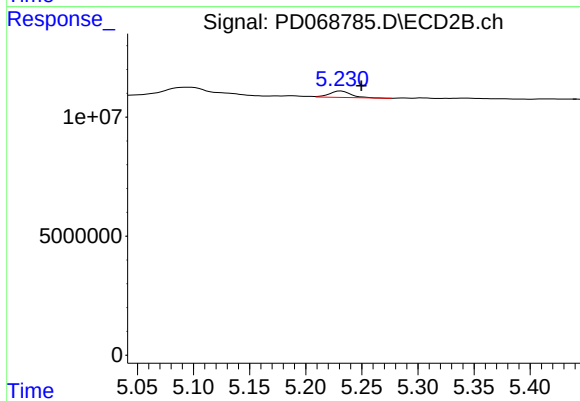

#7 delta-BHC


R.T.: 5.231 min
Delta R.T.: -0.018 min
Response: 3632805
Conc: 0.30 ng/ml

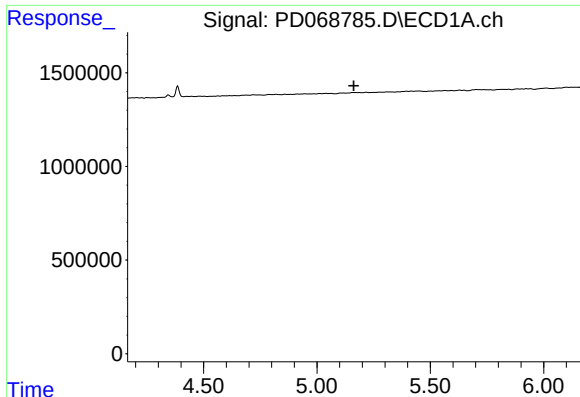

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

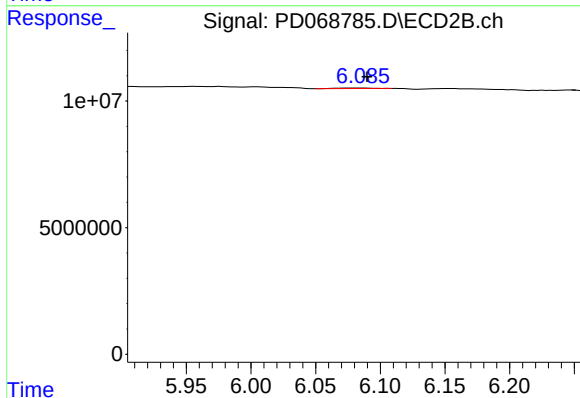


#8 Heptachlor epoxide

R.T.: 6.087 min
Delta R.T.: -0.003 min
Response: 378669
Conc: 0.04 ng/ml

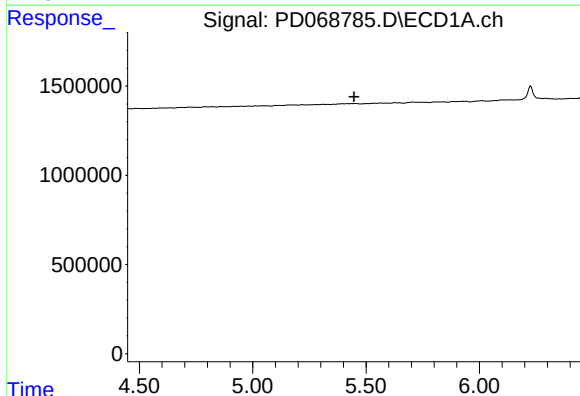


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

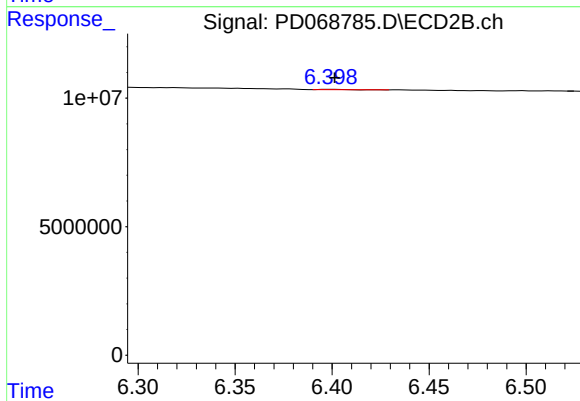

#11 alpha-Chlordane


R.T.: 6.399 min
Delta R.T.: -0.002 min
Response: 111485
Conc: 0.01 ng/ml

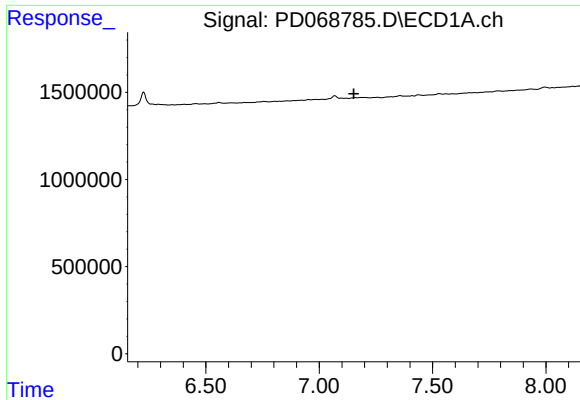

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

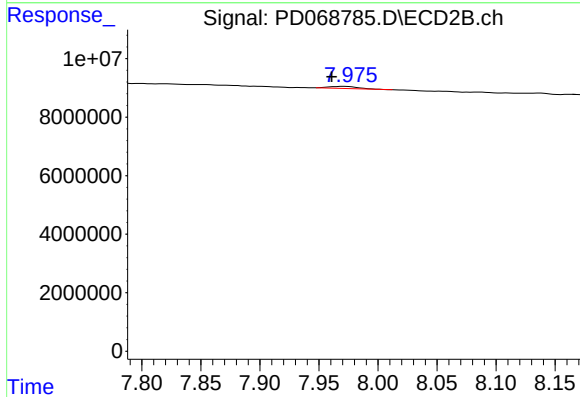


#21 Endrin ketone

R.T.: 7.971 min
Delta R.T.: 0.011 min
Response: 1076371
Conc: 0.14 ng/ml

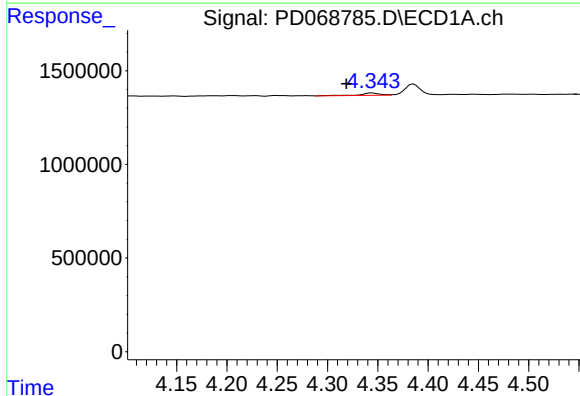


#23 Chlordane-1

R.T.: 4.344 min
Delta R.T.: 0.026 min
Response: 158379
Conc: 3.73 ng/ml

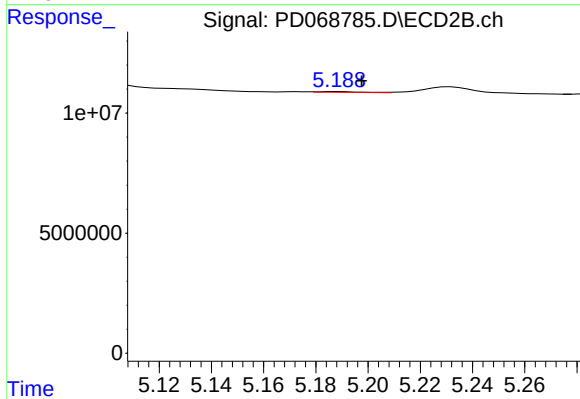

#23 Chlordane-1


R.T.: 5.188 min
Delta R.T.: -0.010 min
Response: 426959
Conc: 1.08 ng/ml

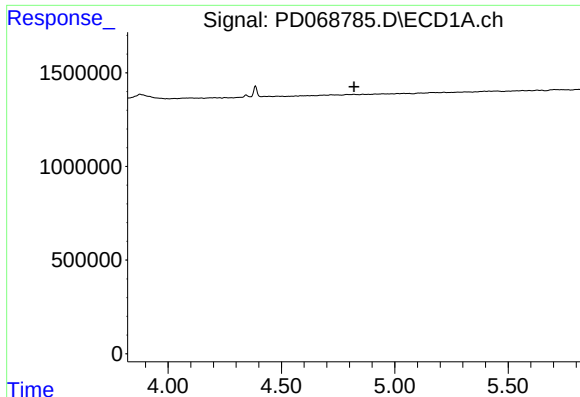

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

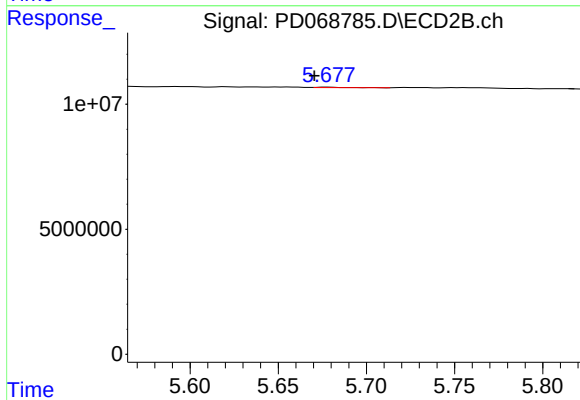


#24 Chlordane-2

R.T.: 5.679 min
Delta R.T.: 0.008 min
Response: 165184
Conc: 0.43 ng/ml

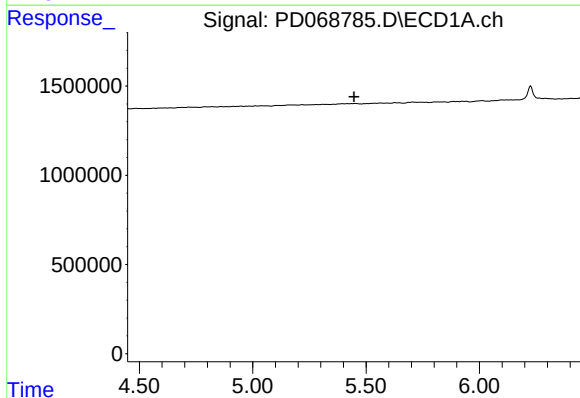


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.447 min
Response: 0
Conc: N.D.

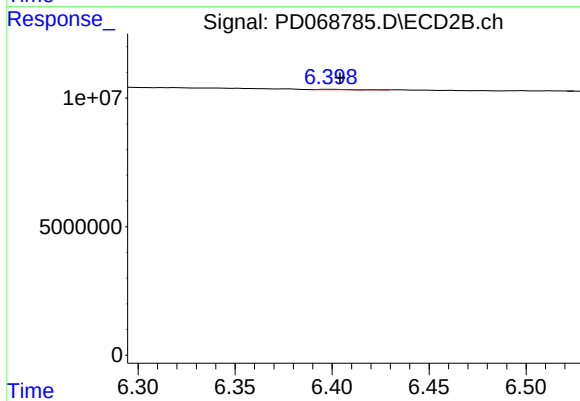

#26 Chlordane-4


R.T.: 6.399 min
Delta R.T.: -0.005 min
Response: 111485
Conc: 0.07 ng/ml

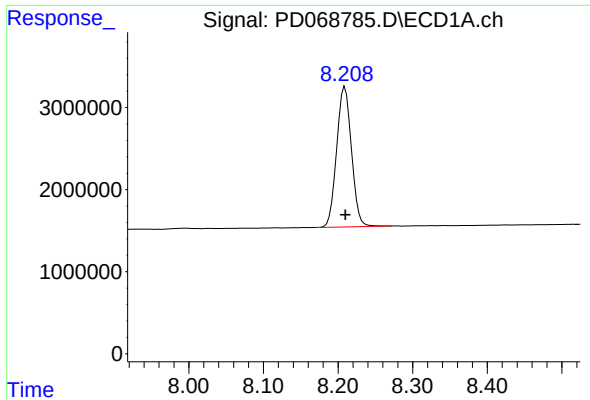

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 23584975
Conc: 18.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

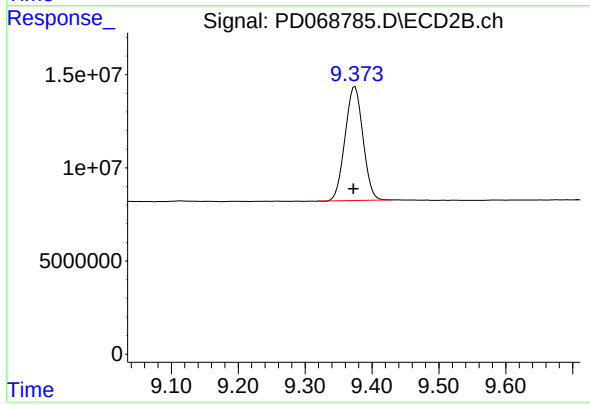

#28 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: 0.002 min
Response: 114126776
Conc: 20.14 ng/ml