

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
 Data File : PD068780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 18:34
 Operator : AR\AJ
 Sample : N2077-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-14A-3-3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/28/2022
 Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 00:06:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.174	19143702	166.9E6	15.767m	17.452m
28)	SA Decachlor...	8.209	9.373	21511468	106.3E6	17.027	18.751

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032622\
Data File : PD068780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 18:34
Operator : AR\AJ
Sample : N2077-16
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WC-14A-3-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/28/2022
Supervised By : mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 00:06:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

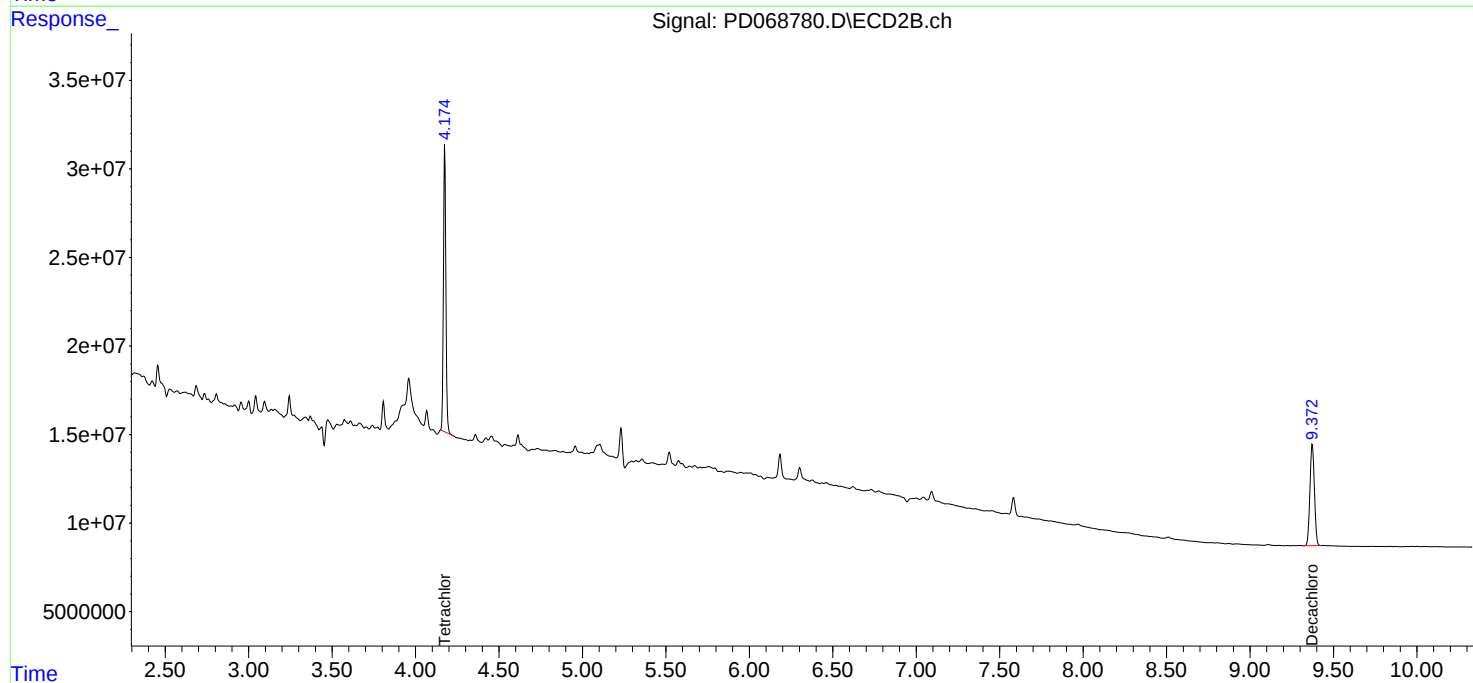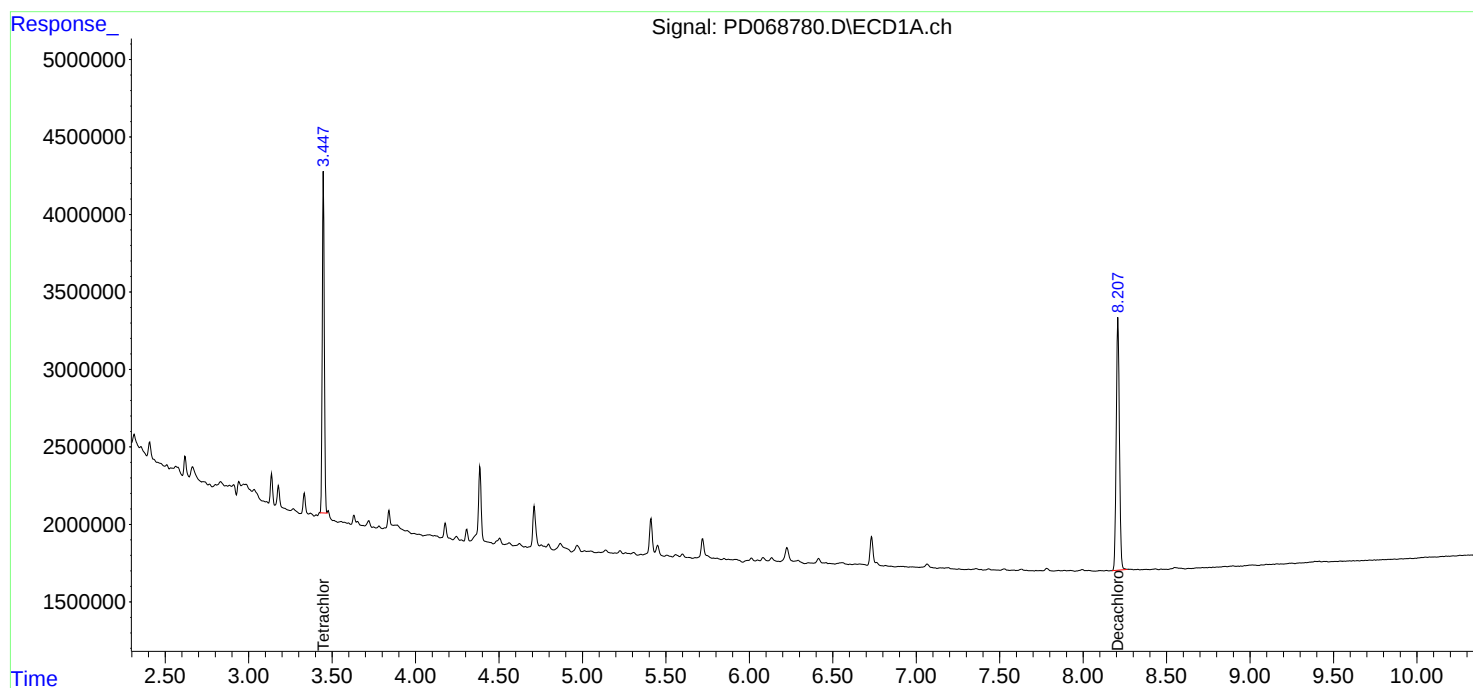

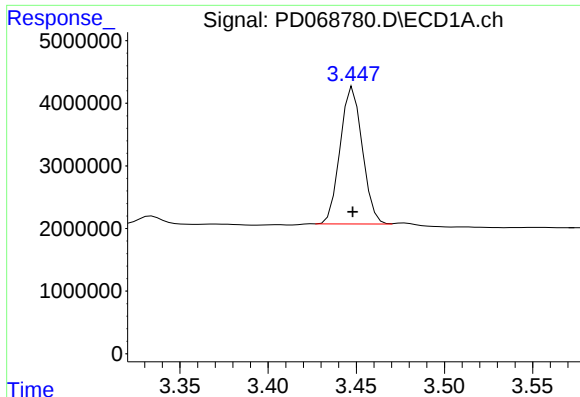


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: -0.001 min
Response: 19143702
Conc: 15.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-14A-3-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

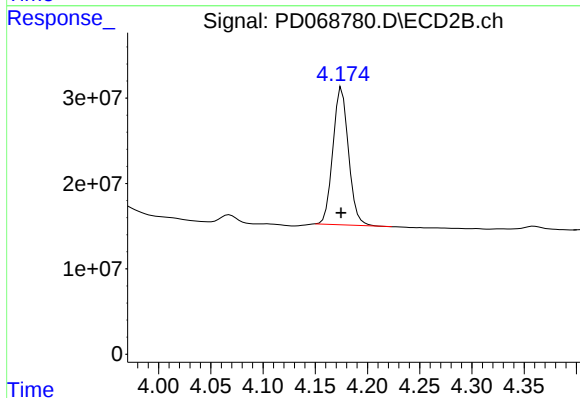


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: 0.000 min
Response: 166851030
Conc: 17.45 ng/ml m

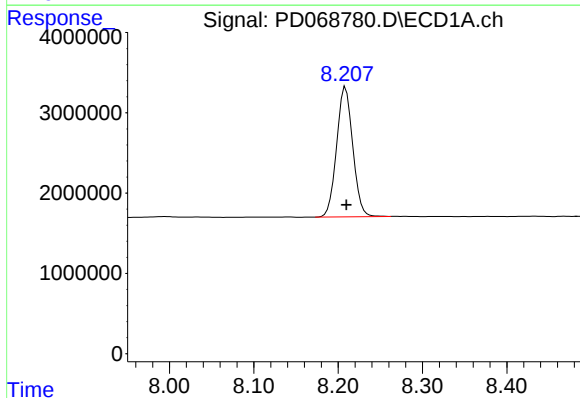

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 21511468
Conc: 17.03 ng/ml

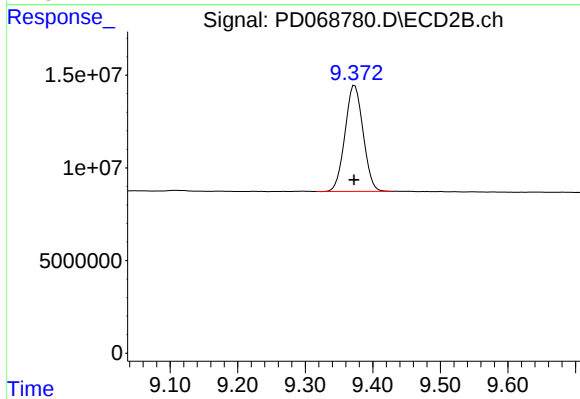

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 106254806
Conc: 18.75 ng/ml