

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
 Data File : PD052174.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 9:54
 Operator : AJ\SJ
 Sample : PB118283BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK83

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 03:09:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.042	25714037	503.9E6	18.116	17.316
27)	SA Decachlor...	7.817	9.152	51275465	532.3E6	32.746	34.483
Target Compounds							
6)	B beta-BHC	0.000	4.931f	0	28171915	N.D.	1.535

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
Data File : PD052174.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 9:54
Operator : AJ\SJ
Sample : PB118283BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 03:09:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

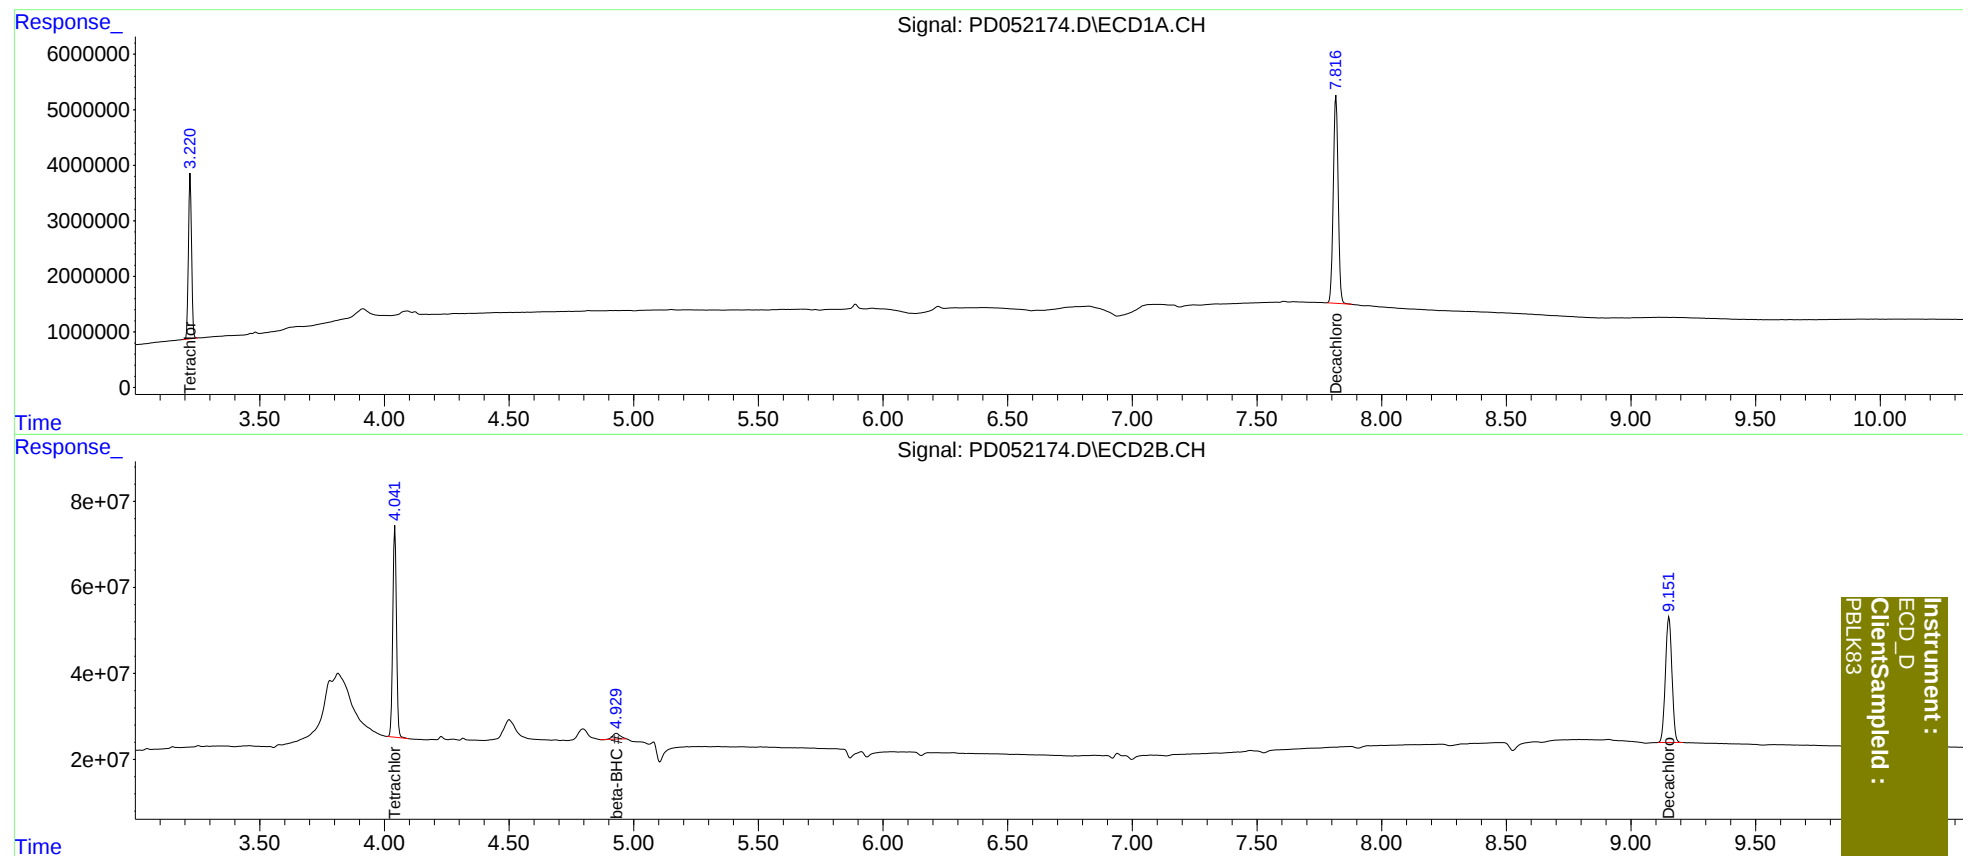


Instrument :
ECD_D
ClientSampleId :
PBLK83

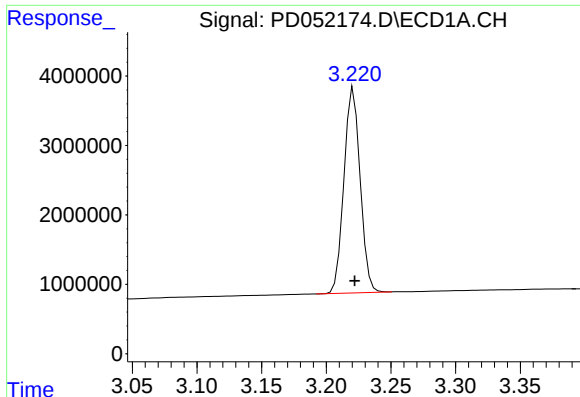

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 25714037
Conc: 18.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK83

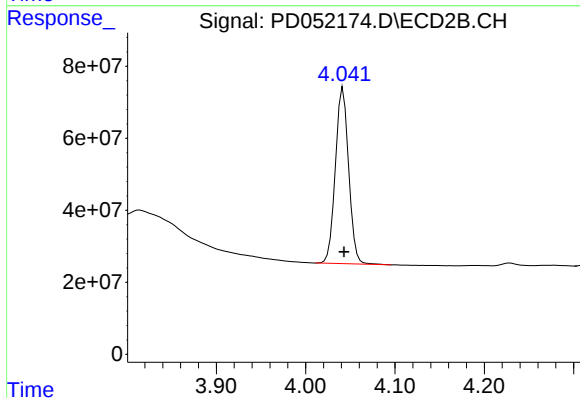


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 503854093
Conc: 17.32 ng/ml

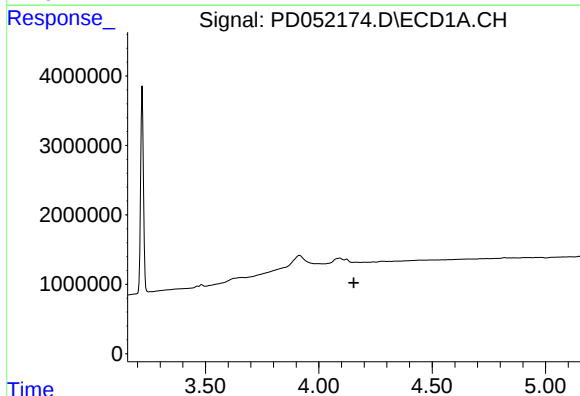


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

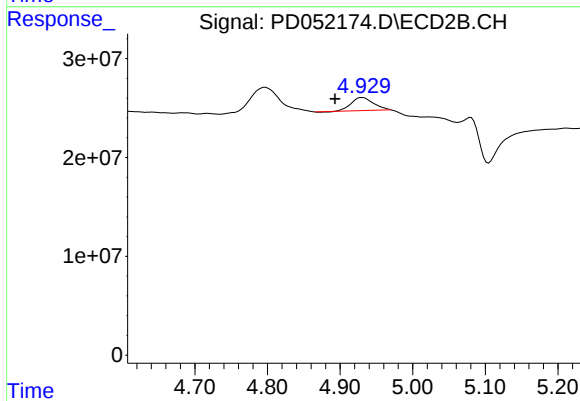

#6 beta-BHC


R.T.: 4.931 min
Delta R.T.: 0.038 min
Response: 28171915
Conc: 1.54 ng/ml

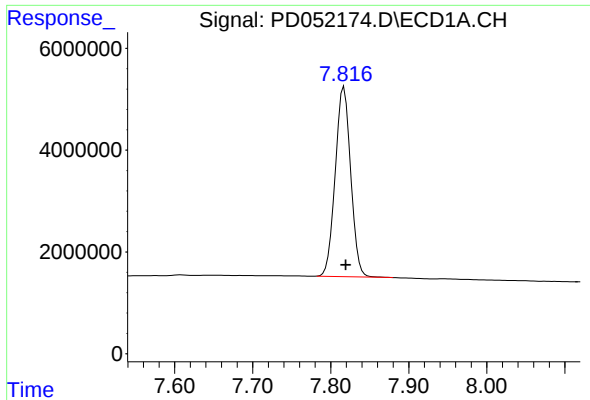

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 51275465
Conc: 32.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK83

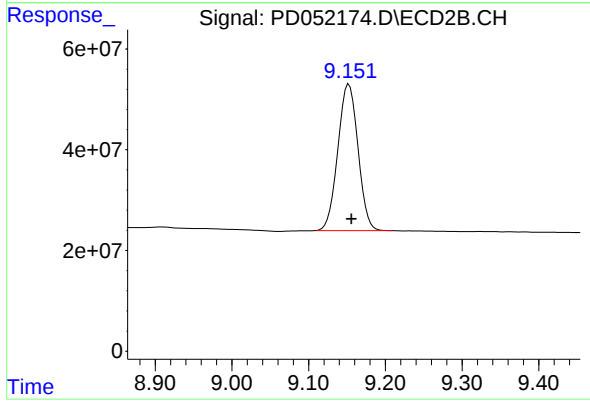

#27 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: -0.003 min
Response: 532309863
Conc: 34.48 ng/ml