

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
 Data File : PD052186.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 12:43
 Operator : AJ\SJ
 Sample : K2084-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF7W7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 03:11:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.221	4.042	23725774	472.3E6	16.715	16.230
2) SA Decachlor...	7.817	9.153	42524543	458.3E6	27.157	29.688
Target Compounds						
2) A alpha-BHC	0.000	4.405f	0	14179635	N.D.	0.324
4) MA Heptachlor	0.000	5.264f	0	10103538	N.D.	0.252
6) B beta-BHC	0.000	4.932f	0	30936424	N.D.	1.686
8) B Heptachlo...	0.000	5.908	0	81604278	N.D.	2.395
10) B trans-Chl...	0.000	6.180	0	20197922	N.D.	0.595
11) B cis-Chlor...	0.000	6.180f	0	20197922	N.D.	0.622

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
Data File : PD052186.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 12:43
Operator : AJ\SJ
Sample : K2084-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 03:11:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

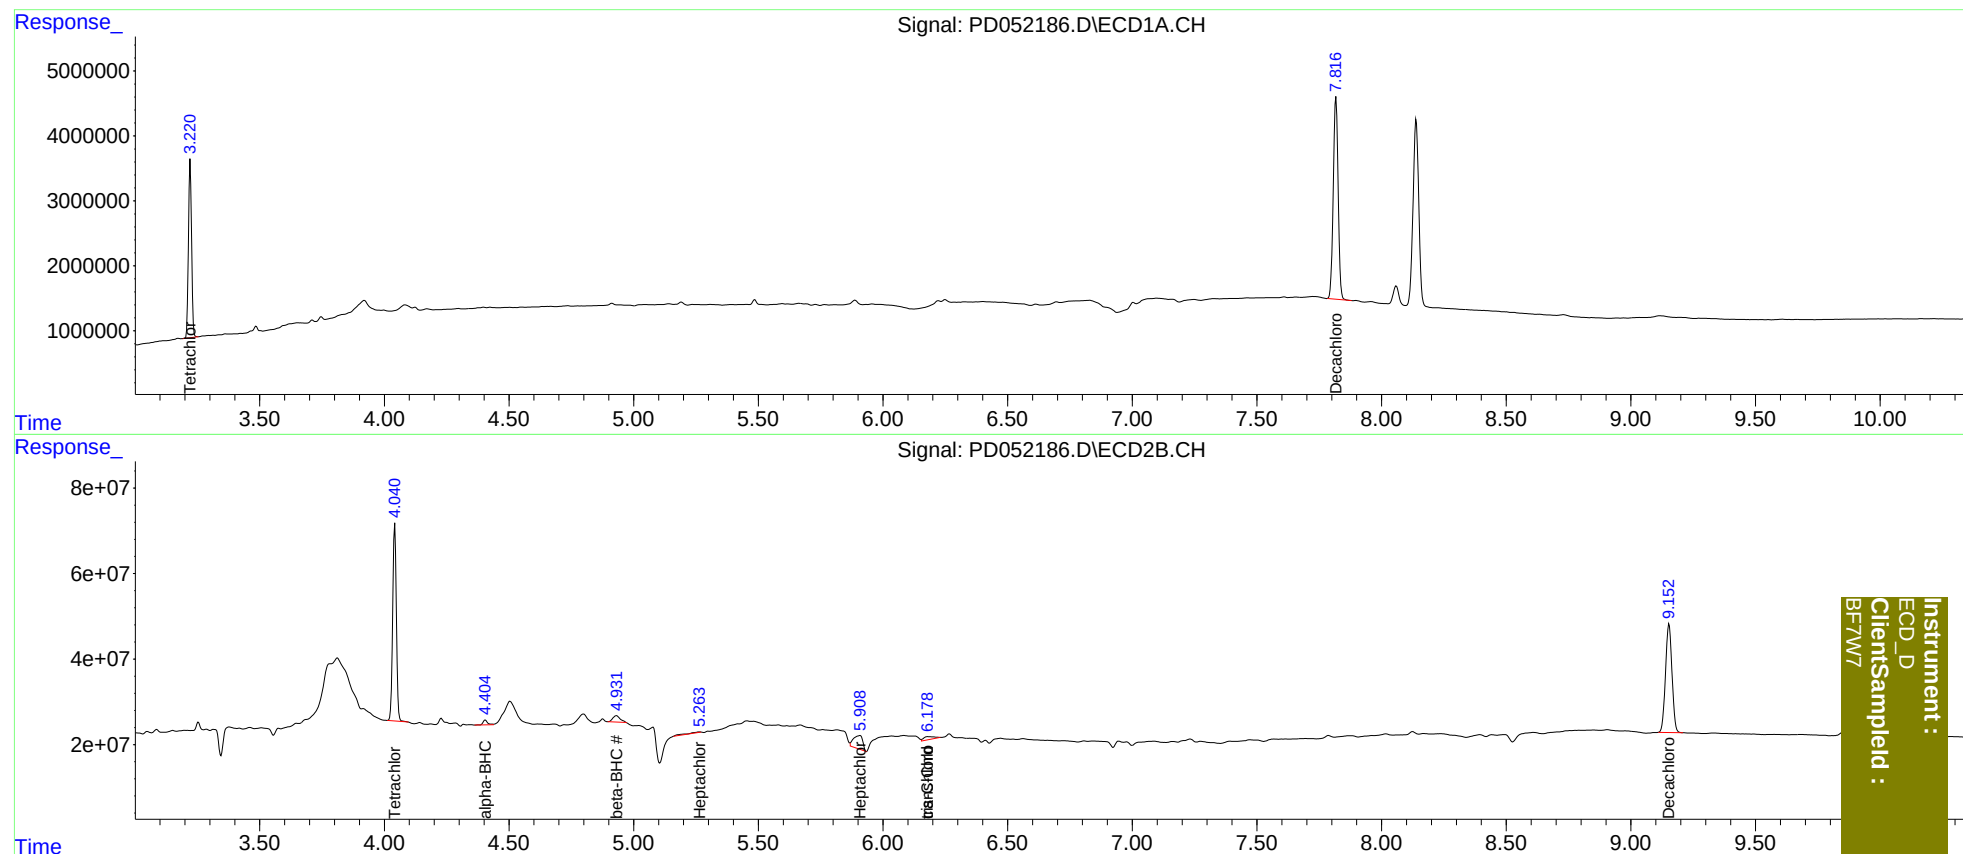


Instrument :
ECD_D
ClientSampleId :
BFTW7

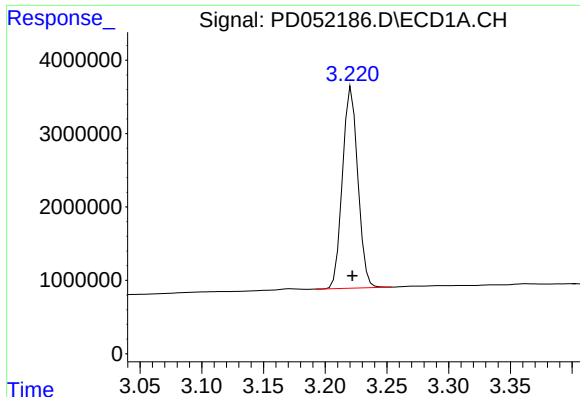

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 23725774
Conc: 16.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF7W7

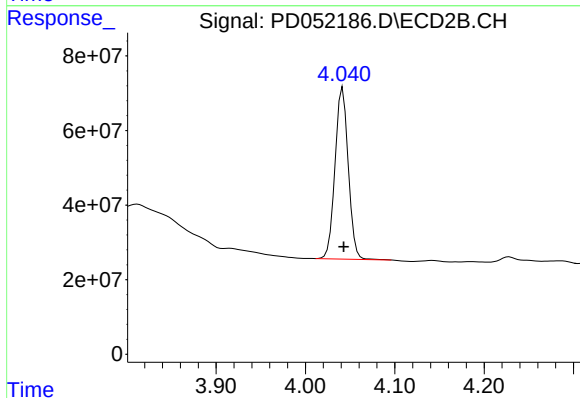


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 472252162
Conc: 16.23 ng/ml

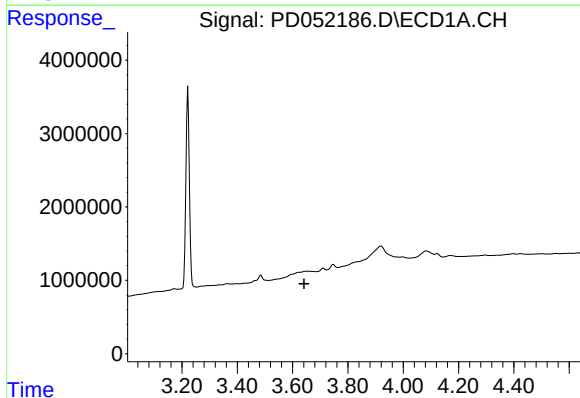


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

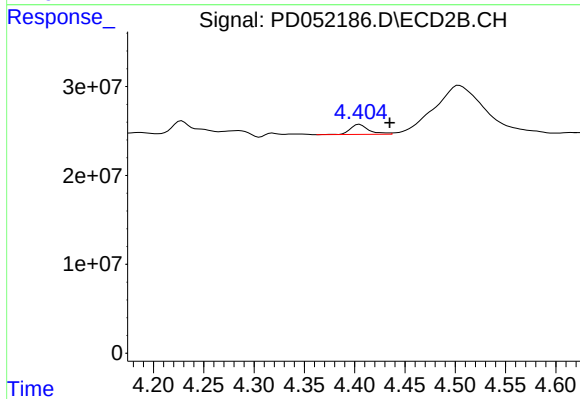

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 14179635
Conc: 0.32 ng/ml

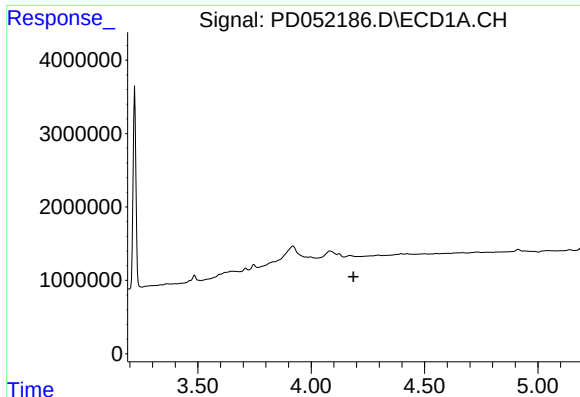

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7W7

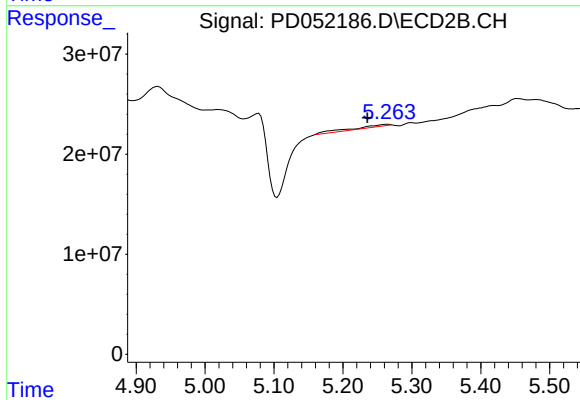


#4 Heptachlor

R.T.: 5.264 min
Delta R.T.: 0.029 min
Response: 10103538
Conc: 0.25 ng/ml

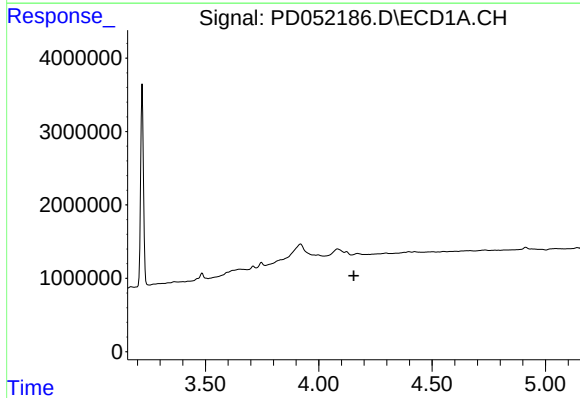


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.154 min
Response: 0
Conc: N.D.

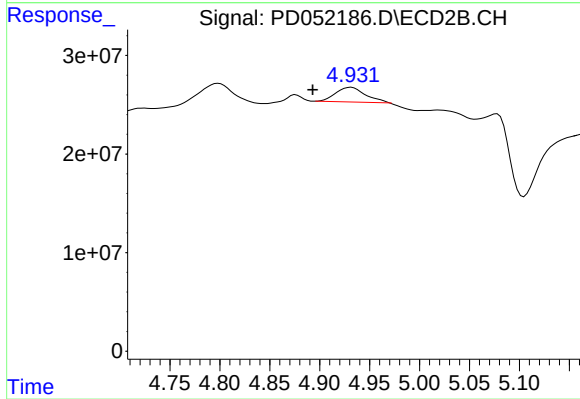

#6 beta-BHC


R.T.: 4.932 min
Delta R.T.: 0.039 min
Response: 30936424
Conc: 1.69 ng/ml

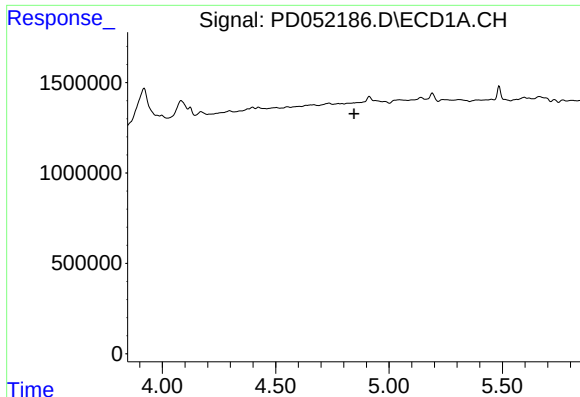

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7W7

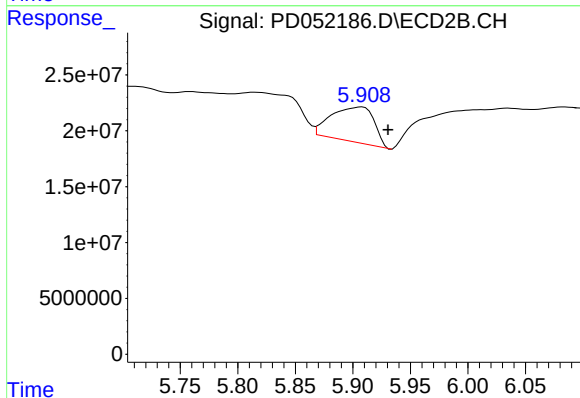


#8 Heptachlor epoxide

R.T.: 5.908 min
Delta R.T.: -0.022 min
Response: 81604278
Conc: 2.40 ng/ml

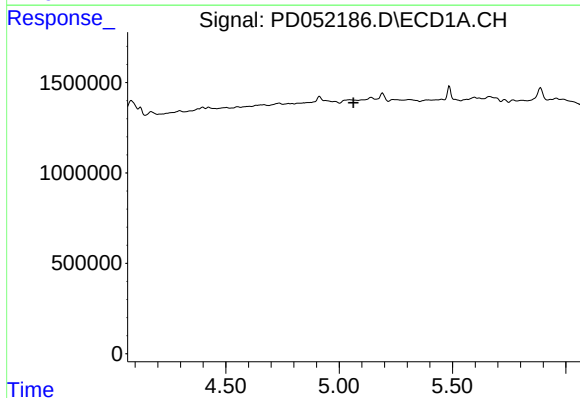


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

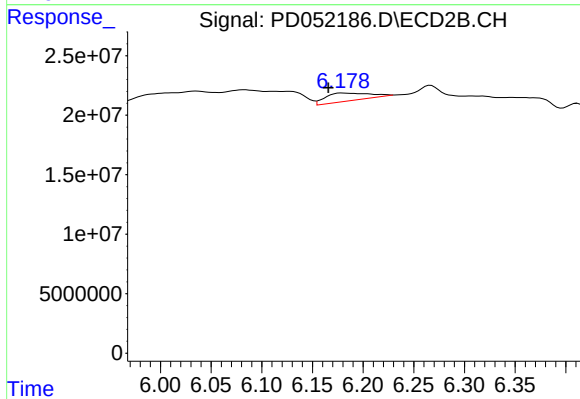

#10 trans-Chlordane


R.T.: 6.180 min
Delta R.T.: 0.014 min
Response: 20197922
Conc: 0.59 ng/ml

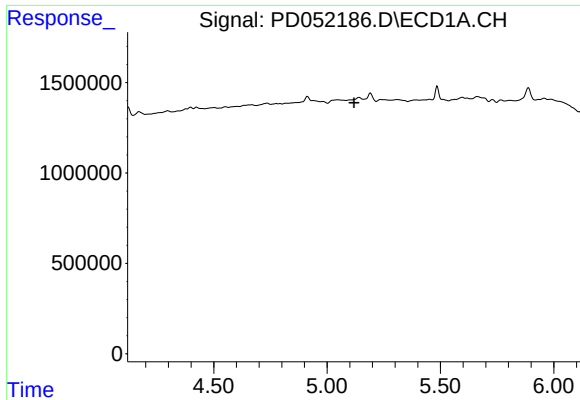

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7W7

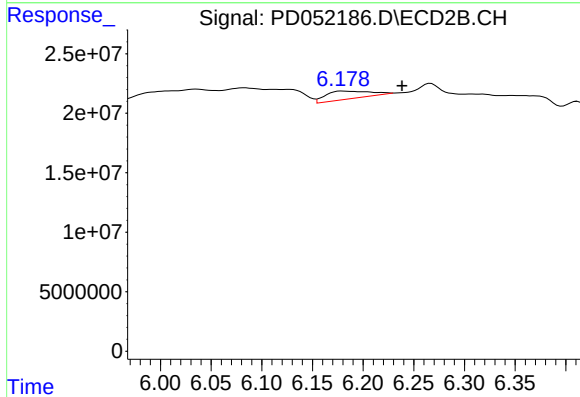


#11 cis-Chlordane

R.T.: 6.180 min
Delta R.T.: -0.058 min
Response: 20197922
Conc: 0.62 ng/ml

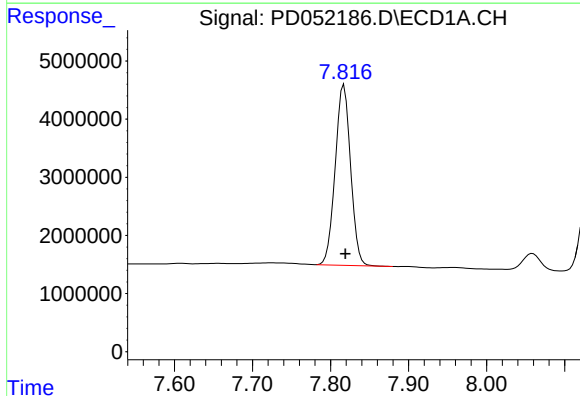

#27 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 42524543
Conc: 27.16 ng/ml

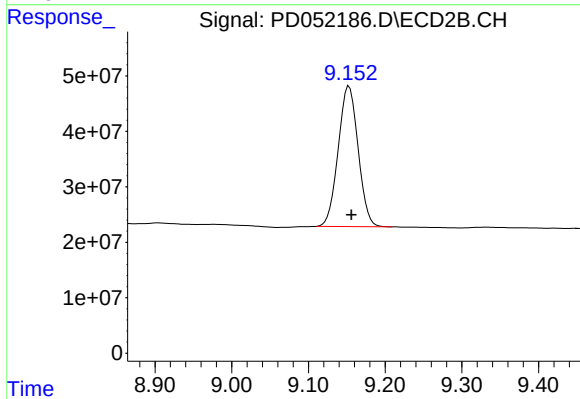

#27 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: -0.003 min
Response: 458291053
Conc: 29.69 ng/ml