

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
 Data File : PD052223.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 22:09
 Operator : AJ\SJ
 Sample : K2085-09
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF7T4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 03:17:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.041	19986524	363.3E6	14.081	12.486
27)	SA Decachlor...	7.816	9.151	34945765	391.3E6	22.317	25.350
Target Compounds							
2)	A alpha-BHC	0.000	4.409f	0 51057382	N.D.	1.168	
3)	MA gamma-BHC...	0.000	4.732	0 16675678	N.D.	0.420	
5)	MB Aldrin	0.000	5.540	0 19529390	N.D.	0.525	
6)	B beta-BHC	0.000	4.934f	0 6767554	N.D.	0.369	
7)	B delta-BHC	0.000	5.078f	0 52929704	N.D.	1.334	
8)	B Heptachlo...	0.000	5.914	0 66913247	N.D.	1.964	
9)	A Endosulfan I	0.000	6.248f	0 73616372	N.D.	2.348	
10)	B trans-Chl...	0.000	6.178	0 92905656	N.D.	2.736	
11)	B cis-Chlor...	0.000	6.248	0 73616372	N.D.	2.267	
13)	MA Dieldrin	0.000	6.544	0 31856231	N.D.	1.022	
15)	B Endosulfa...	0.000	6.982	0 15162451	N.D.	0.598	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
Data File : PD052223.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 22:09
Operator : AJ\SJ
Sample : K2085-09
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 03:17:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

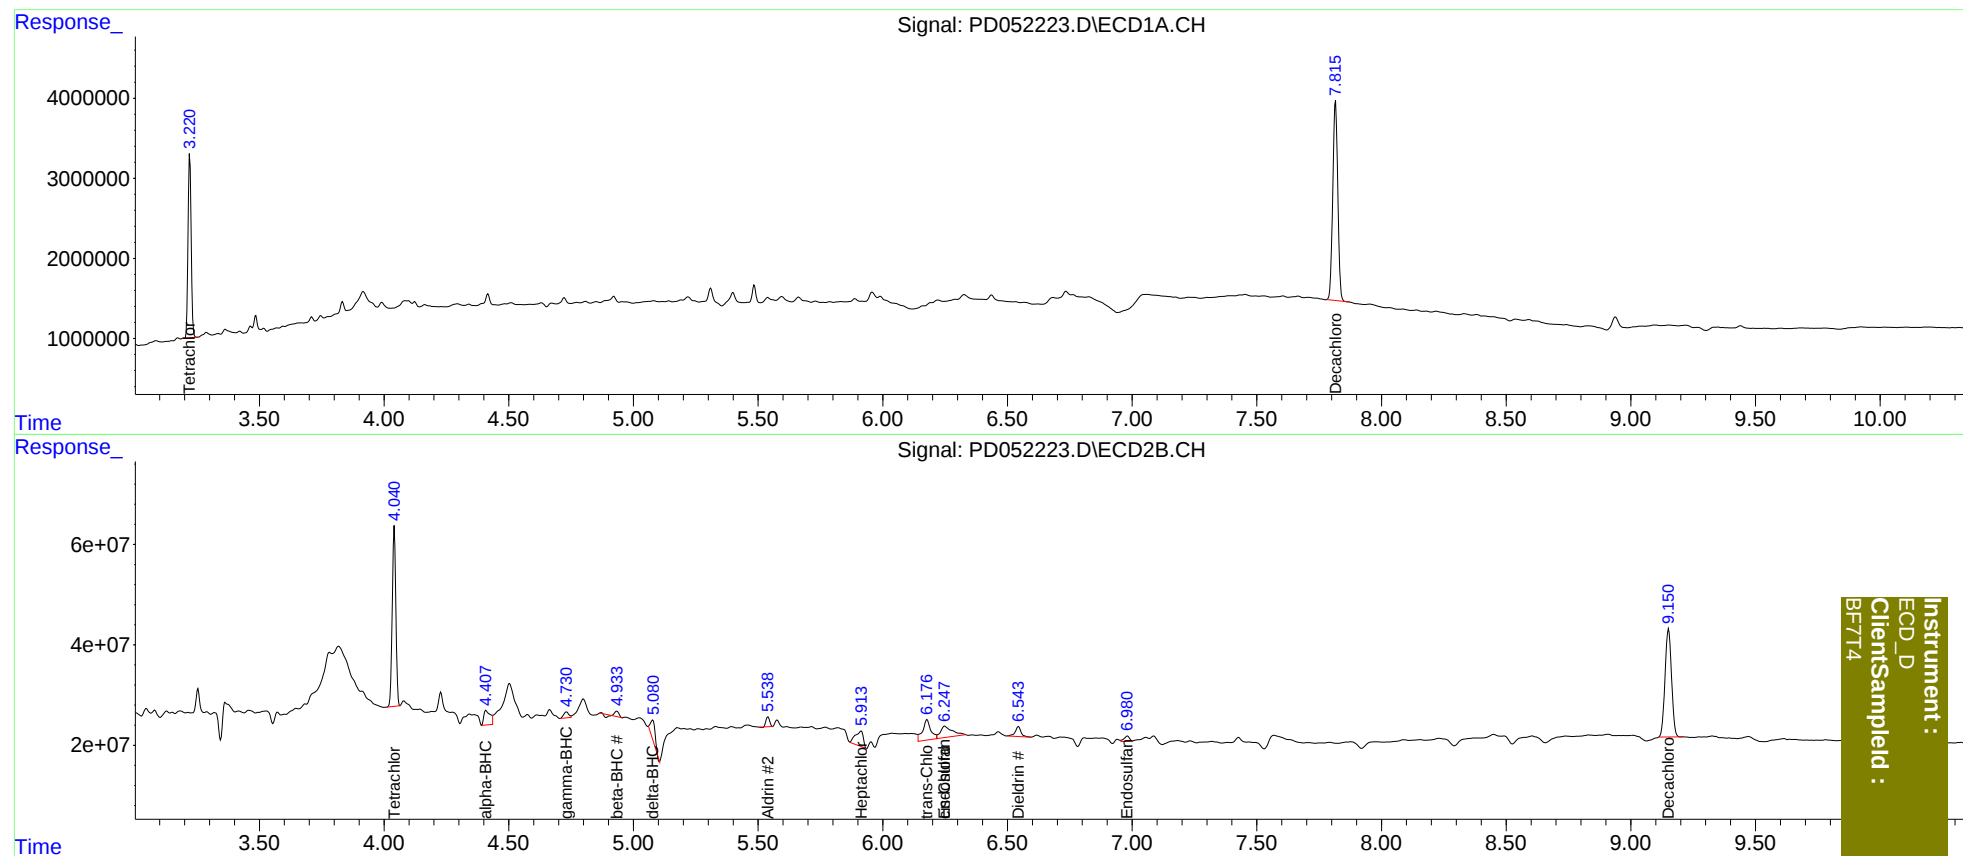


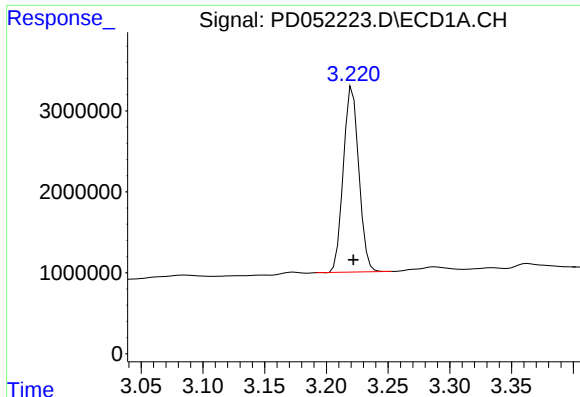

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 19986524
Conc: 14.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF7T4

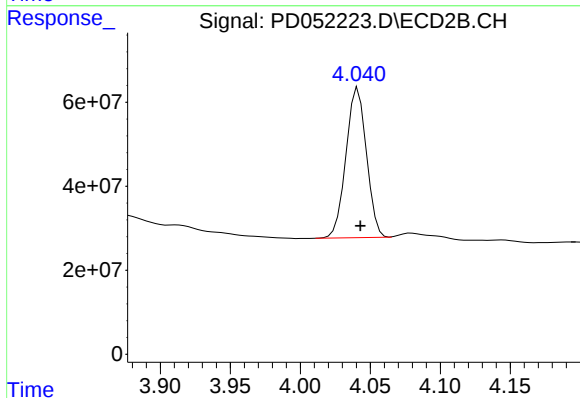


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 363304360
Conc: 12.49 ng/ml

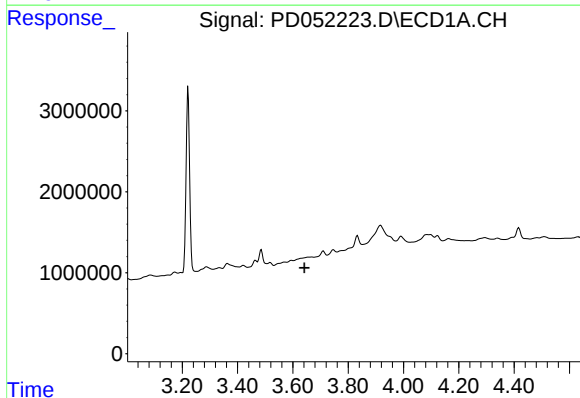


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.641 min
Response: 0
Conc: N.D.

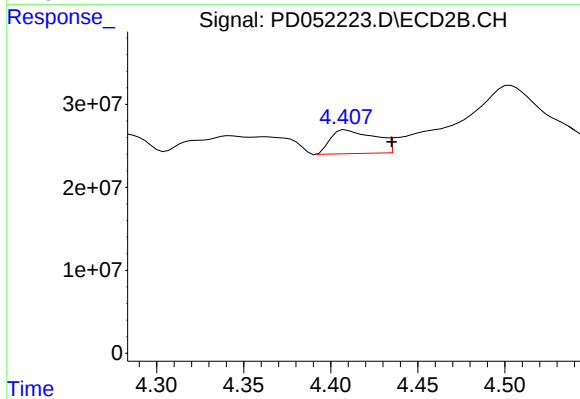

#2 alpha-BHC


R.T.: 4.409 min
Delta R.T.: -0.026 min
Response: 51057382
Conc: 1.17 ng/ml

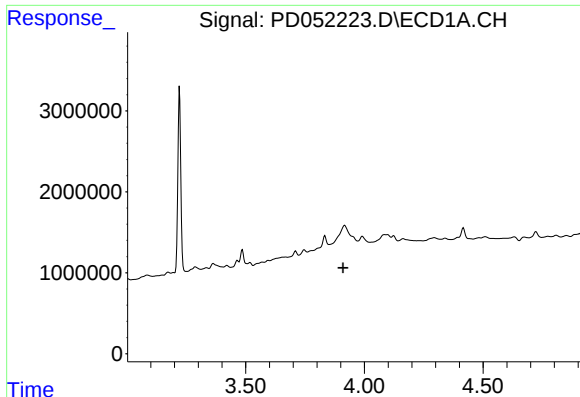

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.910 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7T4

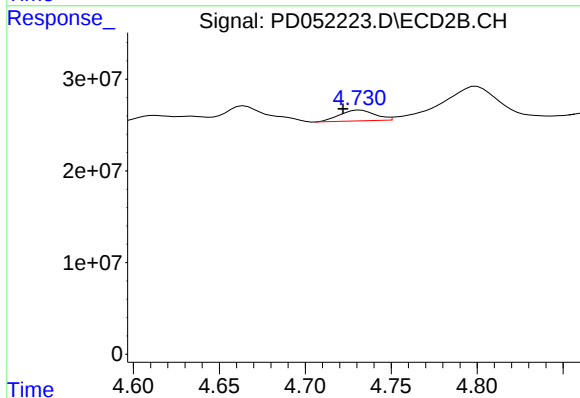


#3 gamma-BHC (Lindane)

R.T.: 4.732 min
Delta R.T.: 0.010 min
Response: 16675678
Conc: 0.42 ng/ml

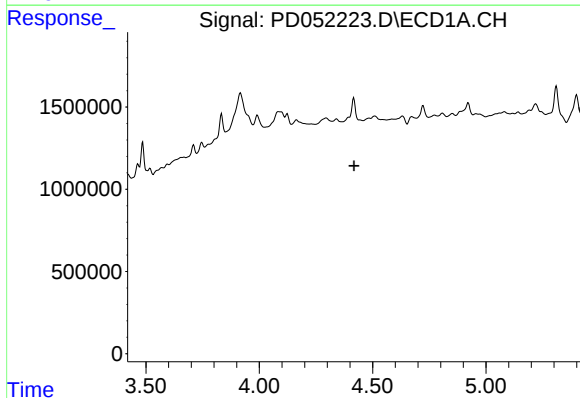


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.419 min
Response: 0
Conc: N.D.

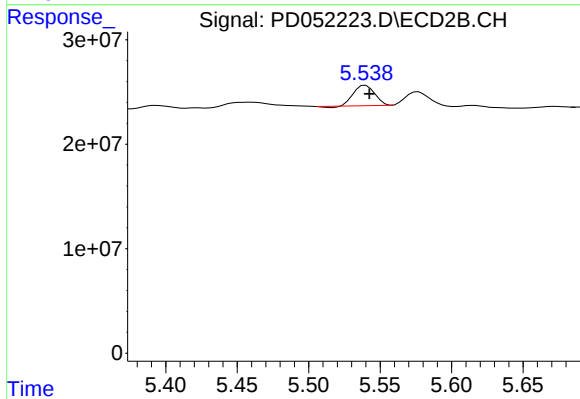

#5 Aldrin


R.T.: 5.540 min
Delta R.T.: -0.003 min
Response: 19529390
Conc: 0.52 ng/ml

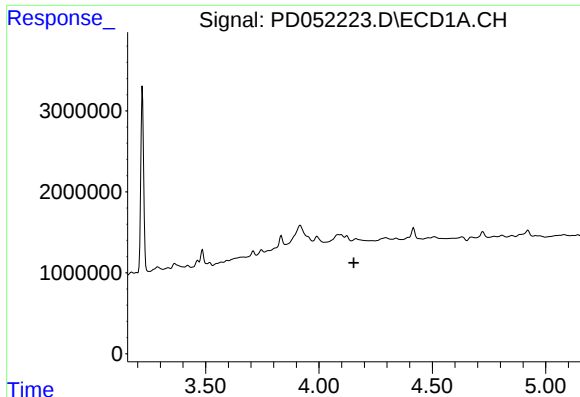

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7T4

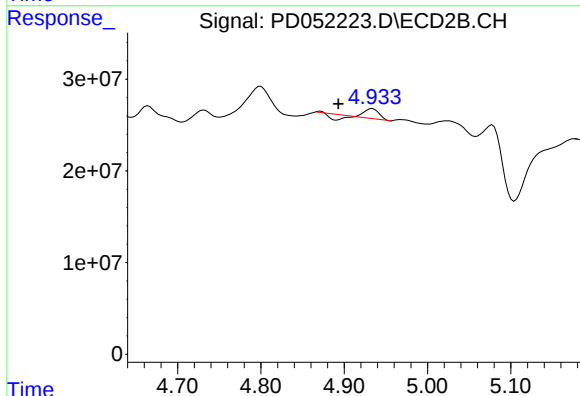


#6 beta-BHC

R.T.: 4.934 min
Delta R.T.: 0.041 min
Response: 6767554
Conc: 0.37 ng/ml

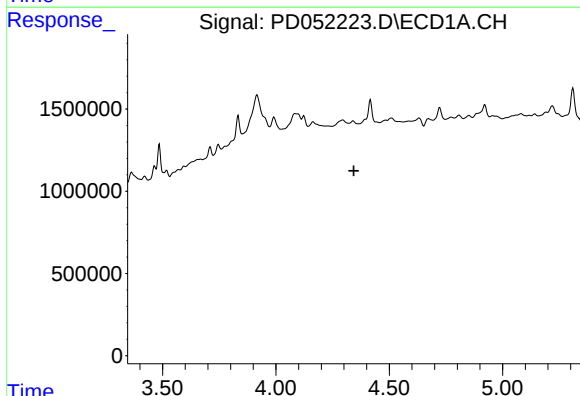


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.344 min
Response: 0
Conc: N.D.

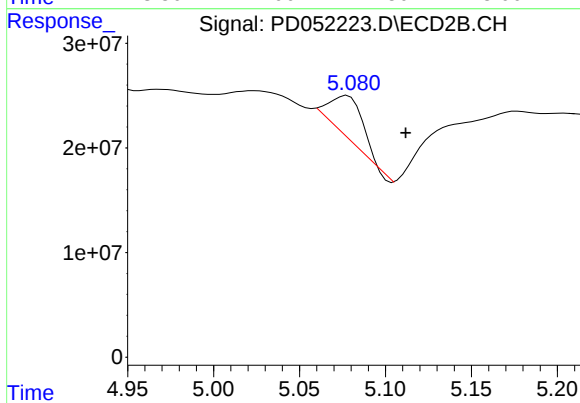

#7 delta-BHC


R.T.: 5.078 min
Delta R.T.: -0.034 min
Response: 52929704
Conc: 1.33 ng/ml

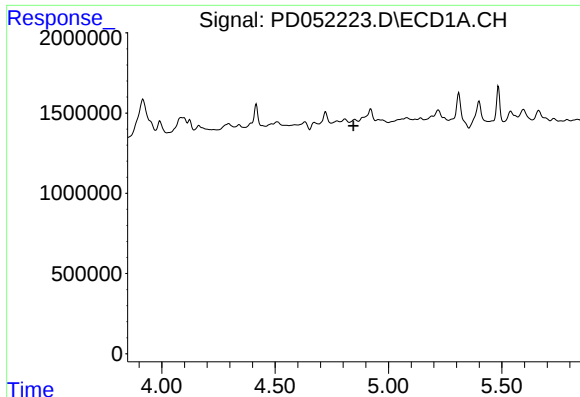

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7T4

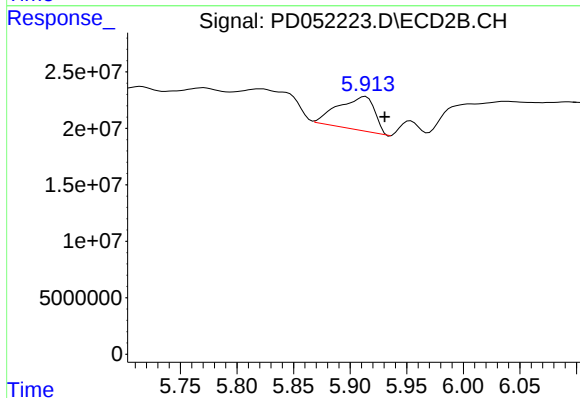


#8 Heptachlor epoxide

R.T.: 5.914 min
Delta R.T.: -0.017 min
Response: 66913247
Conc: 1.96 ng/ml

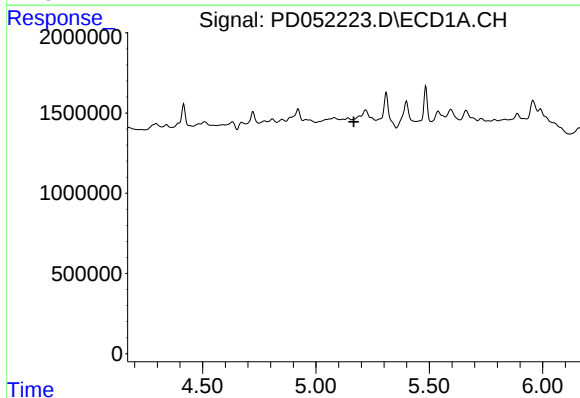


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

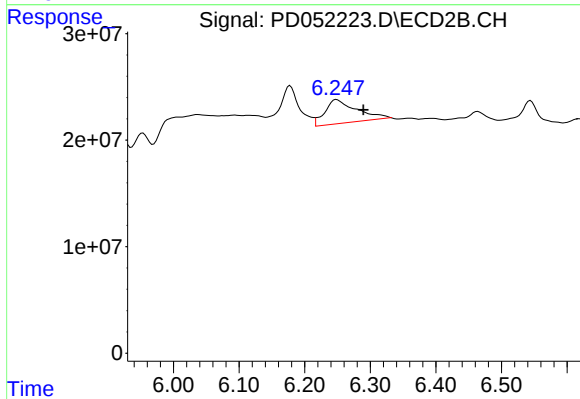

#9 Endosulfan I


R.T.: 6.248 min
Delta R.T.: -0.041 min
Response: 73616372
Conc: 2.35 ng/ml

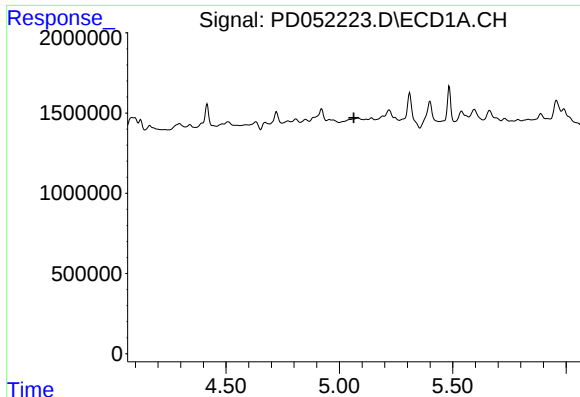

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7T4

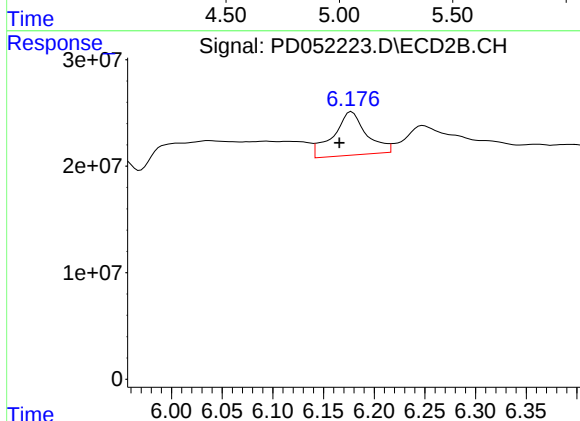


#10 trans-Chlordane

R.T.: 6.178 min
Delta R.T.: 0.012 min
Response: 92905656
Conc: 2.74 ng/ml

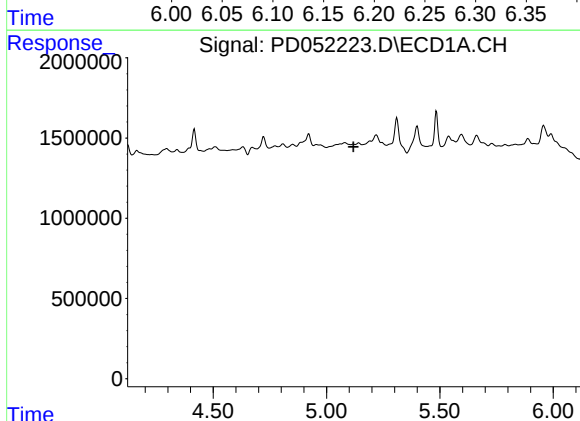


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

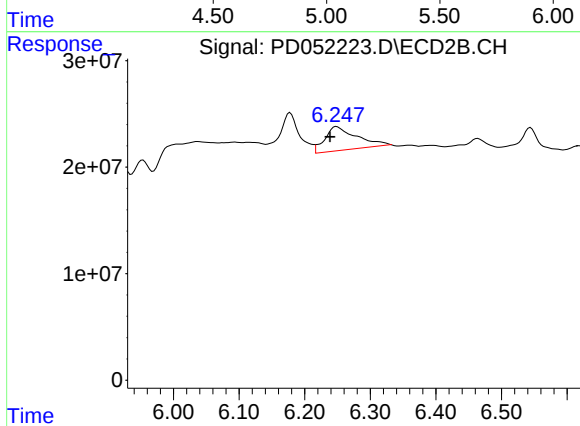

#11 cis-Chlordane


R.T.: 6.248 min
Delta R.T.: 0.010 min
Response: 73616372
Conc: 2.27 ng/ml

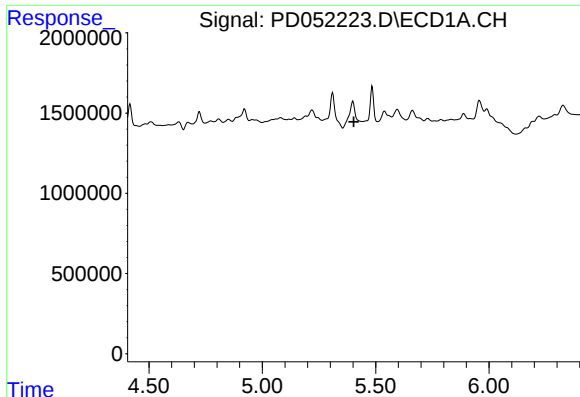

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF7T4

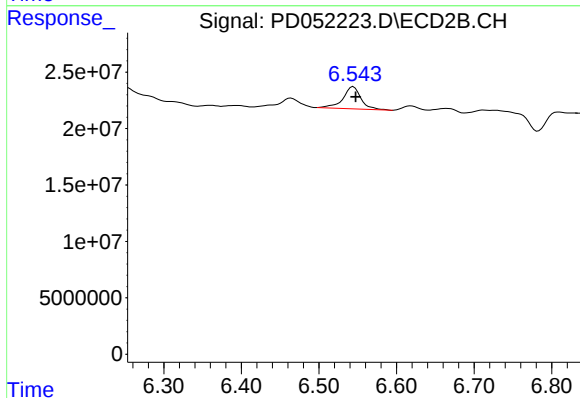


#13 Dieldrin

R.T.: 6.544 min
Delta R.T.: -0.003 min
Response: 31856231
Conc: 1.02 ng/ml

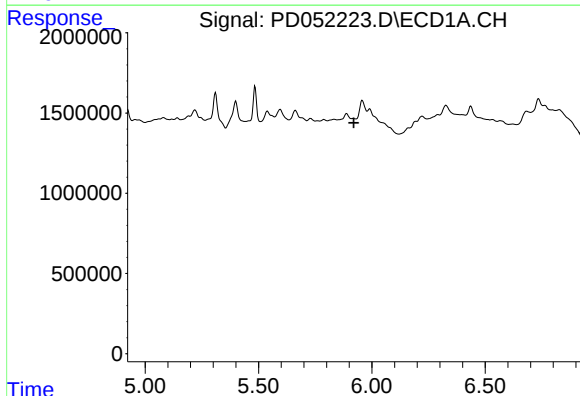


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

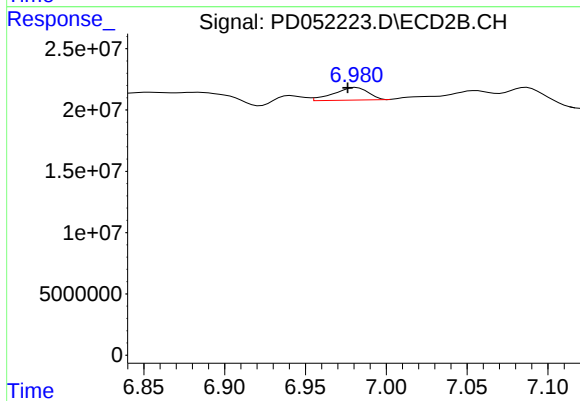

#15 Endosulfan II


R.T.: 6.982 min
Delta R.T.: 0.005 min
Response: 15162451
Conc: 0.60 ng/ml

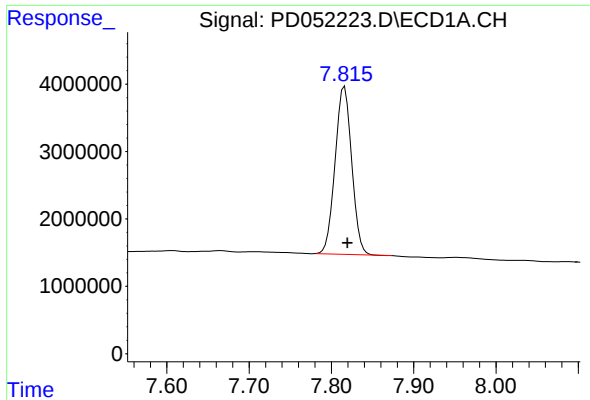

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.003 min
Response: 34945765
Conc: 22.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF7T4

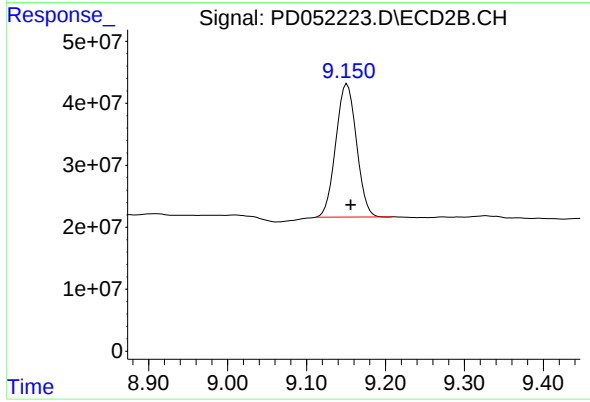

#27 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: -0.004 min
Response: 391316641
Conc: 25.35 ng/ml