

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
 Data File : PD052229.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 23:34
 Operator : AJ\SJ
 Sample : PIBLK03
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 03:18:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.221	4.042	32687508	610.7E6	23.029	20.989
27) SA Decachlor...	7.816	9.151	56574076	568.0E6	36.130	36.797
Target Compounds						
10) B trans-Chl...	0.000	6.139	0	26990603	N.D.	0.795
11) B cis-Chlor...	0.000	6.193f	0	12728200	N.D.	0.392


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
Data File : PD052229.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 23:34
Operator : AJ\SJ
Sample : PIBLK03
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 03:18:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

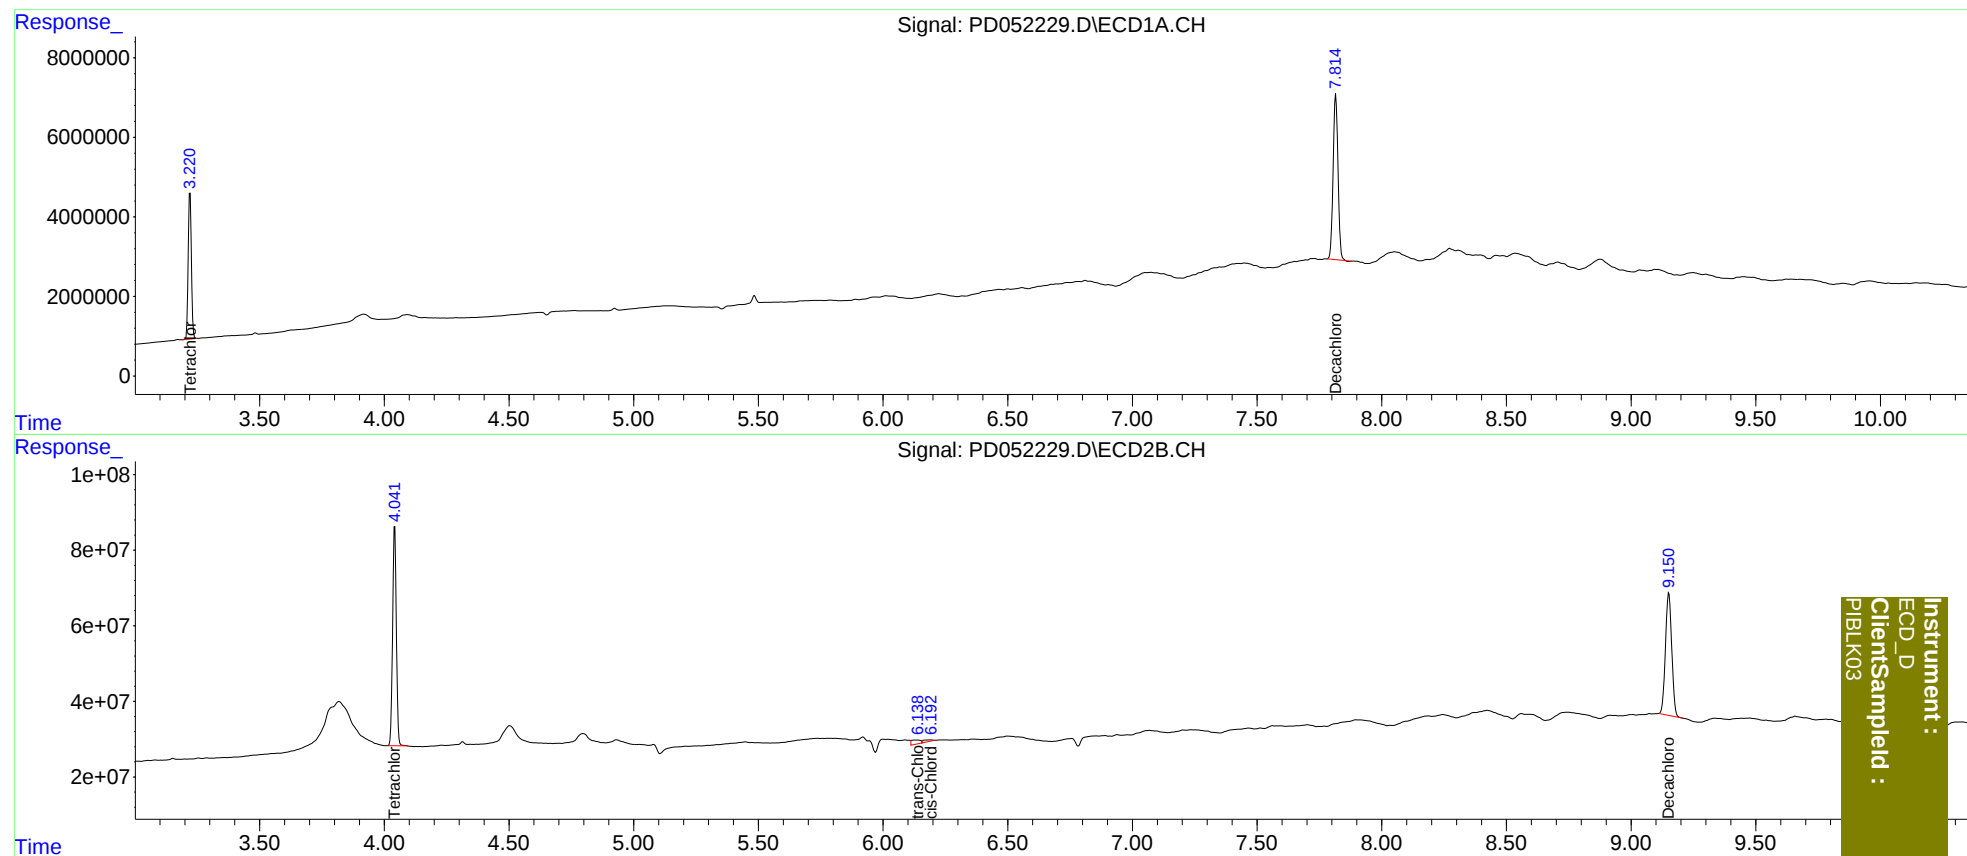


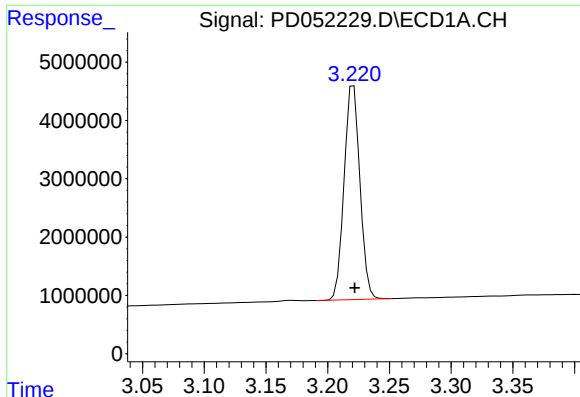

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 32687508
Conc: 23.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK03

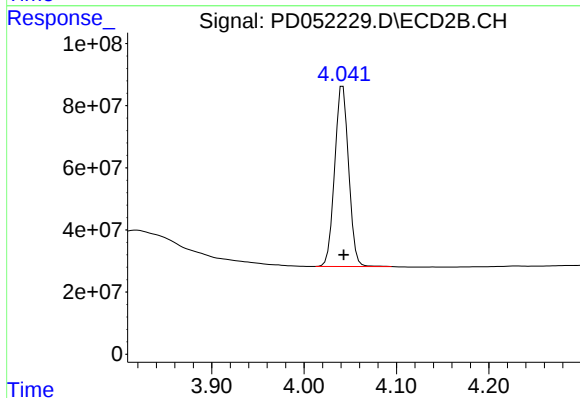


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 610720795
Conc: 20.99 ng/ml

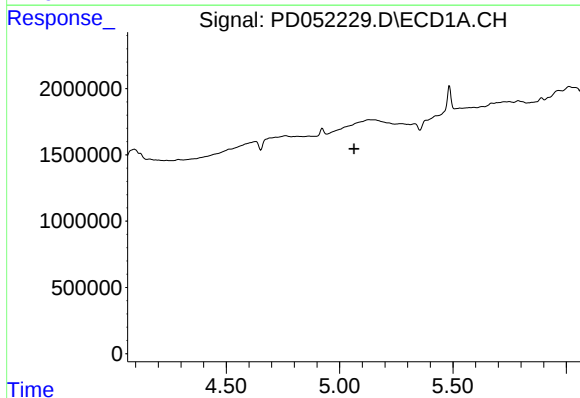


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

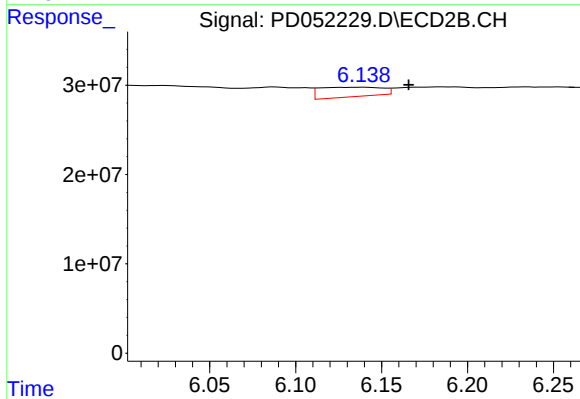

#10 trans-Chlordane


R.T.: 6.139 min
Delta R.T.: -0.027 min
Response: 26990603
Conc: 0.79 ng/ml

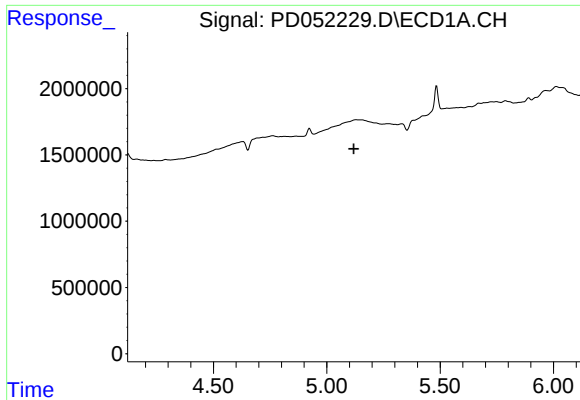

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK03

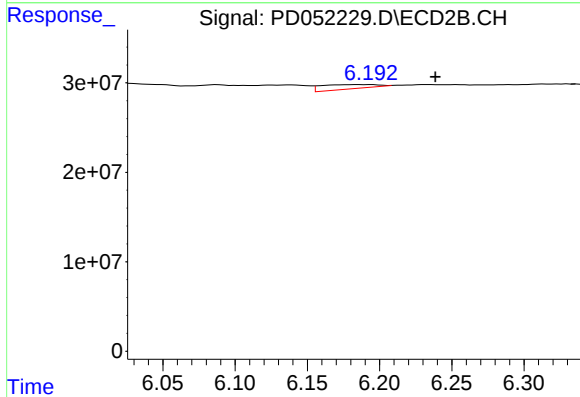


#11 cis-Chlordane

R.T.: 6.193 min
Delta R.T.: -0.045 min
Response: 12728200
Conc: 0.39 ng/ml

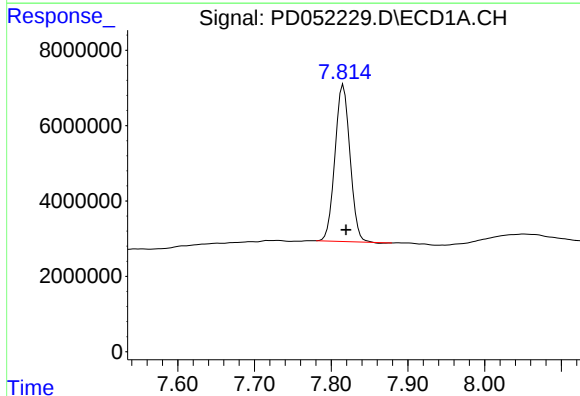

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.003 min
Response: 56574076
Conc: 36.13 ng/ml

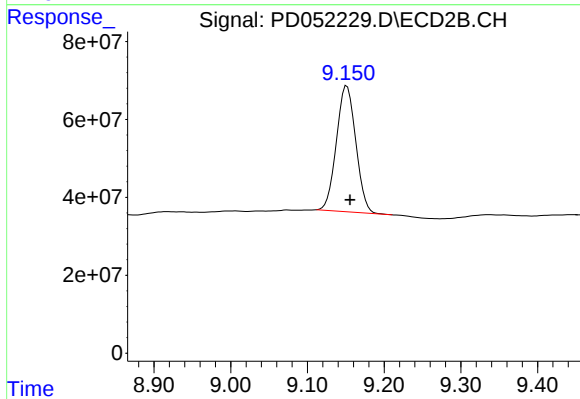

#27 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: -0.004 min
Response: 568028641
Conc: 36.80 ng/ml