

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
 Data File : PD052234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 7:35
 Operator : AJ\SJ
 Sample : PIBLK04
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 08:47:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 25 18:59:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.041	33353246	639.8E6	23.498	21.987
27)	SA Decachlor...	7.816	9.151	59716562	609.3E6	38.136	39.469
Target Compounds							
6)	B beta-BHC	0.000	4.937f	0	22905911	N.D.	1.248
8)	B Heptachlo...	0.000	5.922	0	166.4E6	N.D.	4.884
10)	B trans-Chl...	0.000	6.176	0	195.3E6	N.D.	5.750
11)	B cis-Chlor...	0.000	6.210	0	14950112	N.D.	0.460
20)	A Methoxychlor	0.000	7.579f	0	5825067	N.D.	0.626
22)	Toxaphene-1	5.484	0.000	6808225	0	532.330	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032719\
Data File : PD052234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 7:35
Operator : AJ\SJ
Sample : PIBLK04
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 08:47:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032519CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 25 18:59:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

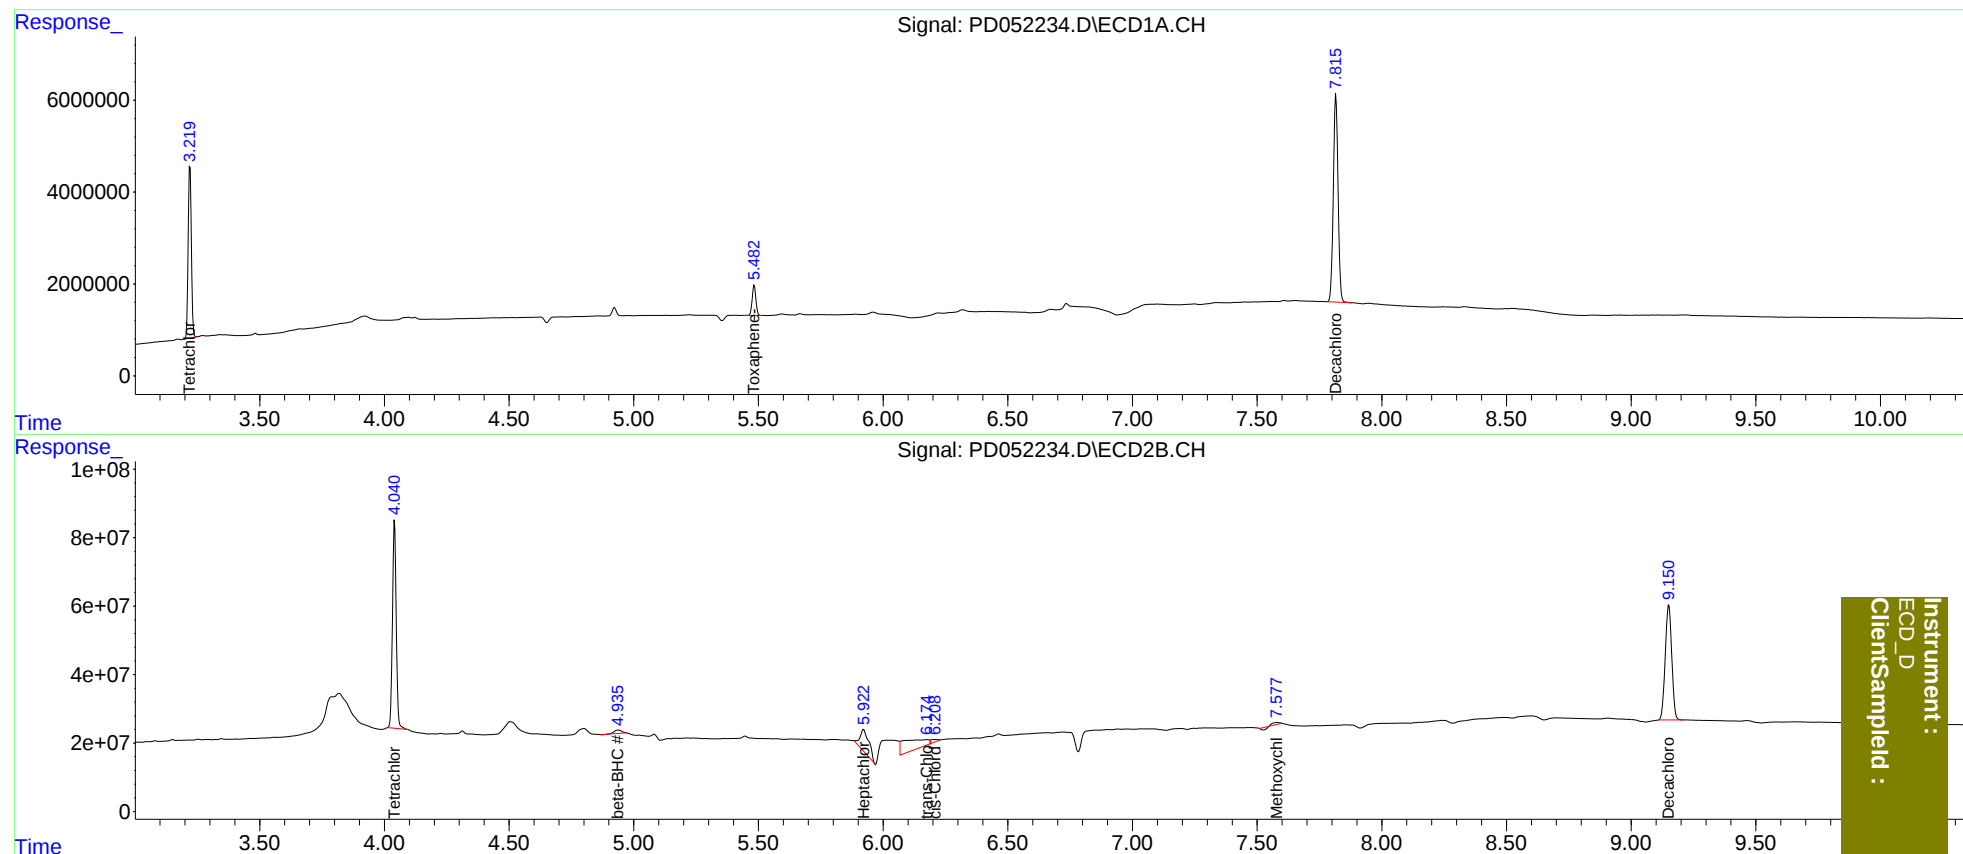


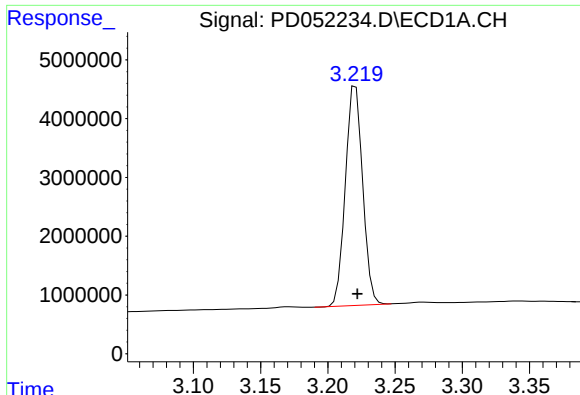

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: -0.001 min
Response: 33353246
Conc: 23.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

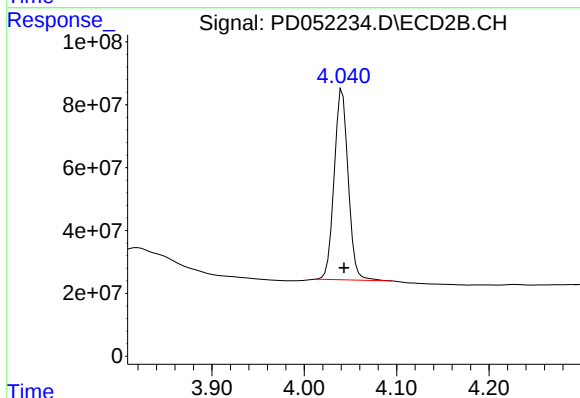


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 639758547
Conc: 21.99 ng/ml

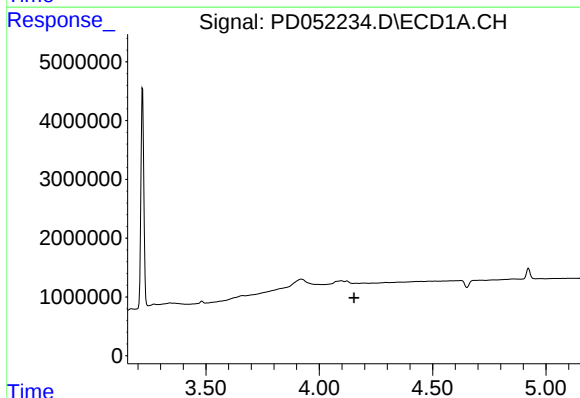


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.154 min
Response: 0
Conc: N.D.

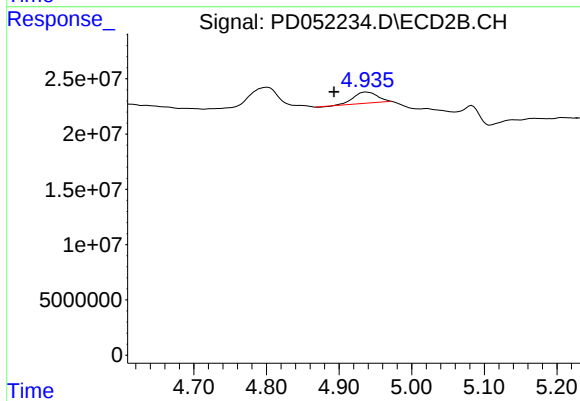

#6 beta-BHC


R.T.: 4.937 min
Delta R.T.: 0.044 min
Response: 22905911
Conc: 1.25 ng/ml

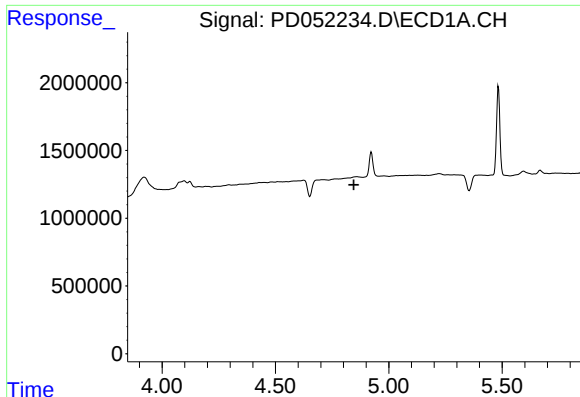

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

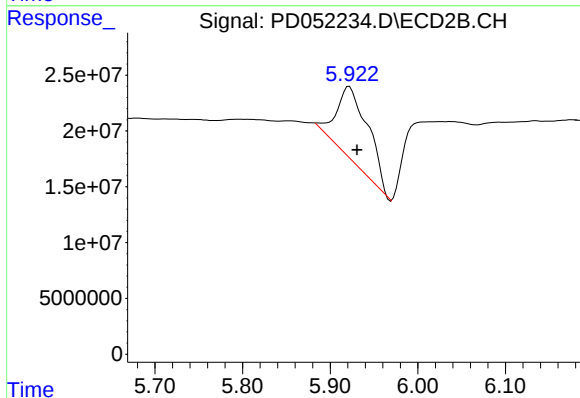


#8 Heptachlor epoxide

R.T.: 5.922 min
Delta R.T.: -0.009 min
Response: 166372213
Conc: 4.88 ng/ml

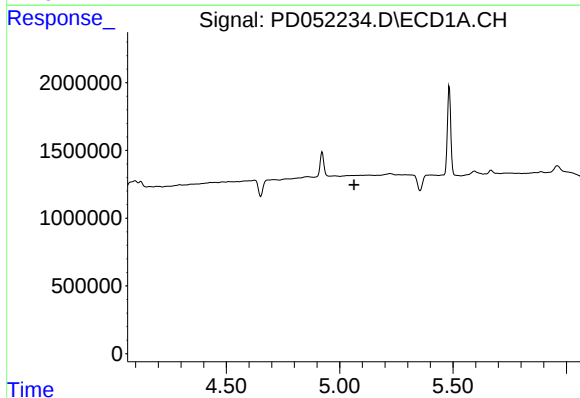


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

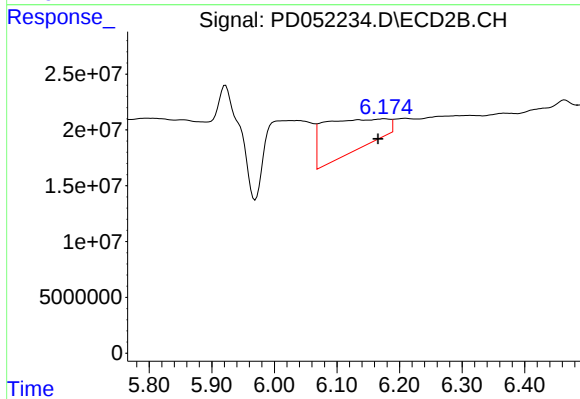

#10 trans-Chlordane


R.T.: 6.176 min
Delta R.T.: 0.010 min
Response: 195274117
Conc: 5.75 ng/ml

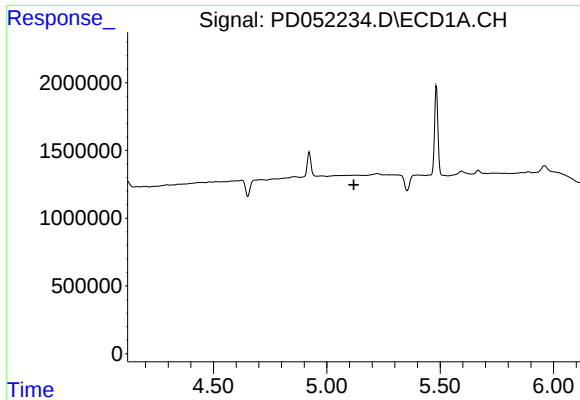

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

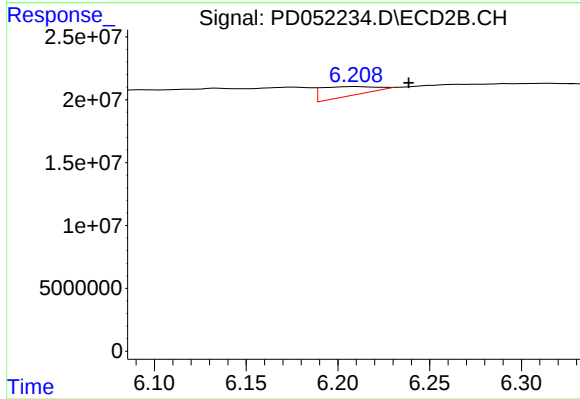


#11 cis-Chlordane

R.T.: 6.210 min
Delta R.T.: -0.029 min
Response: 14950112
Conc: 0.46 ng/ml

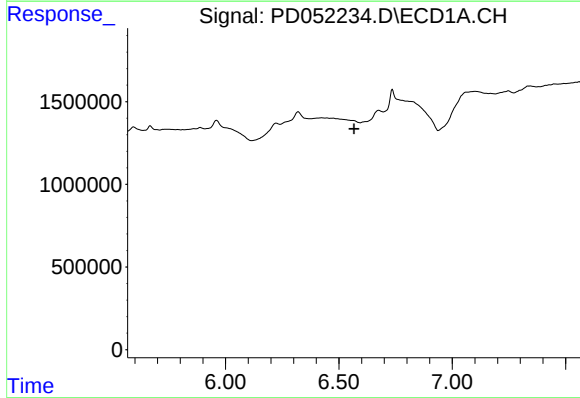


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.567 min
Response: 0
Conc: N.D.

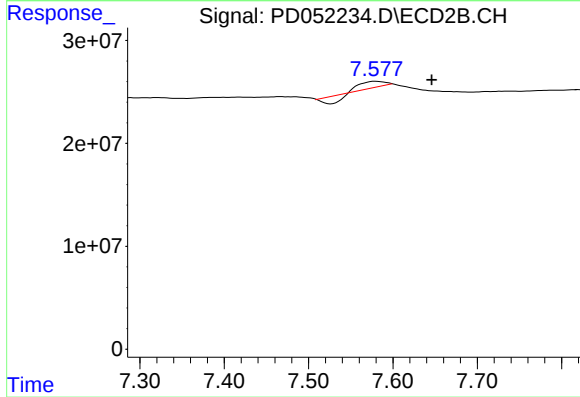

#20 Methoxychlor


R.T.: 7.579 min
Delta R.T.: -0.067 min
Response: 5825067
Conc: 0.63 ng/ml

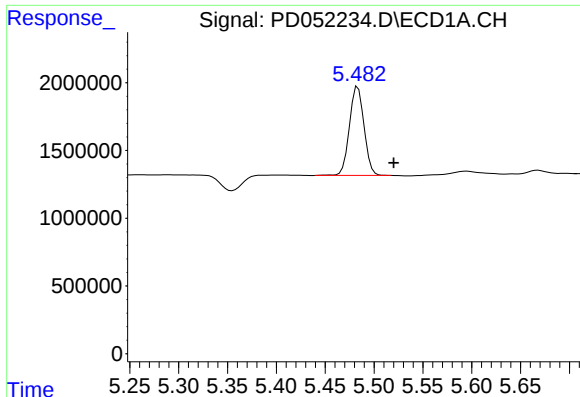

#22 Toxaphene-1


R.T.: 5.484 min
Delta R.T.: -0.037 min
Response: 6808225
Conc: 532.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

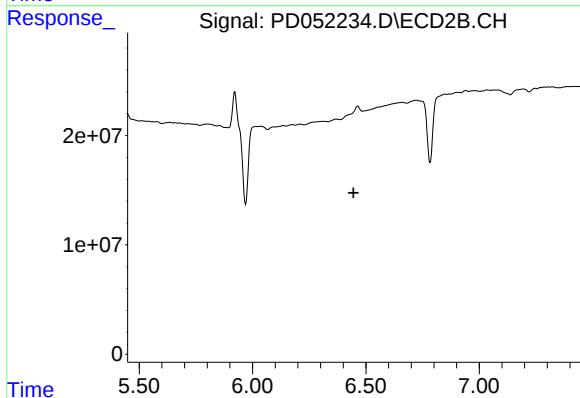


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 6.446 min
Response: 0
Conc: N.D.

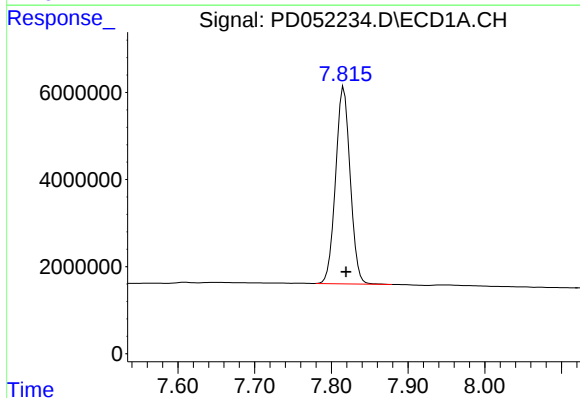

#27 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: -0.003 min
Response: 59716562
Conc: 38.14 ng/ml

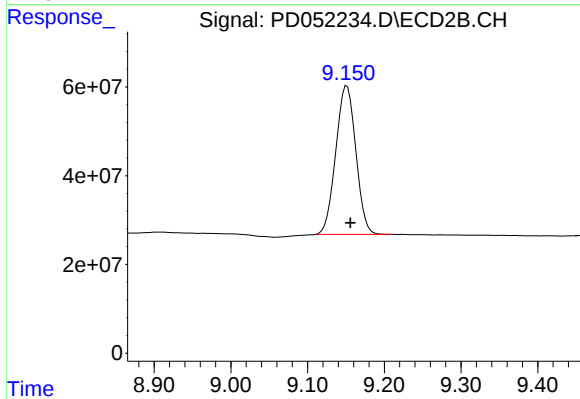

#27 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: -0.005 min
Response: 609272977
Conc: 39.47 ng/ml