

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
 Data File : PD057638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 12:23
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 14:00:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 13:59:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	3.895	58789264	59480632	77.039	76.289
28)	SA Decachlor...	7.866	8.898	55769593	63103920	74.519	74.459
Target Compounds							
23)	Chlordane-1	4.056	4.875	18655609	23718035	756.431	766.550
24)	Chlordane-2	4.541	5.337	20961166	27129754	743.852	724.498
25)	Chlordane-3	5.090	5.978	67271723	109.7E6	782.421	764.117
26)	Chlordane-4	5.145	6.051	61768016	131.2E6	781.548	758.084
27)	Chlordane-5	5.962	6.849	20513390	26005227	764.270	757.726



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD032720\
Data File : PD057638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 12:23
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 14:00:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 13:59:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

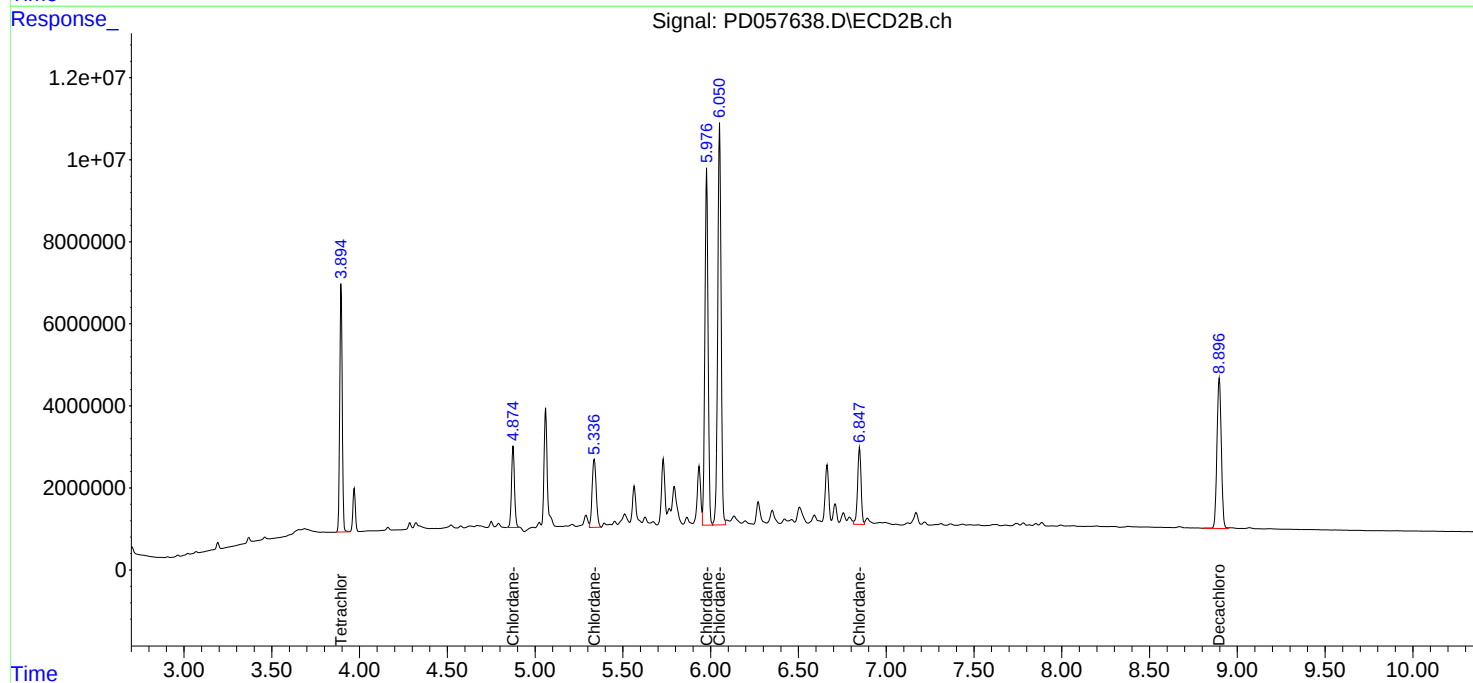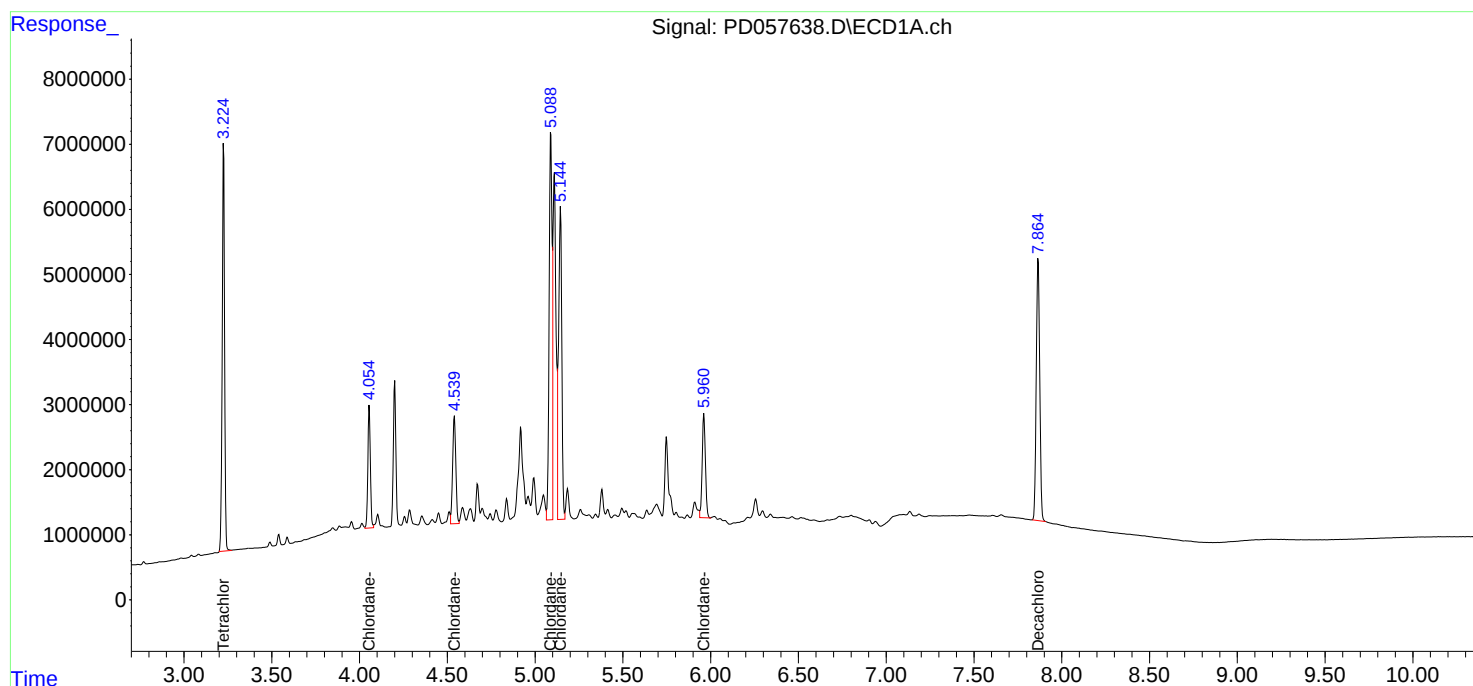


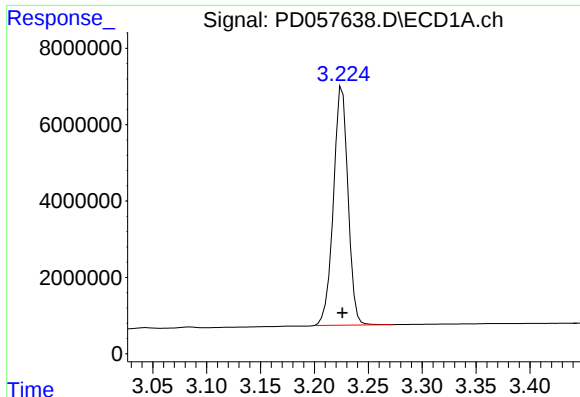

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 58789264
Conc: 77.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

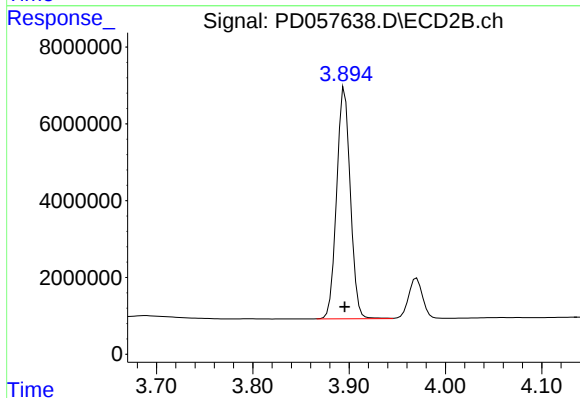


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 59480632
Conc: 76.29 ng/ml

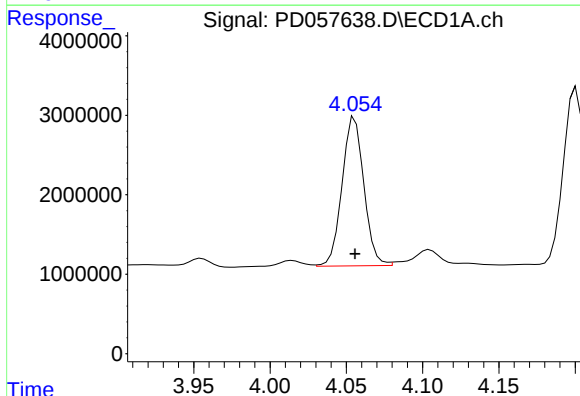


#23 Chlordane-1

R.T.: 4.056 min
Delta R.T.: 0.000 min
Response: 18655609
Conc: 756.43 ng/ml

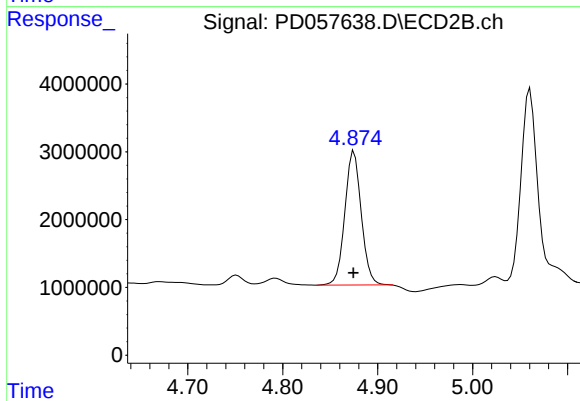

#23 Chlordane-1


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 23718035
Conc: 766.55 ng/ml

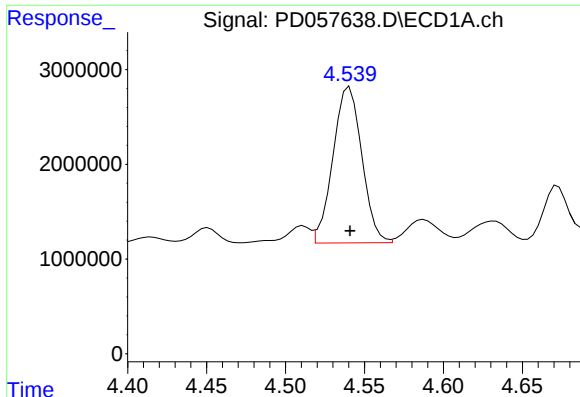

#24 Chlordane-2


R.T.: 4.541 min
Delta R.T.: 0.000 min
Response: 20961166
Conc: 743.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

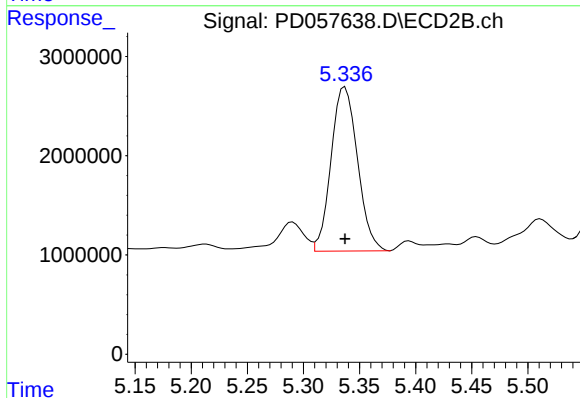


#24 Chlordane-2

R.T.: 5.337 min
Delta R.T.: 0.000 min
Response: 27129754
Conc: 724.50 ng/ml

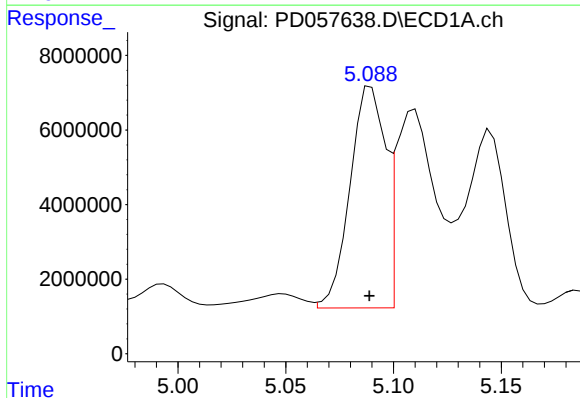


#25 Chlordane-3

R.T.: 5.090 min
Delta R.T.: 0.000 min
Response: 67271723
Conc: 782.42 ng/ml

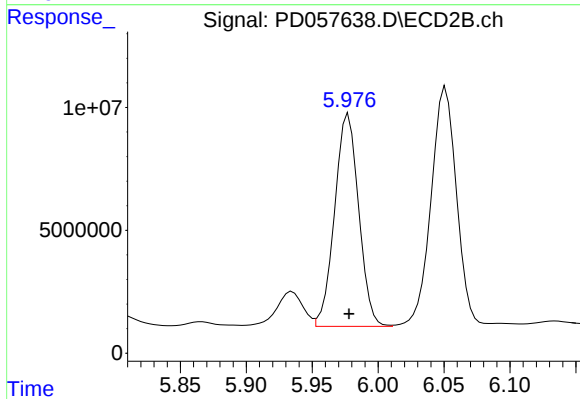

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 109699338
Conc: 764.12 ng/ml

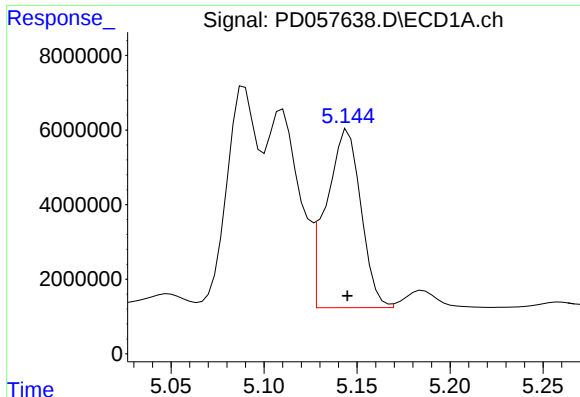

#26 Chlordane-4


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 61768016
Conc: 781.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

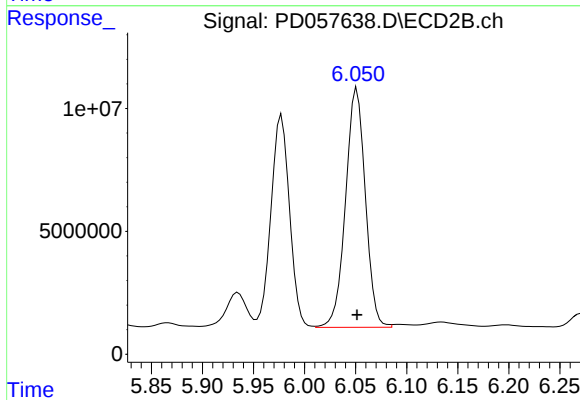


#26 Chlordane-4

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 131219988
Conc: 758.08 ng/ml

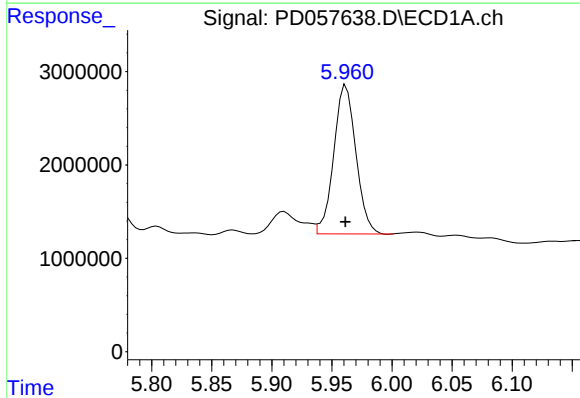


#27 Chlordane-5

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 20513390
Conc: 764.27 ng/ml

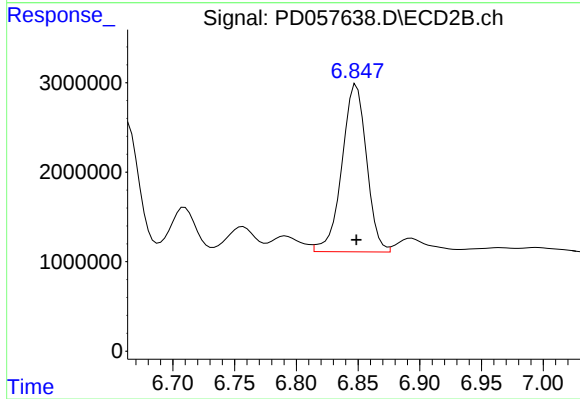

#27 Chlordane-5


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 26005227
Conc: 757.73 ng/ml

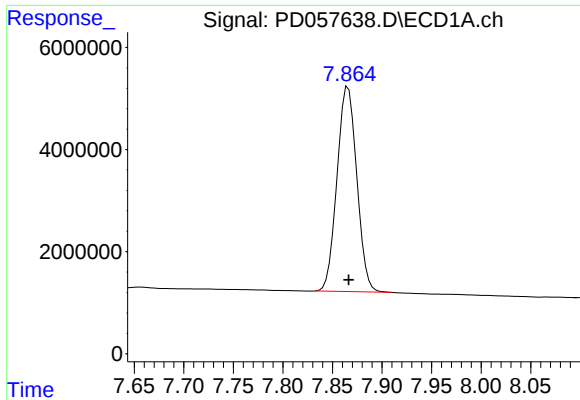

#28 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 55769593
Conc: 74.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

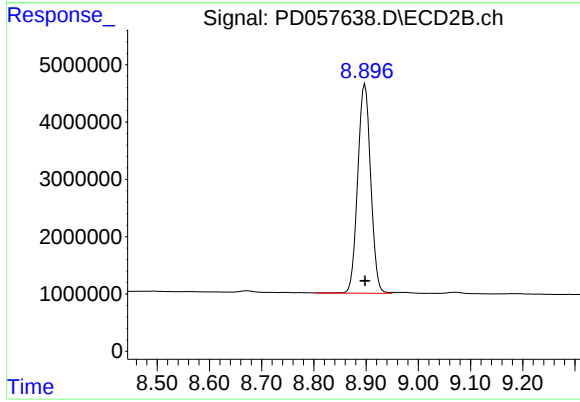

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 63103920
Conc: 74.46 ng/ml